


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX082918\
 Data File : VX004301.D
 Acq On : 29 Aug 2018 19:24
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
 Title : SW846 8260
 Last Update : Thu Aug 23 05:39:44 2018

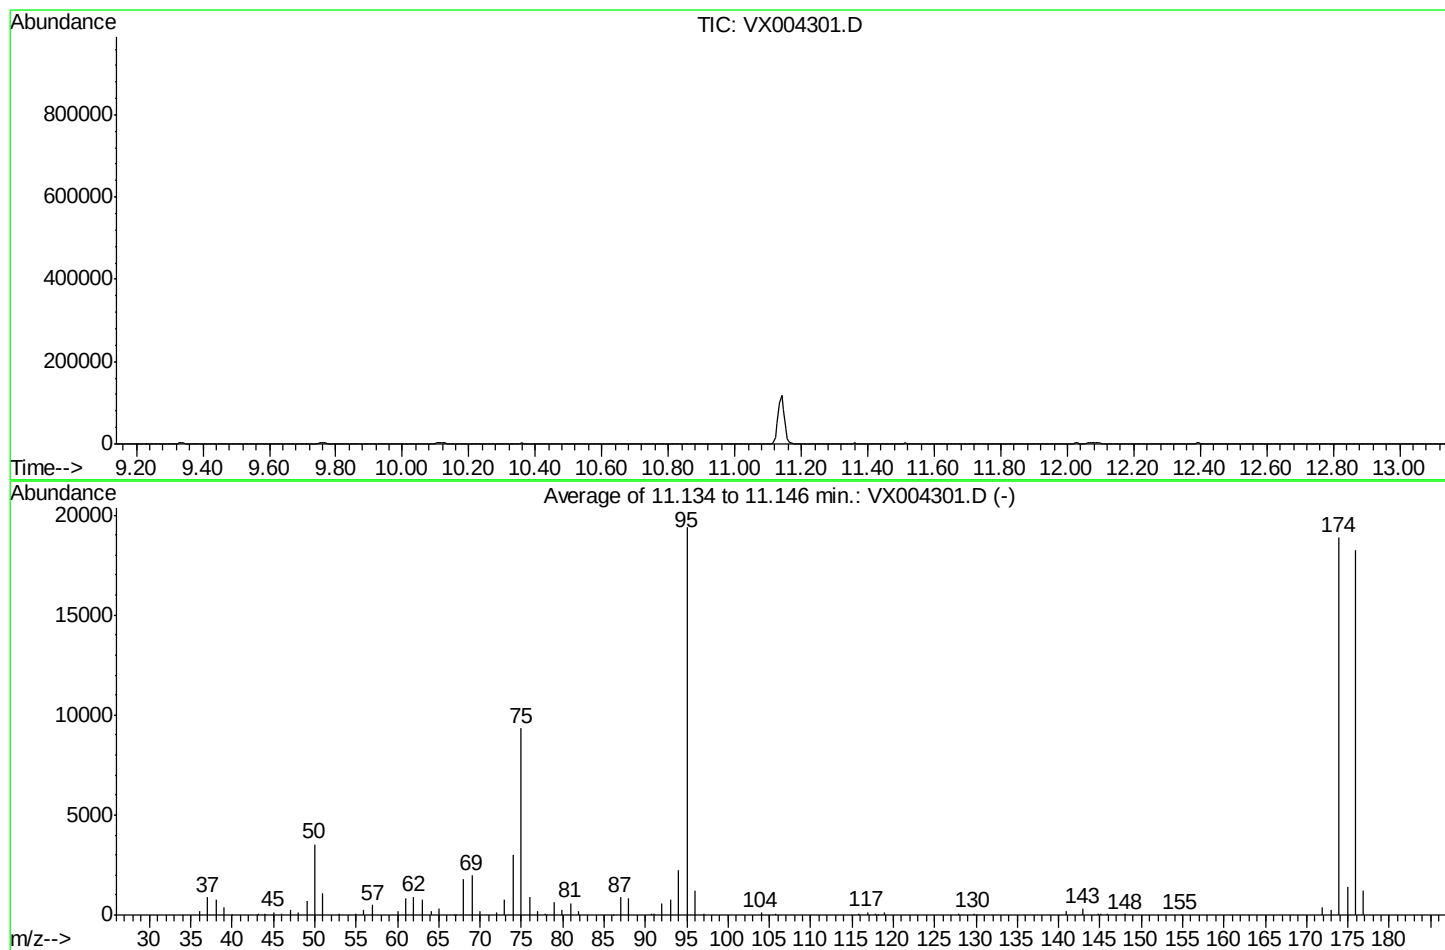

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	3532	PASS
75	95	30	60	48.1	9316	PASS
95	95	100	100	100.0	19382	PASS
96	95	5	9	6.4	1243	PASS
173	174	0.00	2	1.4	266	PASS
174	95	50	100	97.3	18858	PASS
175	174	5	9	7.5	1407	PASS
176	174	95	101	96.8	18248	PASS
177	176	5	9	6.6	1197	PASS