

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082923\
 Data File : VX037361.D
 Acq On : 30 Aug 2023 01:32
 Operator : JC/MD
 Sample : PB155153TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB155153TB

Quant Time: Aug 30 03:48:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 18 09:30:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	191129	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	323282	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	298161	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	136369	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	121655	44.150	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	88.300%		
35) Dibromofluoromethane	5.385	113	102800	48.014	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.020%		
50) Toluene-d8	8.647	98	372542	47.969	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	95.940%		
62) 4-Bromofluorobenzene	11.079	95	148113	48.529	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	97.060%		
Target Compounds						
					Qvalue	
3) Chloromethane	1.252	50	1307	0.673	ug/l #	43
6) Chloroethane	1.709	64	589	0.473	ug/l #	43
11) Tert butyl alcohol	2.953	59	643	0.995	ug/l #	78
13) Acrolein	2.240	56	204	0.415	ug/l #	74
15) Acrylonitrile	3.075	53	273	0.237	ug/l #	71
16) Acetone	2.380	43	24720	22.932	ug/l #	88
18) Methyl Acetate	2.709	43	1681	0.414	ug/l	97
20) Methylene Chloride	2.788	84	11785	4.889	ug/l #	85
25) 2-Butanone	4.568	43	14375	8.857	ug/l	96
29) Tetrahydrofuran	5.026	42	737	0.712	ug/l #	75
31) Cyclohexane	5.544	56	3757	1.213	ug/l #	1
36) 1,1-Dichloropropene	5.550	75	14527	4.776	ug/l #	51
37) Ethyl Acetate	4.721	43	3068	0.987	ug/l #	93
38) Carbon Tetrachloride	5.550	117	20456	6.191	ug/l #	15
41) Methacrylonitrile	5.038	41	376	0.233	ug/l #	37
43) Isopropyl Acetate	6.336	43	102597	20.798	ug/l #	91
48) Methyl methacrylate	7.793	41	87400	36.329	ug/l #	47
49) 1,4-Dioxane	7.787	88	147	2.269	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	120072	40.084	ug/l #	37
53) t-1,3-Dichloropropene	8.952	75	843	0.244	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	45839	12.274	ug/l #	51
57) 1,3-Dichloropropane	9.482	76	5699	1.440	ug/l #	42
58) 2-Chloroethyl Vinyl ether	8.251	63	792	0.449	ug/l	98
59) 2-Hexanone	9.372	43	98885	43.295	ug/l #	26
74) N-amyl acetate	10.817	43	831	0.216	ug/l #	48
76) 1,2,3-Trichloropropane	11.079	75	72660	25.019	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	72660	69.879	ug/l #	5
93) 1,2,4-Trichlorobenzene	13.591	180	691	0.266	ug/l	92
96) 1,2,3-Trichlorobenzene	13.963	180	677	0.262	ug/l	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082923\
Data File : VX037361.D
Acq On : 30 Aug 2023 01:32
Operator : JC/MD
Sample : PB155153TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB155153TB

Quant Time: Aug 30 03:48:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 18 09:30:38 2023
Response via : Initial Calibration




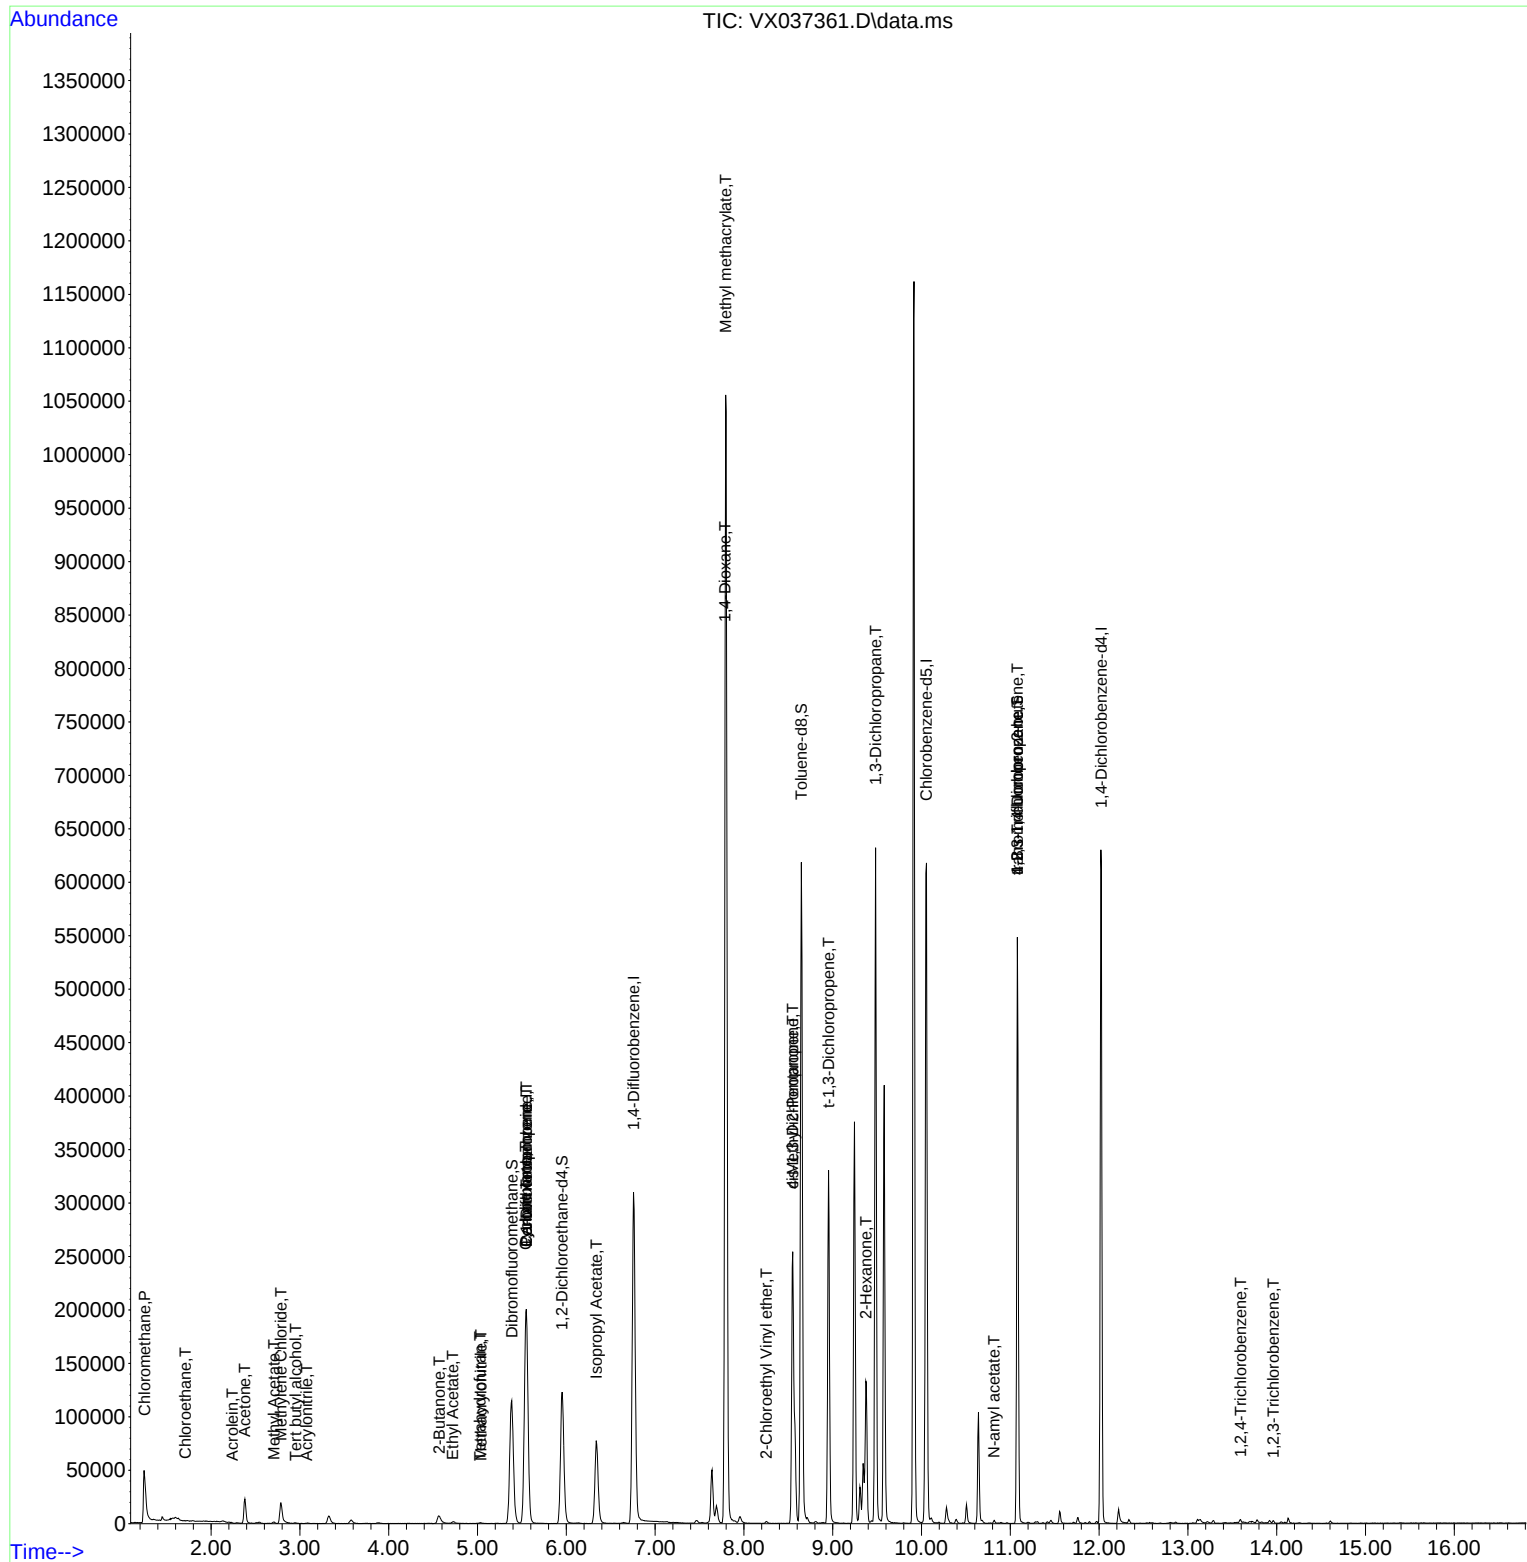


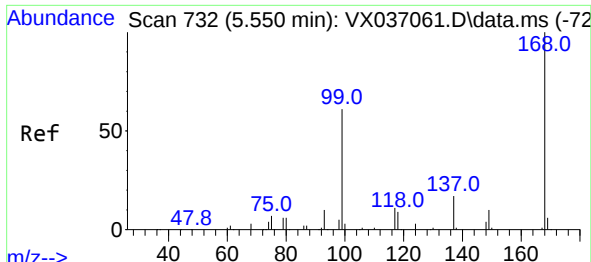

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32




Instrument :
MSVOA_X
ClientSampleId :
PB155153TB

Tgt Ion:168 Resp: 191129
Ion Ratio Lower Upper
168 100
99 62.2 56.6 85.0

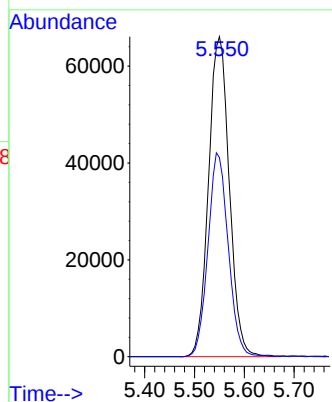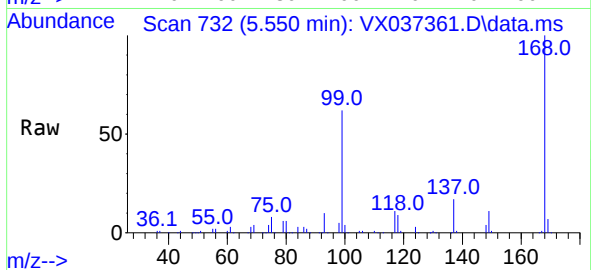


#3
Chloromethane
Concen: 0.673 ug/l
RT: 1.252 min Scan# 27
Delta R.T. -0.049 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Tgt Ion: 50 Resp: 1307
Ion Ratio Lower Upper
50 100
52 0.0 25.5 38.3#

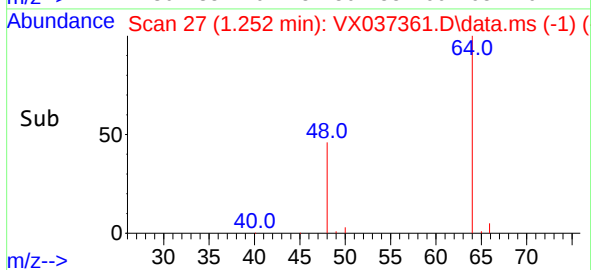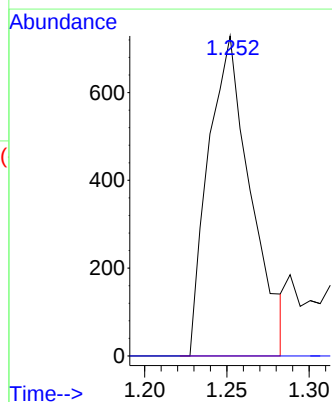

Abundance Scan 96 (1.672 min): VX037061.D\data.ms (-90)

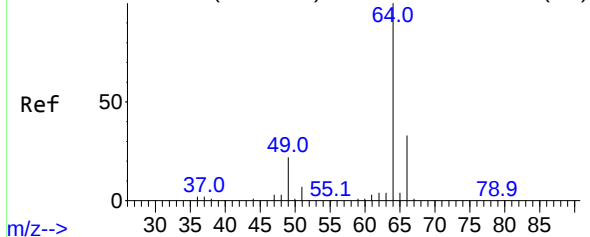

#6

Chloroethane

Concen: 0.473 ug/l

RT: 1.709 min Scan# 102

Delta R.T. 0.037 min

Lab File: VX037361.D

Acq: 30 Aug 2023 01:32

Instrument :

MSVOA_X

ClientSampleId :

PB155153TB


Tgt Ion: 64 Resp: 589

Ion Ratio Lower Upper


64 100

66 0.0 25.1 37.7#


Abundance Scan 102 (1.709 min): VX037361.D\data.ms

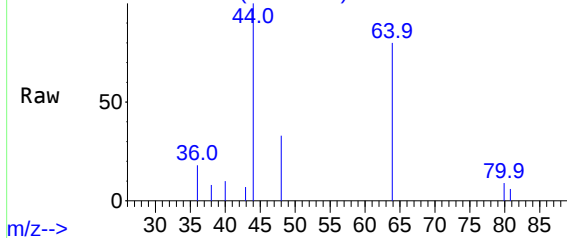


Abundance

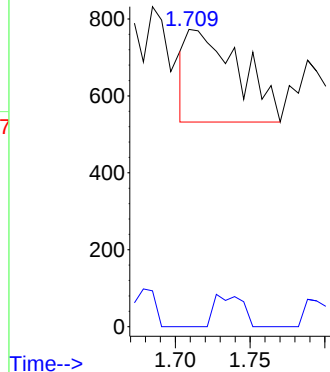

Abundance Scan 102 (1.709 min): VX037361.D\data.ms (-47)

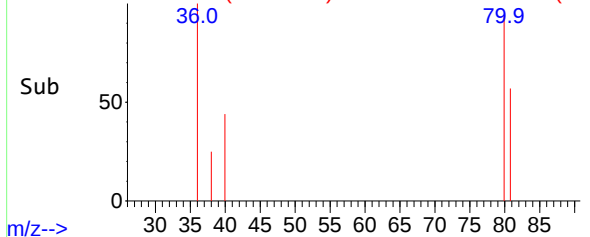

Abundance Scan 310 (2.977 min): VX037061.D\data.ms (-29)

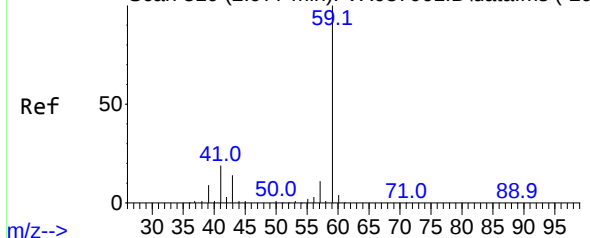

#11

Tert butyl alcohol

Concen: 0.995 ug/l

RT: 2.953 min Scan# 306

Delta R.T. -0.024 min

Lab File: VX037361.D

Acq: 30 Aug 2023 01:32


Tgt Ion: 59 Resp: 643

Ion Ratio Lower Upper


59 100

57 0.0 6.0 9.0#


Abundance Scan 306 (2.953 min): VX037361.D\data.ms

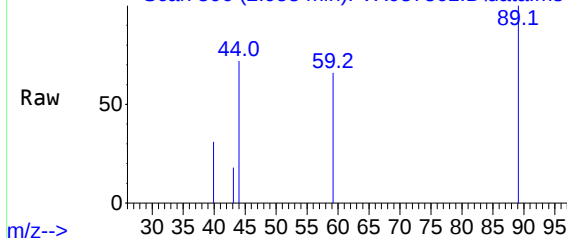


Abundance

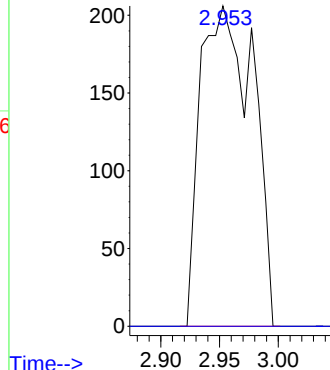

Abundance Scan 306 (2.953 min): VX037361.D\data.ms (-26)




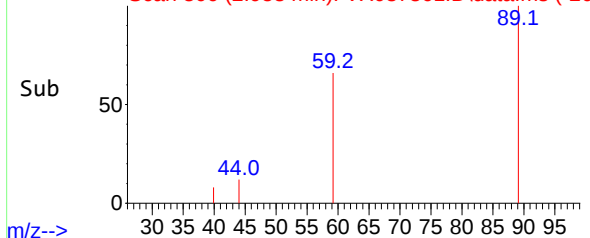




#13
Acrolein
Concen: 0.415 ug/l
RT: 2.240 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32




Instrument :
MSVOA_X
ClientSampleId :
PB155153TB


Tgt Ion: 56 Resp: 204
Ion Ratio Lower Upper
56 100
55 92.6 57.1 85.7#

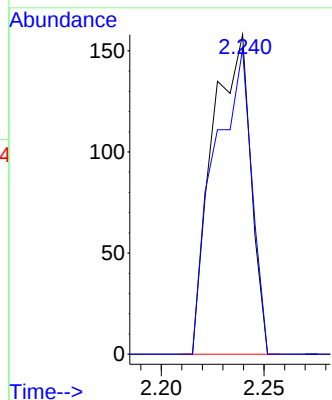

#15
Acrylonitrile
Concen: 0.237 ug/l
RT: 3.075 min Scan# 326
Delta R.T. 0.012 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Tgt Ion: 53 Resp: 273
Ion Ratio Lower Upper
53 100
52 70.0 66.0 99.0
51 0.0 29.8 44.6#


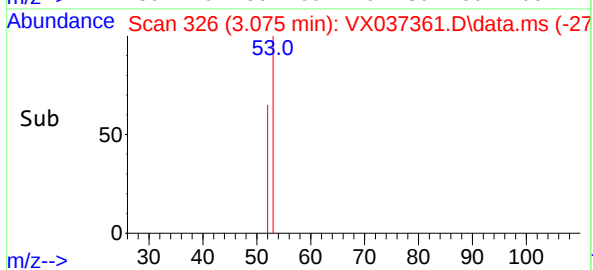
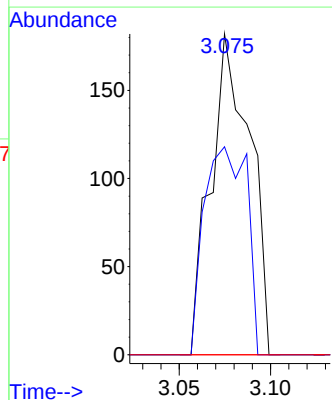





#16
Acetone
Concen: 22.932 ug/l
RT: 2.380 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32




Instrument :
MSVOA_X
ClientSampleId :
PB155153TB


Tgt Ion: 43 Resp: 24720
Ion Ratio Lower Upper
43 100
58 33.9 21.9 32.9#

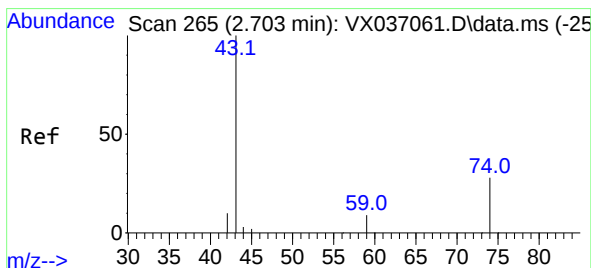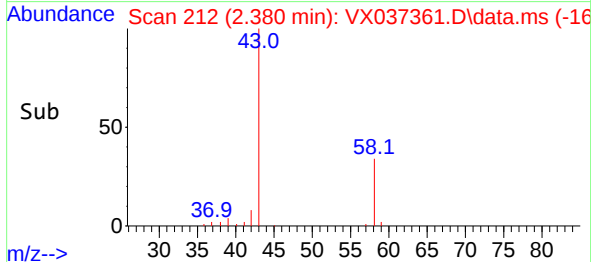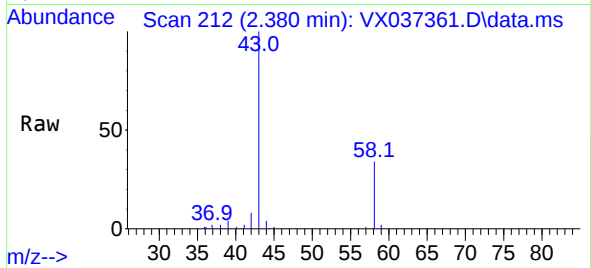

#18
Methyl Acetate
Concen: 0.414 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Tgt Ion: 43 Resp: 1681
Ion Ratio Lower Upper
43 100
74 23.9 17.8 26.8


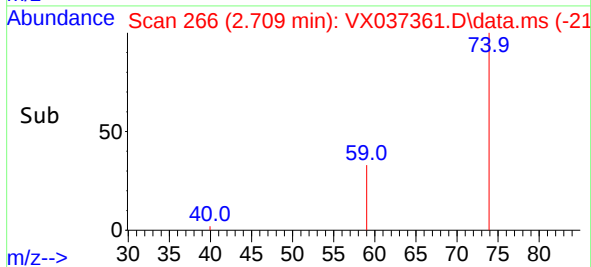

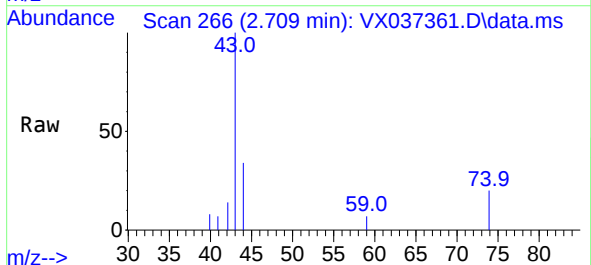




#20
Methylene Chloride
Concen: 4.889 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32




Instrument :
MSVOA_X
ClientSampleId :
PB155153TB


Tgt Ion:	84	Resp:	11785
Ion	Ratio	Lower	Upper
84	100		
49	107.8	103.6	155.4
51	28.2	33.8	50.6#
86	63.8	49.4	74.0

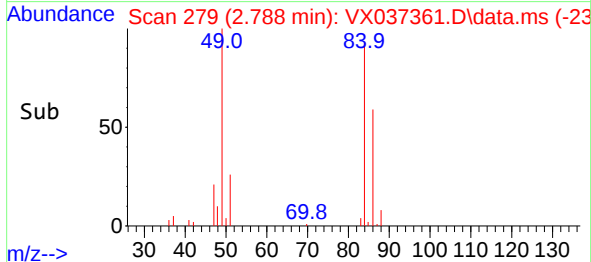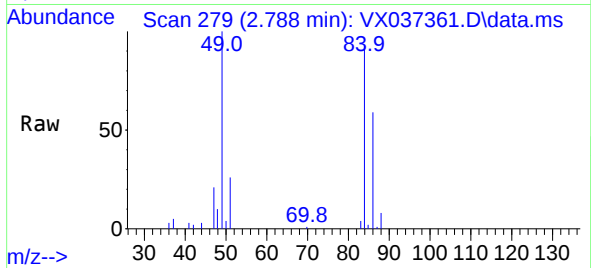

#25
2-Butanone
Concen: 8.857 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.012 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Tgt Ion:	43	Resp:	14375
Ion	Ratio	Lower	Upper
43	100		
72	26.3	19.4	29.2

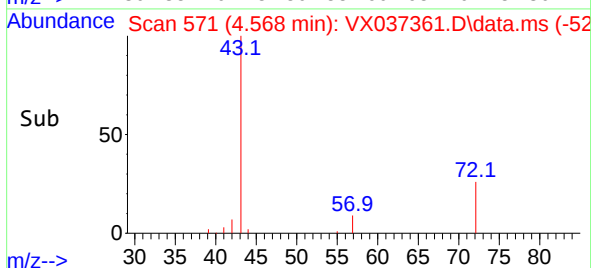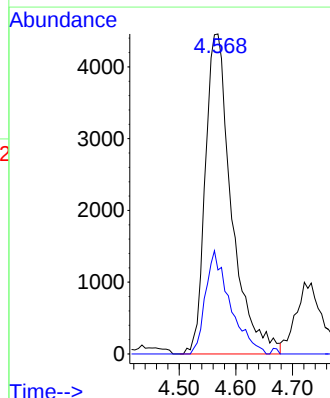



#29

Tetrahydrofuran

Concen: 0.712 ug/l

RT: 5.026 min Scan# 643

Delta R.T. 0.018 min

Lab File: VX037361.D

Acq: 30 Aug 2023 01:32

Instrument :

MSVOA_X

ClientSampleId :

PB155153TB





Tgt Ion: 42 Resp: 737

Ion Ratio Lower Upper

42 100

72 24.8 34.2 51.4#

71 26.2 32.2 48.2#

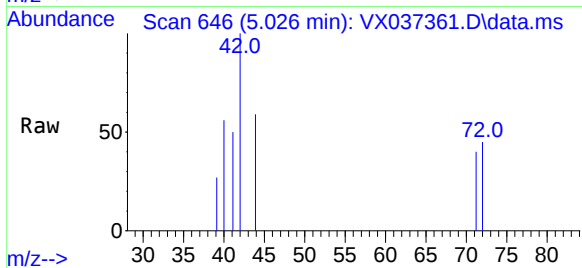

#31

Cyclohexane

Concen: 1.213 ug/l

RT: 5.544 min Scan# 731

Delta R.T. 0.073 min

Lab File: VX037361.D

Acq: 30 Aug 2023 01:32




Tgt Ion: 56 Resp: 3757


Ion Ratio Lower Upper

56 100

69 190.4 23.4 35.2#

84 148.0 65.9 98.9#

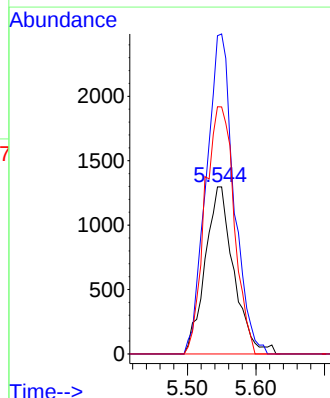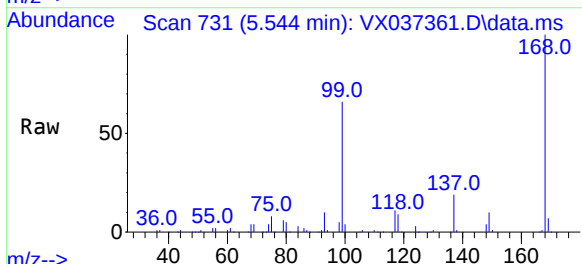



#33

1,2-Dichloroethane-d4

Concen: 44.150 ug/l

RT: 5.952 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX037361.D

Acq: 30 Aug 2023 01:32

Instrument :

MSVOA_X

ClientSampleId :





PB155153TB

Tgt Ion: 65 Resp: 121655

Ion Ratio Lower Upper

65 100

67 51.6 0.0 100.2

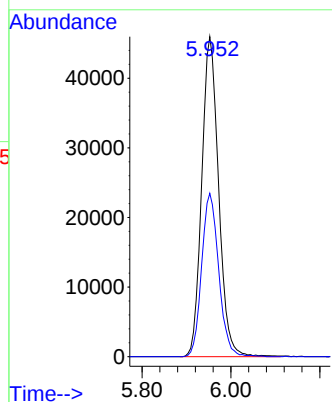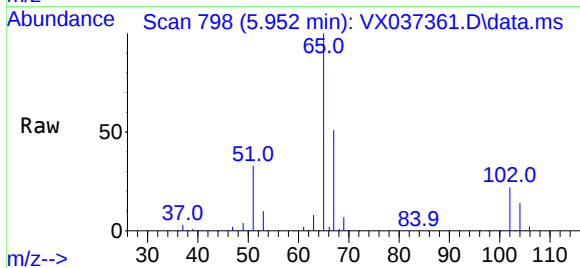

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.006 min

Lab File: VX037361.D

Acq: 30 Aug 2023 01:32




Tgt Ion: 114 Resp: 323282


Ion Ratio Lower Upper

114 100

63 19.4 0.0 45.0


88 16.7 0.0 36.6

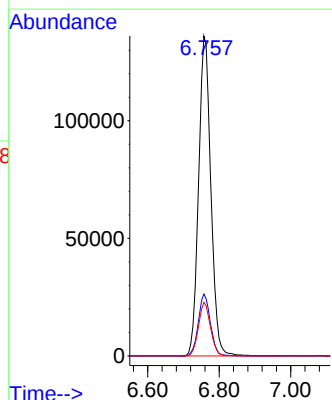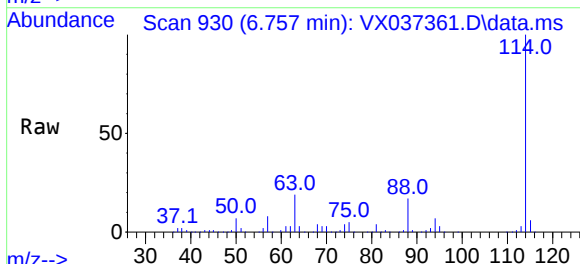



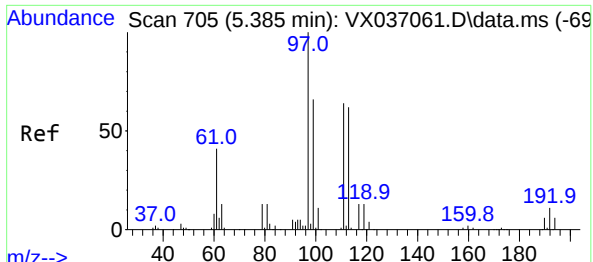


#35
Dibromofluoromethane
Concen: 48.014 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Instrument :
MSVOA_X
ClientSampleId :
PB155153TB



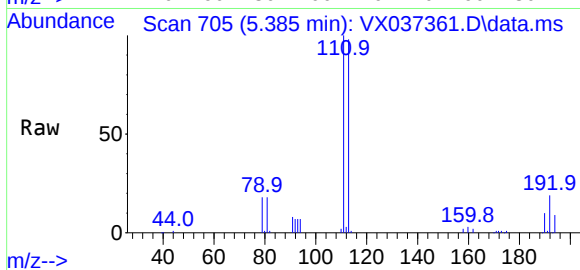



Tgt Ion:113 Resp: 102800
Ion Ratio Lower Upper
113 100
111 102.5 82.9 124.3
192 18.9 13.3 19.9

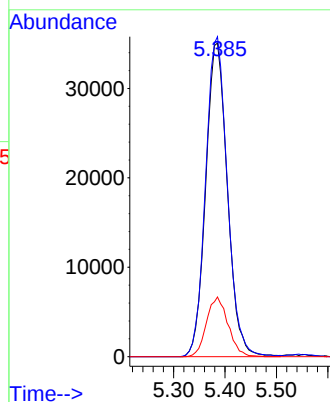

#36
1,1-Dichloropropene
Concen: 4.776 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.146 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Tgt Ion: 75 Resp: 14527
Ion Ratio Lower Upper
75 100
110 9.7 17.0 50.9#
77 0.0 24.7 37.1#


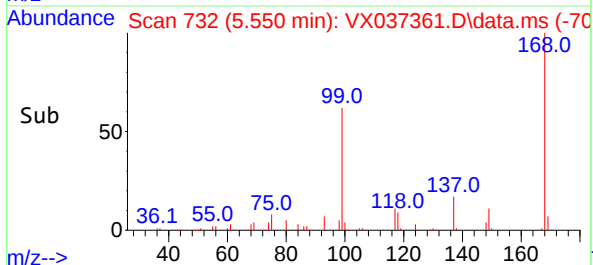

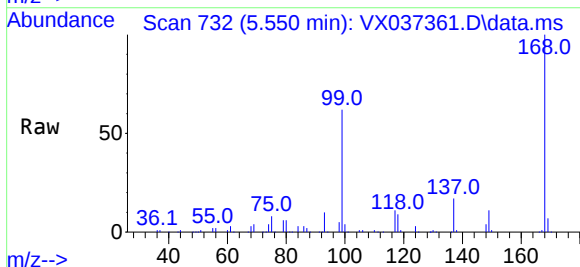




#37
Ethyl Acetate
Concen: 0.987 ug/l
RT: 4.721 min Scan# 595
Delta R.T. 0.006 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32




Instrument :
MSVOA_X
ClientSampleId :
PB155153TB


Tgt Ion:	43	Resp:	3068
Ion	Ratio	Lower	Upper
43	100		
61	9.8	10.6	16.0#
70	8.5	8.3	12.5

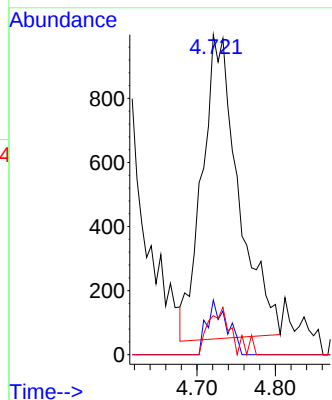

#38
Carbon Tetrachloride
Concen: 6.191 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.122 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Tgt Ion:	117	Resp:	20456
Ion	Ratio	Lower	Upper
117	100		
119	5.2	78.2	117.2#
121	0.0	24.4	36.6#


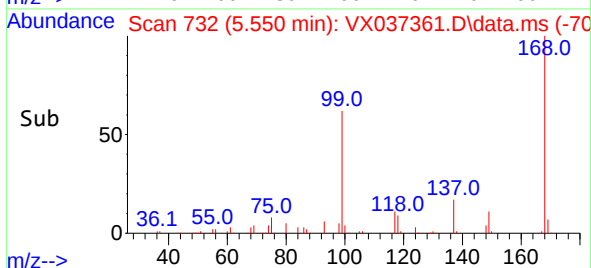
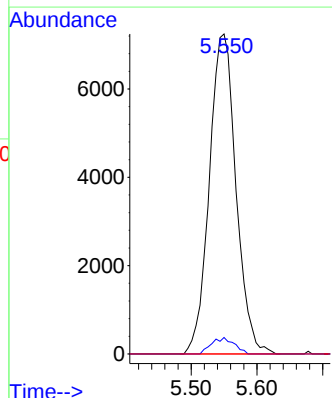



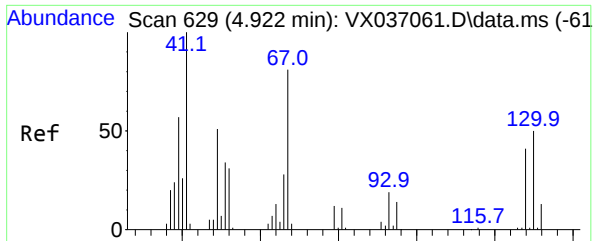

#41
Methacrylonitrile
Concen: 0.233 ug/l
RT: 5.038 min Scan# 641
Delta R.T. 0.116 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32




Instrument :
MSVOA_X
ClientSampleId :
PB155153TB


Tgt Ion: 41	Resp:	376
Ion	Ratio	Lower Upper
41	100	
39	24.5	45.2 67.8#
67	0.0	52.6 78.8#
52	0.0	22.7 34.1#



#43
Isopropyl Acetate
Concen: 20.798 ug/l
RT: 6.336 min Scan# 861
Delta R.T. -0.006 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Tgt Ion: 43	Resp:	102597
Ion	Ratio	Lower Upper
43	100	
61	22.7	15.2 22.8
87	16.3	9.8 14.6#


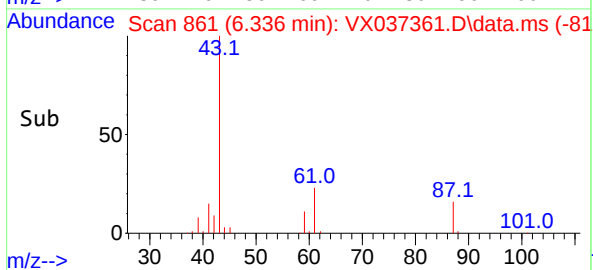






#48
Methyl methacrylate
Concen: 36.329 ug/l
RT: 7.793 min Scan# 1100
Delta R.T. 0.098 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32




Instrument :
MSVOA_X
ClientSampleId :
PB155153TB


Tgt Ion: 41 Resp: 87400
Ion Ratio Lower Upper
41 100
69 0.1 59.2 88.8#
39 51.4 47.7 71.5

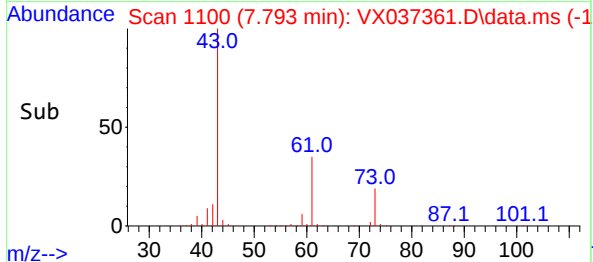

#49
1,4-Dioxane
Concen: 2.269 ug/l
RT: 7.787 min Scan# 1099
Delta R.T. 0.128 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Tgt Ion: 88 Resp: 147
Ion Ratio Lower Upper
88 100
43 640297.3 0.0 0.0#
58 3027.2 60.1 90.1#


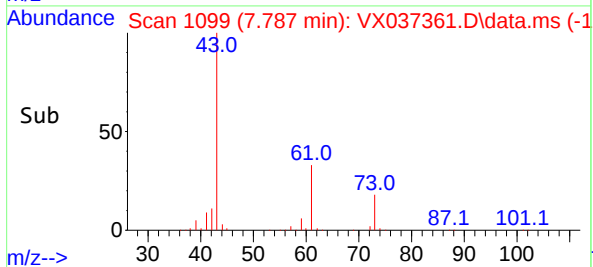

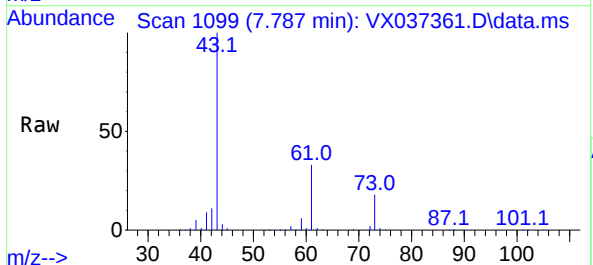




#50
Toluene-d8
Concen: 47.969 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32




Instrument :
MSVOA_X
ClientSampleId :
PB155153TB


Tgt Ion: 98 Resp: 372542
Ion Ratio Lower Upper
98 100
100 66.8 53.1 79.7



#51
4-Methyl-2-Pentanone
Concen: 40.084 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.024 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Tgt Ion: 43 Resp: 120072
Ion Ratio Lower Upper
43 100
58 0.0 30.4 45.6#


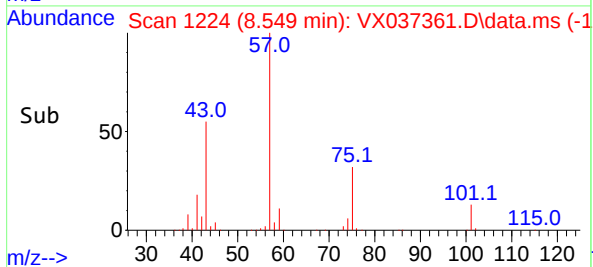

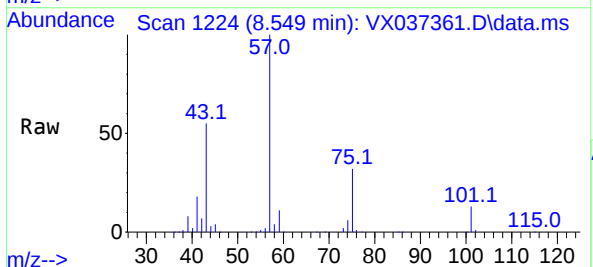




#53
 t-1,3-Dichloropropene
 Concen: 0.244 ug/l
 RT: 8.952 min Scan# 11
 Delta R.T. -0.024 min
 Lab File: VX037361.D
 Acq: 30 Aug 2023 01:32




Instrument :
 MSVOA_X
 ClientSampleId :
 PB155153TB


Tgt Ion: 75 Resp: 843
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.7 38.5#

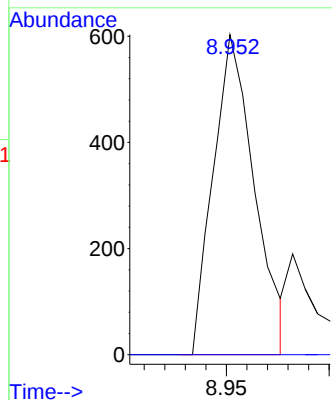

#54
 cis-1,3-Dichloropropene
 Concen: 12.274 ug/l
 RT: 8.549 min Scan# 1224
 Delta R.T. 0.183 min
 Lab File: VX037361.D
 Acq: 30 Aug 2023 01:32

Tgt Ion: 75 Resp: 45839
 Ion Ratio Lower Upper
 75 100
 77 0.6 25.3 37.9#
 39 25.0 46.7 70.1#


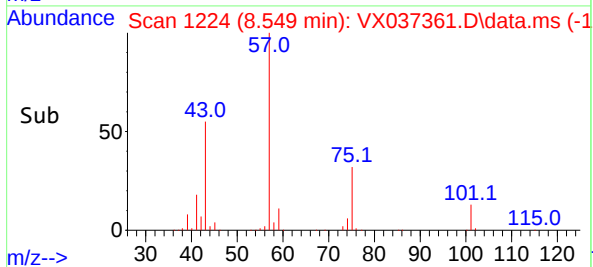
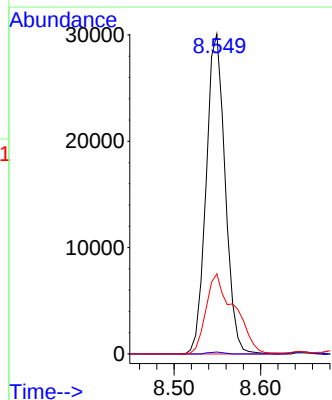
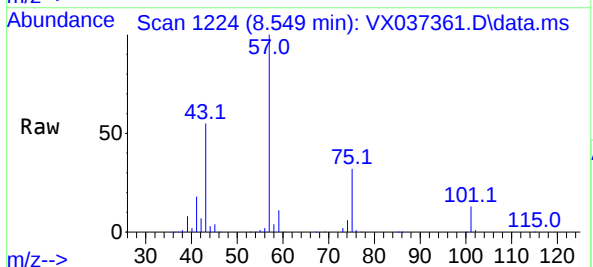




#57
1,3-Dichloropropane
Concen: 1.440 ug/l
RT: 9.482 min Scan# 1175
Delta R.T. 0.177 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32




Instrument :
MSVOA_X
ClientSampleId :
PB155153TB


Tgt Ion: 76 Resp: 5699
Ion Ratio Lower Upper
76 100
78 0.0 26.1 39.1#



#58
2-Chloroethyl Vinyl ether
Concen: 0.449 ug/l
RT: 8.251 min Scan# 1175
Delta R.T. 0.006 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Tgt Ion: 63 Resp: 792
Ion Ratio Lower Upper
63 100
106 29.3 22.5 33.7









#59
2-Hexanone
Concen: 43.295 ug/l
RT: 9.372 min Scan# 11
Delta R.T. -0.061 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32




Instrument :
MSVOA_X
ClientSampleId :
PB155153TB


Tgt Ion: 43 Resp: 98885
Ion Ratio Lower Upper
43 100
58 0.0 26.2 78.5#



#62
4-Bromofluorobenzene
Concen: 48.529 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Tgt Ion: 95 Resp: 148113
Ion Ratio Lower Upper
95 100
174 74.3 0.0 135.6
176 72.3 0.0 131.0


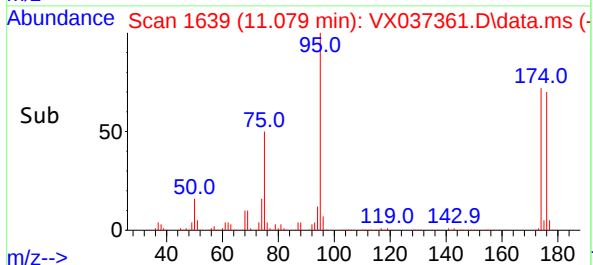
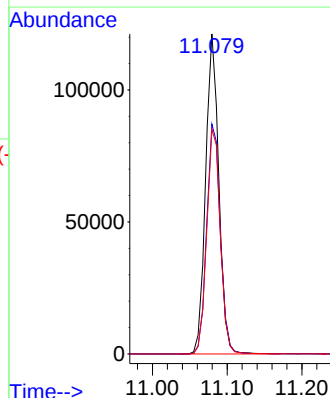
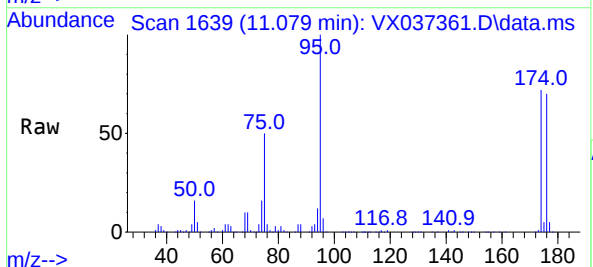




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32




Instrument :
MSVOA_X
ClientSampleId :
PB155153TB


Tgt Ion:117 Resp: 298161
Ion Ratio Lower Upper
117 100
82 53.8 46.2 69.4
119 31.5 25.5 38.3

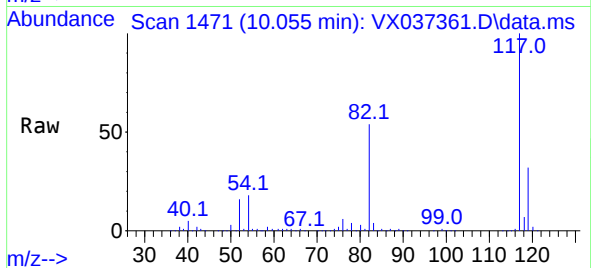

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Tgt Ion:152 Resp: 136369
Ion Ratio Lower Upper
152 100
115 62.8 43.3 129.9
150 156.7 0.0 345.0


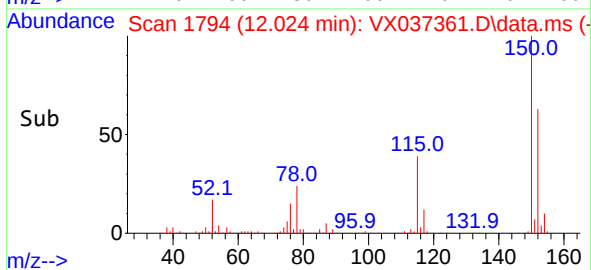






#74
N-amy1 acetate
Concen: 0.216 ug/l
RT: 10.817 min Scan# 11
Delta R.T. -0.024 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32




Instrument :
MSVOA_X
ClientSampleId :
PB155153TB


Tgt Ion:	43	Resp:	831
Ion	Ratio	Lower	Upper
43	100		
70	0.0	32.9	49.3#
55	8.8	19.3	28.9#
61	0.0	18.8	28.2#

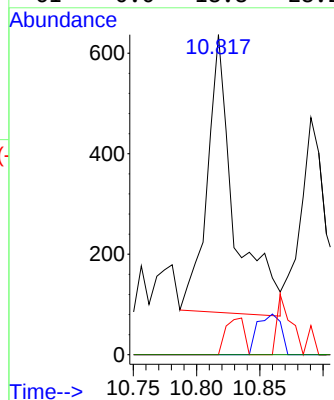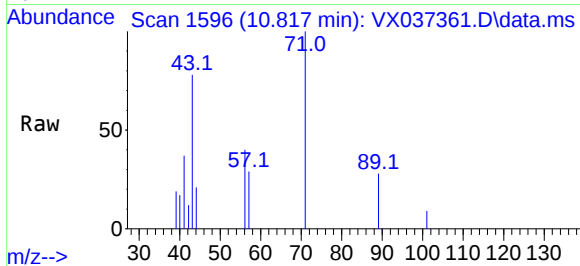

#76
1,2,3-Trichloropropane
Concen: 25.019 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Tgt Ion:	75	Resp:	72660
Ion	Ratio	Lower	Upper
75	100		
77	1.0	19.1	57.5#


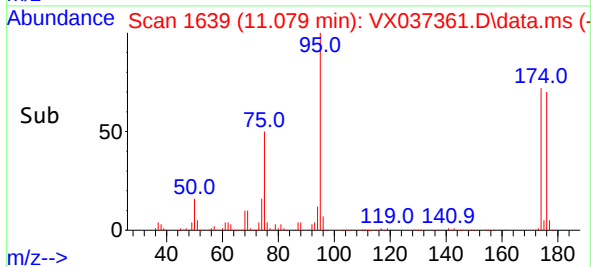
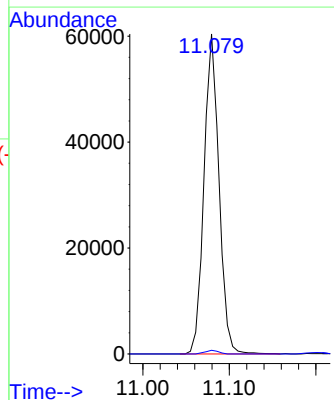
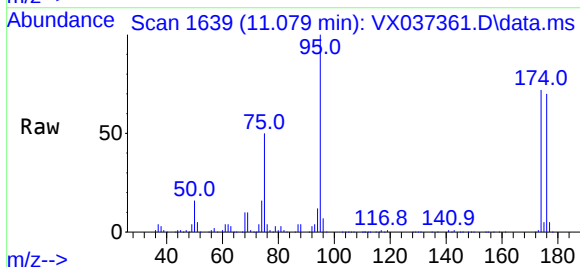




#81
trans-1,4-Dichloro-2-butene
Concen: 69.879 ug/l
RT: 11.079 min Scan# 11
Delta R.T. 0.061 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32




Instrument :
MSVOA_X
ClientSampleId :
PB155153TB


Tgt Ion: 75 Resp: 72660
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

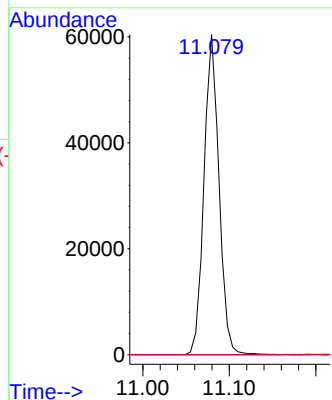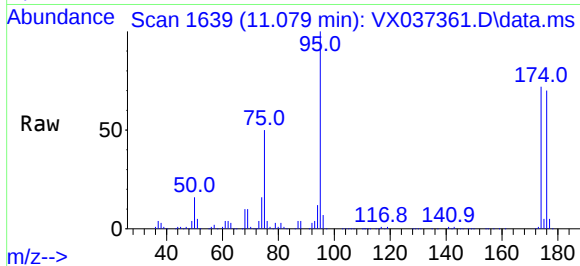

#93
1,2,4-Trichlorobenzene
Concen: 0.266 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.006 min
Lab File: VX037361.D
Acq: 30 Aug 2023 01:32

Tgt Ion:180 Resp: 691
Ion Ratio Lower Upper
180 100
182 104.9 48.3 144.8
145 31.7 18.0 54.0

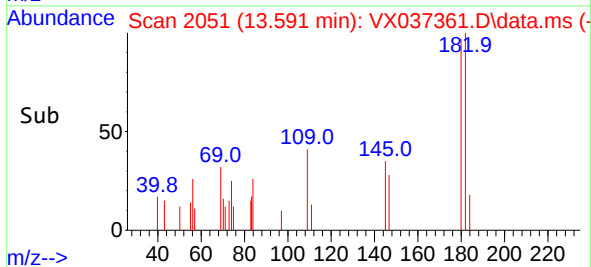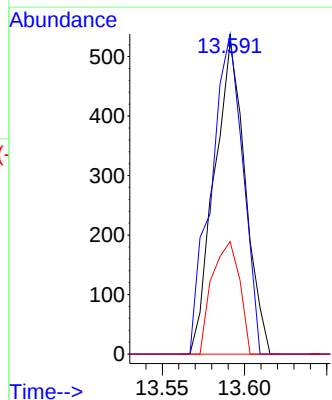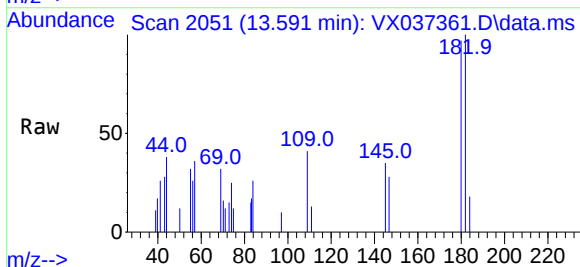



#96

1,2,3-Trichlorobenzene

Concen: 0.262 ug/l

RT: 13.963 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX037361.D


Acq: 30 Aug 2023 01:32

Instrument :

MSVOA_X

ClientSampleId :

PB155153TB

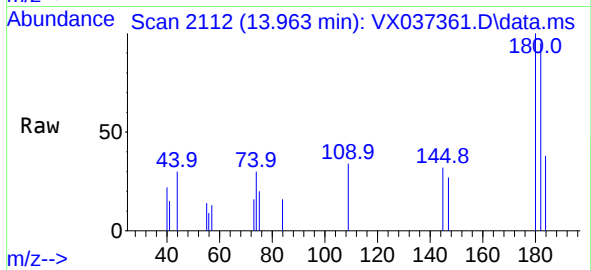

Tgt Ion:180 Resp: 677

Ion Ratio Lower Upper

180 100

182 104.9 46.9 140.6

145 32.8 17.8 53.5

