

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082923\
 Data File : VX037341.D
 Acq On : 29 Aug 2023 14:51
 Operator : JC/MD
 Sample : 04207-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 OW-07B-67-082823-H

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Title : SW846 8260

Signal : TIC: VX037341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rBV2	7269	7198	1.03%	0.146%
2	1.258	21	28	34	rBV2	15246	34852	5.00%	0.709%
3	2.069	157	161	166	rVV	4050	8001	1.15%	0.163%
4	2.136	169	172	181	rVB2	6147	10741	1.54%	0.218%
5	2.313	195	201	211	rBV	246920	391738	56.19%	7.968%
6	3.093	321	329	337	rBV	8916	17843	2.56%	0.363%
7	3.611	403	414	425	rBV	13469	34180	4.90%	0.695%
8	4.489	547	558	574	rBV	159763	436726	62.64%	8.883%
9	5.385	691	705	722	rBV2	80573	235814	33.82%	4.796%
10	5.550	722	732	750	rVB	153255	429176	61.56%	8.729%
11	5.958	789	799	813	rBV	87023	233098	33.43%	4.741%
12	6.092	813	821	833	rVB2	7958	23087	3.31%	0.470%
13	6.763	921	931	950	rBV	218346	524962	75.29%	10.678%
14	7.123	982	990	1005	rBV	91122	201513	28.90%	4.099%
15	7.665	1074	1079	1091	rBV	5234	11278	1.62%	0.229%
16	8.647	1234	1240	1250	rBV	446890	697209	100.00%	14.181%
17	10.055	1465	1471	1485	rBV	441971	597794	85.74%	12.159%
18	11.079	1634	1639	1650	rBV	350065	453601	65.06%	9.226%
19	12.024	1788	1794	1805	rBV	437302	557847	80.01%	11.347%
20	12.219	1820	1826	1838	rBV2	5495	9760	1.40%	0.199%




Sum of corrected areas: 4916418

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082923\
Data File : VX037341.D
Acq On : 29 Aug 2023 14:51
Operator : JC/MD
Sample : 04207-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OW-07B-67-082823-H

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

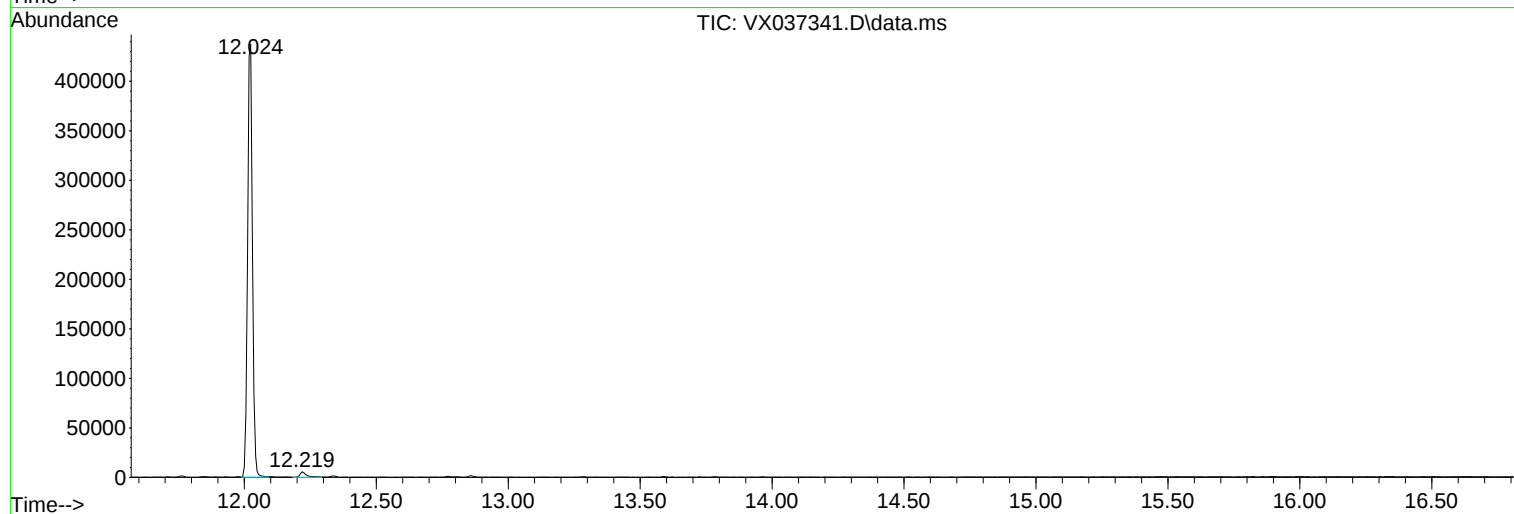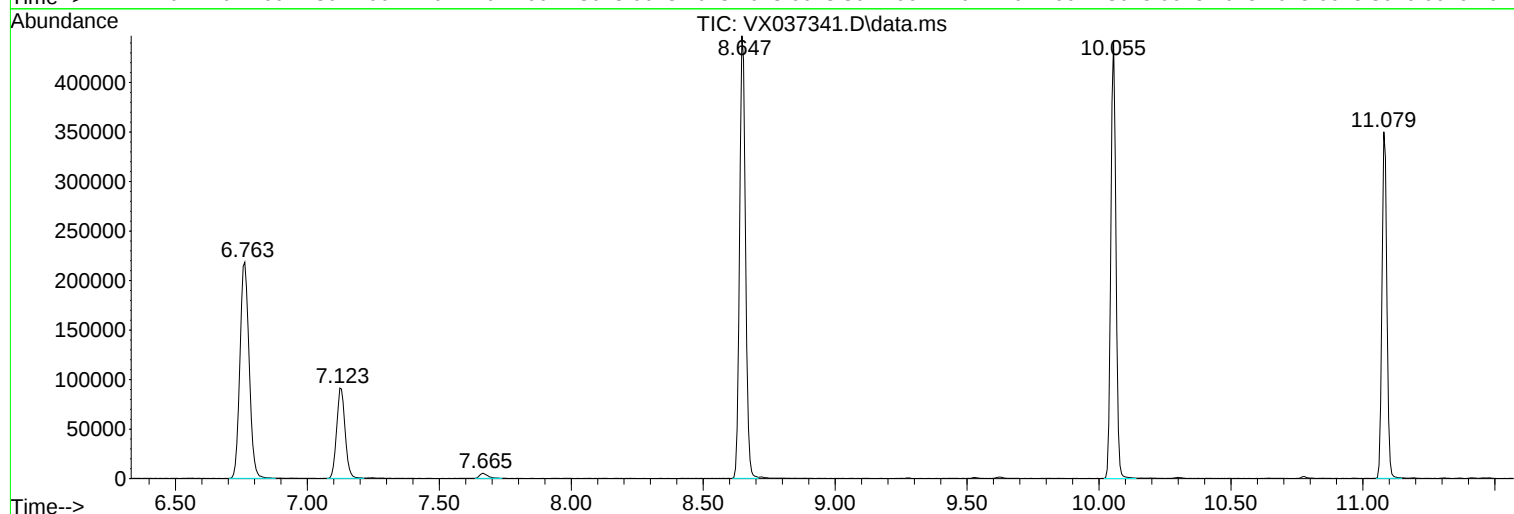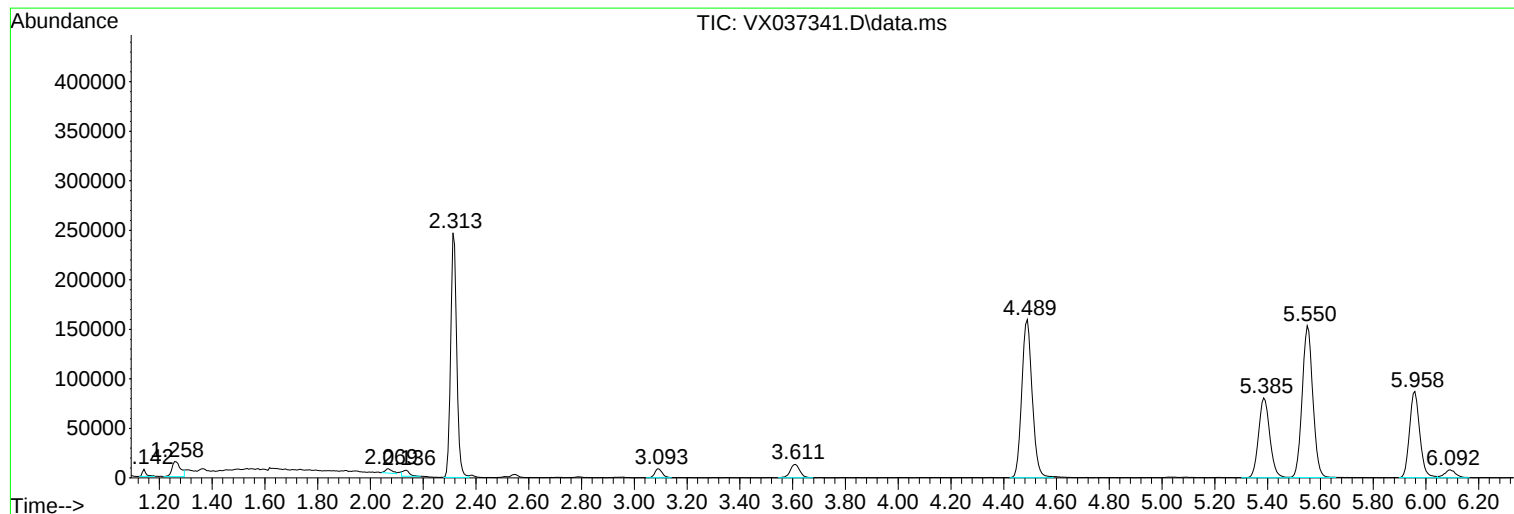

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082923\
Data File : VX037341.D
Acq On : 29 Aug 2023 14:51
Operator : JC/MD
Sample : 04207-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OW-07B-67-082823-H

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082923\
Data File : VX037341.D
Acq On : 29 Aug 2023 14:51
Operator : JC/MD
Sample : 04207-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OW-07B-67-082823-H

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------