


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX083019\
 Data File : VX011919.D
 Acq On : 30 Aug 2019 21:12
 Operator : SY/SP
 Sample : BFB
 Misc : 5.00µ/5.0mL/MSVOA X/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082919S.M
 Title : SW846 8260
 Last Update : Fri Aug 30 01:59:05 2019

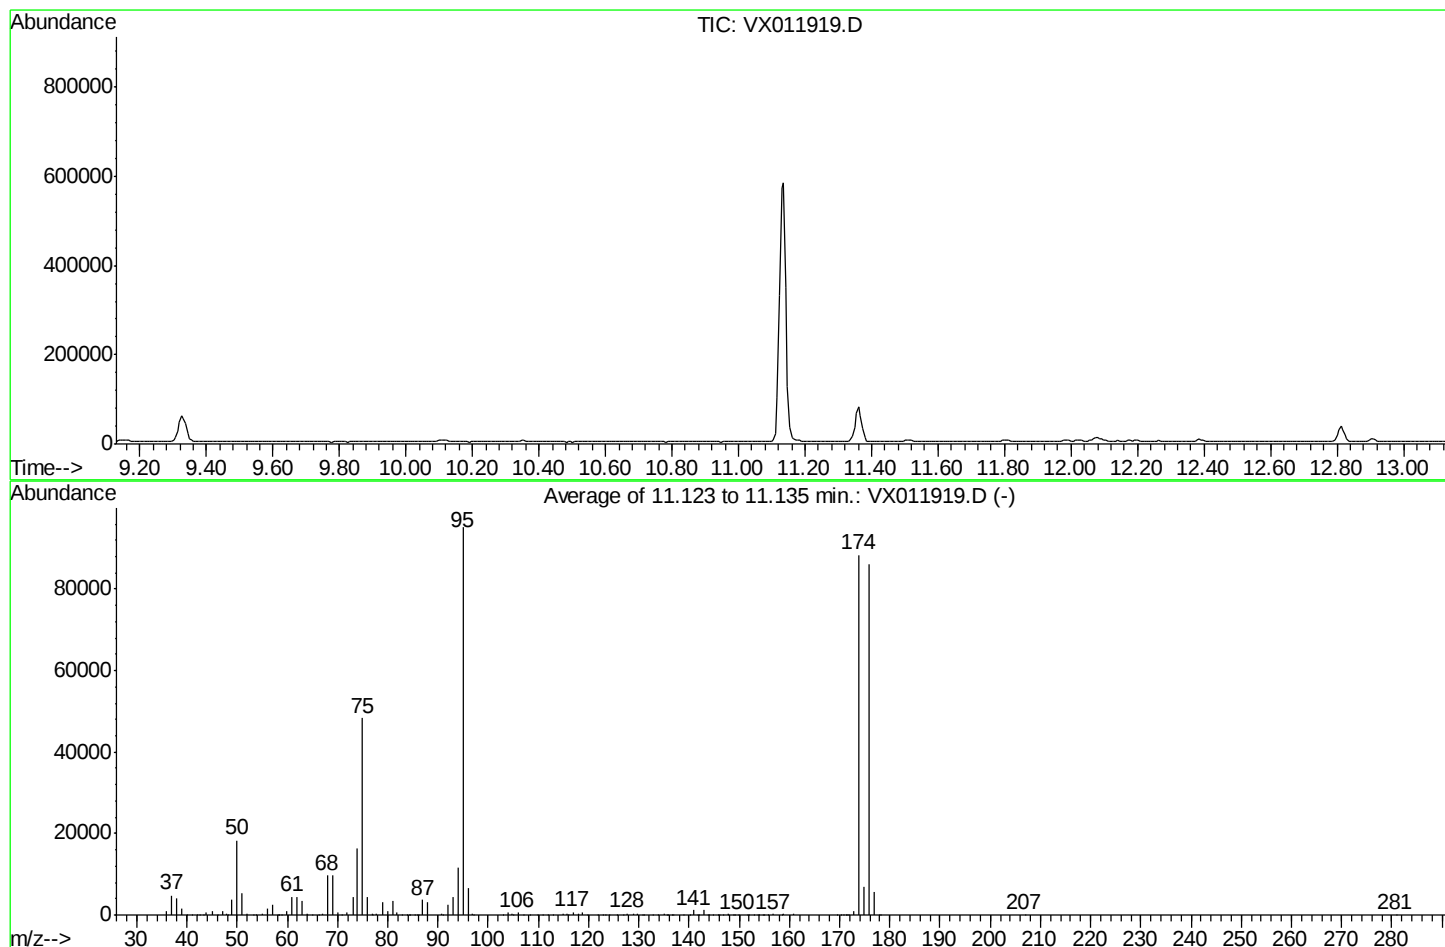

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	18279	PASS
75	95	30	60	50.8	48338	PASS
95	95	100	100	100.0	95190	PASS
96	95	5	9	6.9	6529	PASS
173	174	0.00	2	1.1	1007	PASS
174	95	50	100	92.9	88448	PASS
175	174	5	9	7.8	6922	PASS
176	174	95	101	97.5	86218	PASS
177	176	5	9	6.7	5802	PASS