

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083021\
 Data File : VX024015.D
 Acq On : 30 Aug 2021 15:29
 Operator : JC/MD
 Sample : M3585-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BO-TT-VPB-RW7-GW-610-612

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M

Title : SW846 8260

Signal : TIC: VX024015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.148	7	10	17	rVB2	12303	14172	1.61%	0.301%
2	1.453	57	60	67	rBV	18928	21980	2.50%	0.467%
3	2.386	208	213	221	rBV	20009	31833	3.62%	0.677%
4	4.580	564	573	584	rBV3	3552	11521	1.31%	0.245%
5	5.397	694	707	721	rBV2	101383	293208	33.38%	6.231%
6	5.562	723	734	748	rVB	167275	473846	53.95%	10.070%
7	5.964	786	800	816	rBV	114022	302167	34.40%	6.422%
8	6.769	922	932	946	rBV	271140	635204	72.32%	13.500%
9	8.653	1234	1241	1250	rBV	568960	878362	100.00%	18.667%
10	10.055	1465	1471	1483	rBV	548036	779503	88.75%	16.566%
11	11.085	1634	1640	1652	rBV	473183	591975	67.40%	12.581%
12	12.024	1789	1794	1803	rVB	544722	661216	75.28%	14.053%
13	12.225	1821	1827	1832	rBV	6285	10321	1.18%	0.219%




Sum of corrected areas: 4705308

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083021\
Data File : VX024015.D
Acq On : 30 Aug 2021 15:29
Operator : JC/MD
Sample : M3585-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BO-TT-VPB-RW7-GW-610-612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

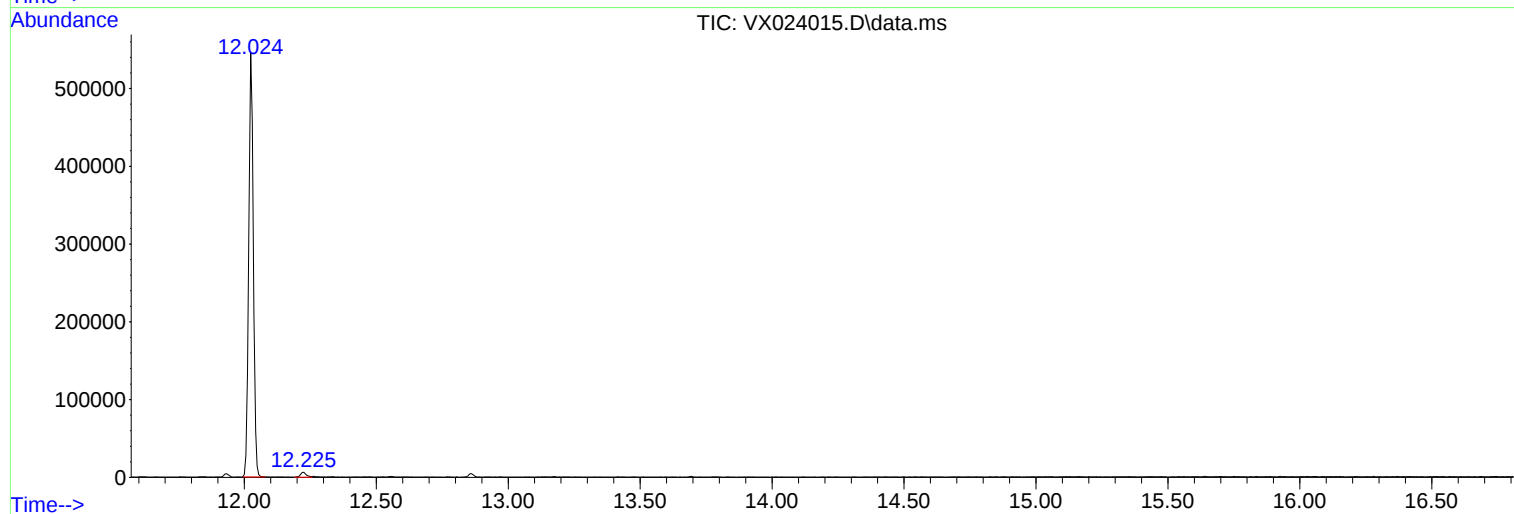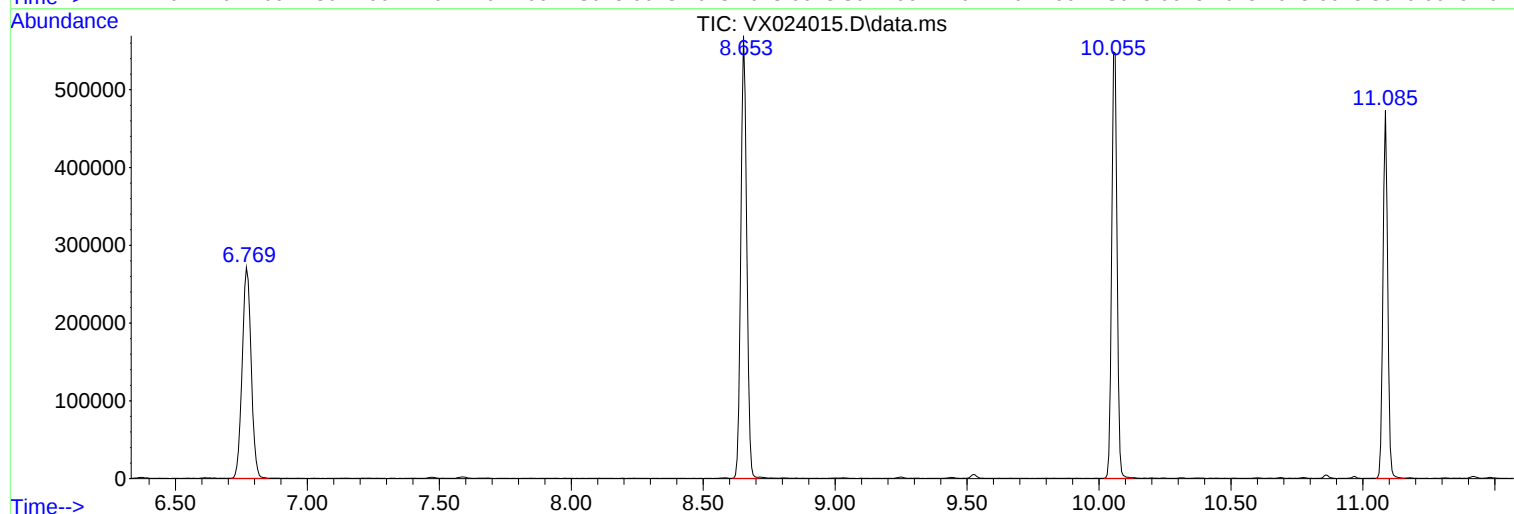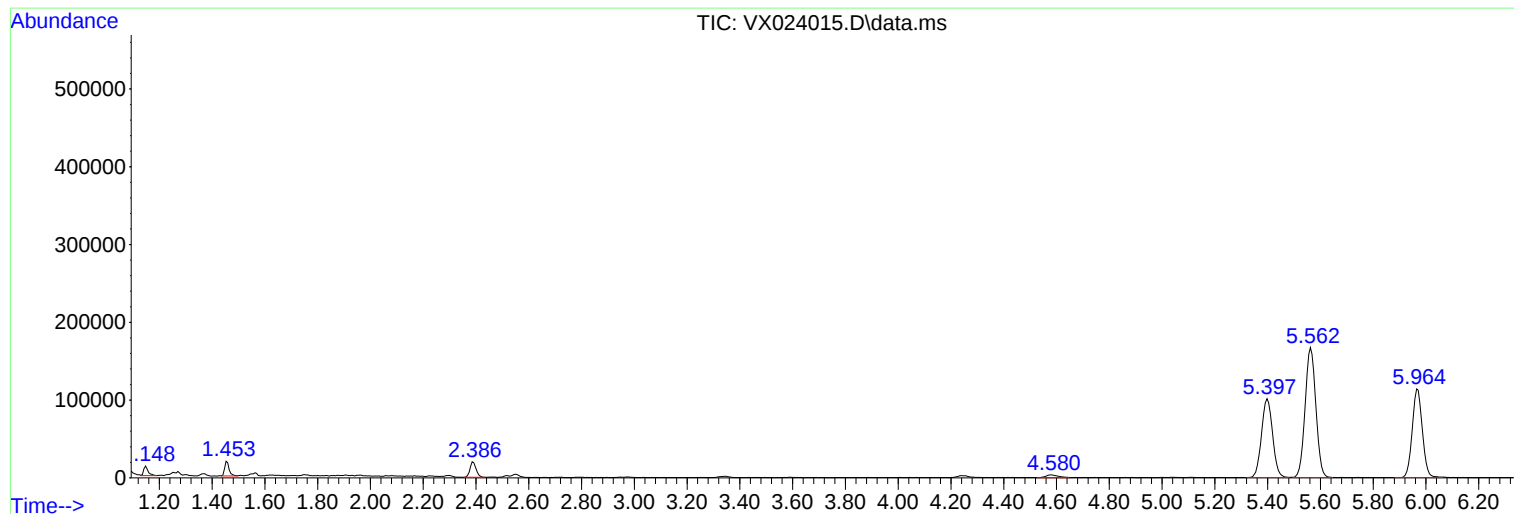

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083021\
Data File : VX024015.D
Acq On : 30 Aug 2021 15:29
Operator : JC/MD
Sample : M3585-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BO-TT-VPB-RW7-GW-610-612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083021\
Data File : VX024015.D
Acq On : 30 Aug 2021 15:29
Operator : JC/MD
Sample : M3585-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BO-TT-VPB-RW7-GW-610-612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
