

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083021\
 Data File : VX024022.D
 Acq On : 30 Aug 2021 18:14
 Operator : JC/MD
 Sample : M3583-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MH-118.5T-20210827

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M

Title : SW846 8260

Signal : TIC: VX024022.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	22	27	33	rBV2	10762	17840	1.98%	0.361%
2	2.550	232	240	245	rBV	8794	16181	1.80%	0.328%
3	4.501	548	560	571	rBV	53924	148510	16.49%	3.008%
4	5.397	696	707	722	rBV2	104517	300977	33.42%	6.097%
5	5.562	722	734	749	rVB	172773	485986	53.97%	9.844%
6	5.964	790	800	816	rBV	114608	306502	34.04%	6.208%
7	6.769	922	932	946	rBV	278770	654614	72.70%	13.260%
8	7.135	984	992	1005	rVB2	36980	81009	9.00%	1.641%
9	8.653	1234	1241	1252	rBV	580902	900470	100.00%	18.240%
10	10.055	1465	1471	1480	rBV	580243	785808	87.27%	15.917%
11	11.085	1634	1640	1651	rBV	472516	591586	65.70%	11.983%
12	12.024	1789	1794	1807	rVB	535881	647348	71.89%	13.113%


Sum of corrected areas: 4936831

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083021\
Data File : VX024022.D
Acq On : 30 Aug 2021 18:14
Operator : JC/MD
Sample : M3583-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-118.5T-20210827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

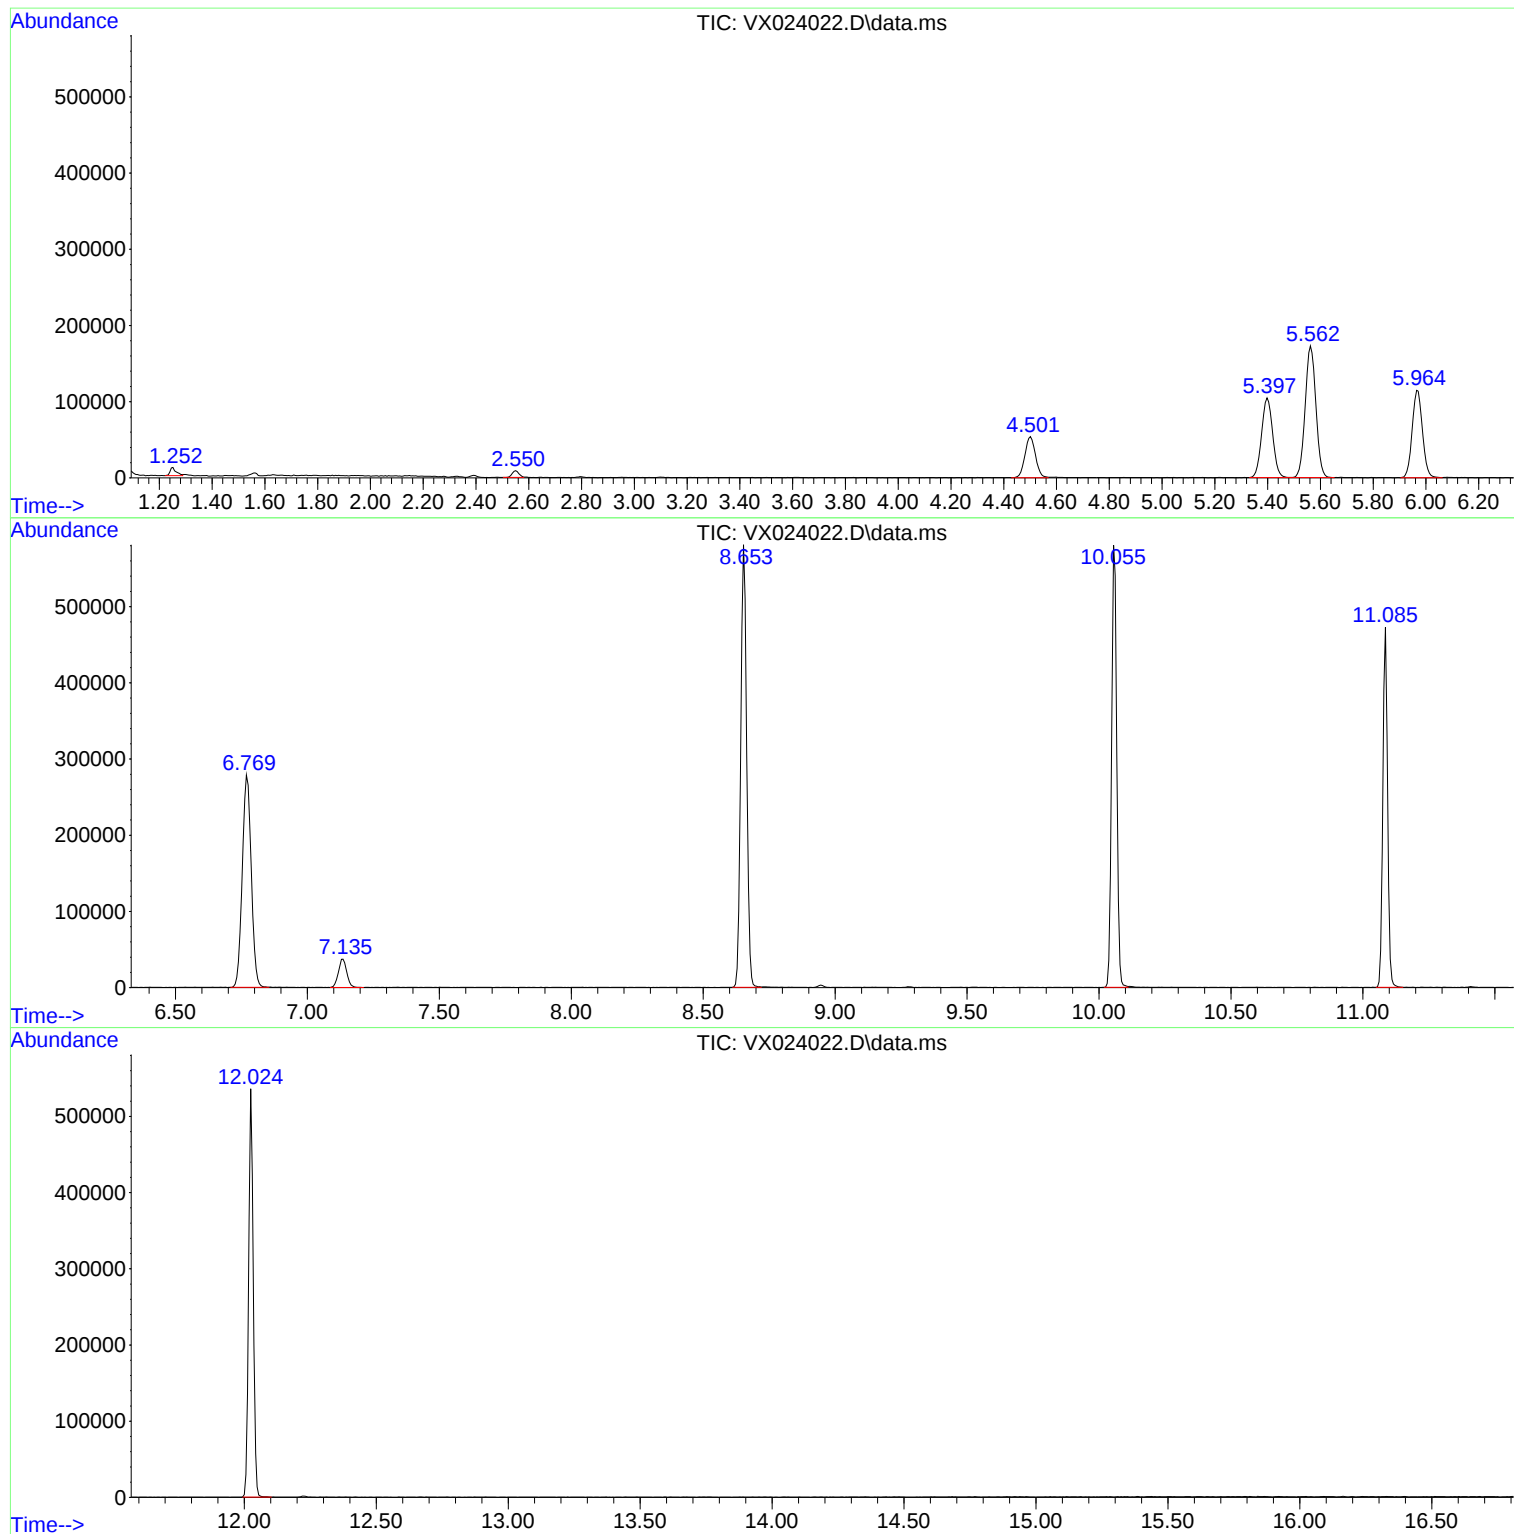

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083021\
Data File : VX024022.D
Acq On : 30 Aug 2021 18:14
Operator : JC/MD
Sample : M3583-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-118.5T-20210827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083021\
Data File : VX024022.D
Acq On : 30 Aug 2021 18:14
Operator : JC/MD
Sample : M3583-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-118.5T-20210827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
