
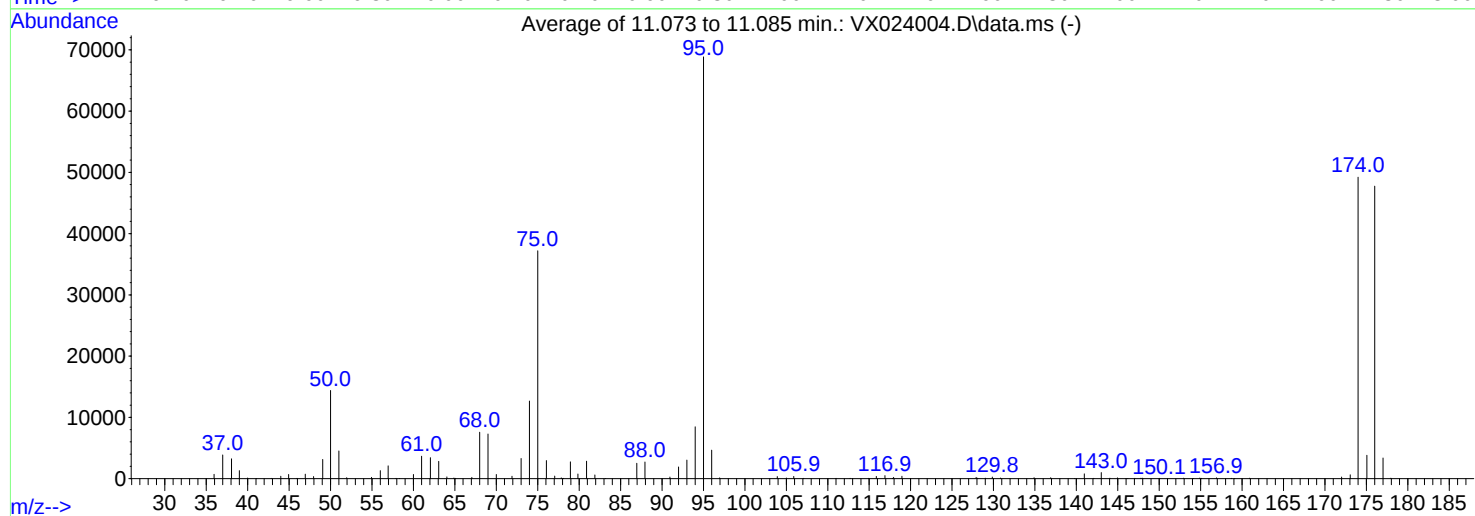


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083021\
 Data File : VX024004.D
 Acq On : 30 Aug 2021 09:02
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Title : SW846 8260
 Last Update : Tue Aug 17 11:57:51 2021

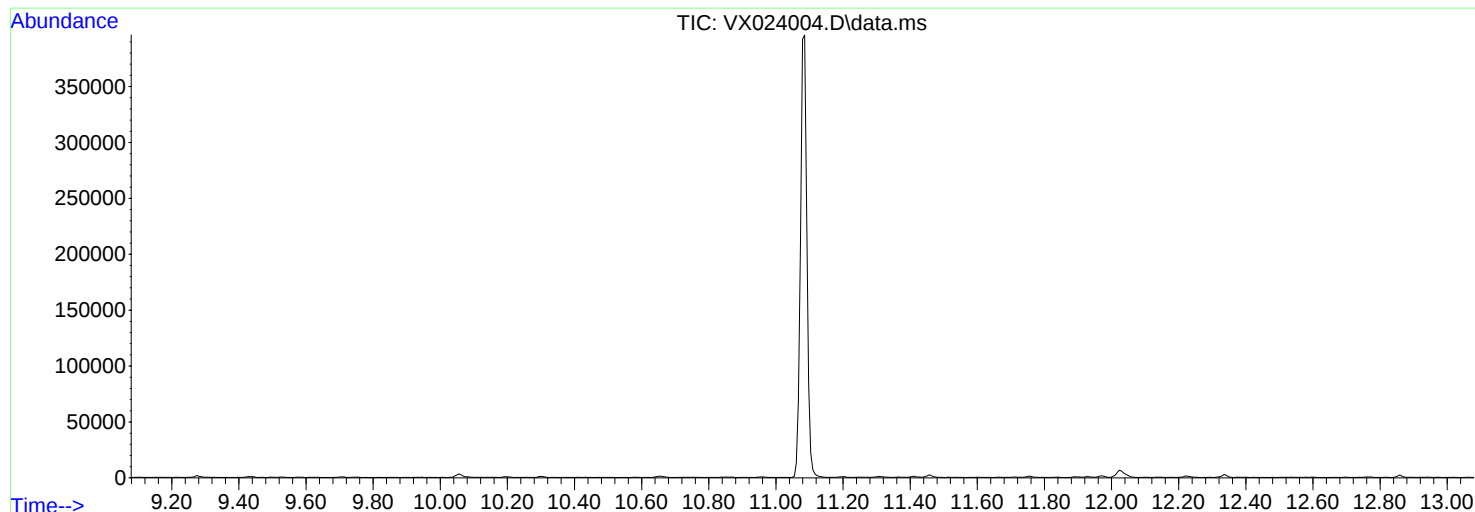

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	14407	PASS
75	95	30	60	54.0	37205	PASS
95	95	100	100	100.0	68864	PASS
96	95	5	9	6.8	4650	PASS
173	174	0.00	2	1.3	627	PASS
174	95	50	100	71.5	49224	PASS
175	174	5	9	7.7	3805	PASS
176	174	95	101	97.0	47763	PASS
177	176	5	9	7.1	3369	PASS