



Bromomethane

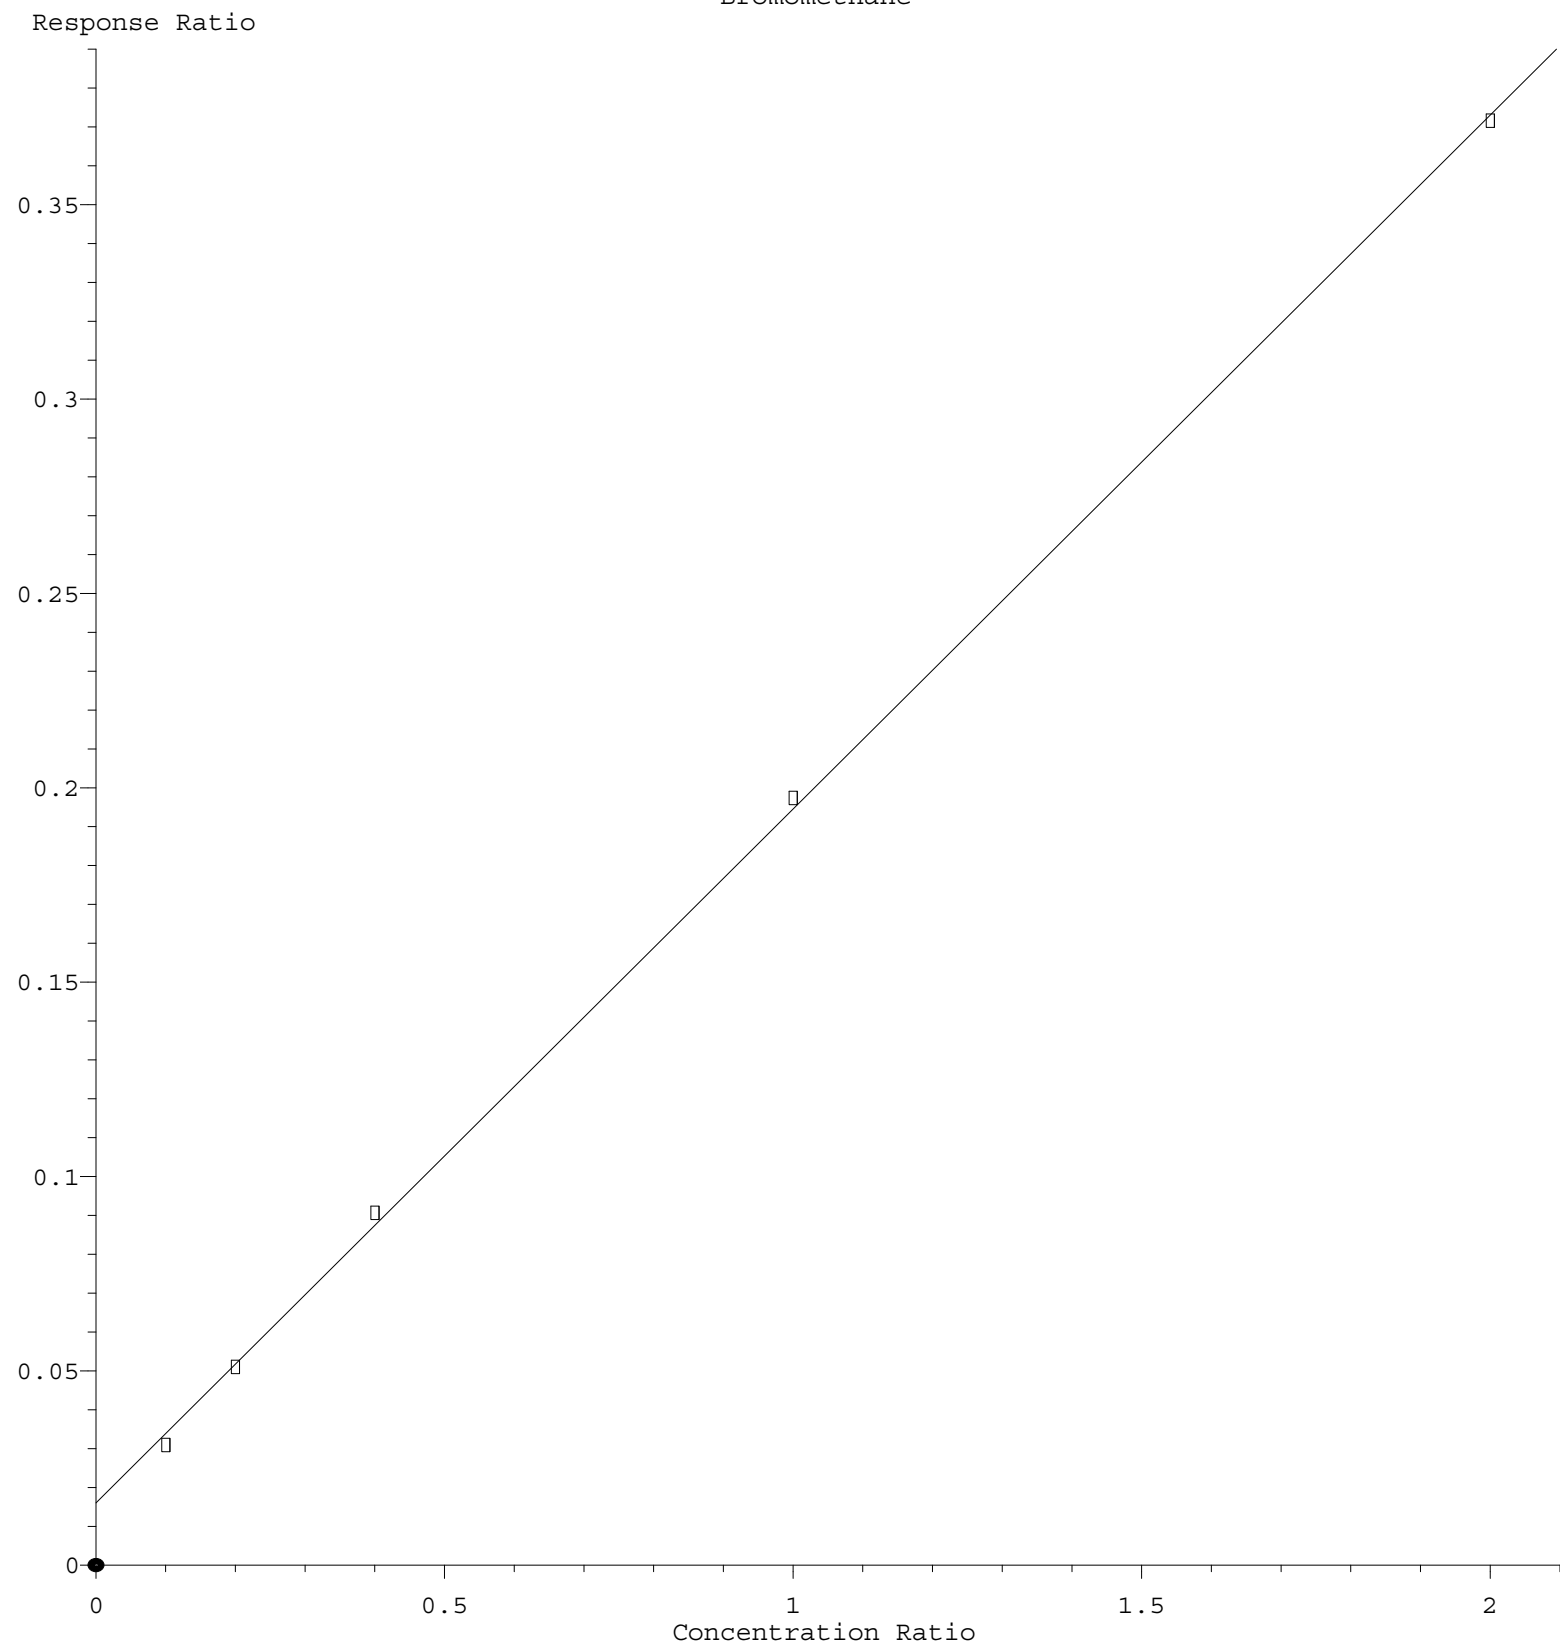

Response = 1.786e-001 * Amt + 1.616e-002
Coef of Det (r^2) = 0.999625 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X083022W.M
Calibration Table Last Updated: Tue Aug 30 14:24:53 2022

Methyl Iodide

Response Ratio

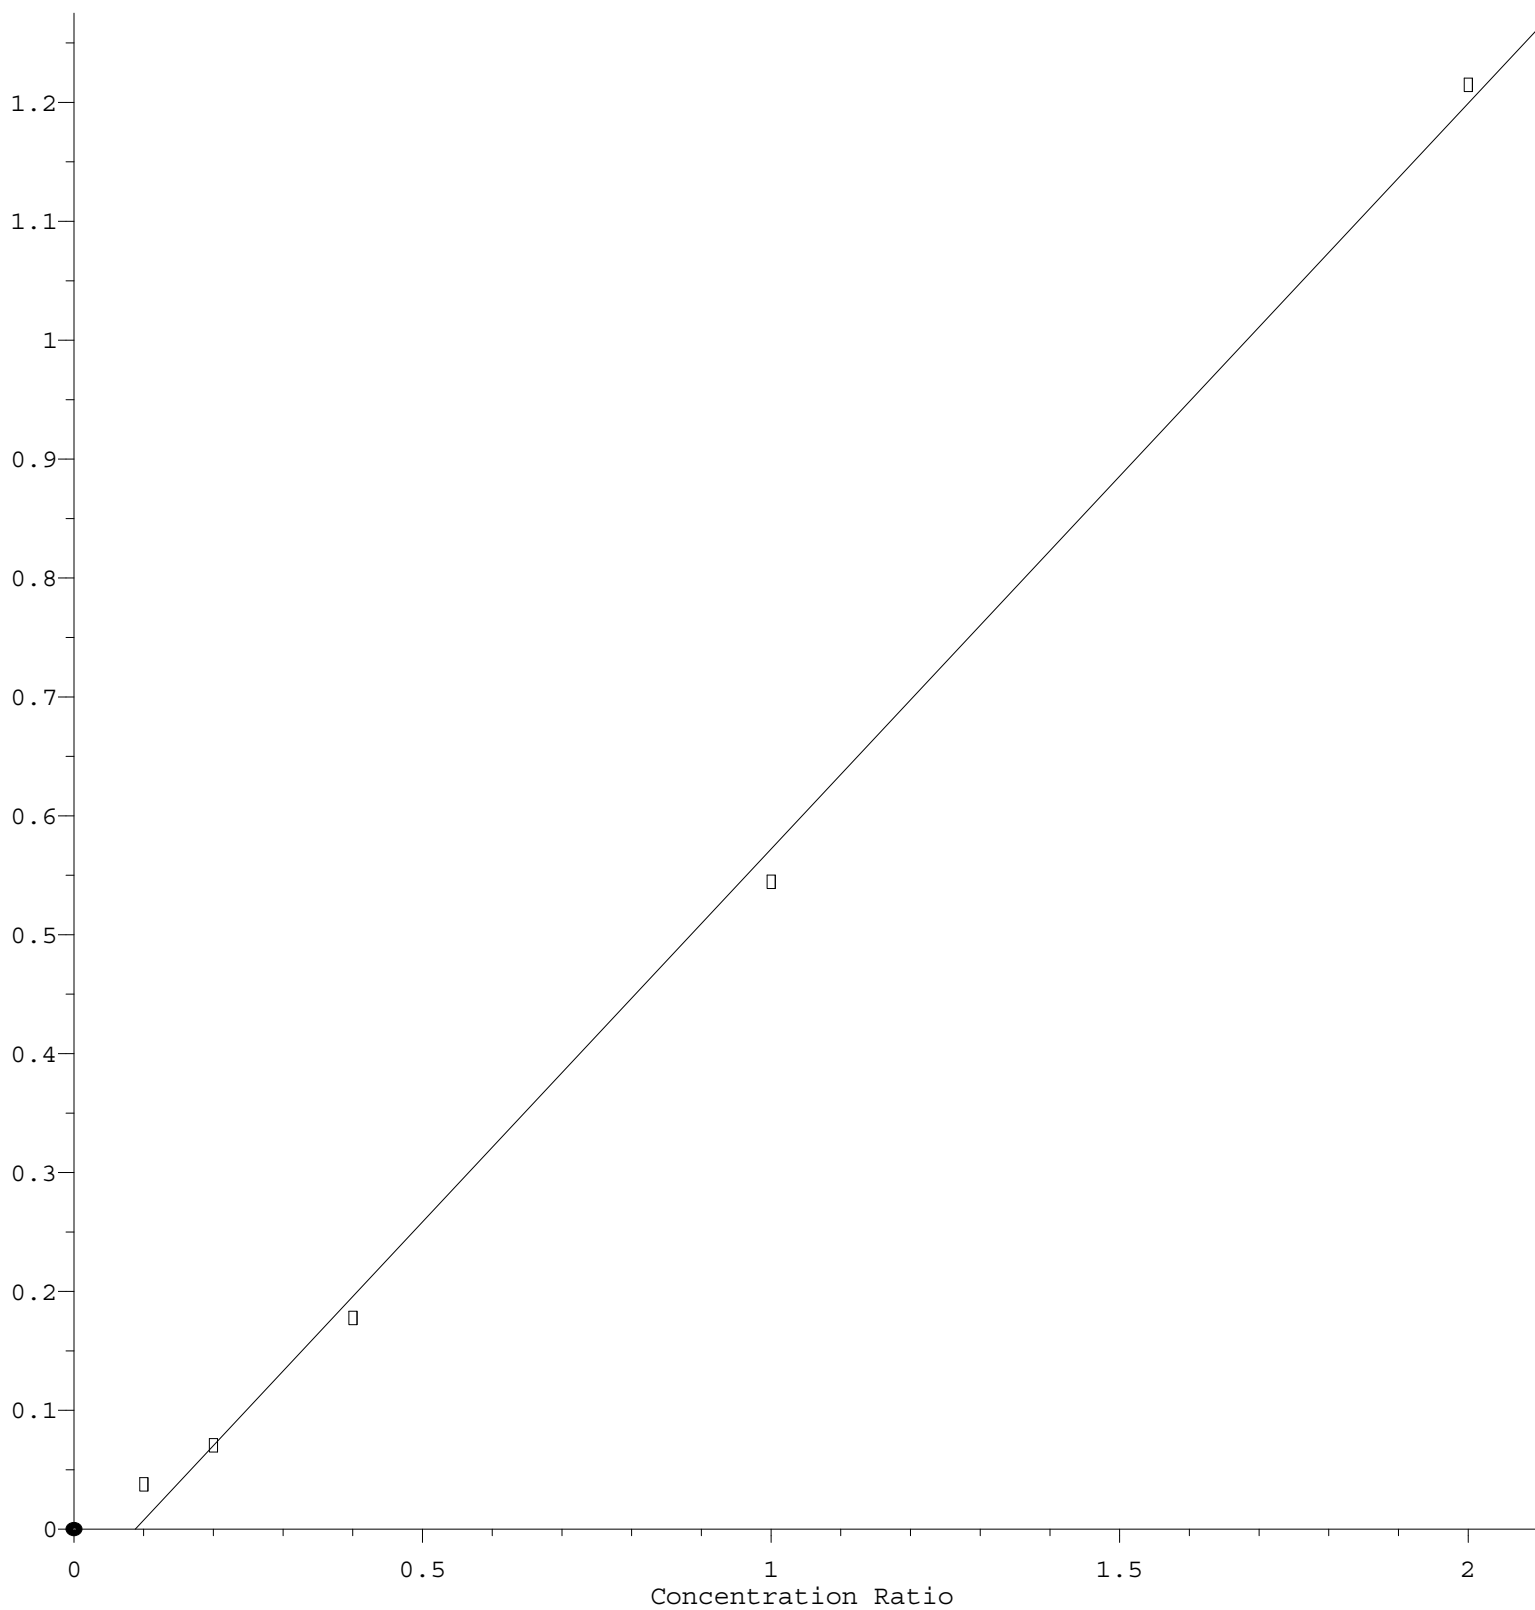

$$\text{Response} = 6.269\text{e-}001 * \text{Amt} - 5.487\text{e-}002$$


Coef of Det (r^2) = 0.997699 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X083022W.M

Calibration Table Last Updated: Tue Aug 30 14:24:53 2022

Acrolein

Response Ratio

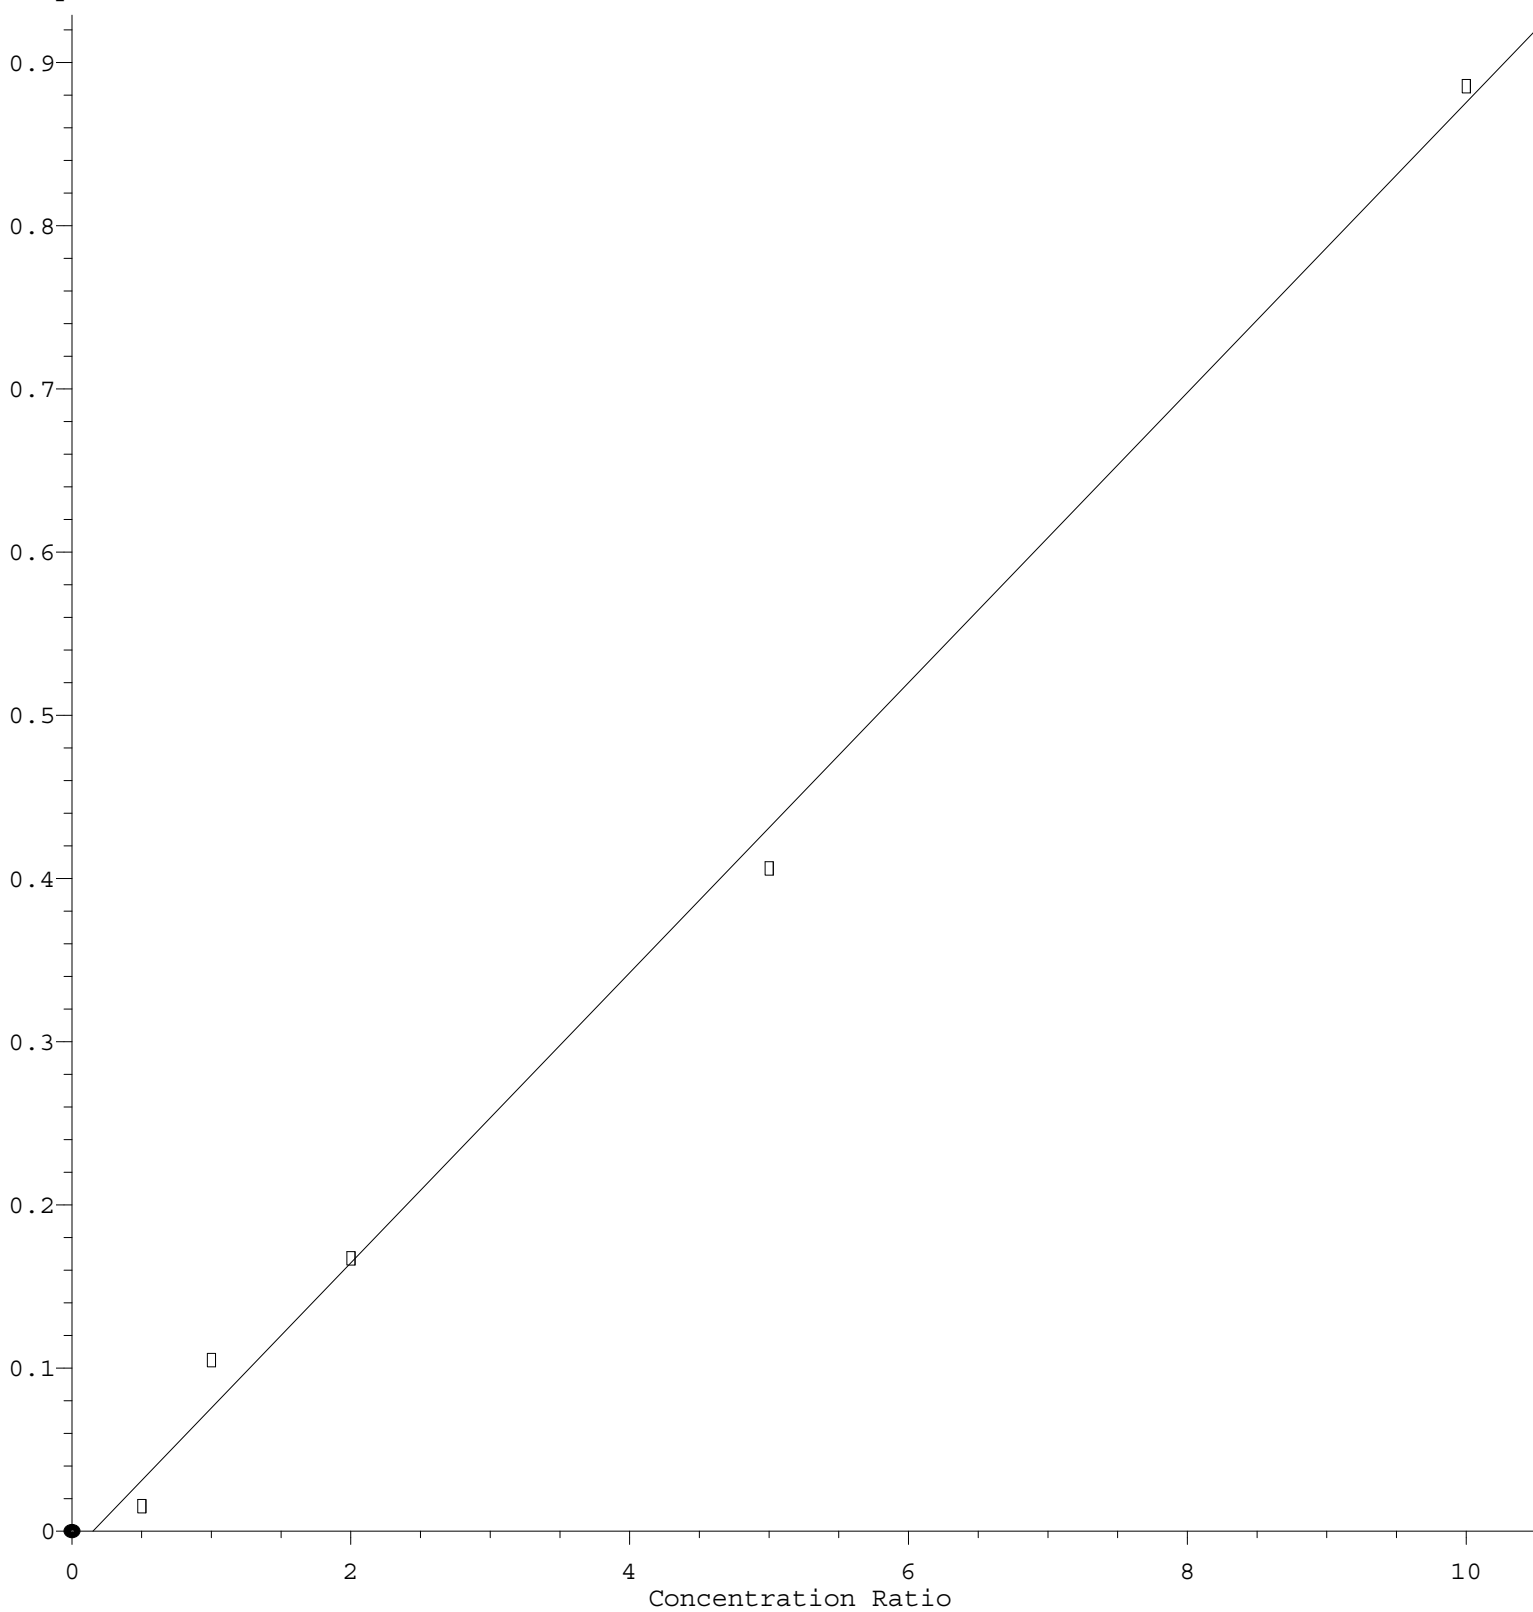

$$\text{Response} = 8.884\text{e-}002 * \text{Amt} - 1.292\text{e-}002$$

Coef of Det (r^2) = 0.996251 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X083022W.M

Calibration Table Last Updated: Tue Aug 30 14:24:53 2022