

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX083022\  
 Data File : VX030946.D  
 Acq On : 30 Aug 2022 18:09  
 Operator : JC/MD  
 Sample : N4371-01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 A4127

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X083022W.M

Title : SW846 8260

Signal : TIC: VX030946.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.246       | 23            | 26          | 40           | rVB      | 565539         | 551458        | 51.63%          | 9.035%        |
| 2         | 2.971       | 299           | 309         | 317          | rVB5     | 4295           | 11930         | 1.12%           | 0.195%        |
| 3         | 5.391       | 693           | 706         | 720          | rBV2     | 124286         | 365736        | 34.24%          | 5.992%        |
| 4         | 5.556       | 722           | 733         | 750          | rVV      | 221920         | 635785        | 59.52%          | 10.416%       |
| 5         | 5.964       | 790           | 800         | 812          | rBV2     | 133166         | 354172        | 33.16%          | 5.802%        |
| 6         | 6.769       | 918           | 932         | 950          | rBV      | 341555         | 816311        | 76.42%          | 13.374%       |
| 7         | 8.653       | 1234          | 1241        | 1250         | rBV      | 688704         | 1068165       | 100.00%         | 17.500%       |
| 8         | 10.055      | 1464          | 1471        | 1485         | rBV      | 677231         | 909739        | 85.17%          | 14.904%       |
| 9         | 11.085      | 1634          | 1640        | 1648         | rBV      | 513126         | 635636        | 59.51%          | 10.414%       |
| 10        | 12.024      | 1789          | 1794        | 1802         | rBV      | 610865         | 754887        | 70.67%          | 12.367%       |




Sum of corrected areas: 6103819

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX083022\  
Data File : VX030946.D  
Acq On : 30 Aug 2022 18:09  
Operator : JC/MD  
Sample : N4371-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
A4127

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X083022W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

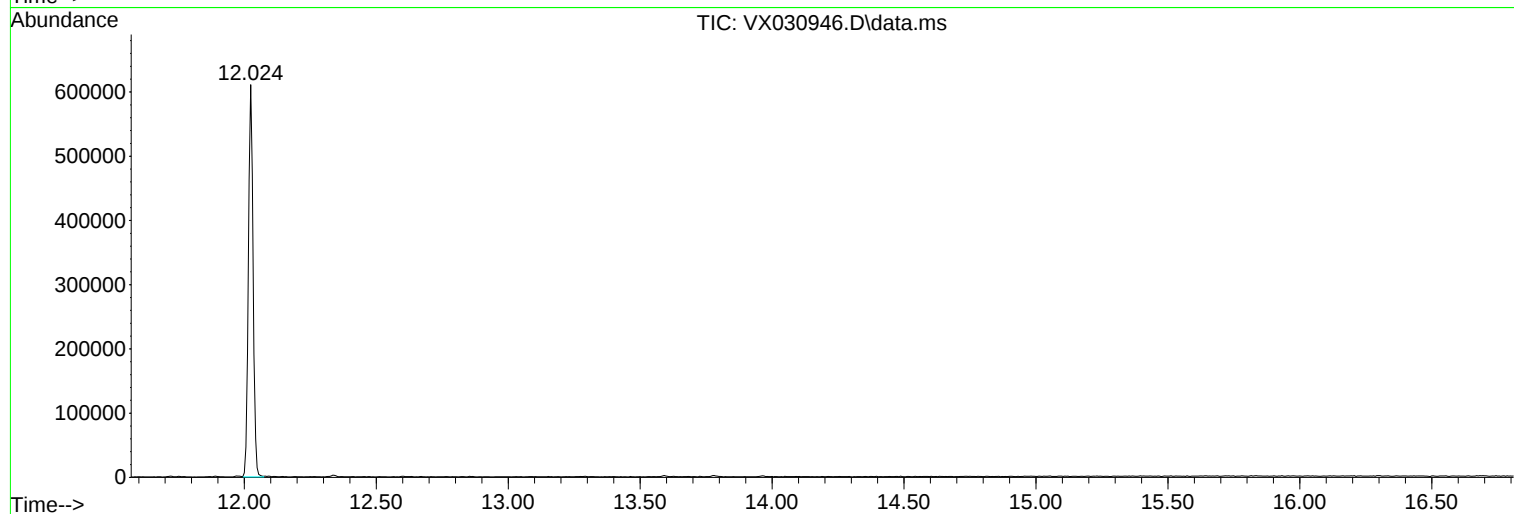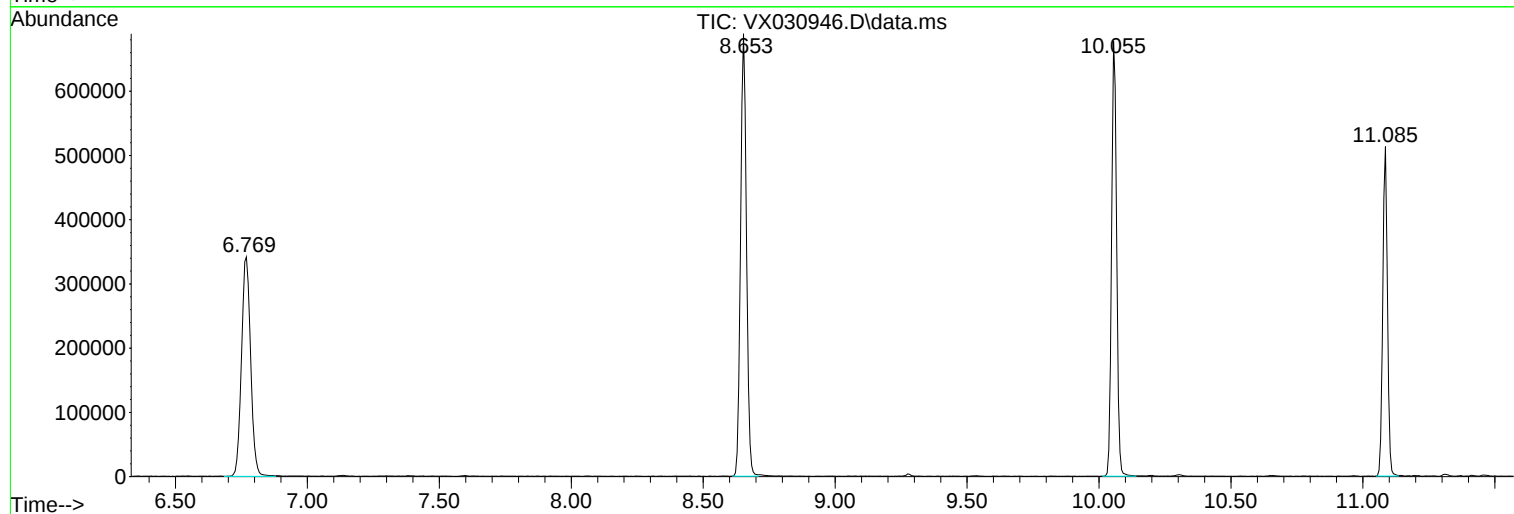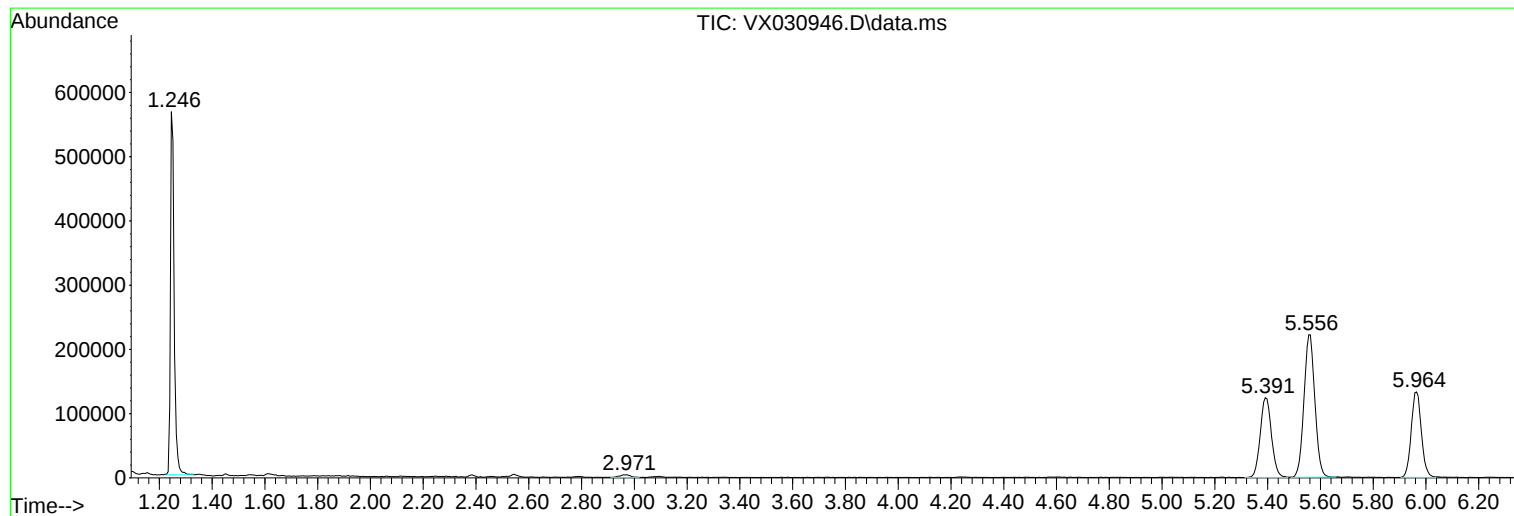

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX083022\  
Data File : VX030946.D  
Acq On : 30 Aug 2022 18:09  
Operator : JC/MD  
Sample : N4371-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
A4127

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X083022W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX083022\  
Data File : VX030946.D  
Acq On : 30 Aug 2022 18:09  
Operator : JC/MD  
Sample : N4371-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
A4127

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X083022W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|