

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083022\
Data File : VX030957.D
Acq On : 30 Aug 2022 22:29
Operator : JC/MD
Sample : N4281-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D1-20220819

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M

Title : SW846 8260

Signal : TIC: VX030957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.324	198	203	210	rVB5	10163	17931	1.50%	0.271%
2	5.391	696	706	722	rBV2	136682	399126	33.38%	6.031%
3	5.555	722	733	747	rBV	209743	598969	50.10%	9.051%
4	5.964	788	800	818	rBV	152418	399249	33.39%	6.033%
5	6.769	922	932	945	rBV	338409	798243	66.76%	12.063%
6	7.128	982	991	1004	rBV	320554	705207	58.98%	10.657%
7	8.652	1234	1241	1251	rBV	769138	1195630	100.00%	18.068%
8	9.280	1337	1344	1349	rBV	29400	44977	3.76%	0.680%
9	10.055	1465	1471	1480	rBV	649987	883918	73.93%	13.357%
10	11.085	1634	1640	1653	rBV	606371	748199	62.58%	11.306%
11	12.024	1789	1794	1802	rBV	671002	826002	69.09%	12.482%




Sum of corrected areas: 6617451

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083022\
Data File : VX030957.D
Acq On : 30 Aug 2022 22:29
Operator : JC/MD
Sample : N4281-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D1-20220819

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

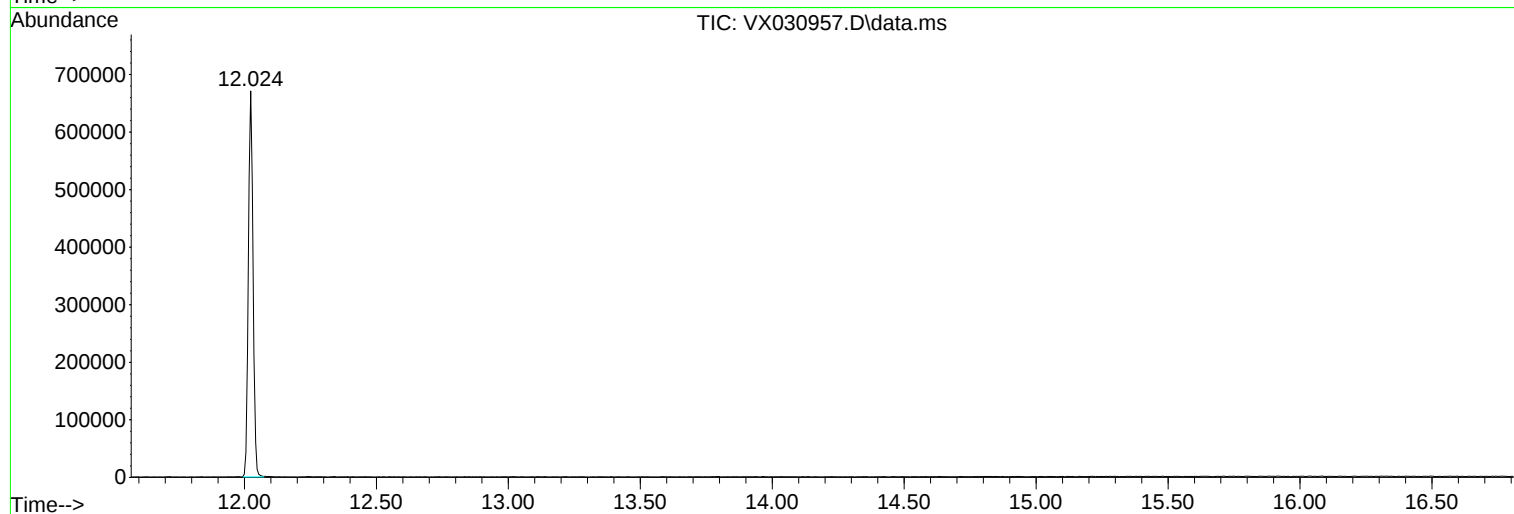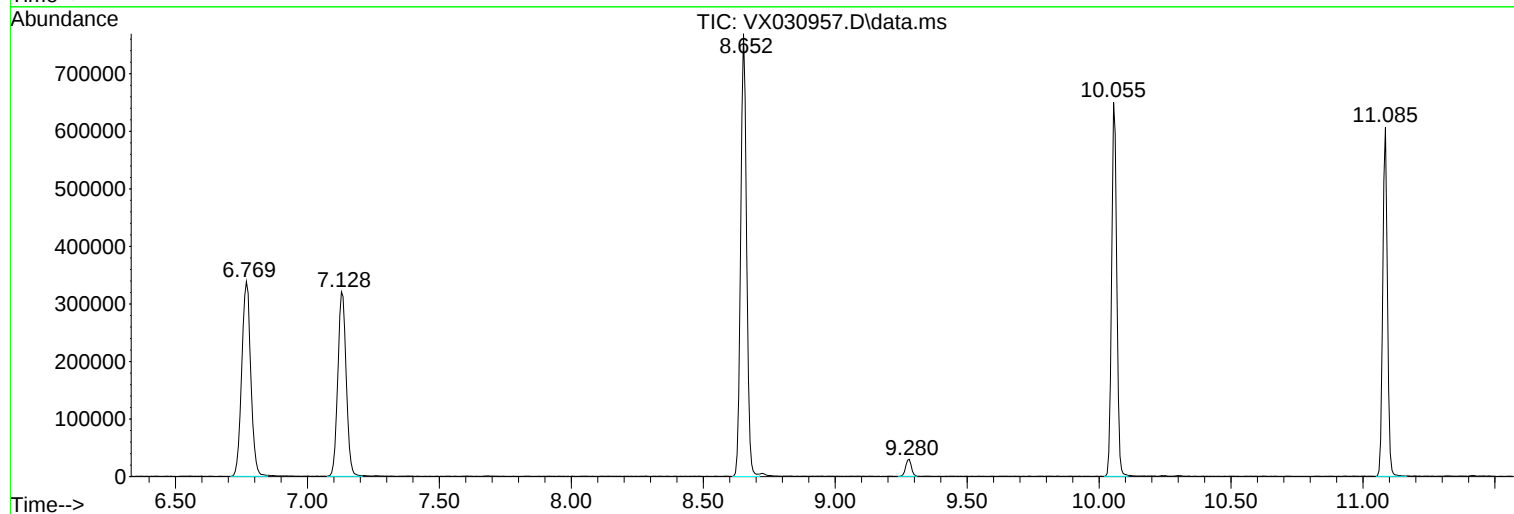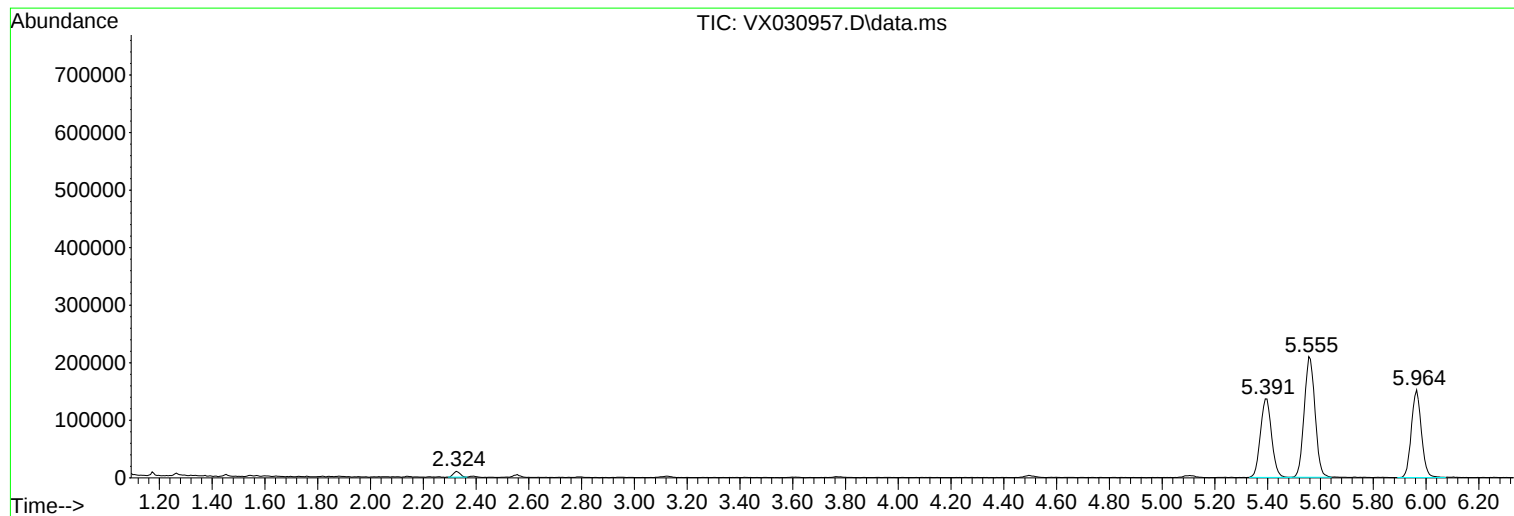

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083022\
Data File : VX030957.D
Acq On : 30 Aug 2022 22:29
Operator : JC/MD
Sample : N4281-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D1-20220819

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083022\
Data File : VX030957.D
Acq On : 30 Aug 2022 22:29
Operator : JC/MD
Sample : N4281-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D1-20220819

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc