
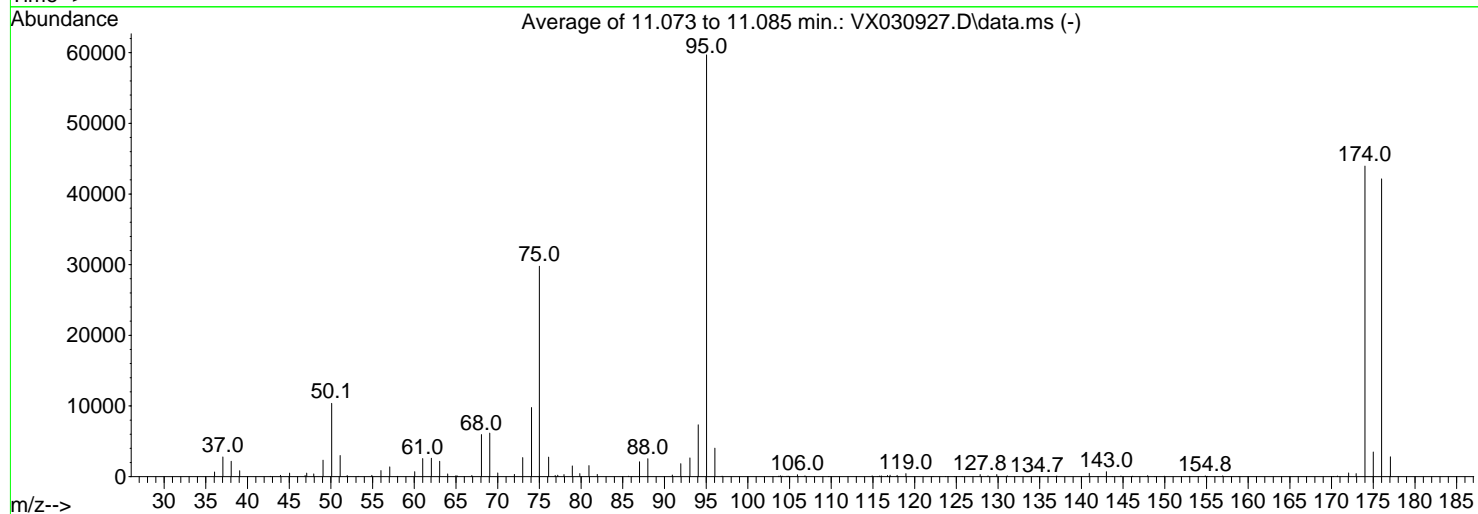


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX083022\  
 Data File : VX030927.D  
 Acq On : 30 Aug 2022 09:19  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X083022W.M  
 Title : SW846 8260  
 Last Update : Tue Aug 30 14:24:53 2022

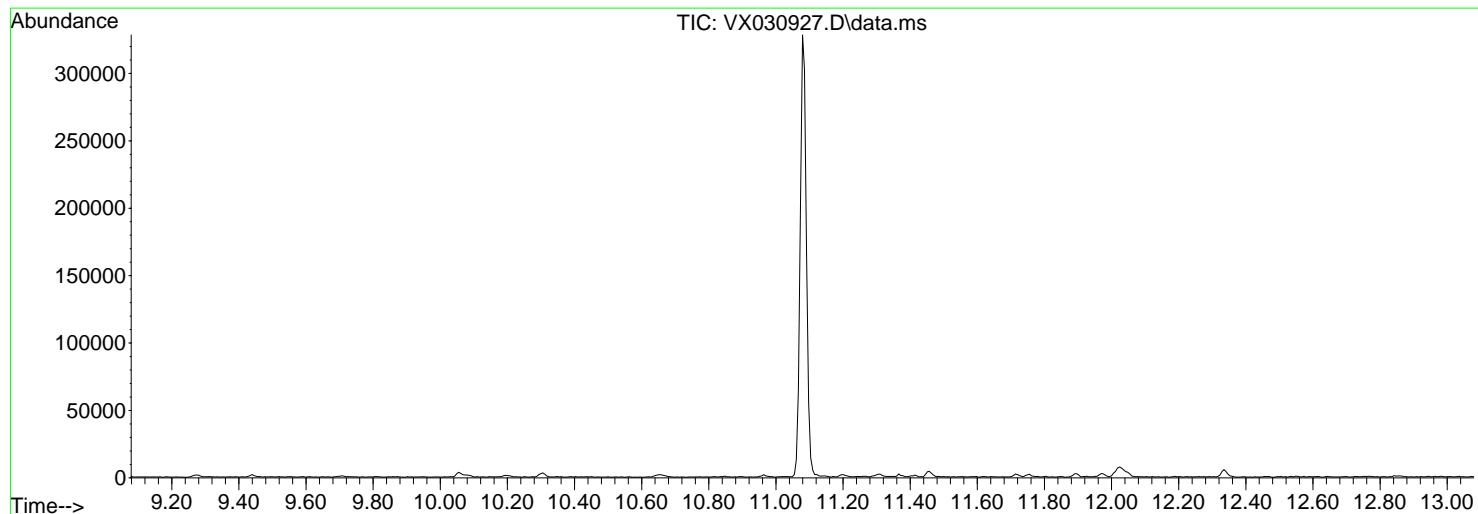

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result
50	95	15	40	17.4	10378	PASS
75	95	30	60	49.9	29770	PASS
95	95	100	100	100.0	59693	PASS
96	95	5	9	6.8	4033	PASS
173	174	0.00	2	1.0	427	PASS
174	95	50	100	73.6	43952	PASS
175	174	5	9	8.0	3499	PASS
176	174	95	101	95.9	42136	PASS
177	176	5	9	6.7	2810	PASS