


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083022\
 Data File : VX030940.D
 Acq On : 30 Aug 2022 15:33
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M
 Title : SW846 8260
 Last Update : Tue Aug 30 14:24:53 2022

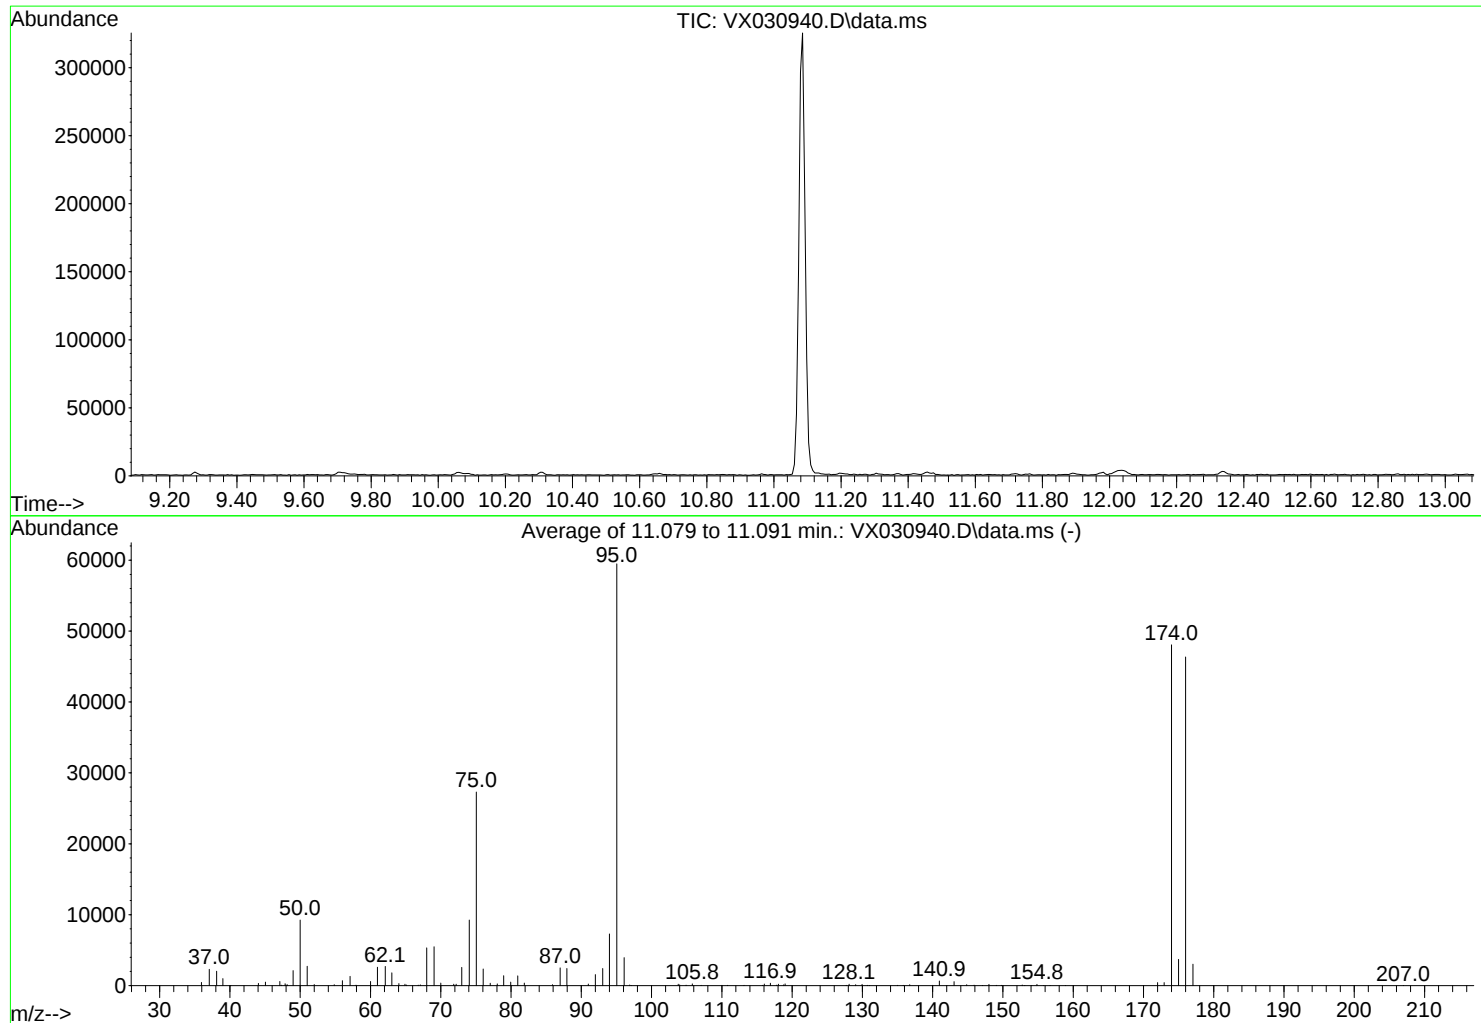

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	9255	PASS
75	95	30	60	45.9	27301	PASS
95	95	100	100	100.0	59483	PASS
96	95	5	9	6.6	3947	PASS
173	174	0.00	2	0.9	437	PASS
174	95	50	100	80.8	48051	PASS
175	174	5	9	7.7	3692	PASS
176	174	95	101	96.5	46347	PASS
177	176	5	9	6.5	3027	PASS