

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083023\
 Data File : VX037403.D
 Acq On : 31 Aug 2023 03:50
 Operator : JC/MD
 Sample : VX0830WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0830WBL02

Quant Time: Aug 31 07:05:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 18 09:30:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	155568	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	256387	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	227675	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	103774	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	94245	42.021	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	84.040%
35) Dibromofluoromethane	5.385	113	78276	46.099	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.200%
50) Toluene-d8	8.647	98	302108	49.049	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.100%
62) 4-Bromofluorobenzene	11.079	95	109919	45.412	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.820%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083023\
Data File : VX037403.D
Acq On : 31 Aug 2023 03:50
Operator : JC/MD
Sample : VX0830WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0830WBL02

Quant Time: Aug 31 07:05:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 18 09:30:38 2023
Response via : Initial Calibration




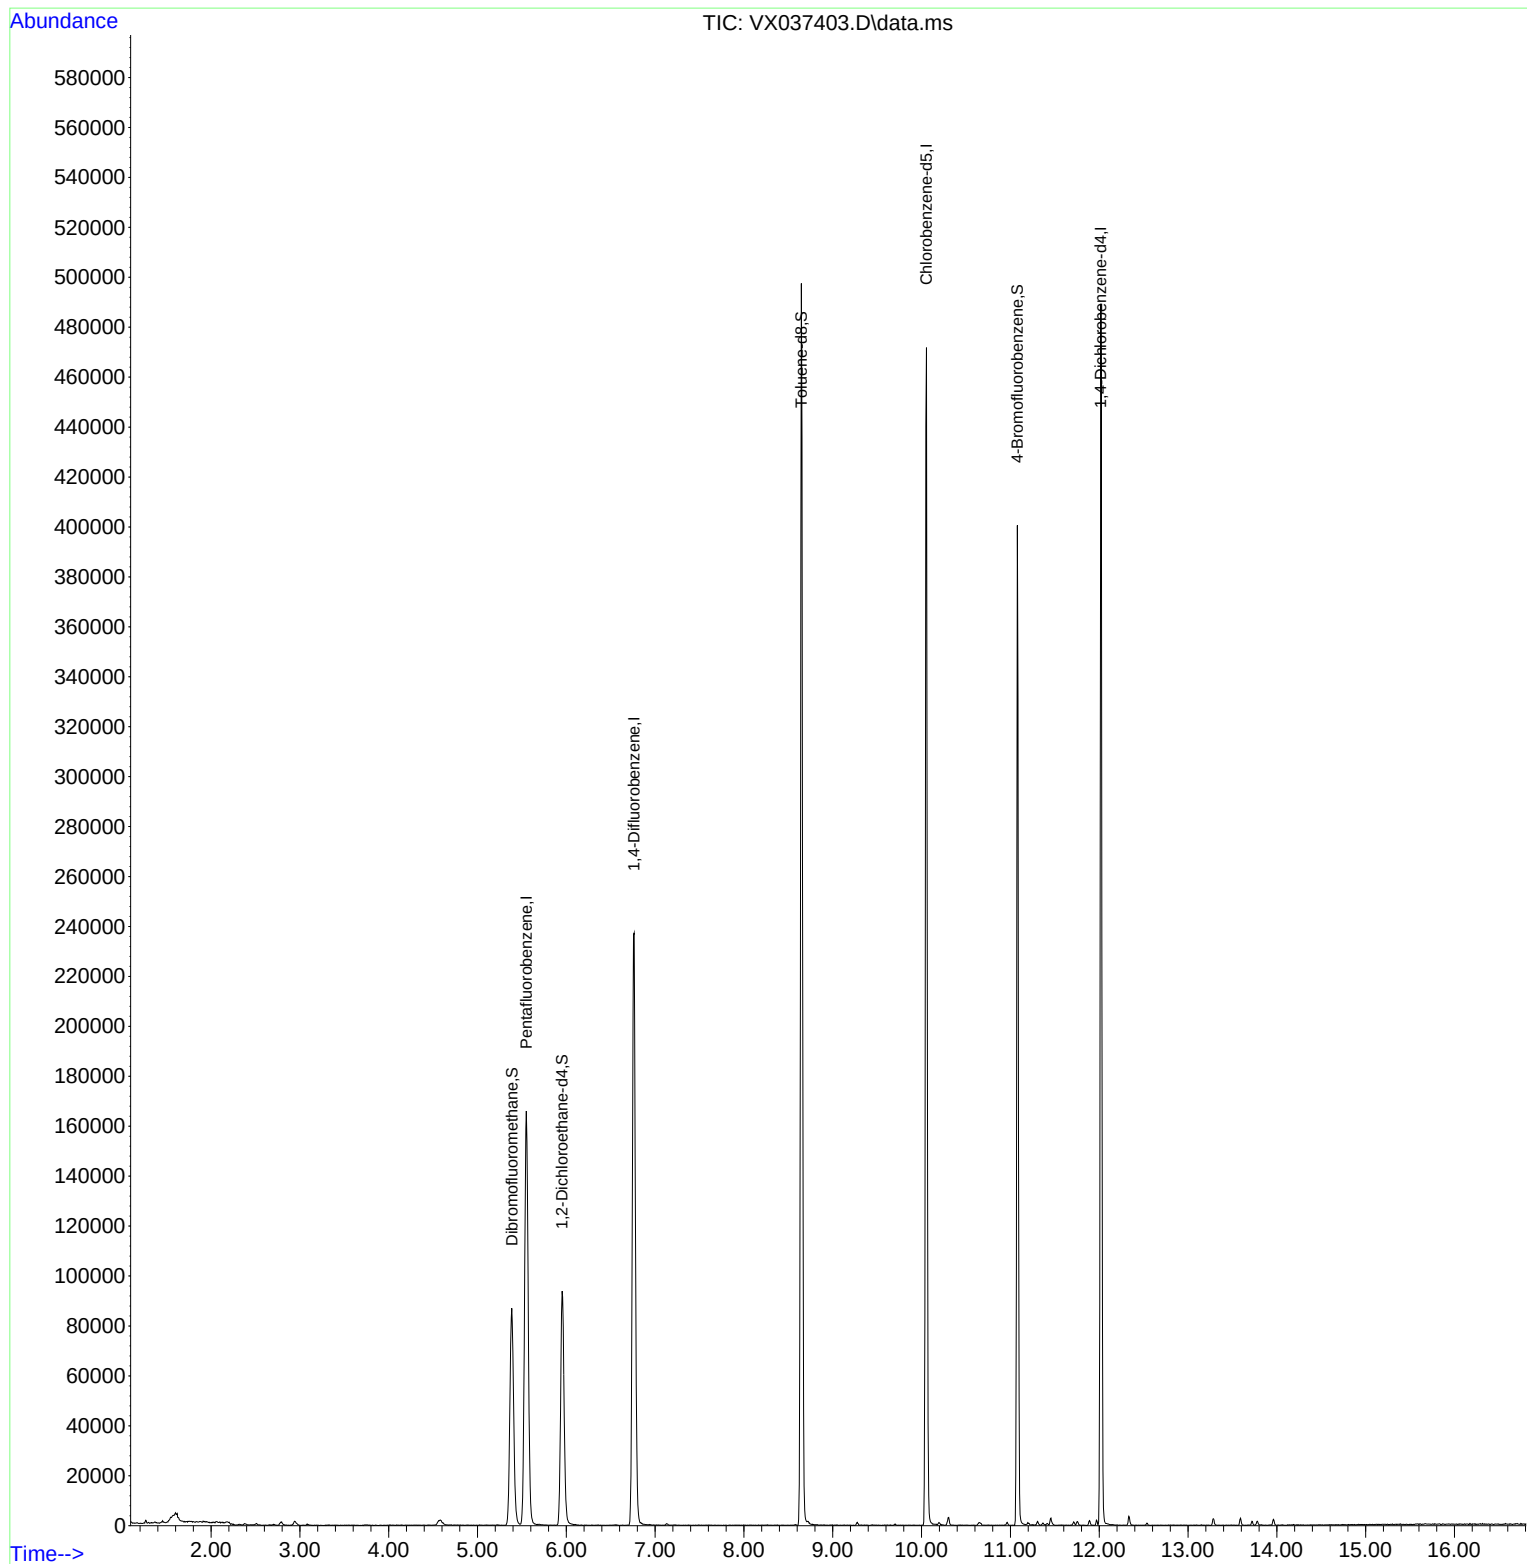


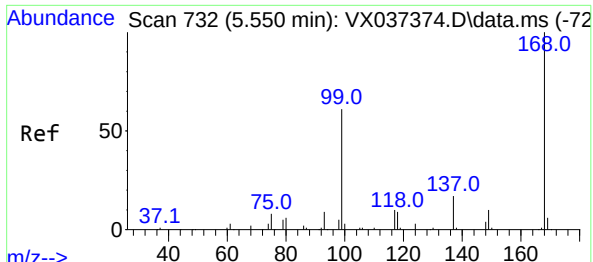

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX037403.D
Acq: 31 Aug 2023 03:50




Instrument :
MSVOA_X
ClientSampleId :
VX0830WBL02


Tgt Ion:168 Resp: 155568
Ion Ratio Lower Upper
168 100
99 63.3 56.6 85.0

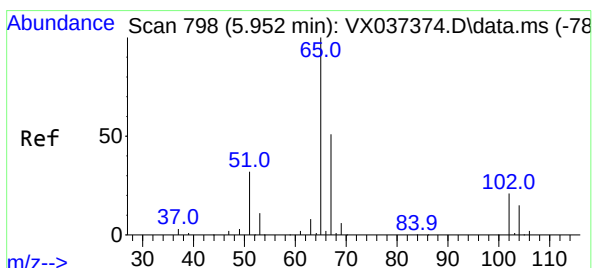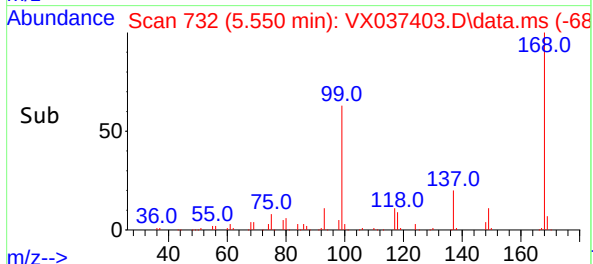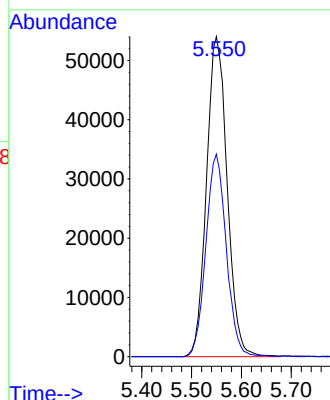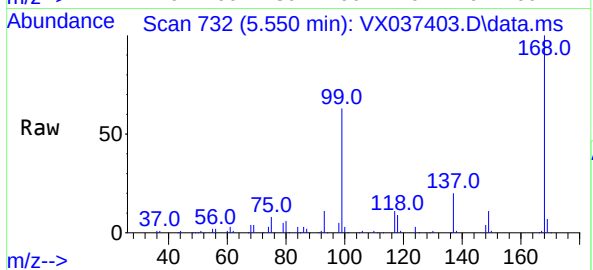

#33
1,2-Dichloroethane-d4
Concen: 42.021 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX037403.D
Acq: 31 Aug 2023 03:50

Tgt Ion: 65 Resp: 94245
Ion Ratio Lower Upper
65 100
67 52.5 0.0 100.2


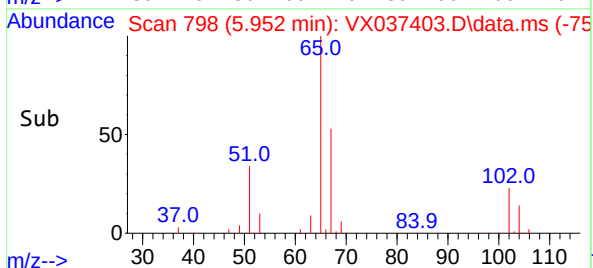
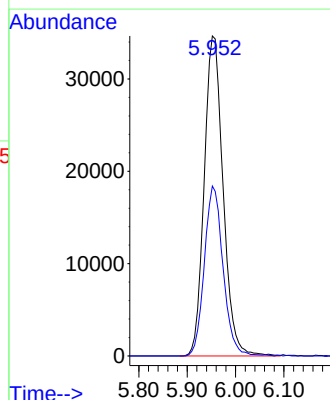
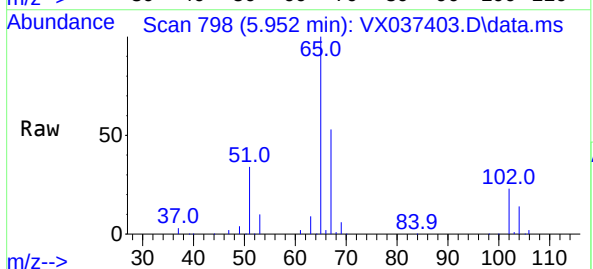


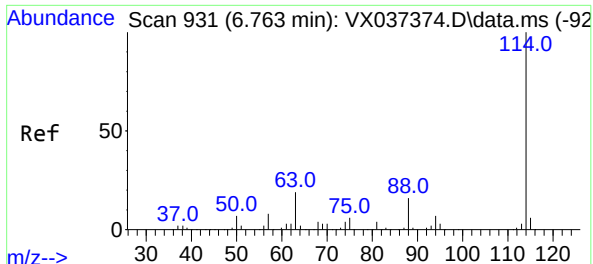

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX037403.D
Acq: 31 Aug 2023 03:50




Instrument :
MSVOA_X
ClientSampleId :
VX0830WBL02


Tgt Ion:114 Resp: 256387
Ion Ratio Lower Upper
114 100
63 19.1 0.0 45.0
88 16.0 0.0 36.6

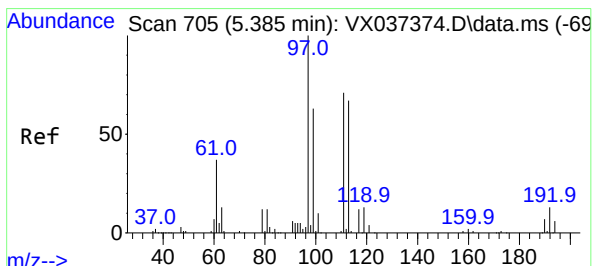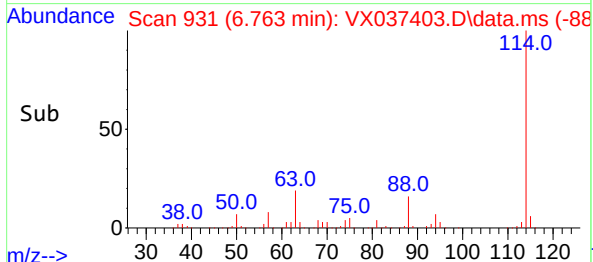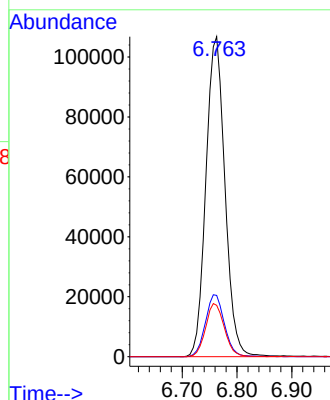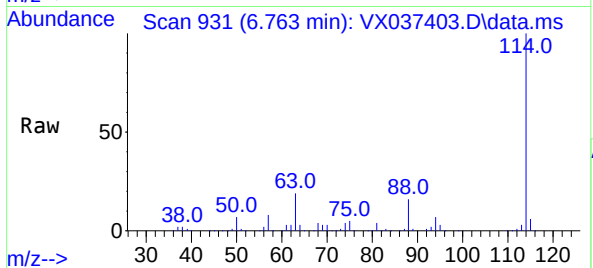

#35
Dibromofluoromethane
Concen: 46.099 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX037403.D
Acq: 31 Aug 2023 03:50

Tgt Ion:113 Resp: 78276
Ion Ratio Lower Upper
113 100
111 102.9 82.9 124.3
192 18.8 13.3 19.9


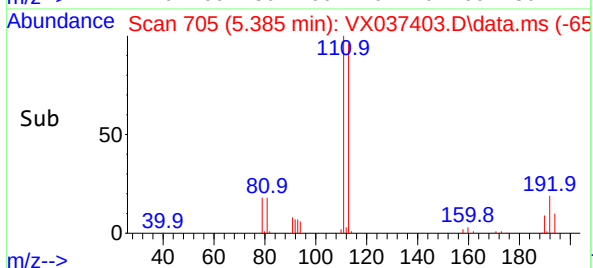
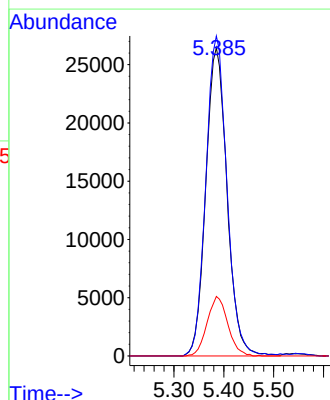
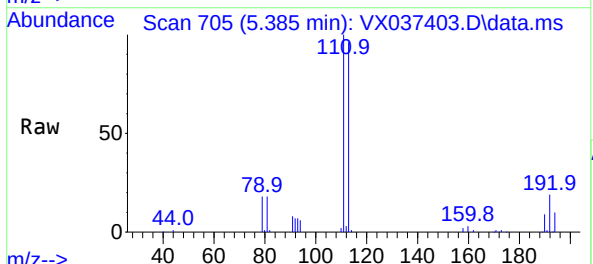


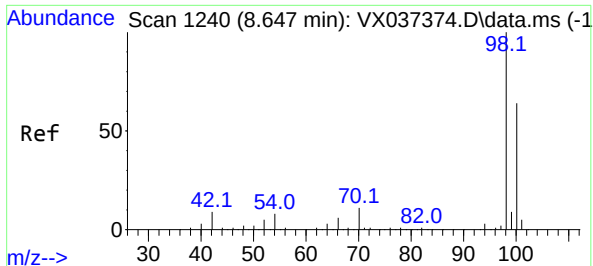

#50
Toluene-d8
Concen: 49.049 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX037403.D
Acq: 31 Aug 2023 03:50




Instrument :
MSVOA_X
ClientSampleId :
VX0830WBL02


Tgt Ion: 98 Resp: 302108
Ion Ratio Lower Upper
98 100
100 66.5 53.1 79.7

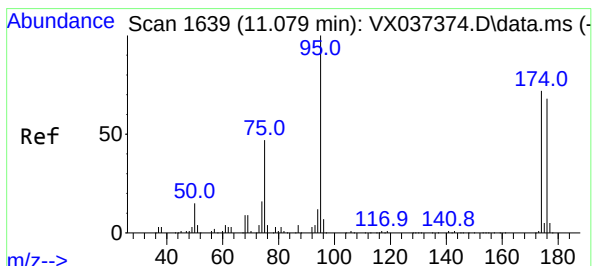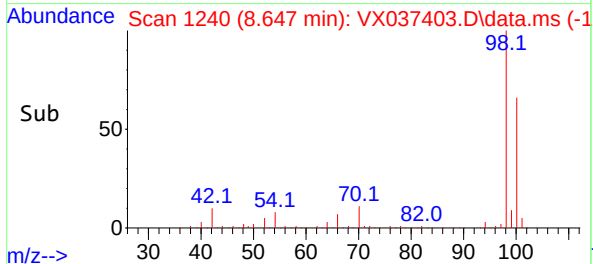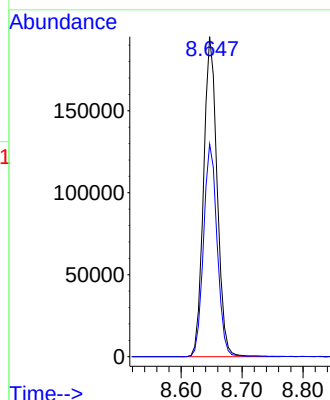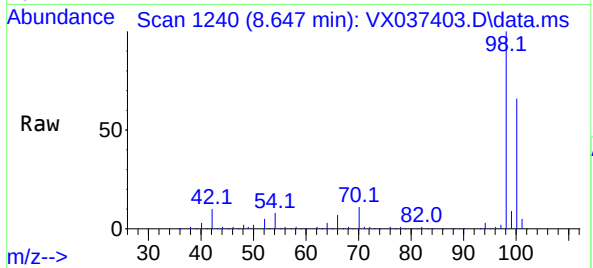

#62
4-Bromofluorobenzene
Concen: 45.412 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX037403.D
Acq: 31 Aug 2023 03:50

Tgt Ion: 95 Resp: 109919
Ion Ratio Lower Upper
95 100
174 73.7 0.0 135.6
176 72.1 0.0 131.0


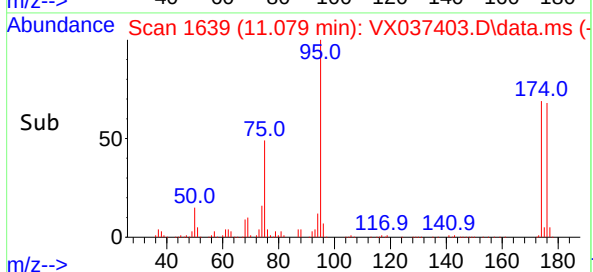
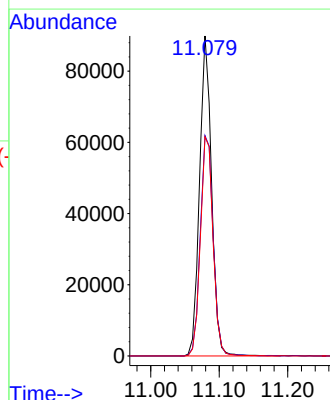
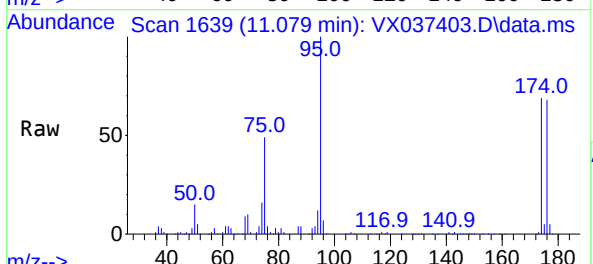


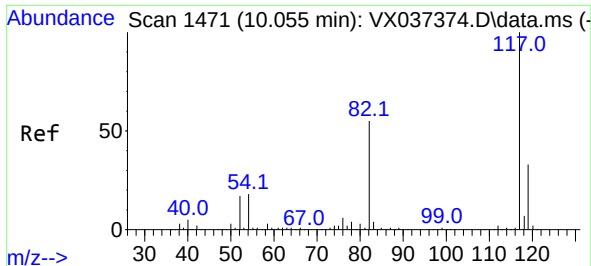

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX037403.D
Acq: 31 Aug 2023 03:50

Instrument :
MSVOA_X
ClientSampleId :
VX0830WBL02

Tgt Ion:117 Resp: 227675
Ion Ratio Lower Upper
117 100
82 53.9 46.2 69.4
119 31.9 25.5 38.3

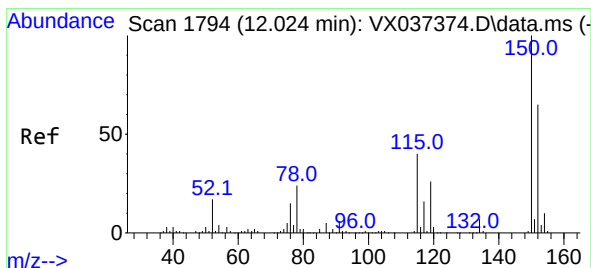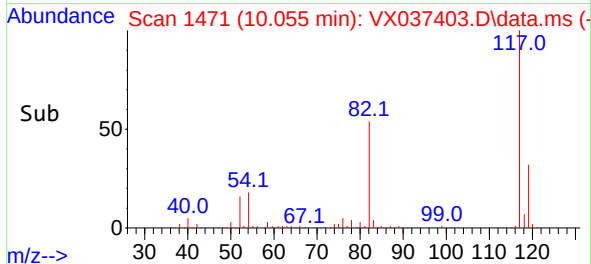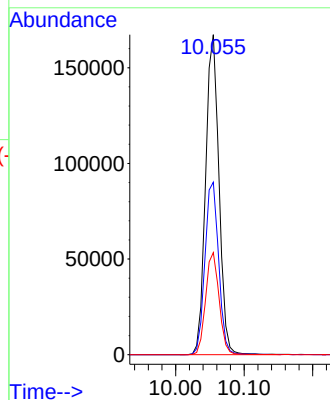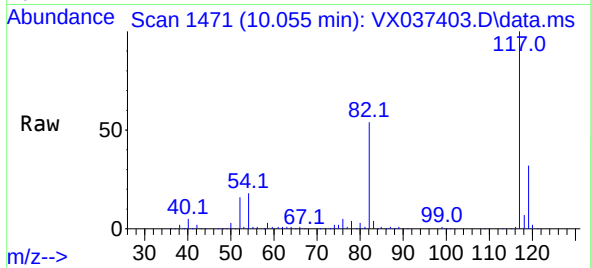

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.006 min
Lab File: VX037403.D
Acq: 31 Aug 2023 03:50

Tgt Ion:152 Resp: 103774
Ion Ratio Lower Upper
152 100
115 62.5 43.3 129.9
150 156.7 0.0 345.0

