

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083023\
 Data File : VX037406.D
 Acq On : 31 Aug 2023 05:02
 Operator : JC/MD
 Sample : 04128-02 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE132D6-20230821

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M

Title : SW846 8260

Signal : TIC: VX037406.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	69	84	85	rBV7	3765	13353	1.79%	0.294%
2	1.624	85	88	97	rVB3	3954	7539	1.01%	0.166%
3	4.580	566	573	585	rVB2	3173	10694	1.43%	0.235%
4	5.385	692	705	721	rBV	84799	248498	33.32%	5.468%
5	5.550	721	732	748	rVB2	160044	456173	61.16%	10.037%
6	5.952	789	798	815	rBV	90350	244413	32.77%	5.378%
7	6.757	921	930	948	rBV	233618	559993	75.09%	12.322%
8	7.123	981	990	1013	rBV	243379	536706	71.96%	11.809%
9	8.647	1233	1240	1250	rBV	482406	745811	100.00%	16.410%
10	10.055	1465	1471	1483	rBV	461911	634935	85.13%	13.971%
11	11.079	1634	1639	1651	rBV	384632	485981	65.16%	10.693%
12	12.024	1788	1794	1803	rBV	462708	600623	80.53%	13.216%


Sum of corrected areas: 4544719

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083023\
Data File : VX037406.D
Acq On : 31 Aug 2023 05:02
Operator : JC/MD
Sample : 04128-02 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D6-20230821

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

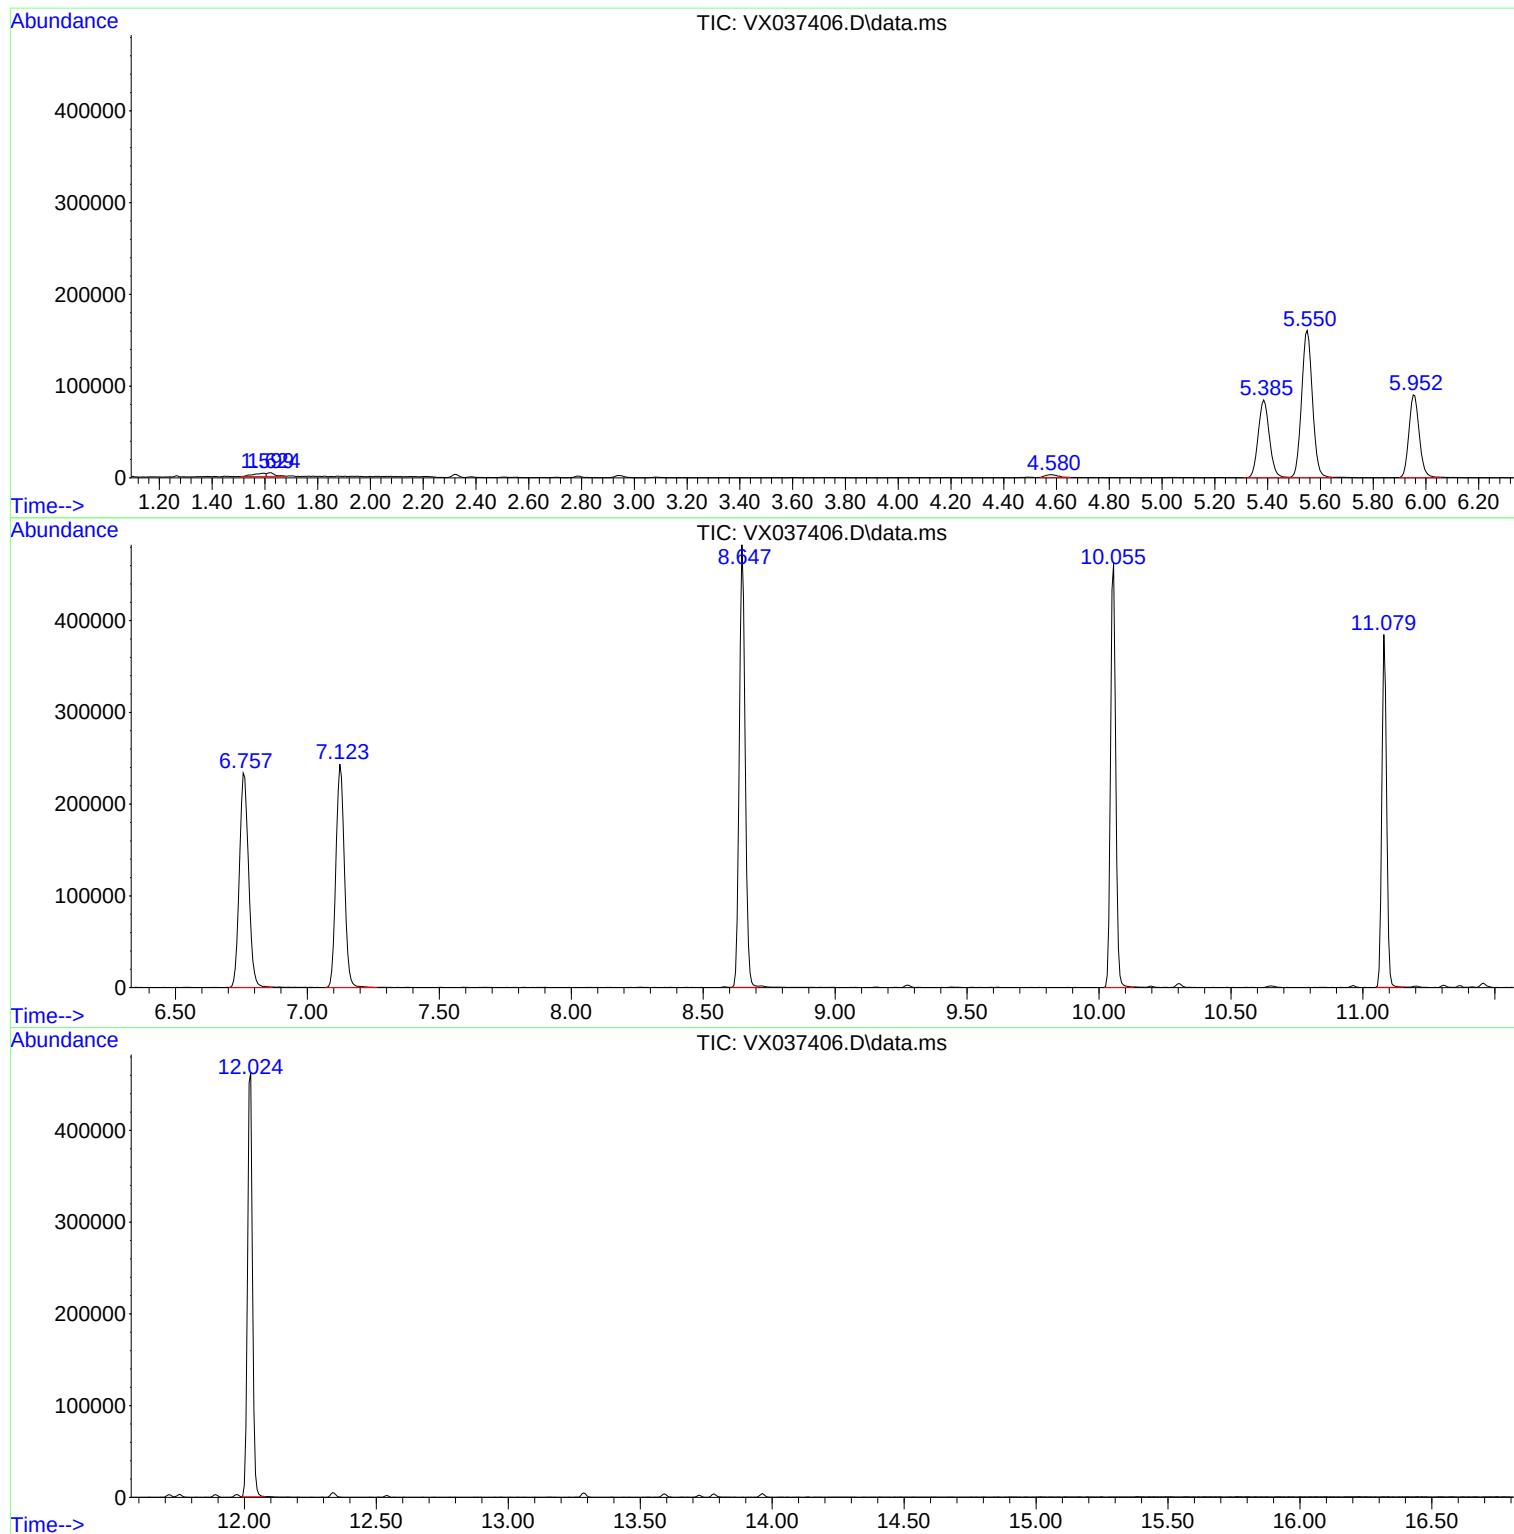

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083023\
Data File : VX037406.D
Acq On : 31 Aug 2023 05:02
Operator : JC/MD
Sample : 04128-02 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D6-20230821

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083023\
Data File : VX037406.D
Acq On : 31 Aug 2023 05:02
Operator : JC/MD
Sample : 04128-02 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D6-20230821

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------