


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX083118\
Data File : VX004327.D
Acq On : 31 Aug 2018 15:08
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
Title : SW846 8260
Last Update : Thu Aug 23 05:39:44 2018

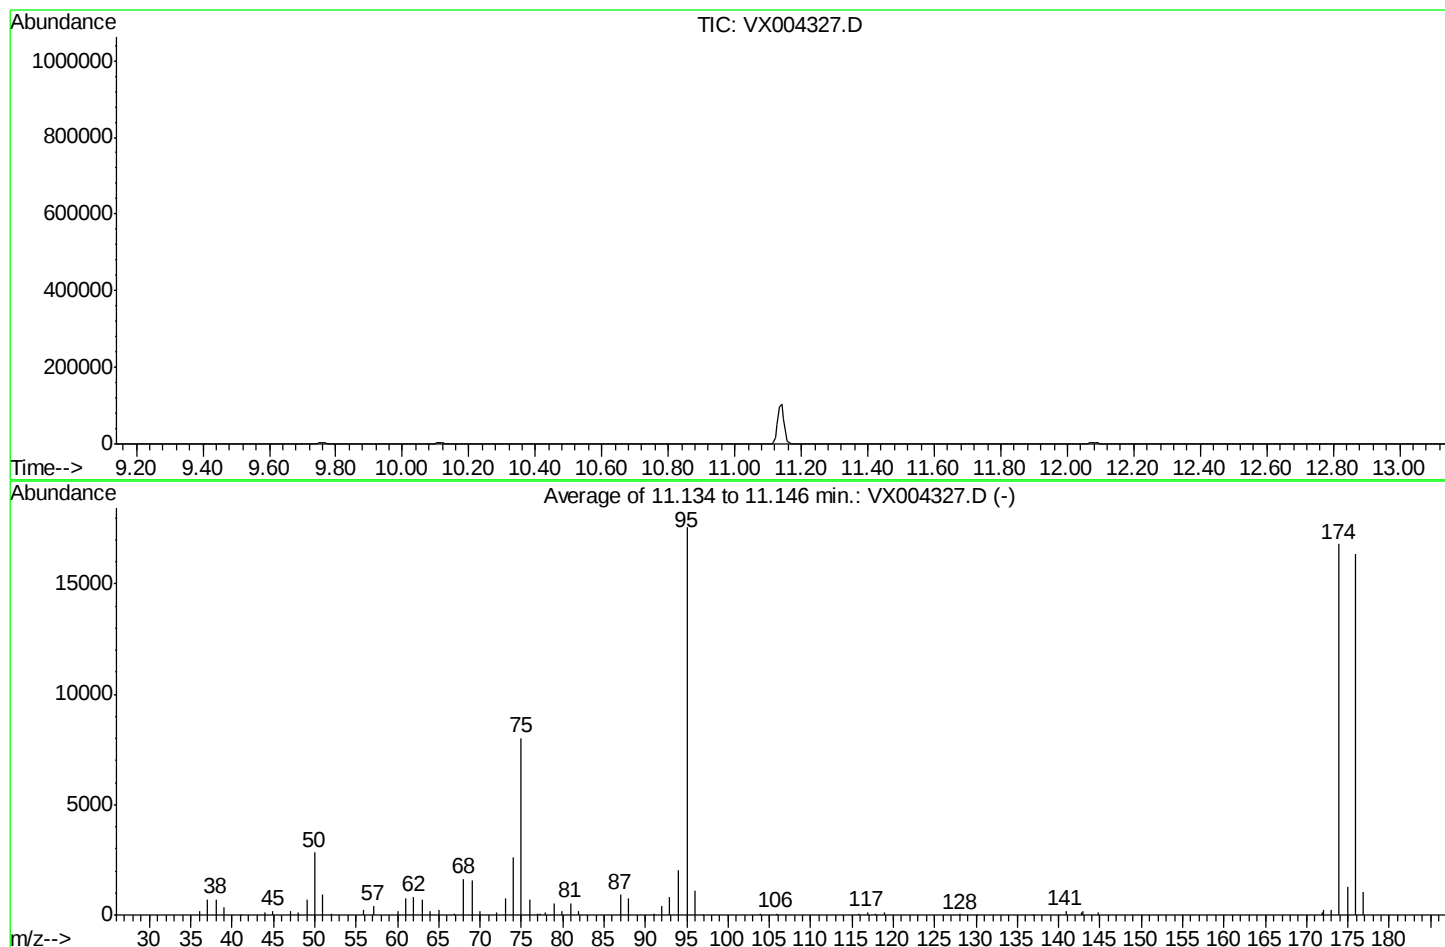

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	2840	PASS
75	95	30	60	45.6	8014	PASS
95	95	100	100	100.0	17556	PASS
96	95	5	9	6.4	1132	PASS
173	174	0.00	2	1.3	214	PASS
174	95	50	100	95.6	16791	PASS
175	174	5	9	7.8	1302	PASS
176	174	95	101	97.5	16364	PASS
177	176	5	9	6.5	1065	PASS