

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083121\
 Data File : VX024040.D
 Acq On : 31 Aug 2021 13:38
 Operator : JC/MD
 Sample : M3584-14 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP02-20210827

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Title : SW846 8260

Signal : TIC: VX024040.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.953	297	306	315	rBV	9362	22042	2.29%	0.401%
2	4.501	549	560	569	rBV	56508	156152	16.22%	2.839%
3	4.593	569	575	591	rVB	12716	38100	3.96%	0.693%
4	5.397	694	707	723	rBV2	96171	278438	28.92%	5.063%
5	5.562	723	734	747	rVV	158679	443639	46.08%	8.067%
6	5.964	789	800	816	rBV	108288	285771	29.68%	5.197%
7	6.769	922	932	944	rBV	259355	597604	62.07%	10.867%
8	7.135	982	992	1005	rBV	441145	962763	100.00%	17.507%
9	8.653	1234	1241	1251	rBV	520147	822479	85.43%	14.956%
10	10.055	1465	1471	1486	rBV	528456	728510	75.67%	13.247%
11	11.085	1634	1640	1651	rBV	442061	548111	56.93%	9.967%
12	12.024	1789	1794	1806	rVB	501412	615673	63.95%	11.196%


Sum of corrected areas: 5499282

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083121\
Data File : VX024040.D
Acq On : 31 Aug 2021 13:38
Operator : JC/MD
Sample : M3584-14 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20210827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

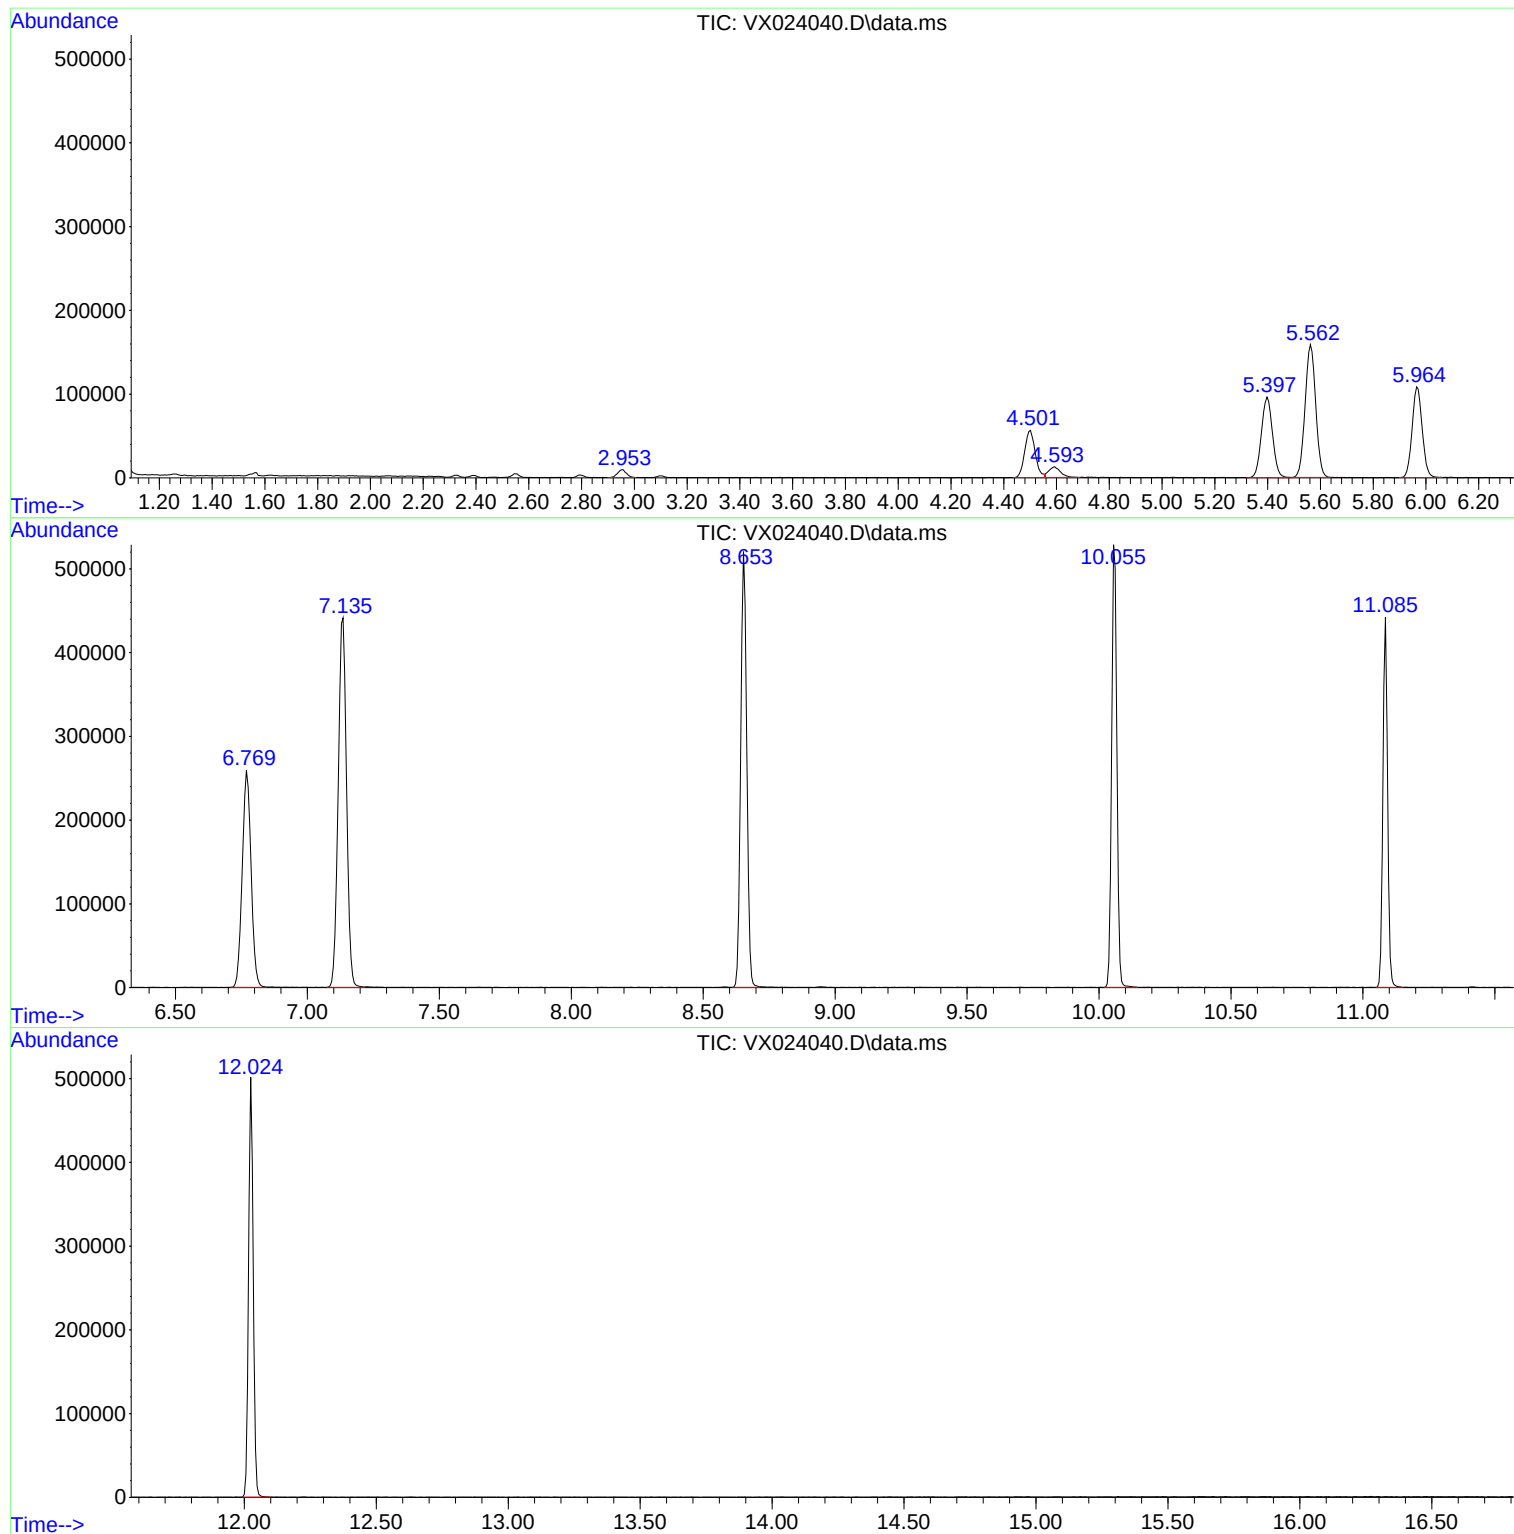

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083121\
Data File : VX024040.D
Acq On : 31 Aug 2021 13:38
Operator : JC/MD
Sample : M3584-14 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20210827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083121\
Data File : VX024040.D
Acq On : 31 Aug 2021 13:38
Operator : JC/MD
Sample : M3584-14 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20210827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------