

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083121\
 Data File : VX024042.D
 Acq On : 31 Aug 2021 14:25
 Operator : JC/MD
 Sample : M3584-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ROOF-DRAIN-20210827

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M

Title : SW846 8260

Signal : TIC: VX024042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.550	234	240	248	rBV	11488	21120	2.57%	0.486%
2	5.397	695	707	722	rBV2	98470	278709	33.97%	6.419%
3	5.562	722	734	747	rBV	155392	440673	53.71%	10.149%
4	5.964	790	800	815	rBV	109363	286052	34.87%	6.588%
5	6.769	922	932	945	rBV	252708	594282	72.43%	13.687%
6	7.135	985	992	1000	rVB4	4293	9453	1.15%	0.218%
7	8.653	1234	1241	1252	rBV	532996	820445	100.00%	18.896%
8	10.055	1466	1471	1488	rVB	537815	726216	88.51%	16.725%
9	11.085	1634	1640	1651	rVB	431797	548329	66.83%	12.628%
10	12.024	1789	1794	1802	rBV	502239	616728	75.17%	14.204%




Sum of corrected areas: 4342007

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083121\
Data File : VX024042.D
Acq On : 31 Aug 2021 14:25
Operator : JC/MD
Sample : M3584-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ROOF-DRAIN-20210827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

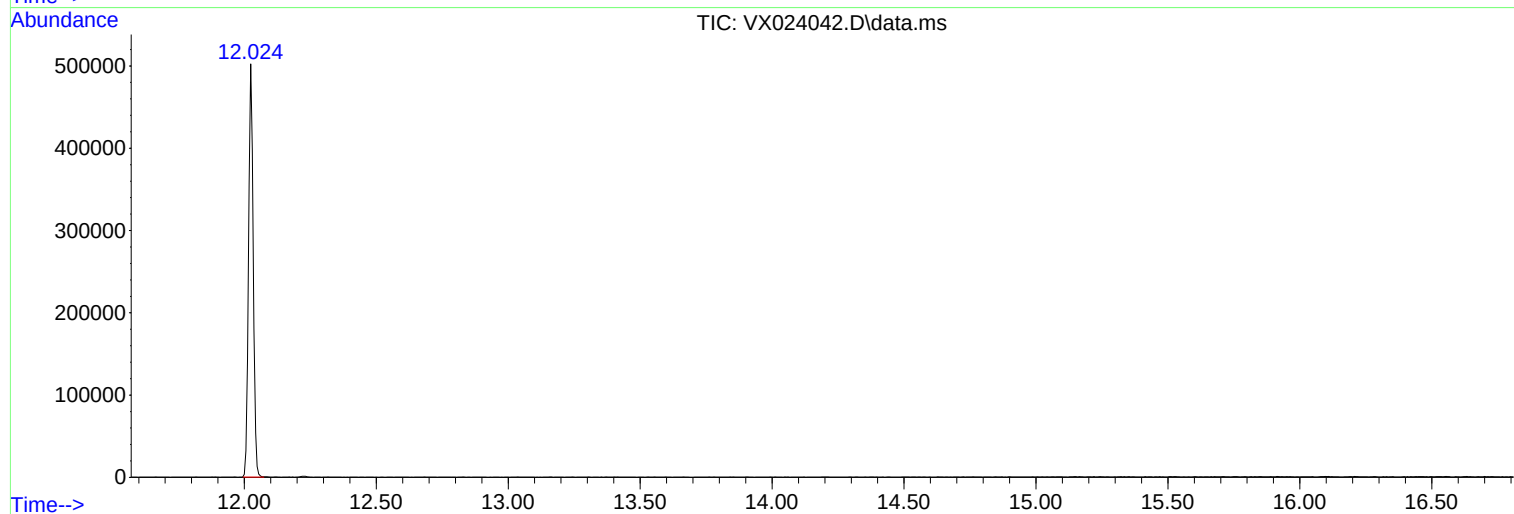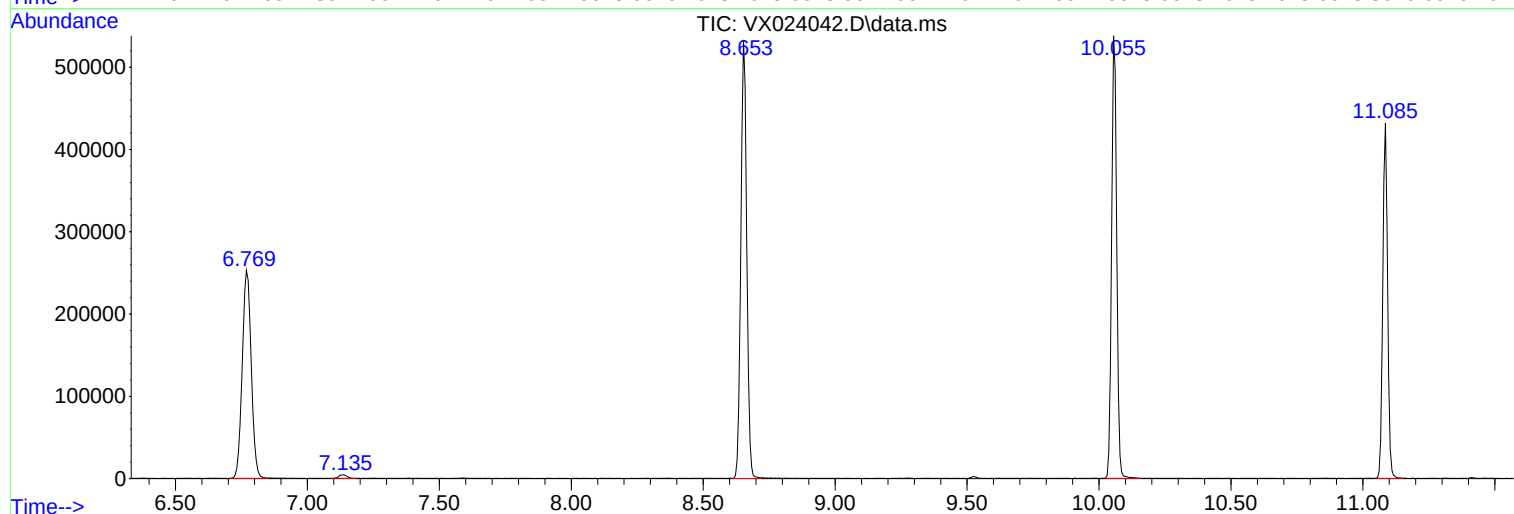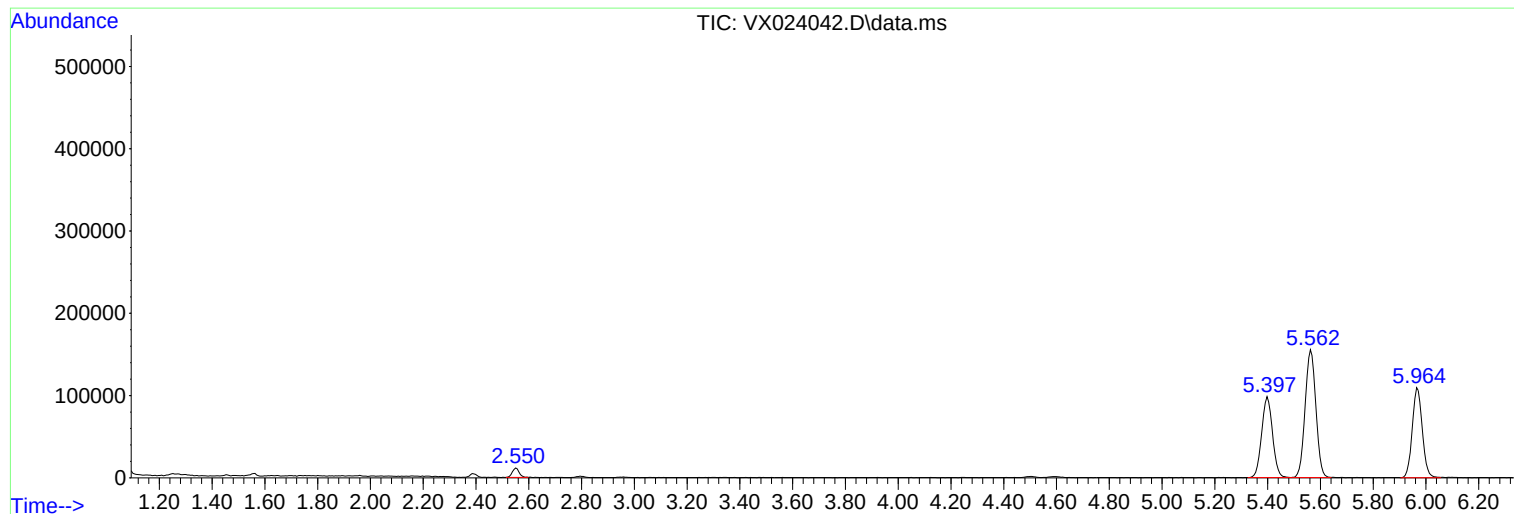

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083121\
Data File : VX024042.D
Acq On : 31 Aug 2021 14:25
Operator : JC/MD
Sample : M3584-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ROOF-DRAIN-20210827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083121\
Data File : VX024042.D
Acq On : 31 Aug 2021 14:25
Operator : JC/MD
Sample : M3584-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ROOF-DRAIN-20210827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------