

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083122\
 Data File : VX030997.D
 Acq On : 31 Aug 2022 23:46
 Operator : JC/MD
 Sample : N4380-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-40

Quant Time: Sep 06 02:26:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 30 14:24:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	213413	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	355102	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	313304	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	139974	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	137214	44.827	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	89.660%		
35) Dibromofluoromethane	5.391	113	126211	48.216	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.440%		
50) Toluene-d8	8.653	98	473499	48.845	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	97.680%		
62) 4-Bromofluorobenzene	11.079	95	162123	46.964	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	93.920%		
Target Compounds			Qvalue			
5) Bromomethane	1.618	94	477	Below Cal	#	72
10) Methyl Iodide	2.465	142	669	4.626	ug/l #	88
11) Tert butyl alcohol	2.971	59	799	1.102	ug/l #	74
13) Acrolein	2.239	56	63	7.440	ug/l #	1
15) Acrylonitrile	3.087	53	594	0.371	ug/l #	47
16) Acetone	2.392	43	2259	1.635	ug/l	91
17) Carbon Disulfide	2.514	76	2334	0.341	ug/l #	89
25) 2-Butanone	4.580	43	504	0.225	ug/l #	48
31) Cyclohexane	5.471	56	6332	1.398	ug/l	97
36) 1,1-Dichloropropene	5.562	75	15188	3.904	ug/l #	50
38) Carbon Tetrachloride	5.562	117	21651	5.845	ug/l #	17
39) Methylcyclohexane	7.379	83	4540	0.954	ug/l #	80
40) Benzene	6.050	78	13232	1.180	ug/l	95
52) Toluene	8.720	92	3401	0.496	ug/l	82
59) 2-Hexanone	9.433	43	652	0.209	ug/l	99
67) Ethyl Benzene	10.195	91	14255	1.085	ug/l	95
68) m/p-Xylenes	10.305	106	3951	0.794	ug/l	95
69) o-Xylene	10.640	106	15030	3.085	ug/l	100
73) Isopropylbenzene	10.963	105	12413	1.121	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	73149	21.227	ug/l #	38
78) n-propylbenzene	11.305	91	6265	0.483	ug/l	98
80) 1,3,5-Trimethylbenzene	11.451	105	3357	0.360	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	73149	63.112	ug/l #	13
84) 1,2,4-Trimethylbenzene	11.756	105	6228	0.652	ug/l	98
85) sec-Butylbenzene	11.890	105	4068	0.342	ug/l	85
89) n-Butylbenzene	12.335	91	3031	0.328	ug/l	87
90) Hexachloroethane	12.616	117	1332	0.769	ug/l #	16
93) 1,2,4-Trichlorobenzene	13.591	180	1133	0.330	ug/l	86
95) Naphthalene	13.780	128	22132	1.804	ug/l	98
96) 1,2,3-Trichlorobenzene	13.969	180	1028	0.297	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083122\
Data File : VX030997.D
Acq On : 31 Aug 2022 23:46
Operator : JC/MD
Sample : N4380-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-40

Quant Time: Sep 06 02:26:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 30 14:24:53 2022
Response via : Initial Calibration




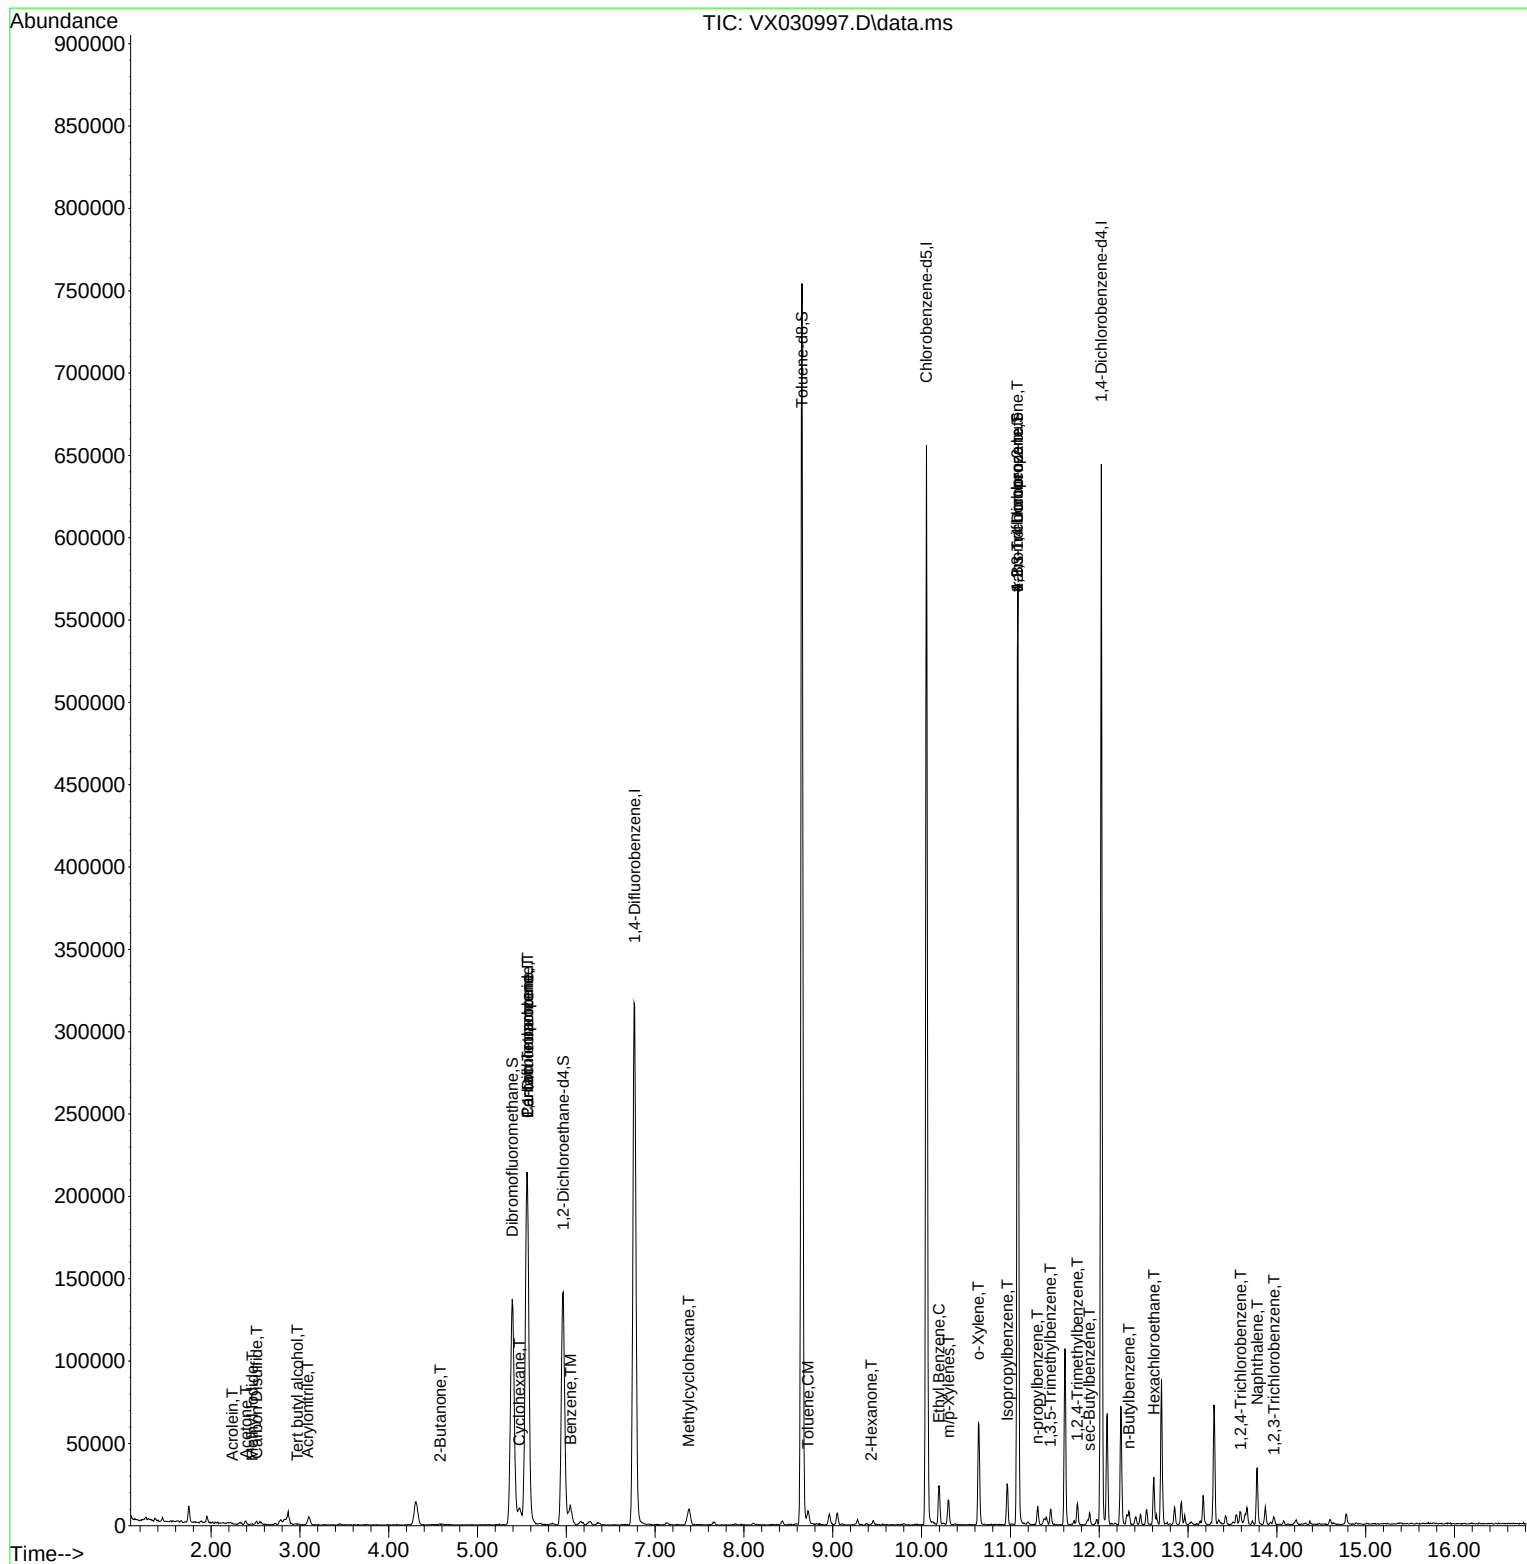


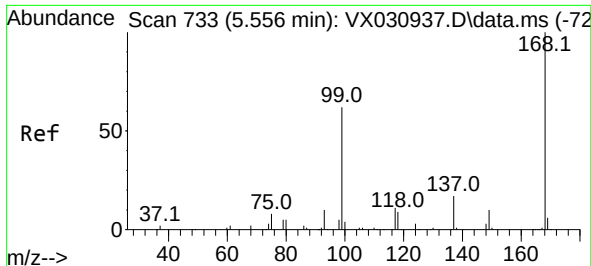

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:168 Resp: 213413
Ion Ratio Lower Upper
168 100
99 55.3 44.0 66.0

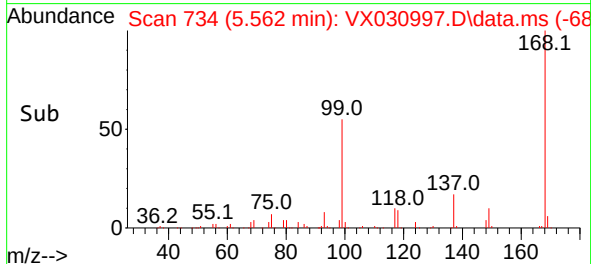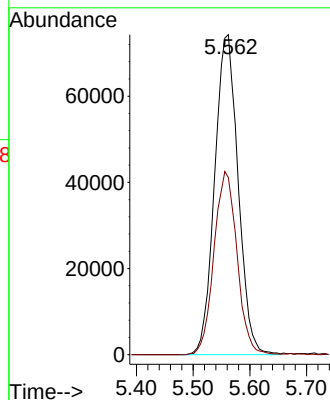

#5
Bromomethane
Concen: Below Cal
RT: 1.618 min Scan# 87
Delta R.T. 0.013 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46


Tgt Ion: 94 Resp: 477
Ion Ratio Lower Upper
94 100
96 69.1 76.9 115.3#

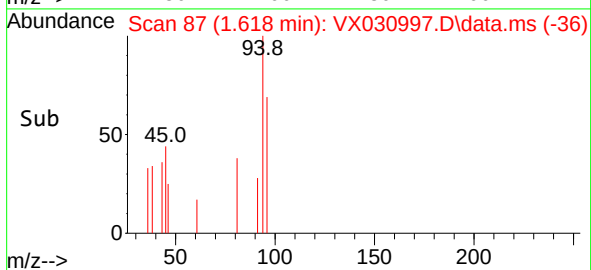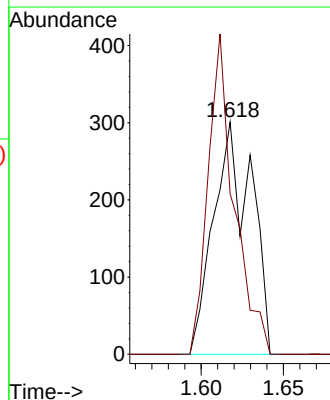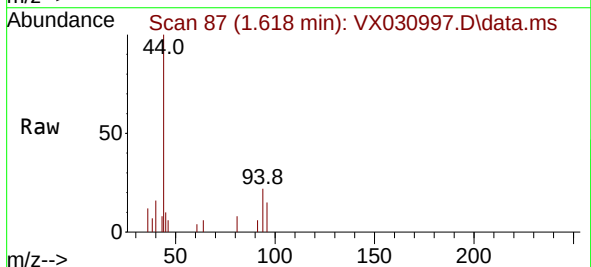






#10
Methyl Iodide
Concen: 4.626 ug/l
RT: 2.465 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46

Instrument :
MSVOA_X
ClientSampleId :
MW-40







Tgt Ion:142 Resp: 669
Ion Ratio Lower Upper
142 100
127 40.1 30.2 45.2
141 0.0 11.3 16.9#

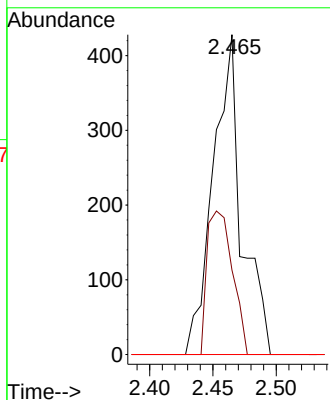

#11
Tert butyl alcohol
Concen: 1.102 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.018 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46

Tgt Ion: 59 Resp: 799
Ion Ratio Lower Upper
59 100
57 0.0 7.4 11.2#


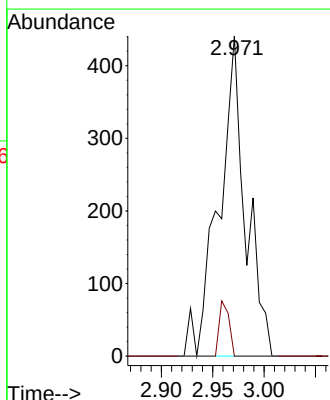

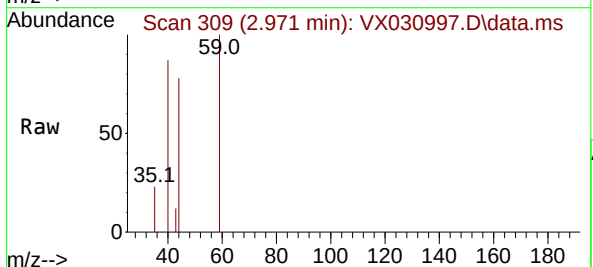




#13
Acrolein
Concen: 7.440 ug/l
RT: 2.239 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 56 Resp: 63
Ion Ratio Lower Upper
56 100
55 187.3 56.6 84.8#

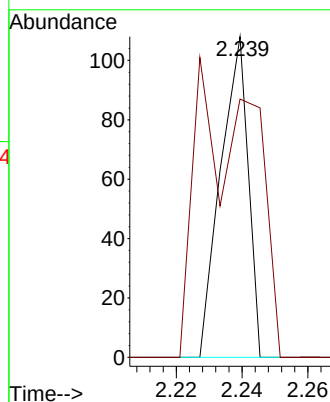

#15
Acrylonitrile
Concen: 0.371 ug/l
RT: 3.087 min Scan# 328
Delta R.T. 0.018 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46

Tgt Ion: 53 Resp: 594
Ion Ratio Lower Upper
53 100
52 30.6 65.4 98.0#
51 9.8 27.7 41.5#


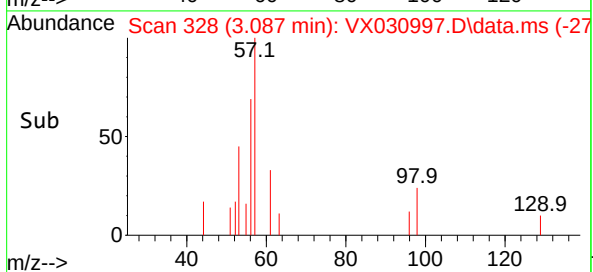
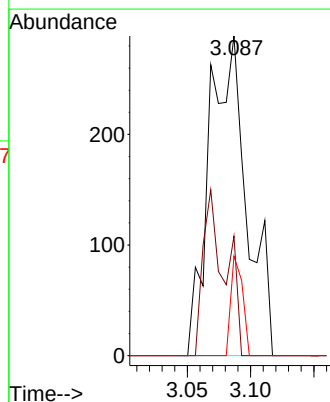



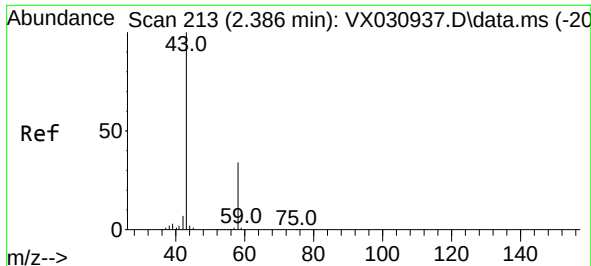

#16
Acetone
Concen: 1.635 ug/l
RT: 2.392 min Scan# 213
Delta R.T. 0.006 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 43 Resp: 2259
Ion Ratio Lower Upper
43 100
58 29.2 27.7 41.5

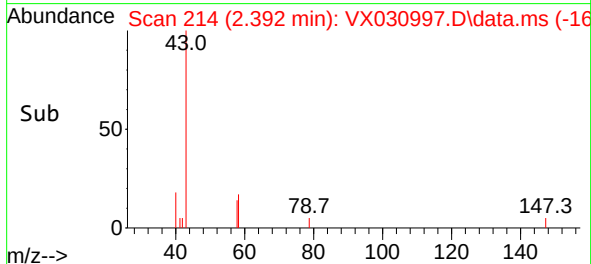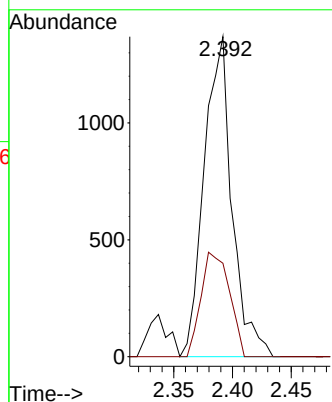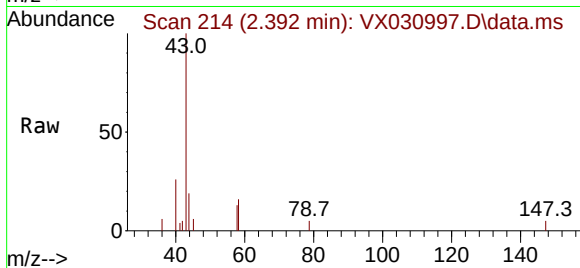

#17
Carbon Disulfide
Concen: 0.341 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46

Tgt Ion: 76 Resp: 2334
Ion Ratio Lower Upper
76 100
78 13.9 7.8 11.6#

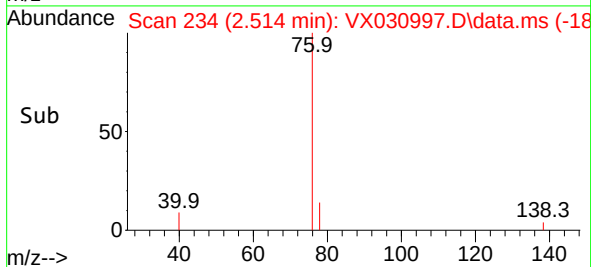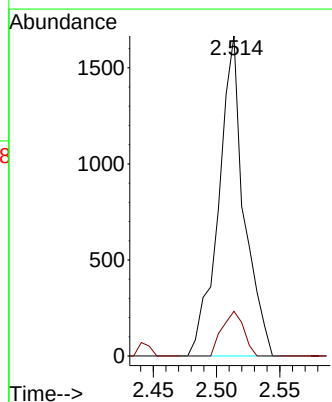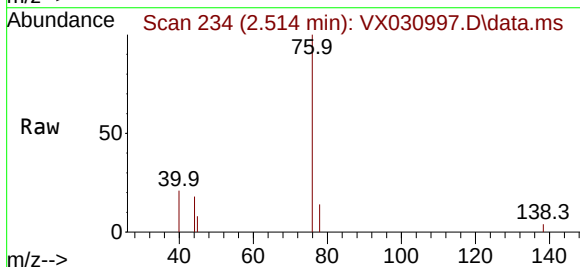



#25

2-Butanone

Concen: 0.225 ug/l

RT: 4.580 min Scan# 51

Delta R.T. 0.012 min

Lab File: VX030997.D

Acq: 31 Aug 2022 23:46

Instrument :

MSVOA_X

ClientSampleId :





MW-40

Tgt Ion: 43 Resp: 504

Ion Ratio Lower Upper

43 100

72 0.0 21.7 32.5#

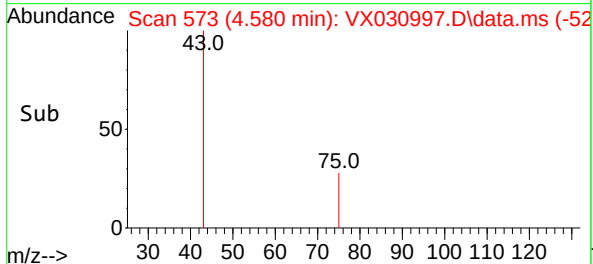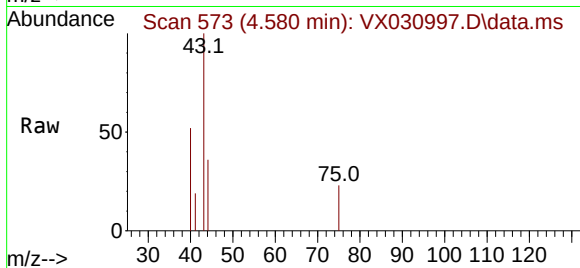

#31

Cyclohexane

Concen: 1.398 ug/l

RT: 5.471 min Scan# 719

Delta R.T. -0.006 min

Lab File: VX030997.D

Acq: 31 Aug 2022 23:46




Tgt Ion: 56 Resp: 6332


Ion Ratio Lower Upper

56 100

69 33.0 25.4 38.0

84 82.8 68.9 103.3


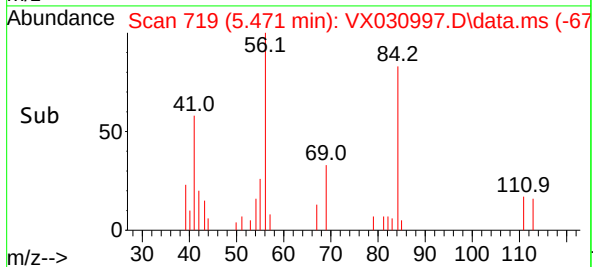

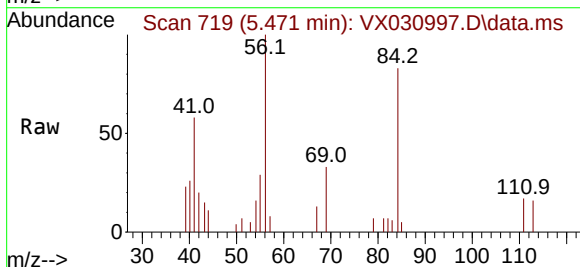




#33
 1,2-Dichloroethane-d4
 Concen: 44.827 ug/l
 RT: 5.964 min Scan# 800
 Delta R.T. 0.006 min
 Lab File: VX030997.D
 Acq: 31 Aug 2022 23:46




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-40


Tgt Ion: 65 Resp: 137214
 Ion Ratio Lower Upper
 65 100
 67 53.6 0.0 109.6

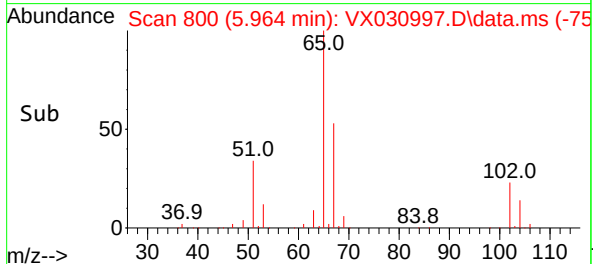

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.769 min Scan# 932
 Delta R.T. 0.000 min
 Lab File: VX030997.D
 Acq: 31 Aug 2022 23:46

Tgt Ion: 114 Resp: 355102
 Ion Ratio Lower Upper
 114 100
 63 18.2 0.0 38.4
 88 14.5 0.0 31.8


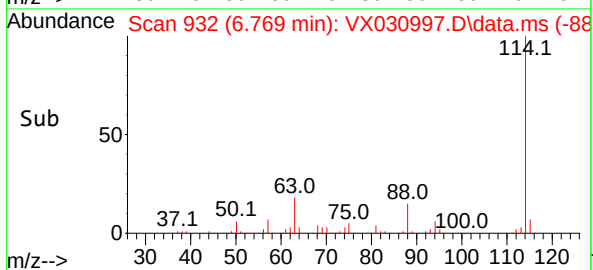

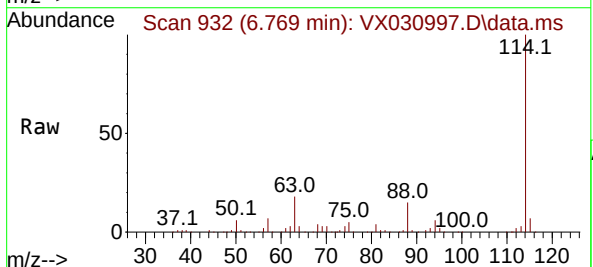




#35
Dibromofluoromethane
Concen: 48.216 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:113 Resp: 126211
Ion Ratio Lower Upper
113 100
111 102.6 83.2 124.8
192 19.5 14.8 22.2

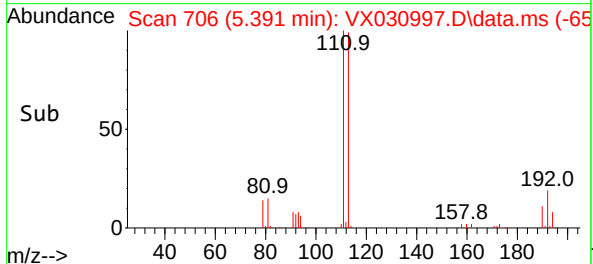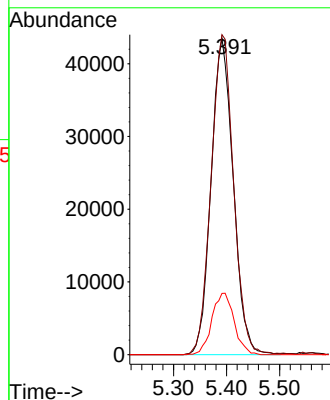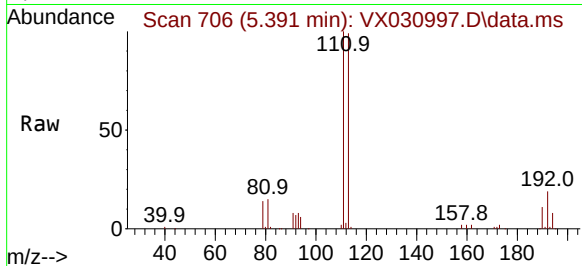

#36
1,1-Dichloropropene
Concen: 3.904 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.134 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46


Tgt Ion: 75 Resp: 15188
Ion Ratio Lower Upper
75 100
110 10.6 19.3 57.9#
77 0.2 24.4 36.6#

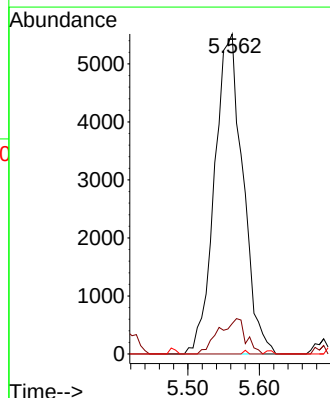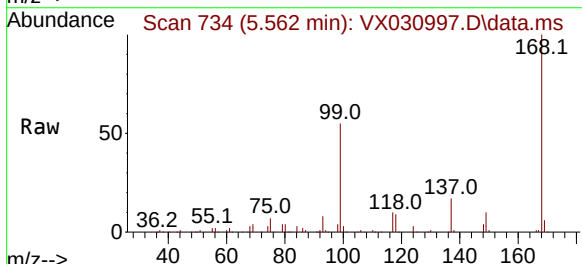






#38
Carbon Tetrachloride
Concen: 5.845 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46

Instrument :
MSVOA_X
ClientSampleId :
MW-40







Tgt Ion:117 Resp: 21651
Ion Ratio Lower Upper
117 100
119 4.8 74.1 111.1#
121 0.0 25.8 38.8#

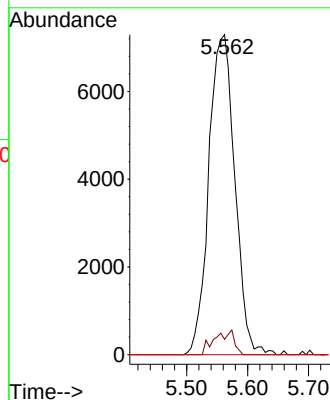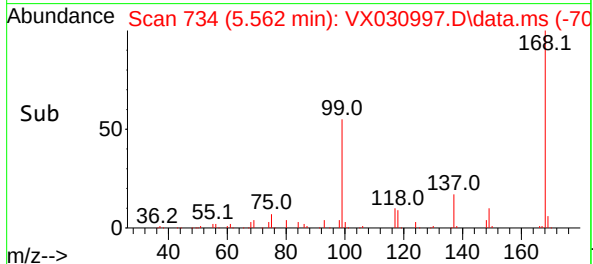

#39
Methylcyclohexane
Concen: 0.954 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46

Tgt Ion: 83 Resp: 4540
Ion Ratio Lower Upper
83 100
55 53.6 57.7 86.5#
98 35.1 36.5 54.7#


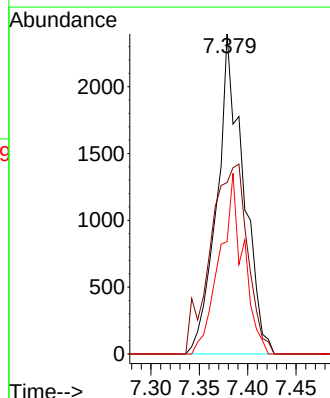
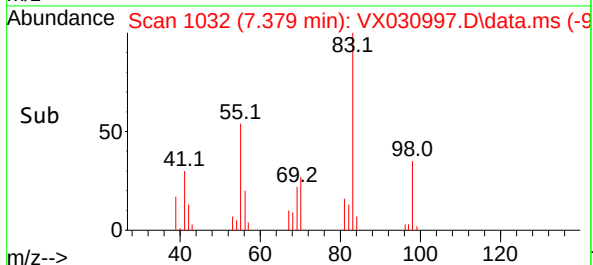
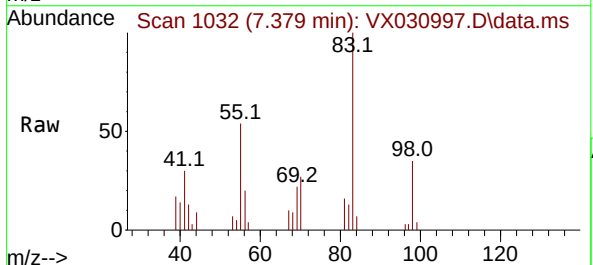




#40
Benzene
Concen: 1.180 ug/l
RT: 6.050 min Scan# 813
Delta R.T. 0.006 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 78 Resp: 13232
Ion Ratio Lower Upper
78 100
77 20.3 18.0 27.0

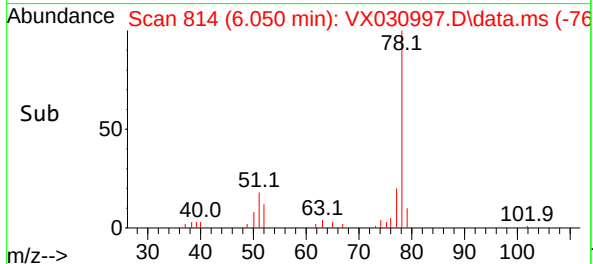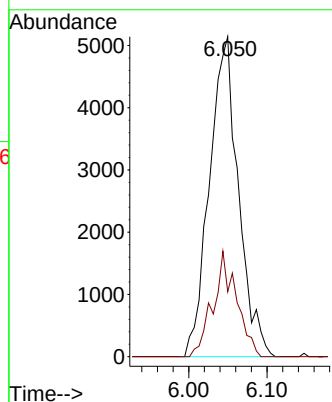

#50
Toluene-d8
Concen: 48.845 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46

Tgt Ion: 98 Resp: 473499
Ion Ratio Lower Upper
98 100
100 63.2 52.3 78.5


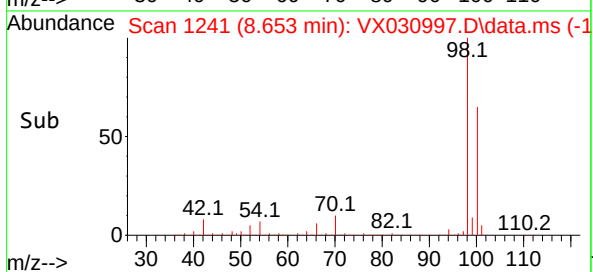
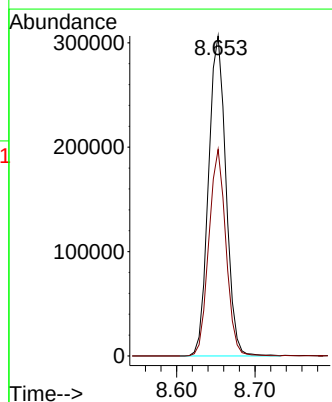





#52
Toluene
Concen: 0.496 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 92 Resp: 3401
Ion Ratio Lower Upper
92 100
91 148.5 139.2 208.8

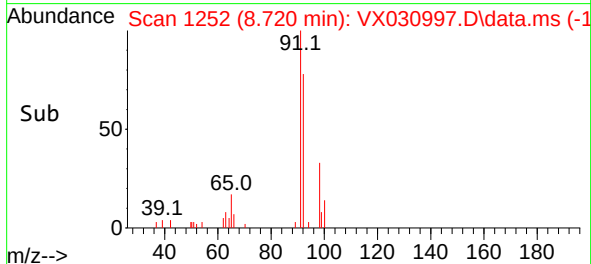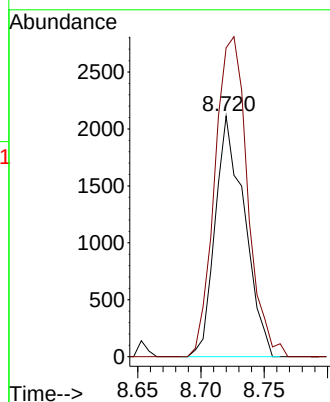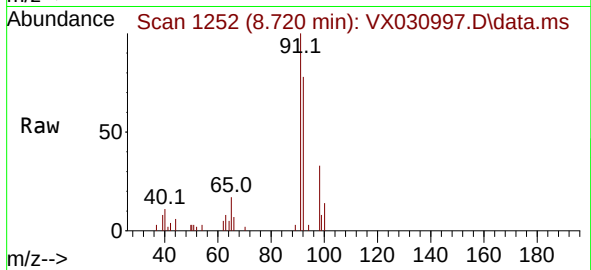

#59
2-Hexanone
Concen: 0.209 ug/l
RT: 9.433 min Scan# 1369
Delta R.T. 0.000 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46

Tgt Ion: 43 Resp: 652
Ion Ratio Lower Upper
43 100
58 54.3 27.6 82.8

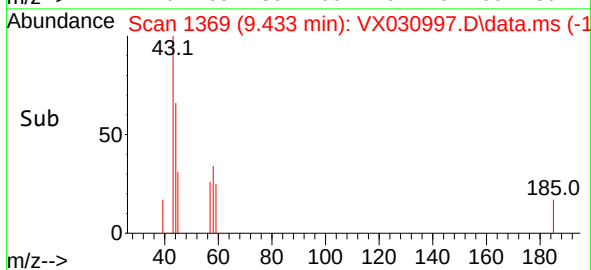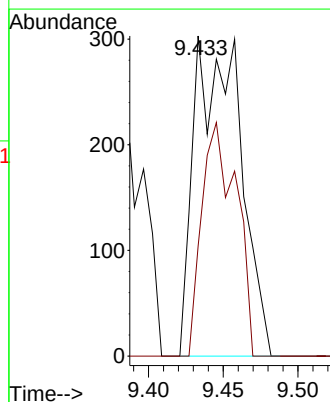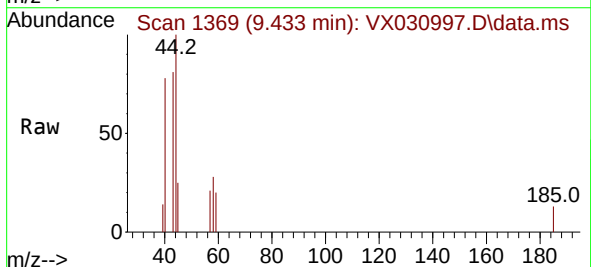

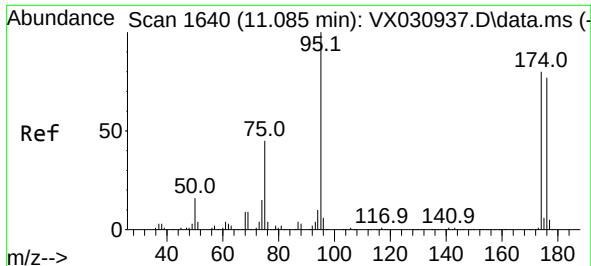

#62

4-Bromofluorobenzene

Concen: 46.964 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX030997.D

Acq: 31 Aug 2022 23:46

Instrument :

MSVOA_X

ClientSampleId :

MW-40





Tgt Ion: 95 Resp: 162123

Ion Ratio Lower Upper

95 100

174 81.2 0.0 149.0

176 78.2 0.0 146.0

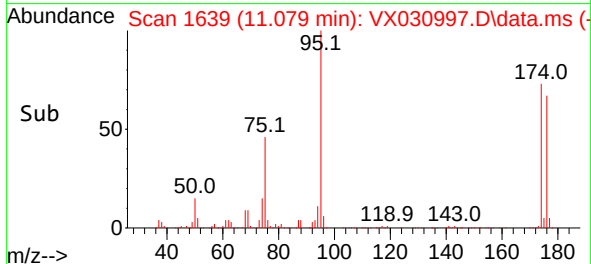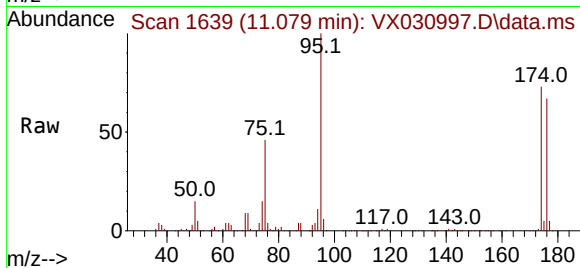

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX030997.D

Acq: 31 Aug 2022 23:46




Tgt Ion: 117 Resp: 313304


Ion Ratio Lower Upper

117 100

82 52.4 42.7 64.1

119 33.3 25.4 38.2

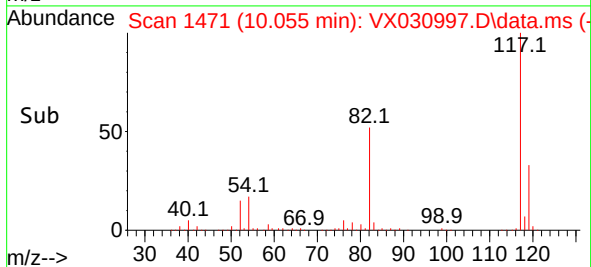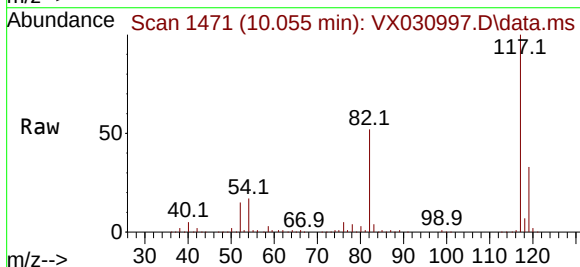

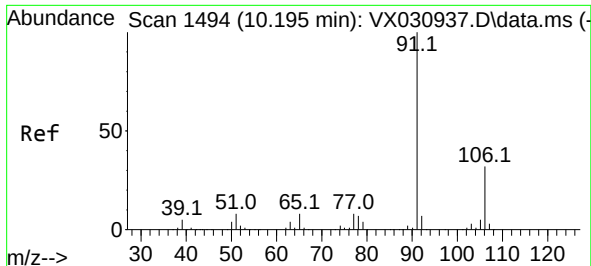

#67

Ethyl Benzene

Concen: 1.085 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX030997.D

Acq: 31 Aug 2022 23:46

Instrument :

MSVOA_X

ClientSampleId :





MW-40

Tgt Ion: 91 Resp: 14255

Ion Ratio Lower Upper

91 100

106 34.7 25.5 38.3

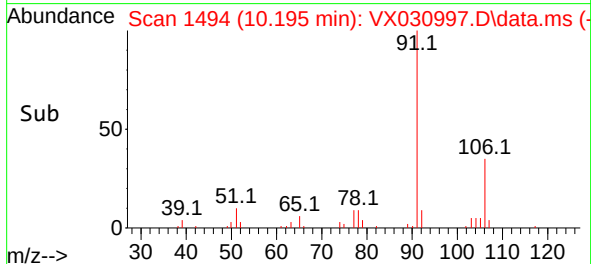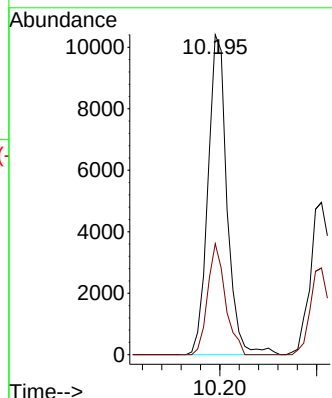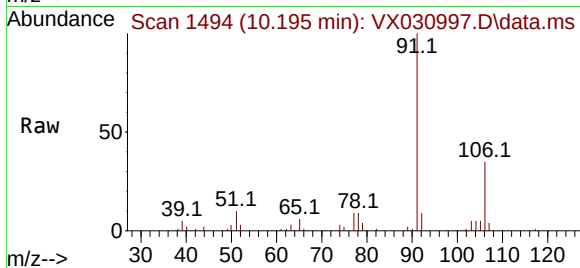

#68

m/p-Xylenes

Concen: 0.794 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. 0.000 min

Lab File: VX030997.D




Acq: 31 Aug 2022 23:46


Tgt Ion: 106 Resp: 3951

Ion Ratio Lower Upper

106 100

91 190.9 158.2 237.4


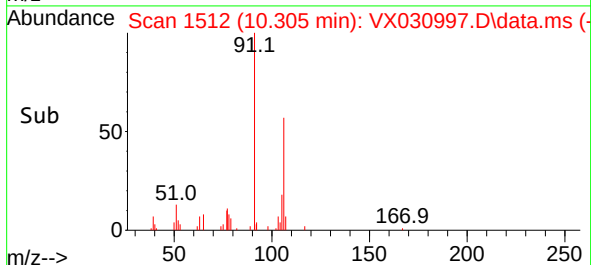
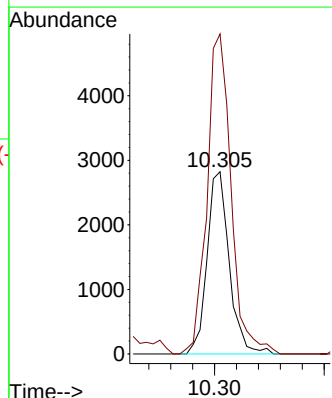
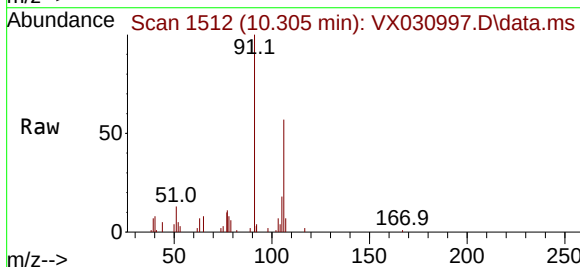




#69
o-Xylene
Concen: 3.085 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:106 Resp: 15030
Ion Ratio Lower Upper
106 100
91 208.4 103.8 311.6

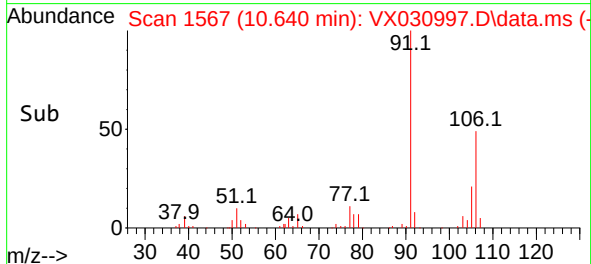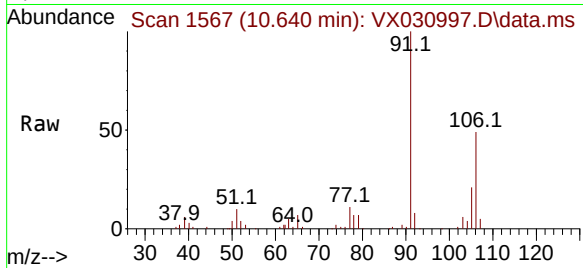

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46

Tgt Ion:152 Resp: 139974
Ion Ratio Lower Upper
152 100
115 57.7 40.5 121.5
150 156.1 0.0 347.0

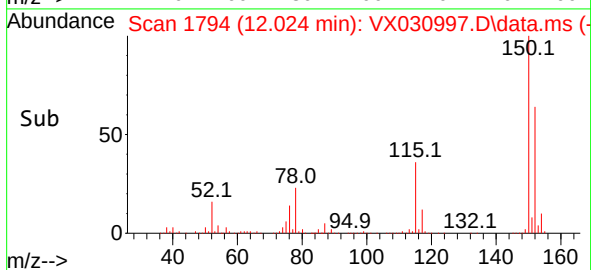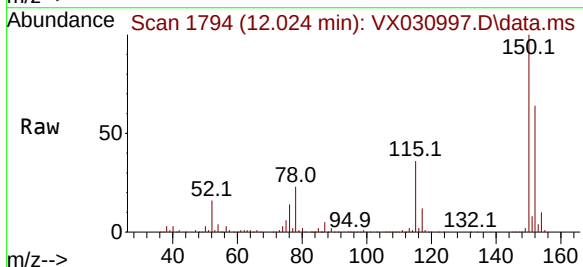

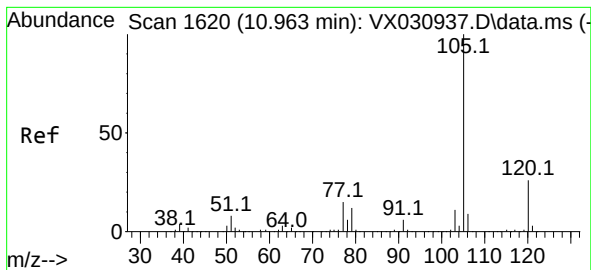

#73

Isopropylbenzene

Concen: 1.121 ug/l

RT: 10.963 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX030997.D

Acq: 31 Aug 2022 23:46

Instrument :

MSVOA_X

ClientSampleId :





MW-40

Tgt Ion:105 Resp: 12413

Ion Ratio Lower Upper

105 100

120 27.6 13.5 40.4

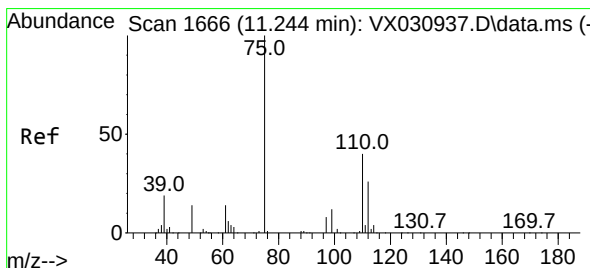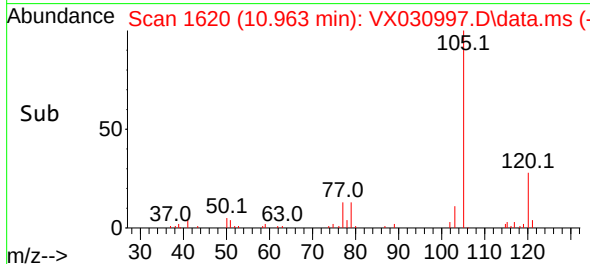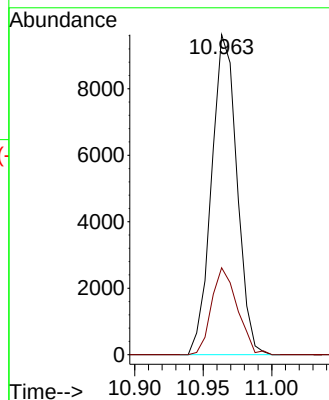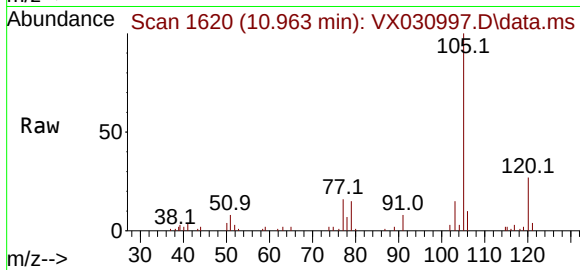

#76

1,2,3-Trichloropropane

Concen: 21.227 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.165 min

Lab File: VX030997.D




Acq: 31 Aug 2022 23:46


Tgt Ion: 75 Resp: 73149

Ion Ratio Lower Upper

75 100

77 1.3 19.8 59.3#


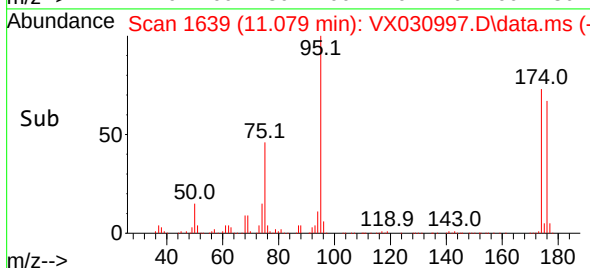
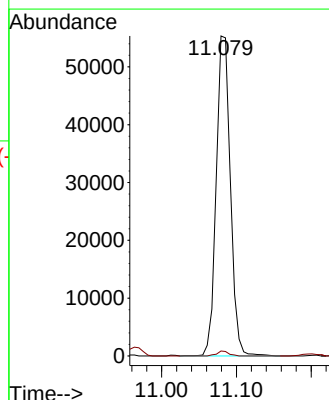
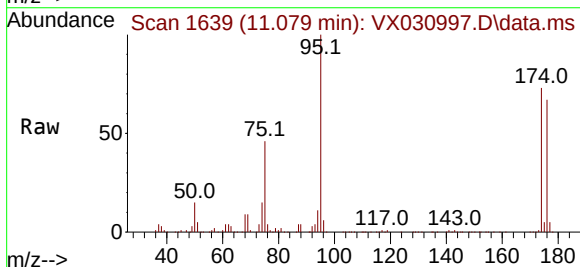


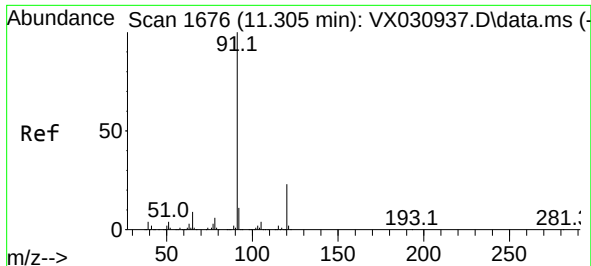

#78
n-propylbenzene
Concen: 0.483 ug/l
RT: 11.305 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 91 Resp: 6265
Ion Ratio Lower Upper
91 100
120 24.3 11.6 34.8

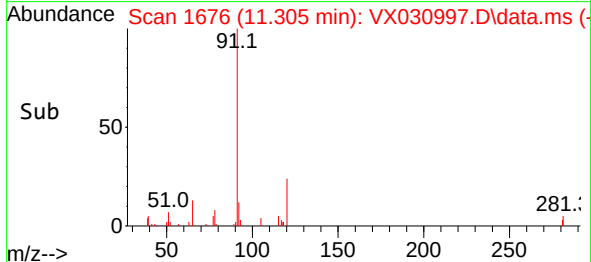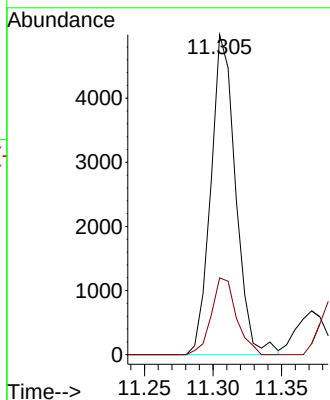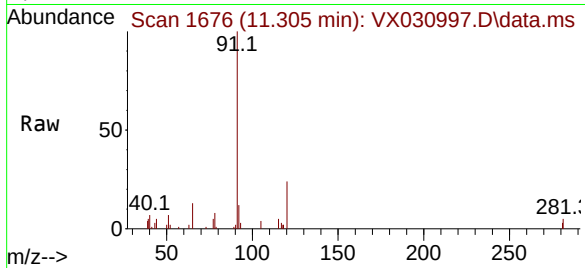

#80
1,3,5-Trimethylbenzene
Concen: 0.360 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46

Tgt Ion: 105 Resp: 3357
Ion Ratio Lower Upper
105 100
120 50.2 24.4 73.2


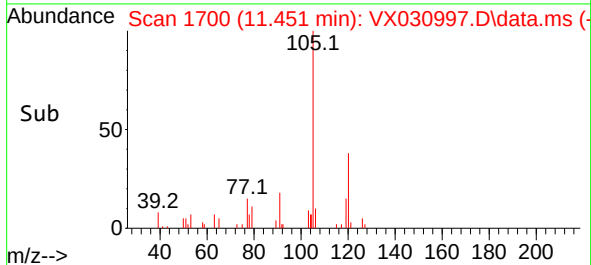
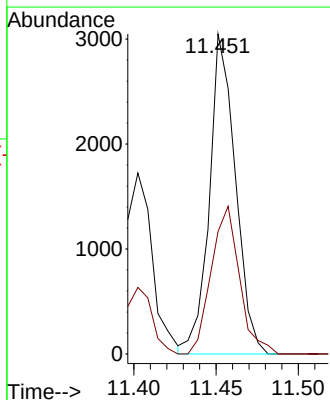
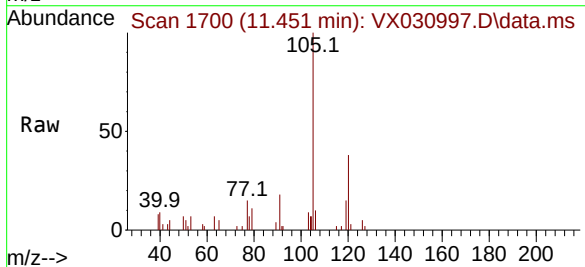


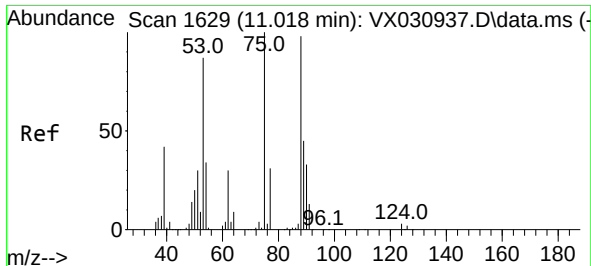

#81
trans-1,4-Dichloro-2-butene
Concen: 63.112 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.055 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 75 Resp: 73149
Ion Ratio Lower Upper
75 100
53 0.1 74.2 111.4#
89 0.1 34.8 52.2#

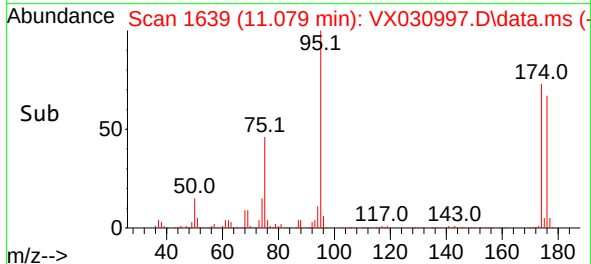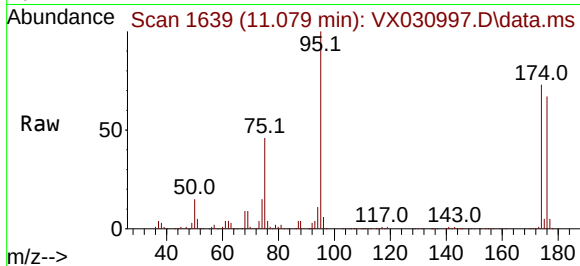

#84
1,2,4-Trimethylbenzene
Concen: 0.652 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46

Tgt Ion: 105 Resp: 6228
Ion Ratio Lower Upper
105 100
120 44.4 22.9 68.8


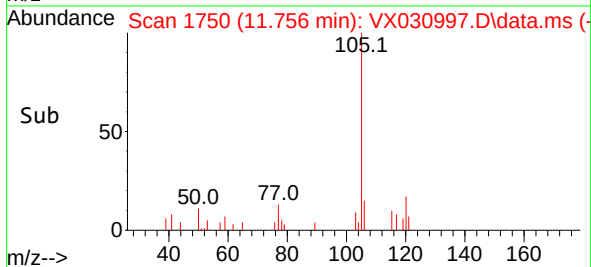

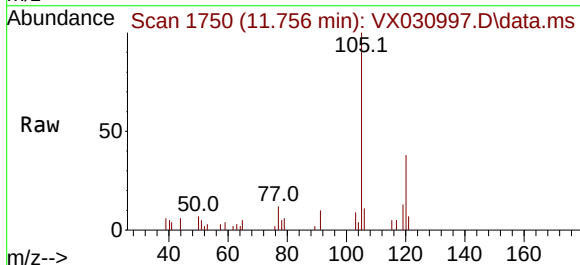


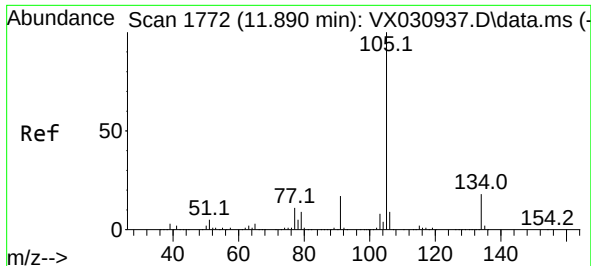

#85
 sec-Butylbenzene
 Concen: 0.342 ug/l
 RT: 11.890 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: VX030997.D
 Acq: 31 Aug 2022 23:46




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-40


Tgt Ion:105 Resp: 4068
 Ion Ratio Lower Upper
 105 100
 134 26.8 10.0 30.0

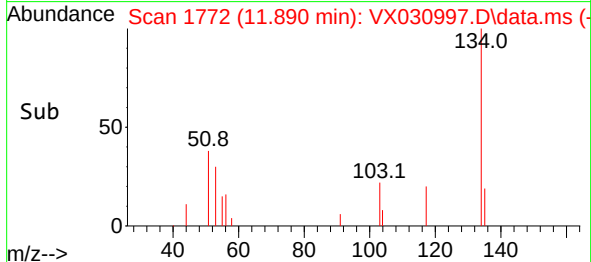

#89
 n-Butylbenzene
 Concen: 0.328 ug/l
 RT: 12.335 min Scan# 1845
 Delta R.T. 0.000 min
 Lab File: VX030997.D
 Acq: 31 Aug 2022 23:46

Tgt Ion: 91 Resp: 3031
 Ion Ratio Lower Upper
 91 100
 92 47.3 26.2 78.5
 134 37.6 12.6 37.8

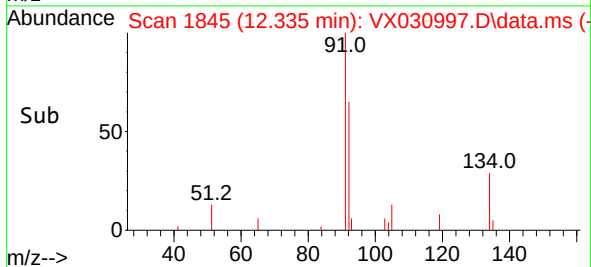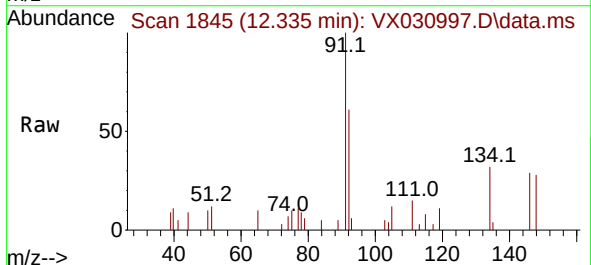



#90

Hexachloroethane

Concen: 0.769 ug/l

RT: 12.616 min Scan# 1879

Delta R.T. 0.074 min

Lab File: VX030997.D

Acq: 31 Aug 2022 23:46

Instrument :

MSVOA_X

ClientSampleId :





MW-40

Tgt Ion:117 Resp: 1332

Ion Ratio Lower Upper

117 100

201 0.0 34.2 102.5#

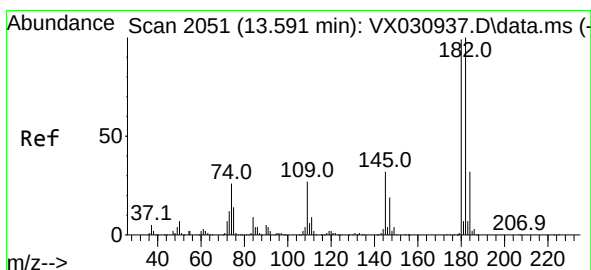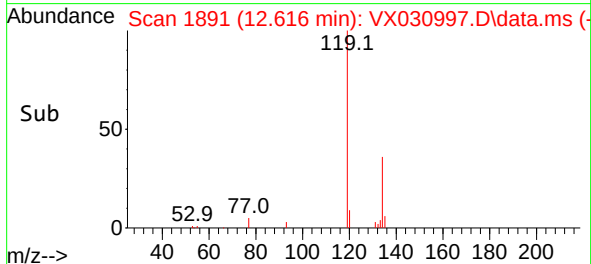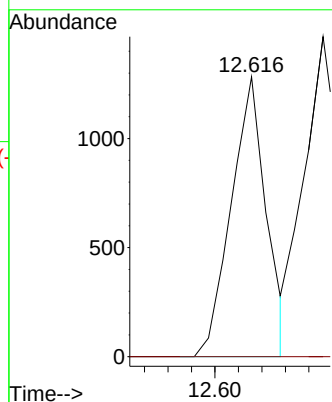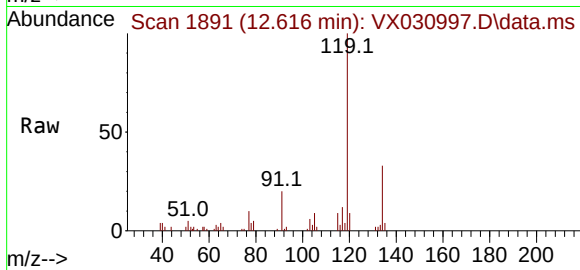

#93

1,2,4-Trichlorobenzene

Concen: 0.330 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. -0.000 min

Lab File: VX030997.D

Acq: 31 Aug 2022 23:46




Tgt Ion:180 Resp: 1133


Ion Ratio Lower Upper

180 100

182 83.8 48.2 144.6

145 41.7 15.9 47.6




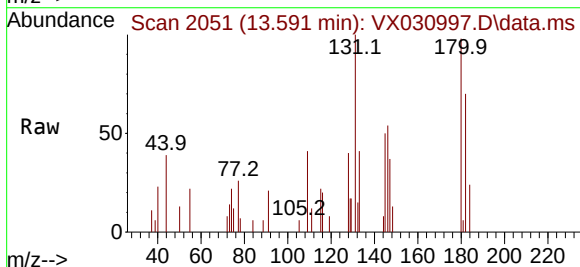


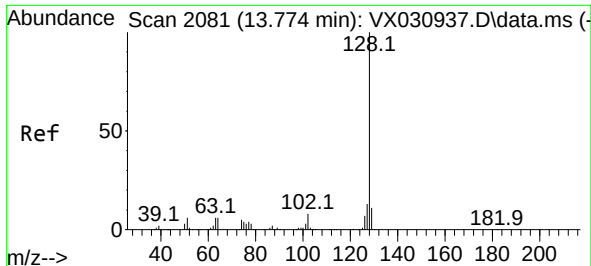

#95
Naphthalene
Concen: 1.804 ug/l
RT: 13.780 min Scan# 2081
Delta R.T. 0.006 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46

Instrument :
MSVOA_X
ClientSampleId :
MW-40

Tgt Ion:128	Resp:	22132
Ion Ratio	Lower	Upper
128	100	
127	13.3	10.2 15.2
129	11.6	8.6 13.0

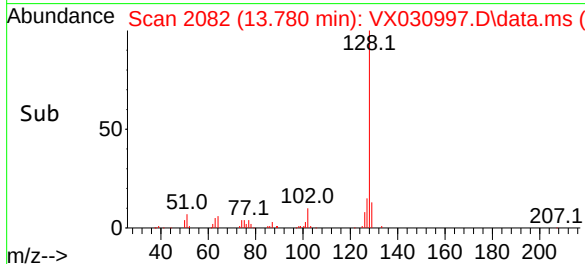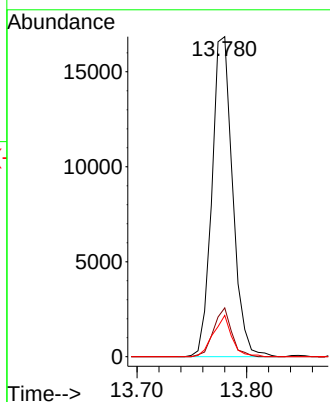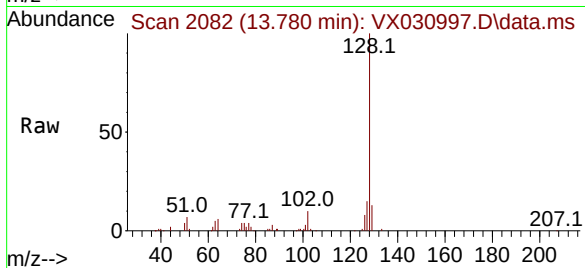

#96
1,2,3-Trichlorobenzene
Concen: 0.297 ug/l
RT: 13.969 min Scan# 2113
Delta R.T. 0.006 min
Lab File: VX030997.D
Acq: 31 Aug 2022 23:46

Tgt Ion:180	Resp:	1028
Ion Ratio	Lower	Upper
180	100	
182	99.9	47.0 141.0
145	40.5	17.0 50.9

