

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083122\
 Data File : VX030970.D
 Acq On : 31 Aug 2022 12:02
 Operator : JC/MD
 Sample : N4381-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-32

Quant Time: Sep 01 00:55:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 30 14:24:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	220909	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	373860	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	329743	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	148727	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	148522	46.875	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	93.760%
35) Dibromofluoromethane	5.391	113	136201	49.422	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.840%
50) Toluene-d8	8.653	98	516563	50.613	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.220%
62) 4-Bromofluorobenzene	11.085	95	169820	46.725	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.460%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083122\
Data File : VX030970.D
Acq On : 31 Aug 2022 12:02
Operator : JC/MD
Sample : N4381-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-32

Quant Time: Sep 01 00:55:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 30 14:24:53 2022
Response via : Initial Calibration




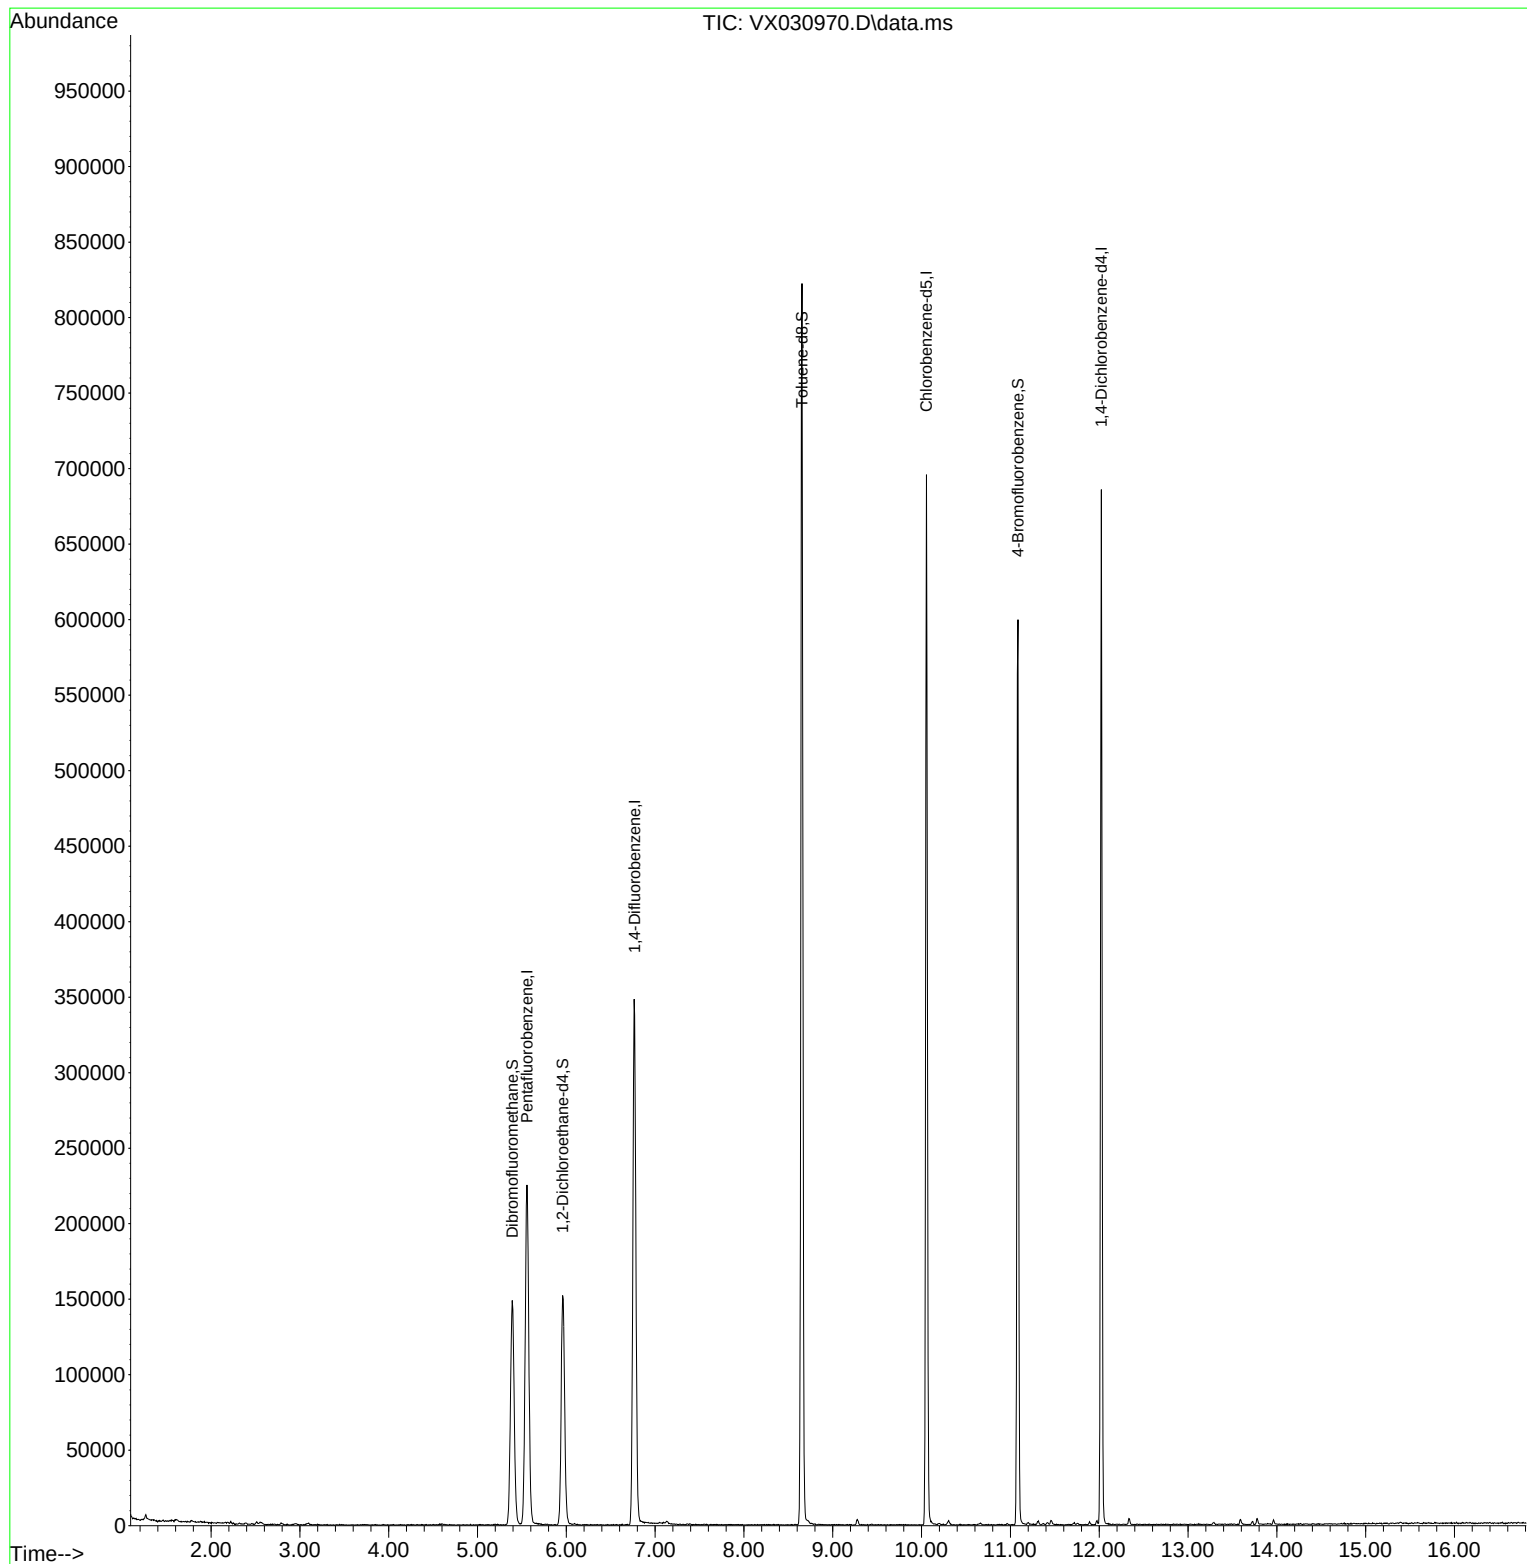


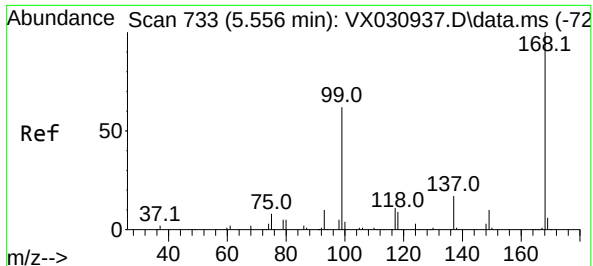

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 719
Delta R.T. -0.000 min
Lab File: VX030970.D
Acq: 31 Aug 2022 12:02




Instrument :
MSVOA_X
ClientSampleId :
MW-32


Tgt Ion:168 Resp: 220909
Ion Ratio Lower Upper
168 100
99 55.9 44.0 66.0

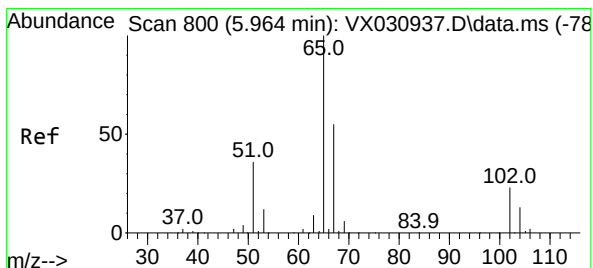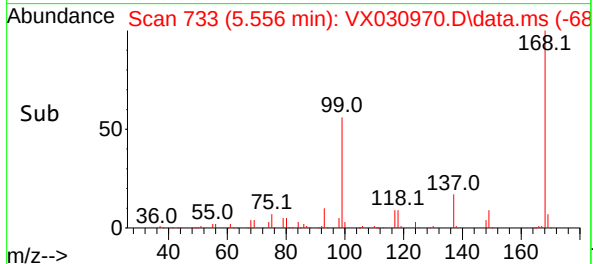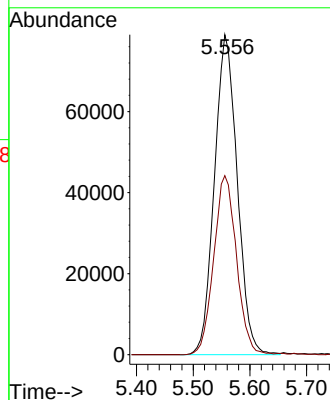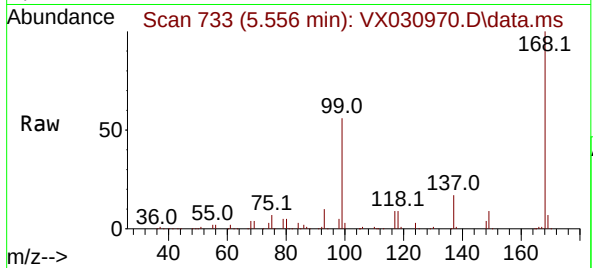

#33
1,2-Dichloroethane-d4
Concen: 46.875 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX030970.D
Acq: 31 Aug 2022 12:02

Tgt Ion: 65 Resp: 148522
Ion Ratio Lower Upper
65 100
67 54.7 0.0 109.6


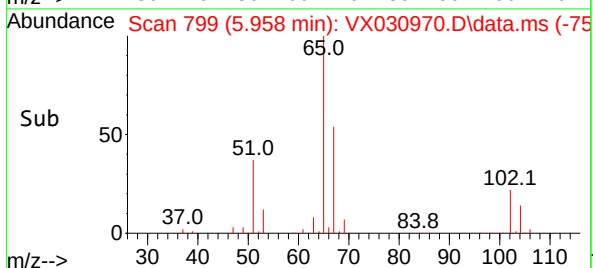
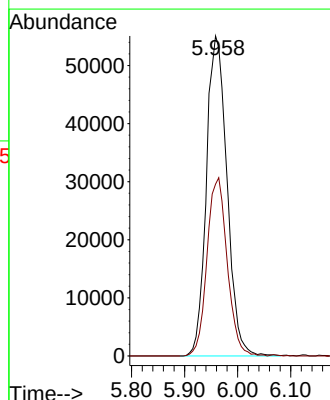
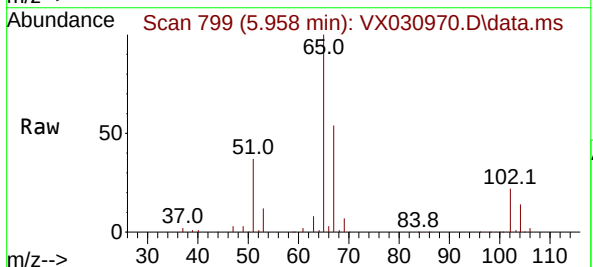


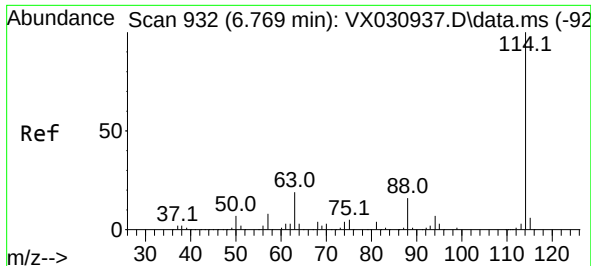

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX030970.D
Acq: 31 Aug 2022 12:02




Instrument :
MSVOA_X
ClientSampleId :
MW-32


Tgt Ion:114 Resp: 373860
Ion Ratio Lower Upper
114 100
63 17.9 0.0 38.4
88 14.8 0.0 31.8

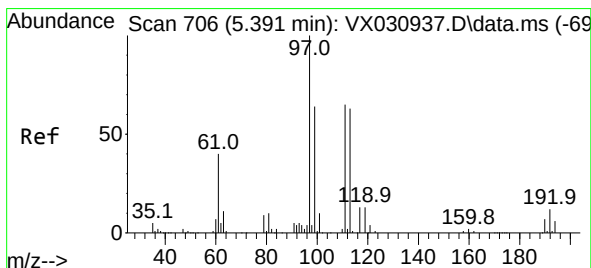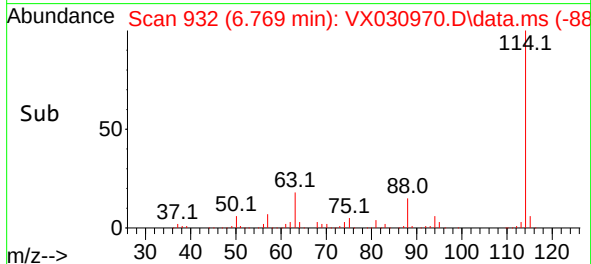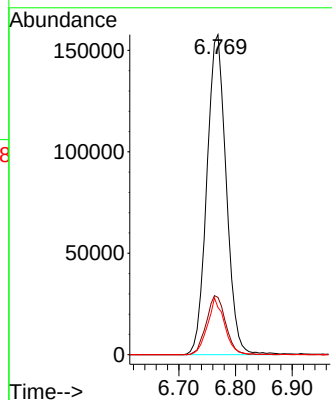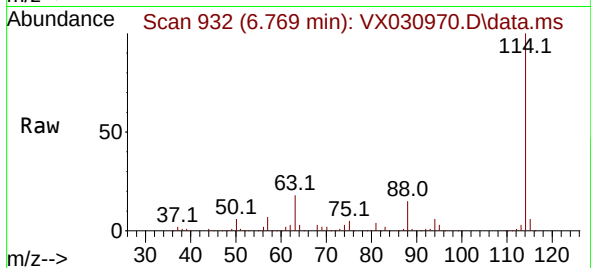

#35
Dibromofluoromethane
Concen: 49.422 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX030970.D
Acq: 31 Aug 2022 12:02

Tgt Ion:113 Resp: 136201
Ion Ratio Lower Upper
113 100
111 102.9 83.2 124.8
192 19.1 14.8 22.2


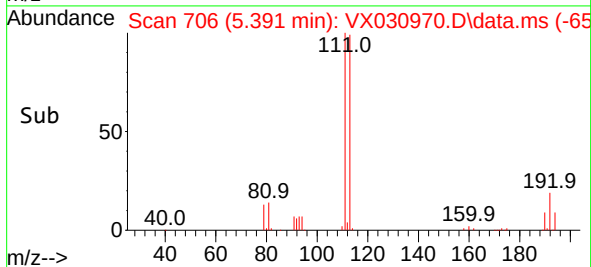
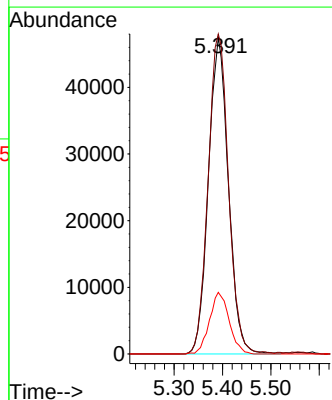
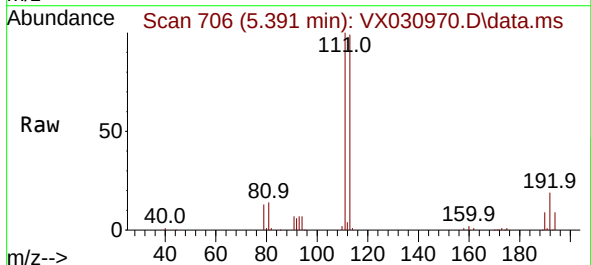


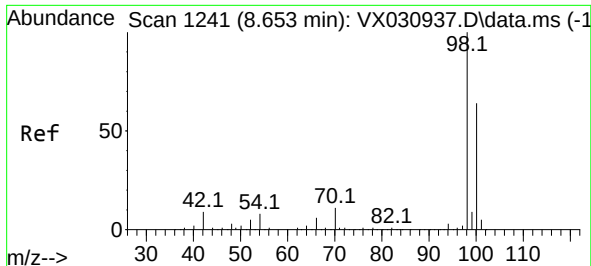

#50
Toluene-d8
Concen: 50.613 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX030970.D
Acq: 31 Aug 2022 12:02




Instrument :
MSVOA_X
ClientSampleId :
MW-32


Tgt Ion: 98 Resp: 516563
Ion Ratio Lower Upper
98 100
100 63.0 52.3 78.5

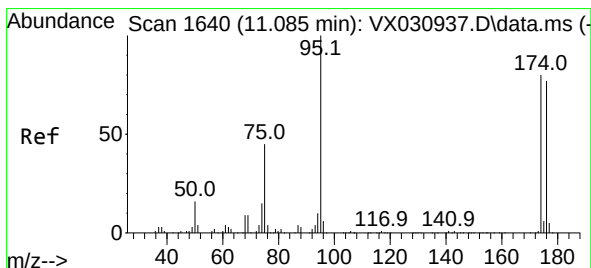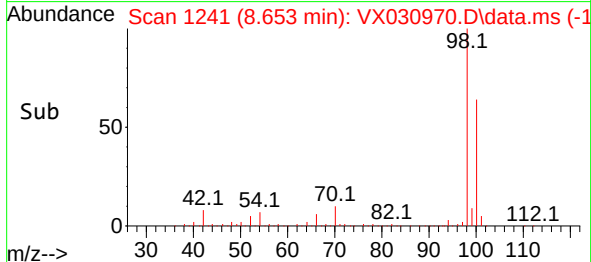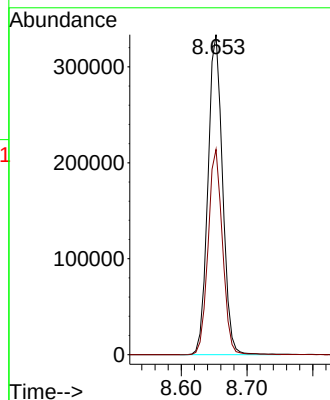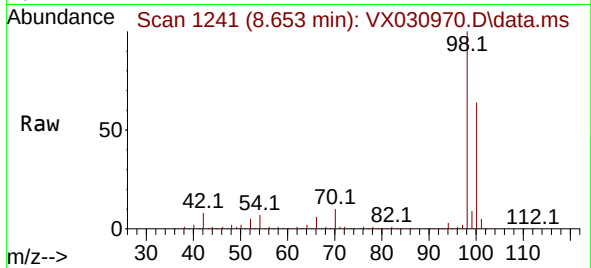

#62
4-Bromofluorobenzene
Concen: 46.725 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX030970.D
Acq: 31 Aug 2022 12:02

Tgt Ion: 95 Resp: 169820
Ion Ratio Lower Upper
95 100
174 80.8 0.0 149.0
176 78.3 0.0 146.0


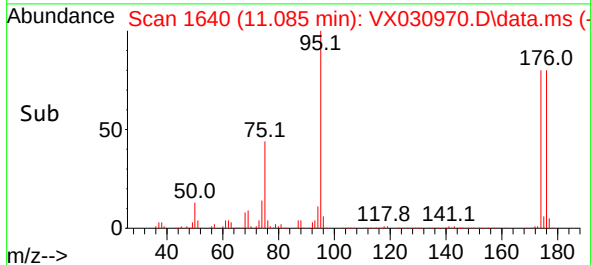
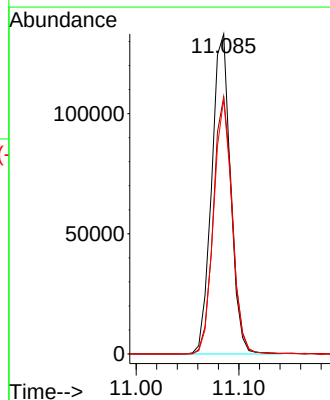
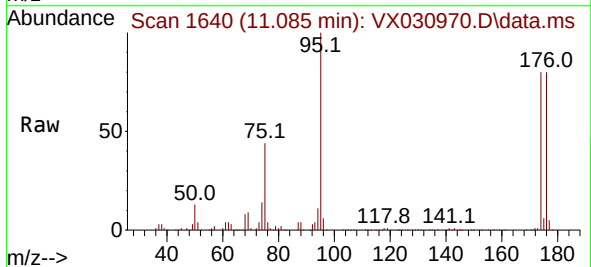


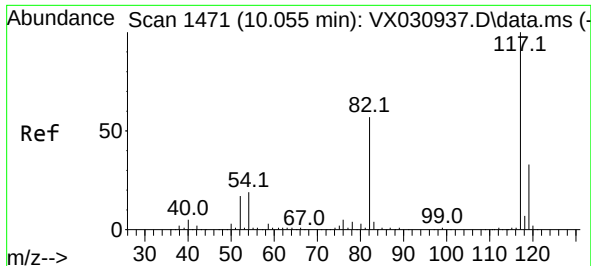

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX030970.D
Acq: 31 Aug 2022 12:02

Instrument :
MSVOA_X
ClientSampleId :
MW-32

Tgt Ion:117 Resp: 329743
Ion Ratio Lower Upper
117 100
82 53.8 42.7 64.1
119 32.1 25.4 38.2

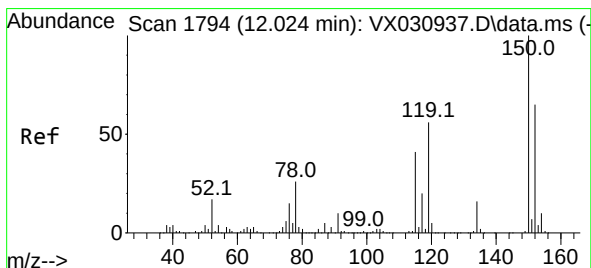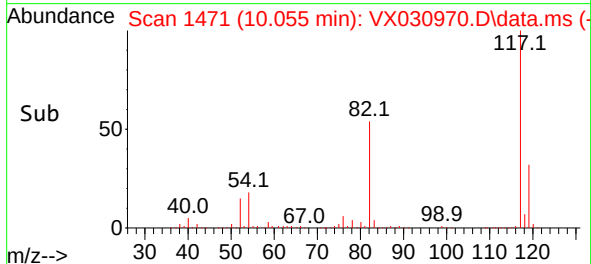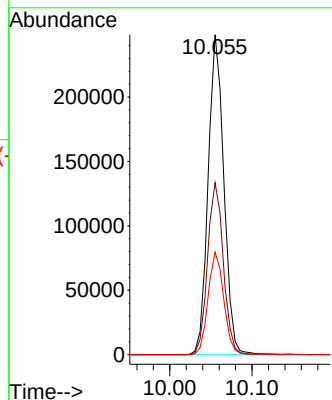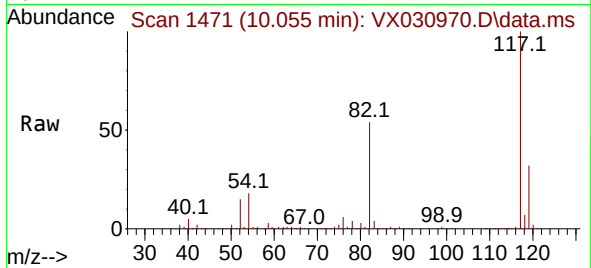

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX030970.D
Acq: 31 Aug 2022 12:02

Tgt Ion:152 Resp: 148727
Ion Ratio Lower Upper
152 100
115 58.8 40.5 121.5
150 153.1 0.0 347.0

