

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083122\
 Data File : VX030990.D
 Acq On : 31 Aug 2022 19:52
 Operator : JC/MD
 Sample : N4381-08DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-34DL

Quant Time: Sep 01 00:58:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 30 14:24:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	205253	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	348758	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	304011	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	138118	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	136122	46.238	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	92.480%
35) Dibromofluoromethane	5.397	113	125612	48.860	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.720%
50) Toluene-d8	8.653	98	461300	48.452	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	96.900%
62) 4-Bromofluorobenzene	11.085	95	152403	44.951	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.900%
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	2.971	59	38224	54.804	ug/l #	74
19) Methyl tert-butyl Ether	3.117	73	701598	86.354	ug/l	95
20) Methylene Chloride	2.788	84	1307	0.433	ug/l	90
40) Benzene	6.050	78	13326	1.210	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083122\
Data File : VX030990.D
Acq On : 31 Aug 2022 19:52
Operator : JC/MD
Sample : N4381-08DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-34DL

Quant Time: Sep 01 00:58:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 30 14:24:53 2022
Response via : Initial Calibration




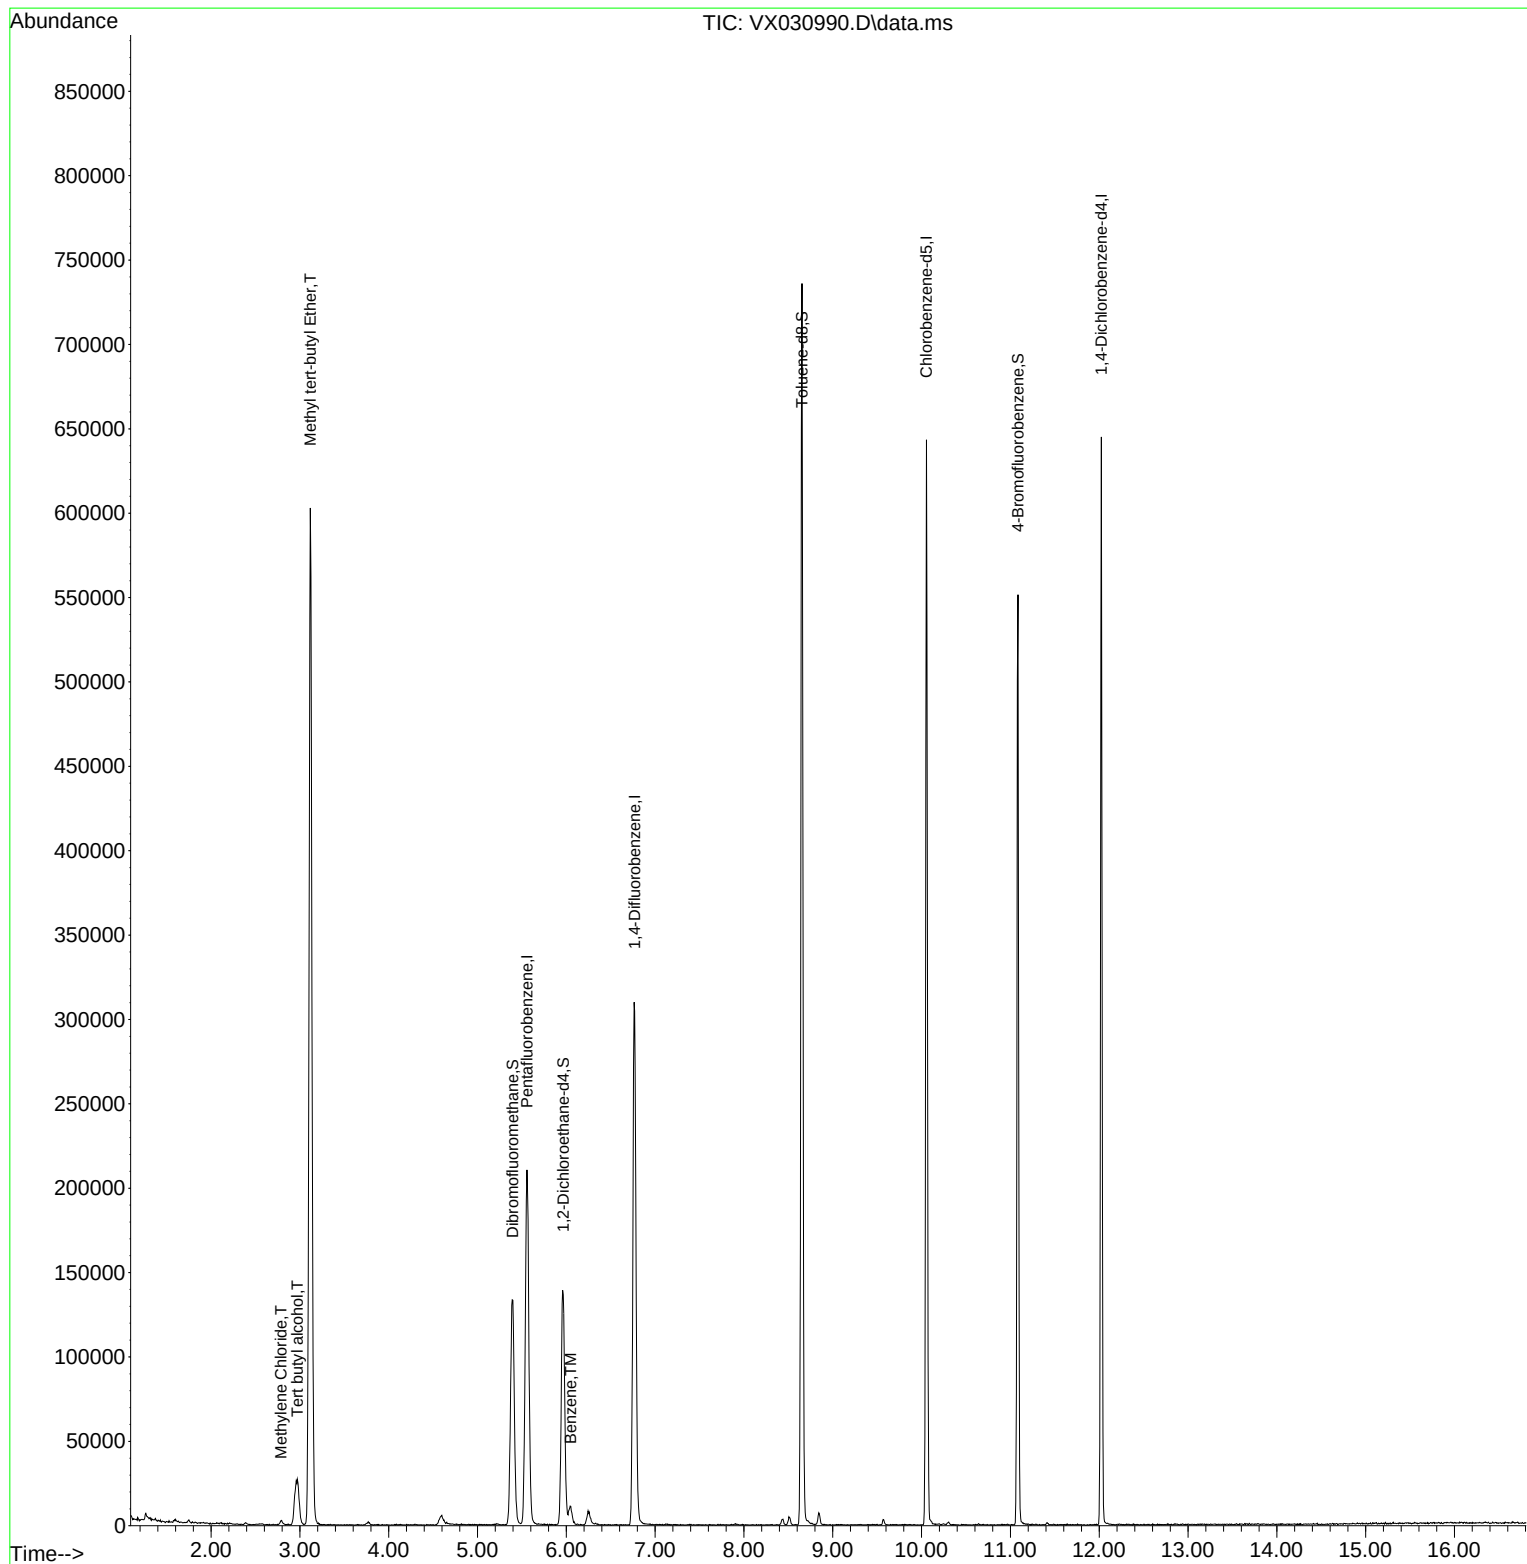


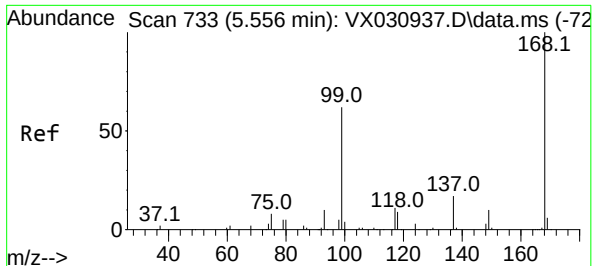

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX030990.D
Acq: 31 Aug 2022 19:52




Instrument :
MSVOA_X
ClientSampleId :
MW-34DL


Tgt Ion:168 Resp: 205253
Ion Ratio Lower Upper
168 100
99 56.3 44.0 66.0

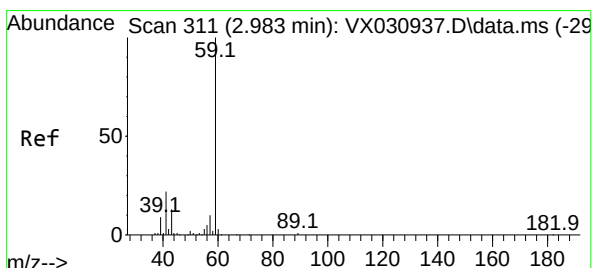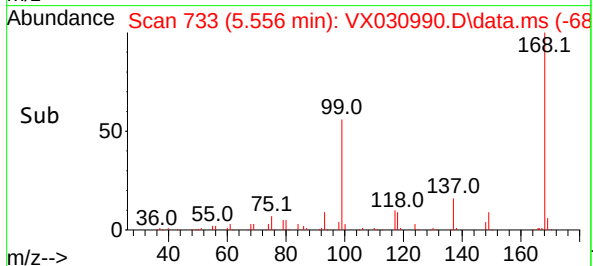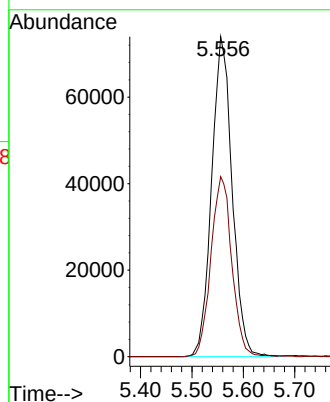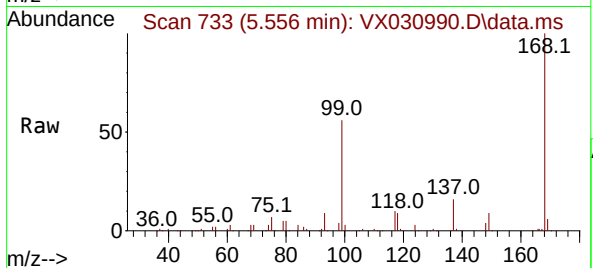

#11
Tert butyl alcohol
Concen: 54.804 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.018 min
Lab File: VX030990.D
Acq: 31 Aug 2022 19:52

Tgt Ion: 59 Resp: 38224
Ion Ratio Lower Upper
59 100
57 0.0 7.4 11.2#


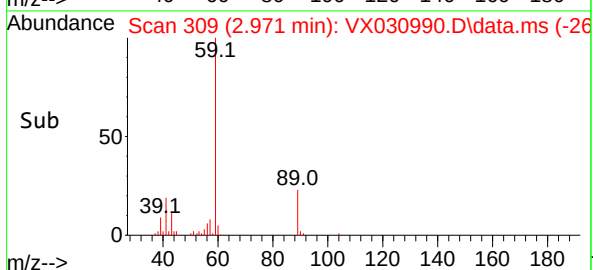
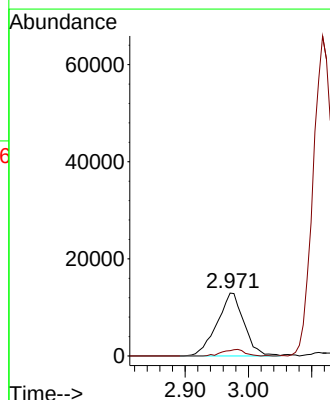
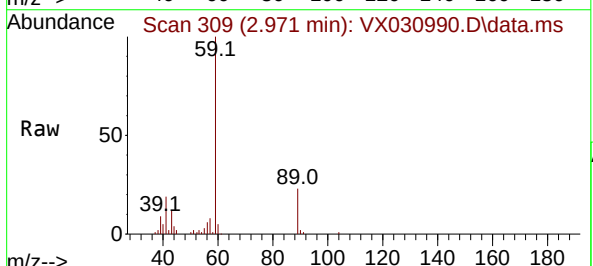


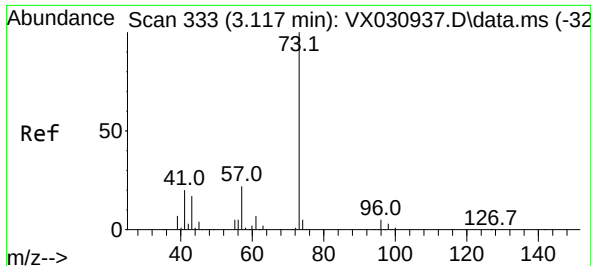

#19
Methyl tert-butyl Ether
Concen: 86.354 ug/l
RT: 3.117 min Scan# 311
Delta R.T. 0.000 min
Lab File: VX030990.D
Acq: 31 Aug 2022 19:52




Instrument :
MSVOA_X
ClientSampleId :
MW-34DL


Tgt Ion: 73 Resp: 701598
Ion Ratio Lower Upper
73 100
57 21.4 19.0 28.6

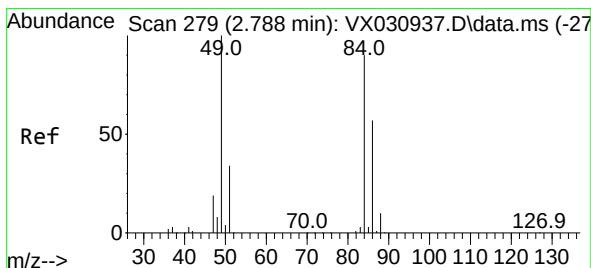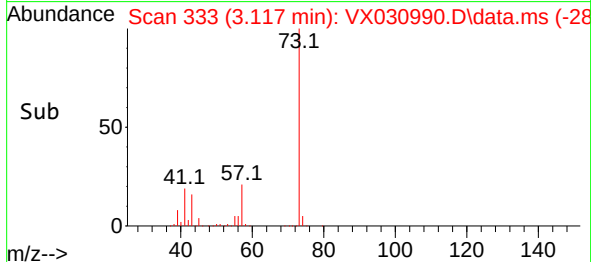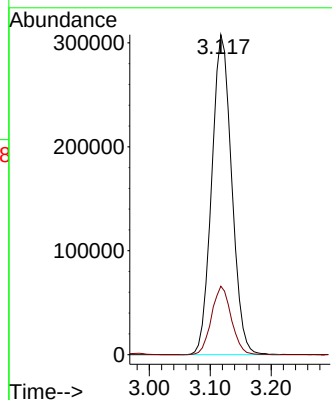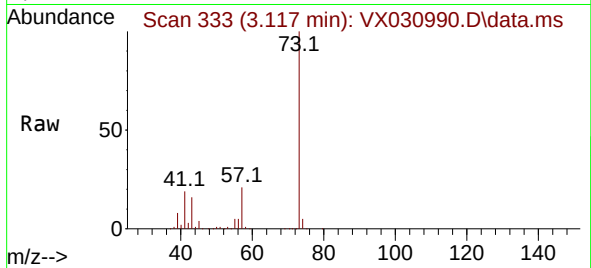

#20
Methylene Chloride
Concen: 0.433 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX030990.D
Acq: 31 Aug 2022 19:52

Tgt Ion: 84 Resp: 1307
Ion Ratio Lower Upper
84 100
49 99.4 93.8 140.6
51 38.1 29.4 44.0
86 65.6 51.0 76.4

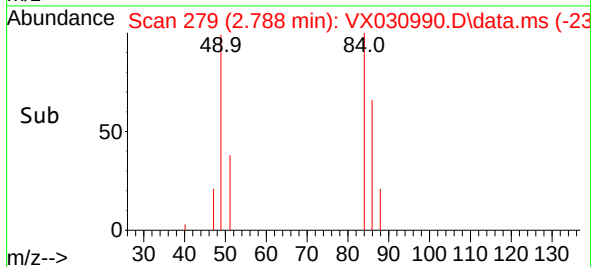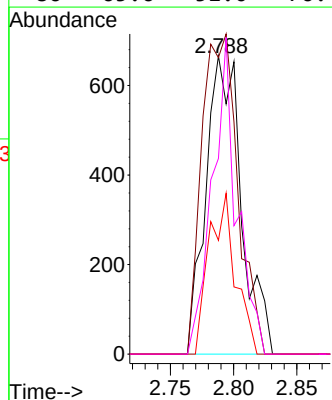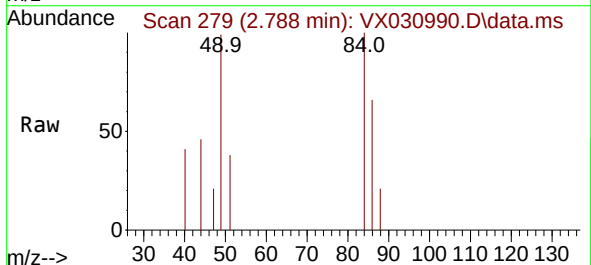

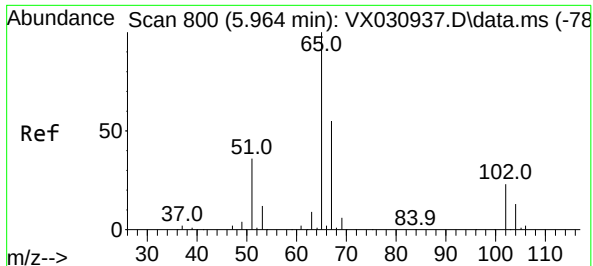

#33

1,2-Dichloroethane-d4

Concen: 46.238 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.006 min

Lab File: VX030990.D

Acq: 31 Aug 2022 19:52

Instrument :

MSVOA_X

ClientSampleId :





MW-34DL

Tgt Ion: 65 Resp: 136122

Ion Ratio Lower Upper

65 100

67 54.9 0.0 109.6

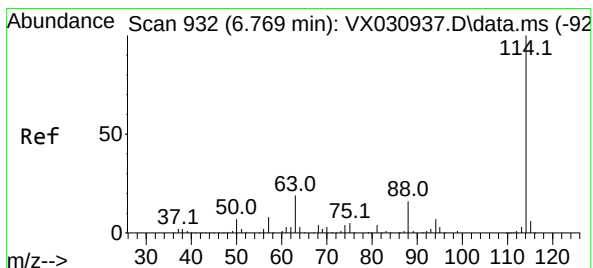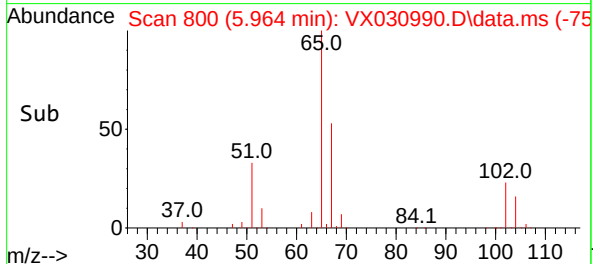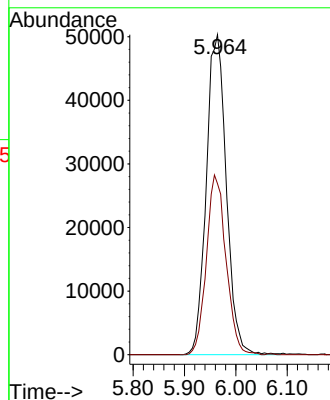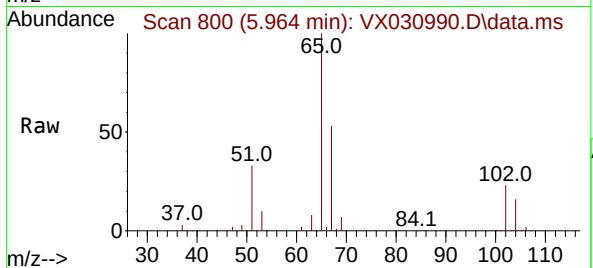

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. -0.000 min

Lab File: VX030990.D

Acq: 31 Aug 2022 19:52




Tgt Ion: 114 Resp: 348758


Ion Ratio Lower Upper

114 100

63 18.5 0.0 38.4

88 13.9 0.0 31.8

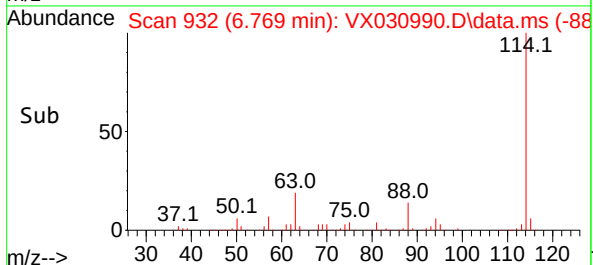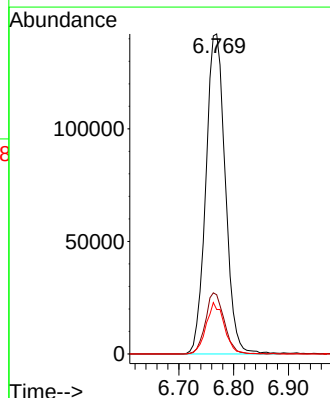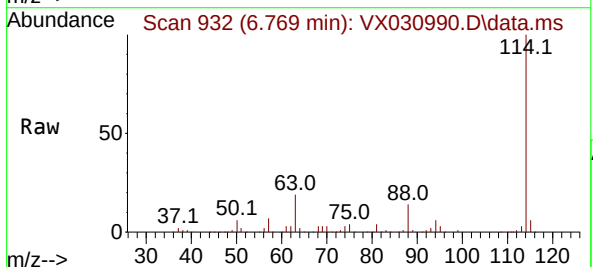

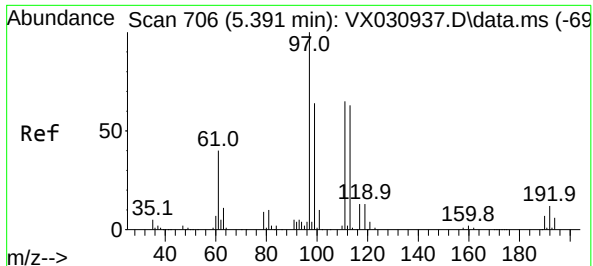

#35

Dibromofluoromethane

Concen: 48.860 ug/l

RT: 5.397 min Scan# 706

Delta R.T. 0.006 min

Lab File: VX030990.D


Acq: 31 Aug 2022 19:52

Instrument :

MSVOA_X

ClientSampleId :

MW-34DL

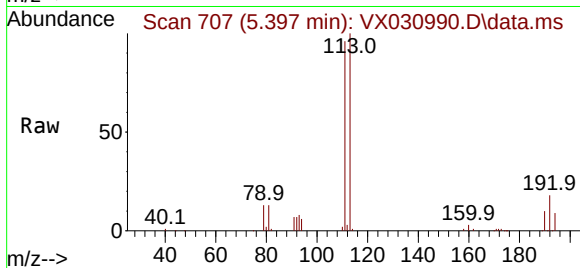




Tgt Ion:113 Resp: 125612

Ion Ratio Lower Upper

113 100

111 101.3 83.2 124.8

192 19.6 14.8 22.2

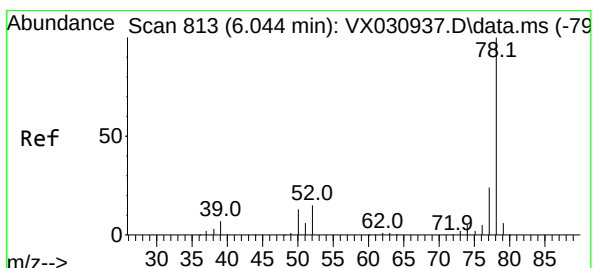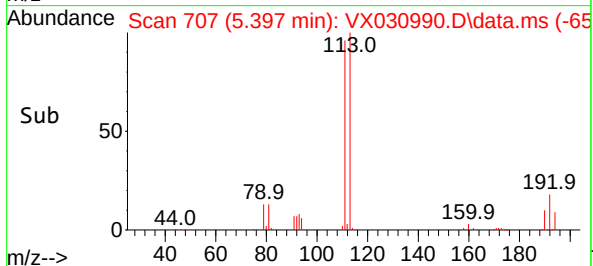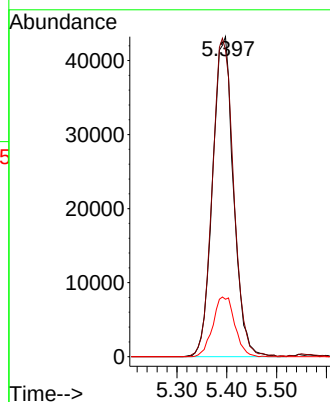

#40

Benzene

Concen: 1.210 ug/l

RT: 6.050 min Scan# 814

Delta R.T. 0.006 min

Lab File: VX030990.D




Acq: 31 Aug 2022 19:52


Tgt Ion: 78 Resp: 13326

Ion Ratio Lower Upper

78 100

77 26.4 18.0 27.0


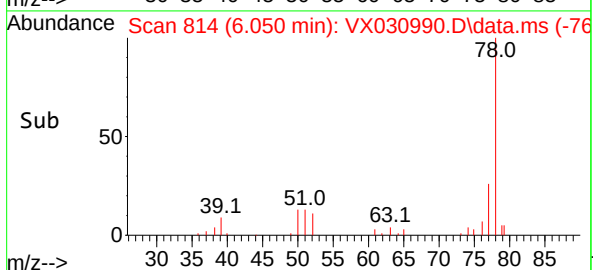
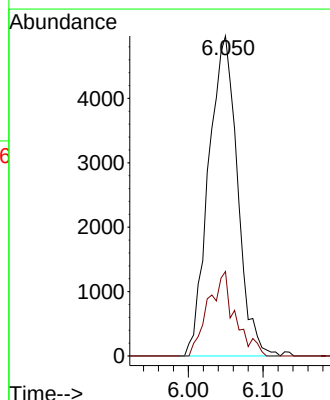
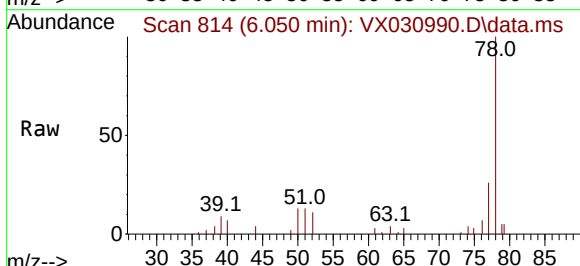


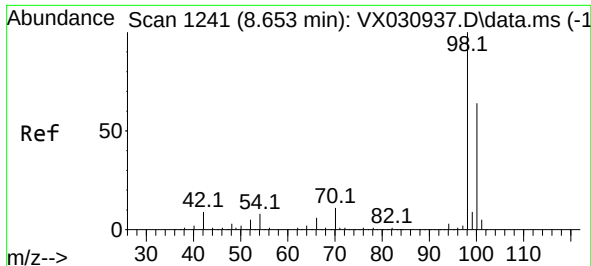

#50
Toluene-d8
Concen: 48.452 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX030990.D
Acq: 31 Aug 2022 19:52




Instrument :
MSVOA_X
ClientSampleId :
MW-34DL


Tgt Ion: 98 Resp: 461300
Ion Ratio Lower Upper
98 100
100 64.6 52.3 78.5

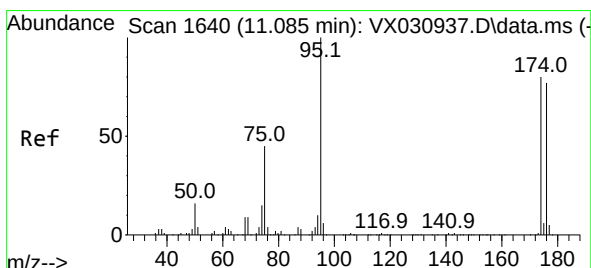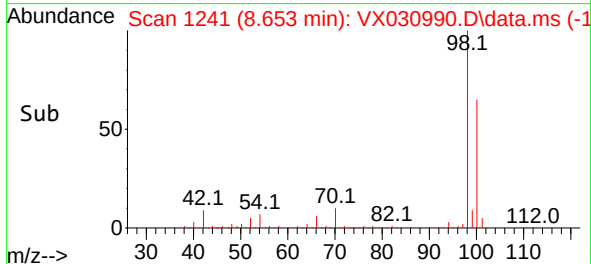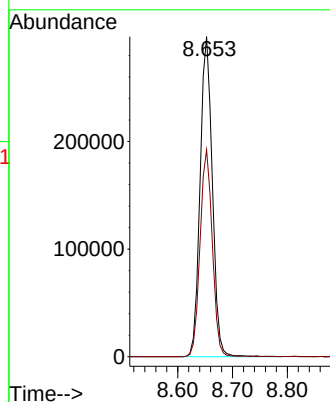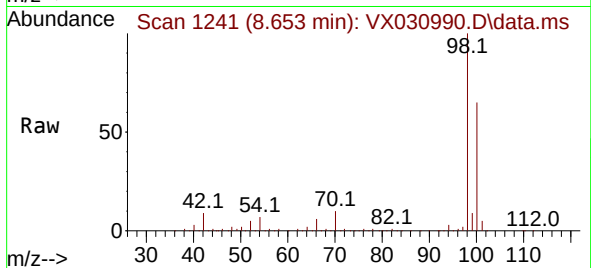

#62
4-Bromofluorobenzene
Concen: 44.951 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX030990.D
Acq: 31 Aug 2022 19:52

Tgt Ion: 95 Resp: 152403
Ion Ratio Lower Upper
95 100
174 82.0 0.0 149.0
176 80.3 0.0 146.0


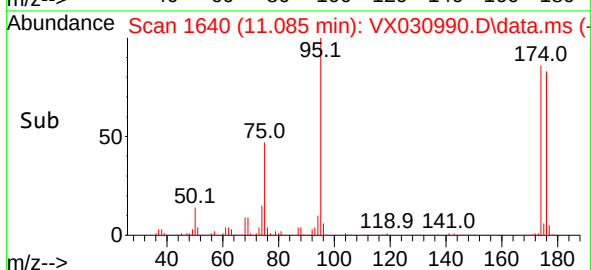
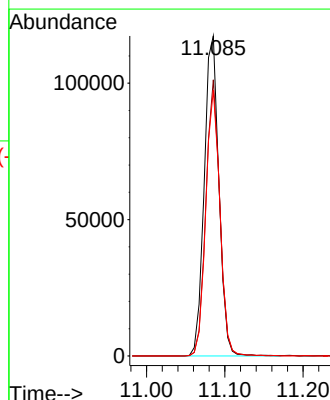
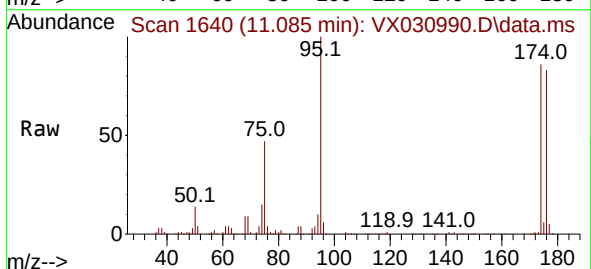


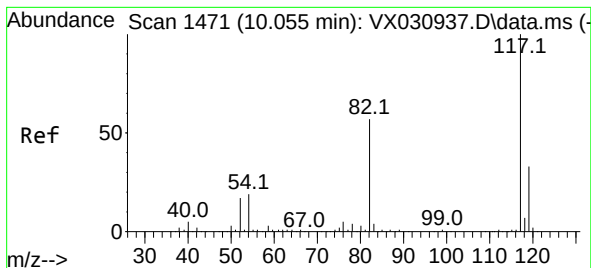

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX030990.D
Acq: 31 Aug 2022 19:52

Instrument :
MSVOA_X
ClientSampleId :
MW-34DL

Tgt Ion:117 Resp: 304011
Ion Ratio Lower Upper
117 100
82 56.5 42.7 64.1
119 31.9 25.4 38.2

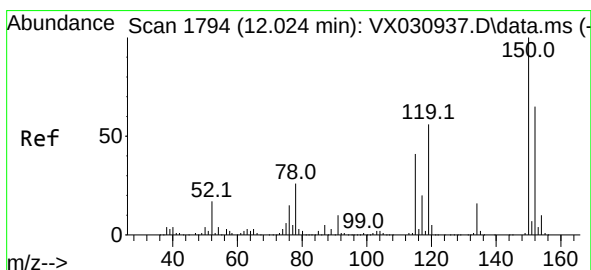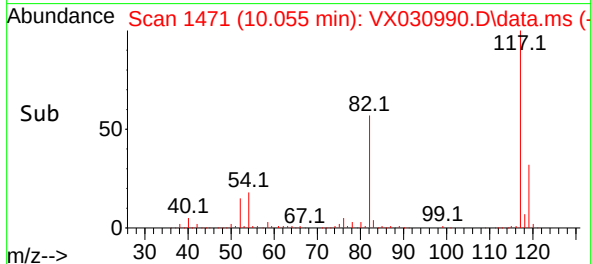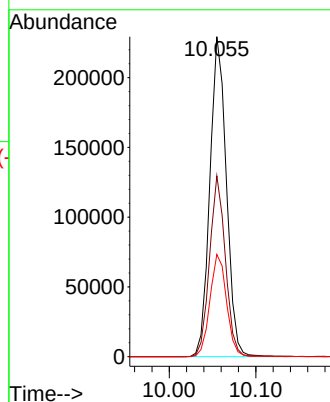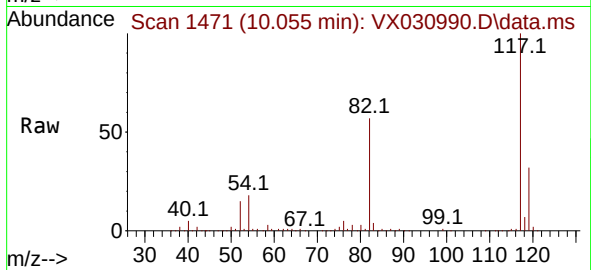

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX030990.D
Acq: 31 Aug 2022 19:52

Tgt Ion:152 Resp: 138118
Ion Ratio Lower Upper
152 100
115 59.1 40.5 121.5
150 153.7 0.0 347.0

