

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083122\
Data File : VX030972.D
Acq On : 31 Aug 2022 12:49
Operator : JC/MD
Sample : N4381-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-24

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M

Title : SW846 8260

Signal : TIC: VX030972.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.971	301	309	321	rBV2	27605	66210	2.13%	0.708%
2	3.117	321	333	349	rBV	1360304	3106868	100.00%	33.221%
3	5.391	694	706	721	rBV	149202	434352	13.98%	4.644%
4	5.556	721	733	748	rVV	218962	627257	20.19%	6.707%
5	5.958	788	799	813	rBV2	153045	413816	13.32%	4.425%
6	6.239	837	845	861	rBV4	31747	96088	3.09%	1.027%
7	6.769	921	932	942	rBV	344375	807886	26.00%	8.639%
8	8.653	1234	1241	1252	rBV	828126	1267693	40.80%	13.555%
9	10.055	1465	1471	1479	rBV	673680	902013	29.03%	9.645%
10	11.085	1634	1640	1650	rBV	617612	781627	25.16%	8.358%
11	12.024	1788	1794	1802	rBV	710889	848246	27.30%	9.070%




Sum of corrected areas: 9352056

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083122\
Data File : VX030972.D
Acq On : 31 Aug 2022 12:49
Operator : JC/MD
Sample : N4381-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

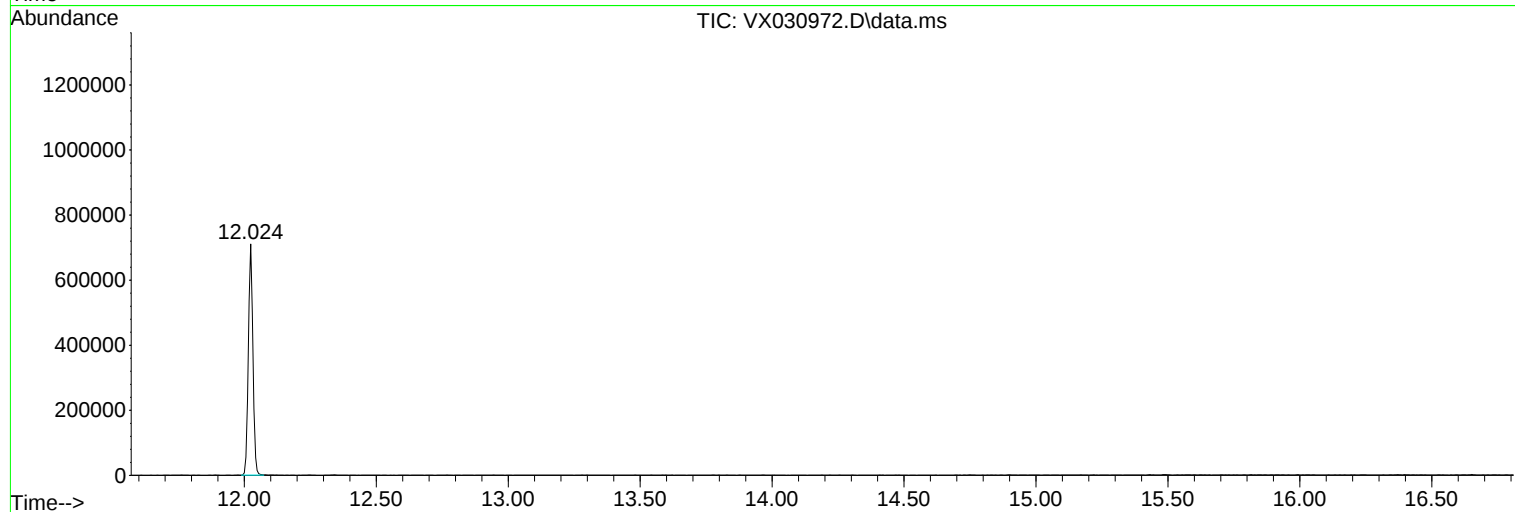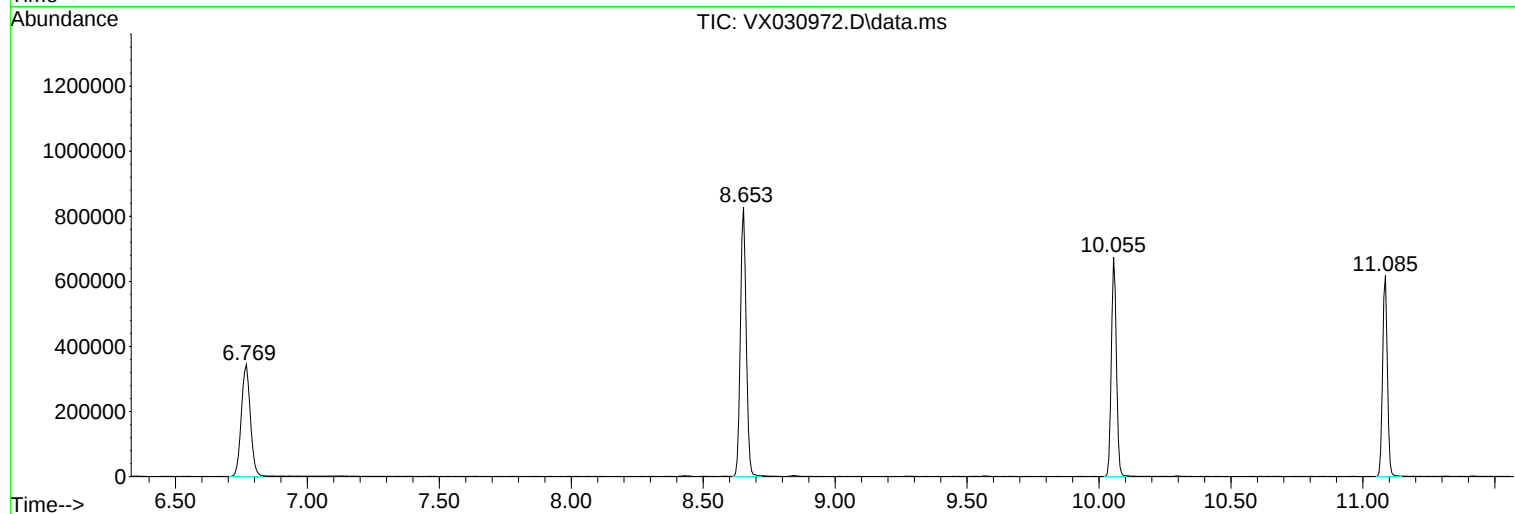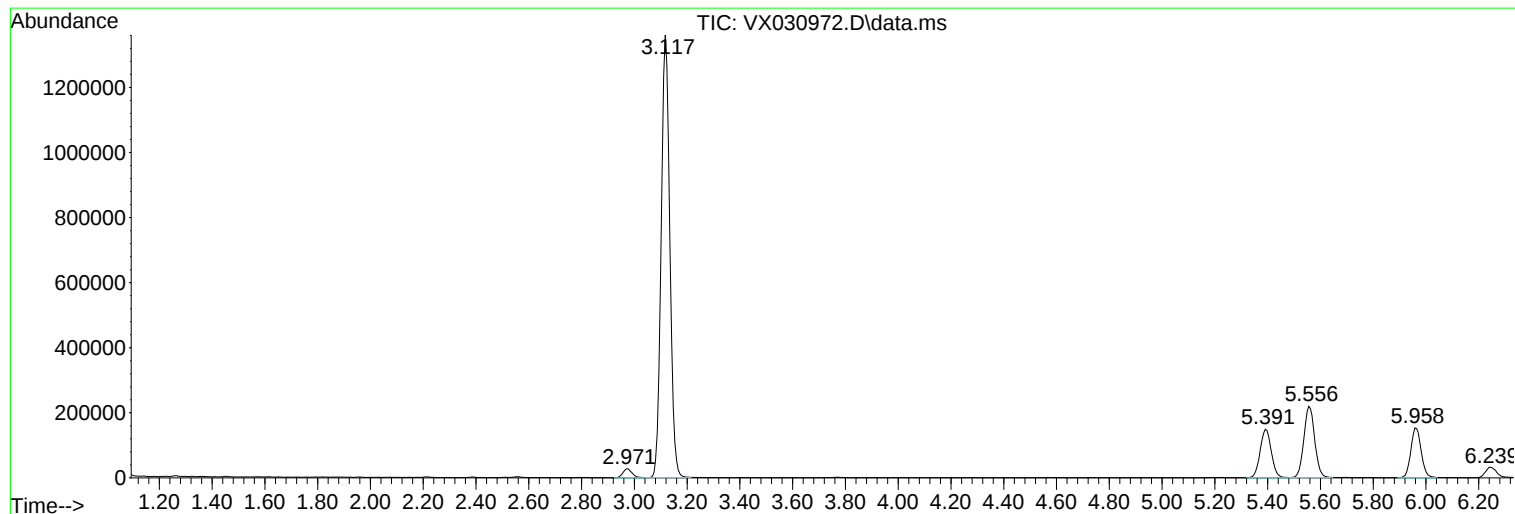

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083122\
Data File : VX030972.D
Acq On : 31 Aug 2022 12:49
Operator : JC/MD
Sample : N4381-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-24










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Amylene hydrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.239	5.95 ug/l	96088	1,4-Difluorobenzene	6.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Amylene hydrate	88	C5H12O	000075-85-4	83
2			Propanoic acid, 2-nitro-, methyl...	133	C4H7NO4	006118-50-9	42
3			3-Hexanol	102	C6H14O	000623-37-0	42
4			3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	40
5			3-Heptanol, 4-methyl-	130	C8H18O	014979-39-6	39

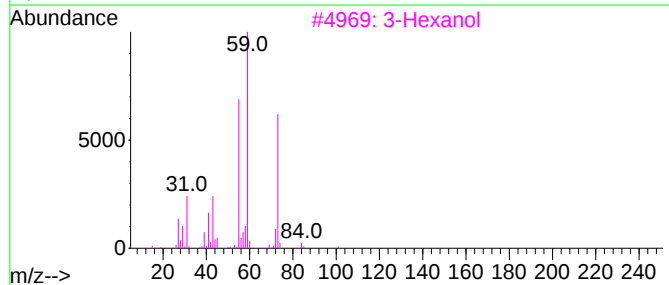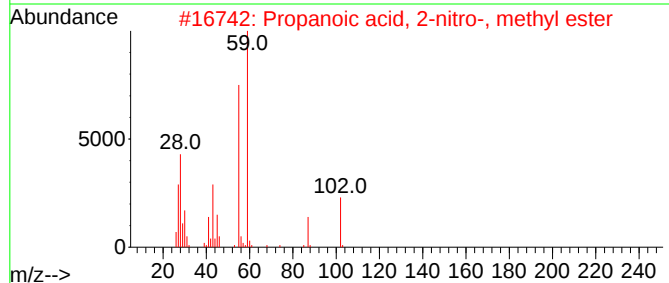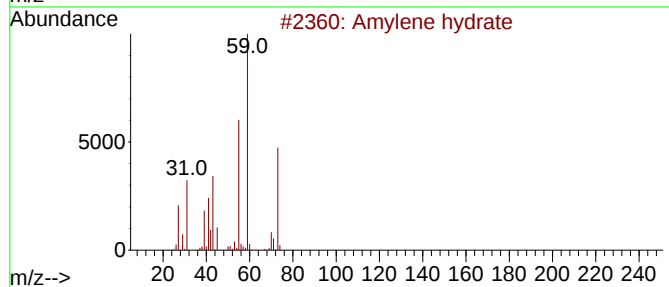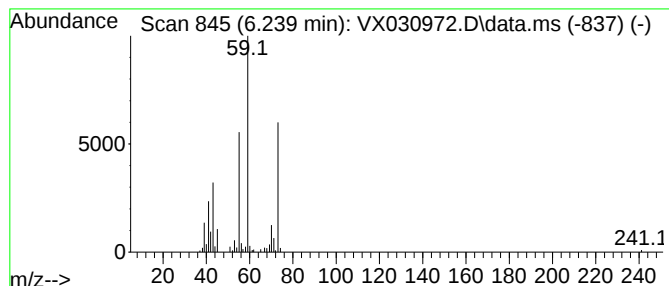

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083122\
Data File : VX030972.D
Acq On : 31 Aug 2022 12:49
Operator : JC/MD
Sample : N4381-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Amylene hydrate	6.239	6.0	ug/l	96088	2	6.769	807886	50.0