

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX083122\  
Data File : VX030985.D  
Acq On : 31 Aug 2022 17:54  
Operator : JC/MD  
Sample : N4381-16  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-50

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X083022W.M

Title : SW846 8260

Signal : TIC: VX030985.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.391       | 695           | 706         | 720          | rBV2     | 135615         | 388226        | 34.31%          | 7.104%        |
| 2         | 5.556       | 722           | 733         | 746          | rBV      | 199110         | 565835        | 50.01%          | 10.354%       |
| 3         | 5.964       | 788           | 800         | 811          | rBV      | 139576         | 368648        | 32.58%          | 6.746%        |
| 4         | 6.763       | 921           | 931         | 943          | rBV2     | 305625         | 748631        | 66.17%          | 13.699%       |
| 5         | 8.653       | 1234          | 1241        | 1256         | rBV      | 752683         | 1131420       | 100.00%         | 20.703%       |
| 6         | 10.055      | 1465          | 1471        | 1483         | rBV      | 609334         | 823591        | 72.79%          | 15.070%       |
| 7         | 11.085      | 1634          | 1640        | 1649         | rBV      | 539127         | 685601        | 60.60%          | 12.545%       |
| 8         | 12.024      | 1789          | 1794        | 1806         | rBV      | 644540         | 753101        | 66.56%          | 13.780%       |




Sum of corrected areas: 5465053

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX083122\  
Data File : VX030985.D  
Acq On : 31 Aug 2022 17:54  
Operator : JC/MD  
Sample : N4381-16  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X083022W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

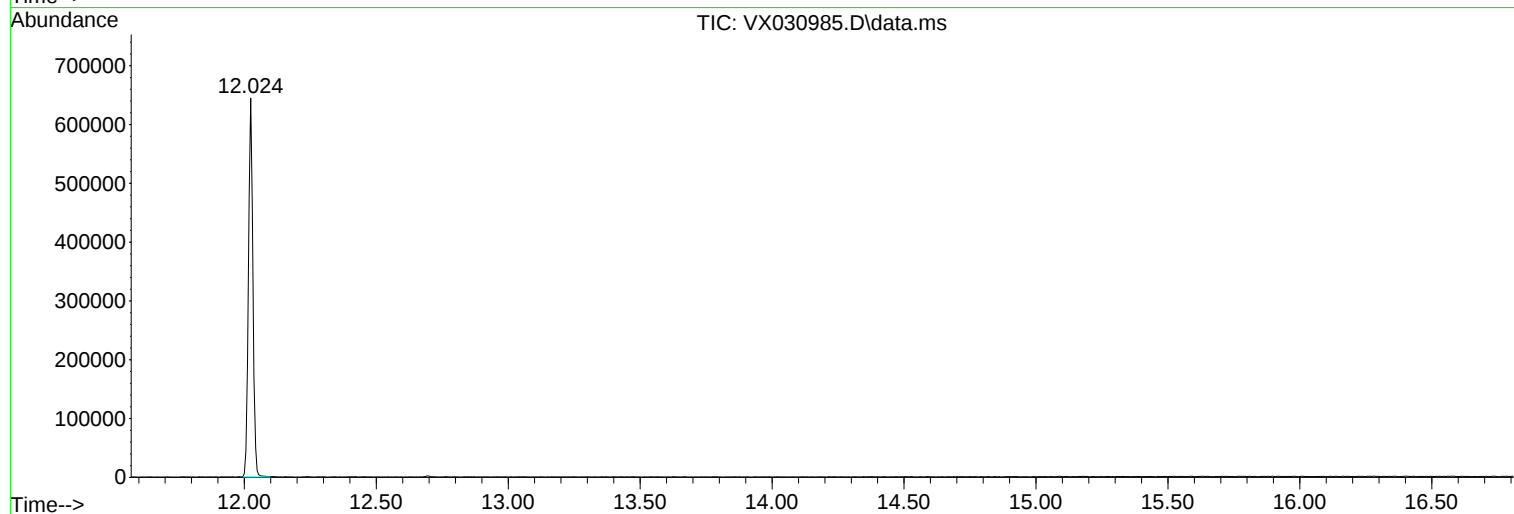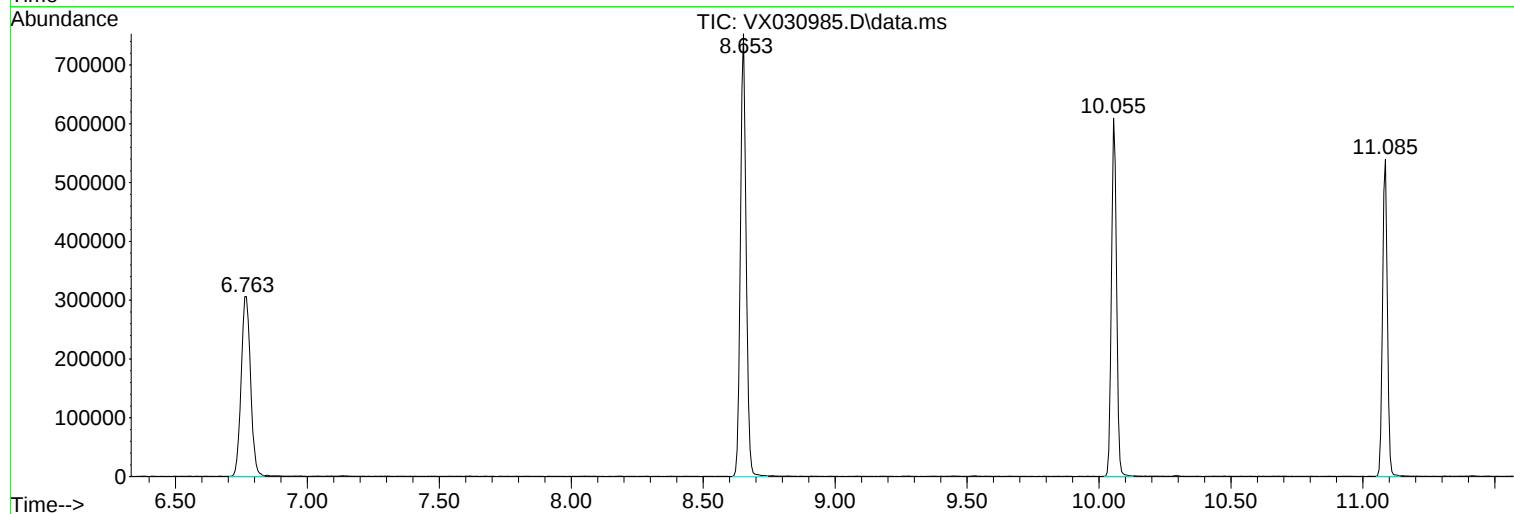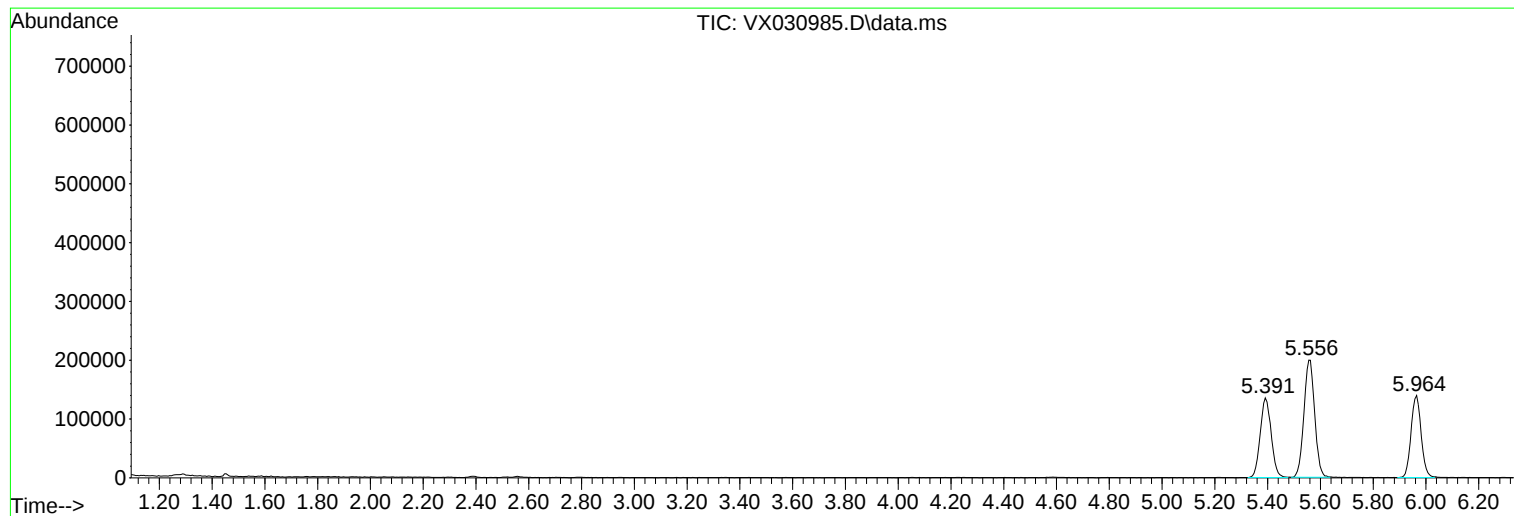

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX083122\  
Data File : VX030985.D  
Acq On : 31 Aug 2022 17:54  
Operator : JC/MD  
Sample : N4381-16  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X083022W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX083122\  
Data File : VX030985.D  
Acq On : 31 Aug 2022 17:54  
Operator : JC/MD  
Sample : N4381-16  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X083022W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|