
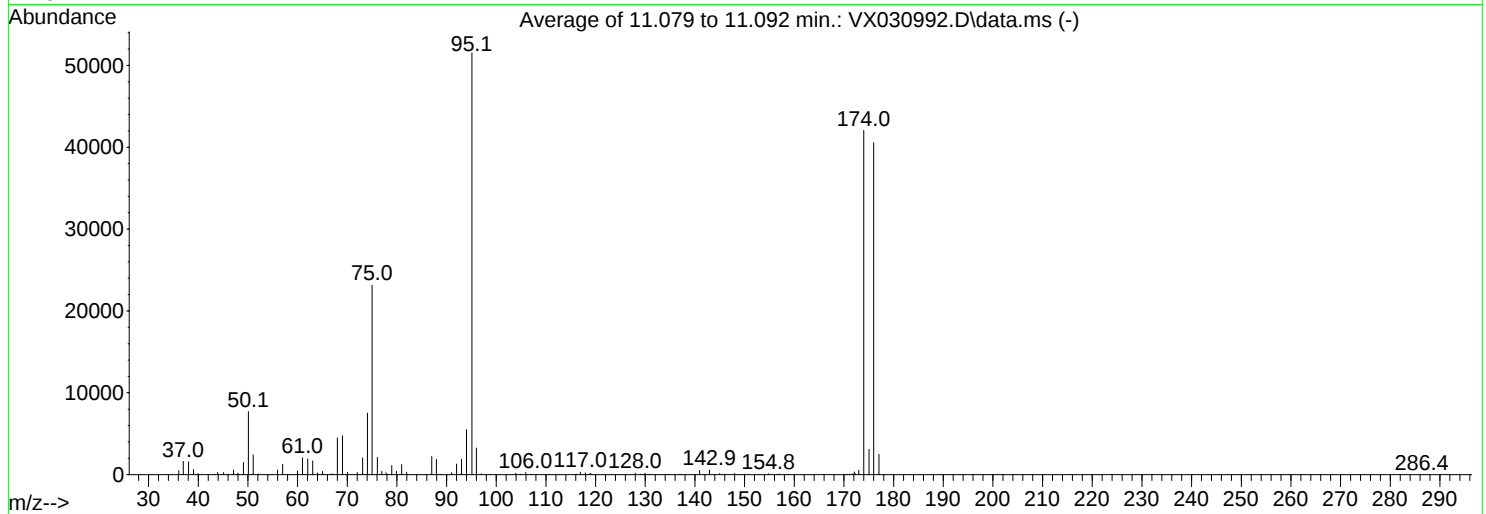


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083122\
 Data File : VX030992.D
 Acq On : 31 Aug 2022 20:39
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X083022W.M
 Title : SW846 8260
 Last Update : Tue Aug 30 14:24:53 2022

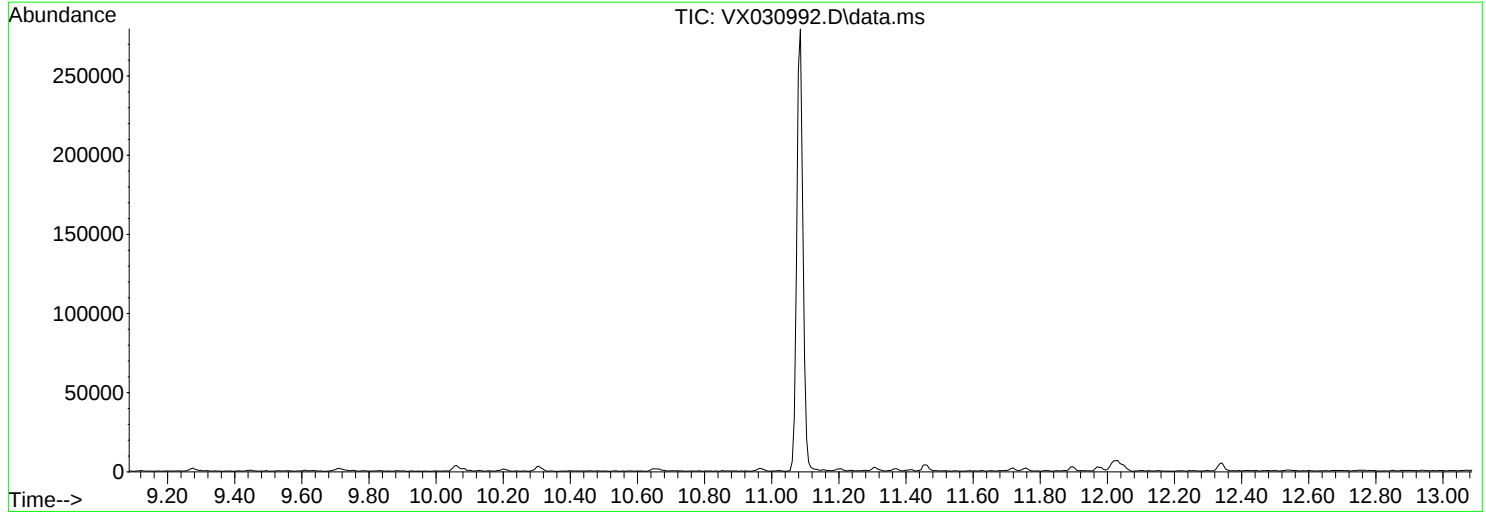

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.0	7710	PASS
75	95	30	60	44.9	23156	PASS
95	95	100	100	100.0	51536	PASS
96	95	5	9	6.3	3246	PASS
173	174	0.00	2	1.3	549	PASS
174	95	50	100	81.6	42067	PASS
175	174	5	9	7.4	3095	PASS
176	174	95	101	96.4	40563	PASS
177	176	5	9	6.1	2477	PASS