

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083123\
 Data File : VX037452.D
 Acq On : 31 Aug 2023 23:57
 Operator : JC/MD
 Sample : 04232-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 50088

Manual Integrations
 APPROVED

Reviewed By : John Carlone 09/01/2023
 Supervised By : Mahesh Dadoda 09/01/2023

Quant Time: Sep 01 08:25:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 18 09:30:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	158241	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	260507	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	241954	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	120974	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	92543	40.565	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	81.140%		
35) Dibromofluoromethane	5.385	113	75721	43.889	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	87.780%		
50) Toluene-d8	8.659	98	317374	50.713	ug/l	0.01
Spiked Amount 50.000	Range 92 - 112		Recovery =	101.420%		
62) 4-Bromofluorobenzene	11.079	95	120203	48.875	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	97.740%		
Target Compounds					Qvalue	
9) 1,1,2-Trichlorotrifluo...	2.319	101	10798	6.455	ug/l	94
11) Tert butyl alcohol	3.026	59	34739	64.915	ug/l #	91
16) Acetone	2.404	43	416644	466.840	ug/l #	84
18) Methyl Acetate	2.715	43	10754	3.200	ug/l #	82
19) Methyl tert-butyl Ether	3.123	73	243031	39.339	ug/l	99
22) Diisopropyl ether	3.763	45	46520	8.992	ug/l #	66
25) 2-Butanone	4.568	43	104905	78.066	ug/l #	81
31) Cyclohexane	5.471	56	144252	56.235	ug/l	87
37) Ethyl Acetate	4.715	43	800446	319.685	ug/l #	91
39) Methylcyclohexane	7.379	83	204382	79.363	ug/l	92
40) Benzene	6.037	78	6554965	932.442	ug/l	98
44) Trichloroethene	7.123	130	84784	42.533	ug/l	95
52) Toluene	8.756	92	22032073	4743.390	ug/l #	73
59) 2-Hexanone	9.439	43	9523	5.174	ug/l	73
64) Tetrachloroethene	9.275	164	666	0.377	ug/l	93
67) Ethyl Benzene	10.201	91	10566314	1174.255	ug/l #	75
68) m/p-Xylenes	10.323	106	11462122	3298.523	ug/l #	67
69) o-Xylene	10.659	106	7285292	2124.981	ug/l	70
73) Isopropylbenzene	10.963	105	963104	109.531	ug/l	97
78) n-propylbenzene	11.305	91	1870110	191.000	ug/l	97
80) 1,3,5-Trimethylbenzene	11.451	105	2262045	308.393	ug/l	97
84) 1,2,4-Trimethylbenzene	11.756	105	7763644	1047.298	ug/l	84
85) sec-Butylbenzene	11.890	105	110911m	13.574	ug/l	
86) p-Isopropyltoluene	12.012	119	68647m	9.760	ug/l	
89) n-Butylbenzene	12.329	91	253670	43.499	ug/l #	29
95) Naphthalene	13.774	128	2037879	201.954	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083123\
Data File : VX037452.D
Acq On : 31 Aug 2023 23:57
Operator : JC/MD
Sample : 04232-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
50088

Manual Integrations
APPROVED

Reviewed By : John Carlone 09/01/2023
Supervised By : Mahesh Dadoda 09/01/2023


Quant Time: Sep 01 08:25:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 18 09:30:38 2023
Response via : Initial Calibration

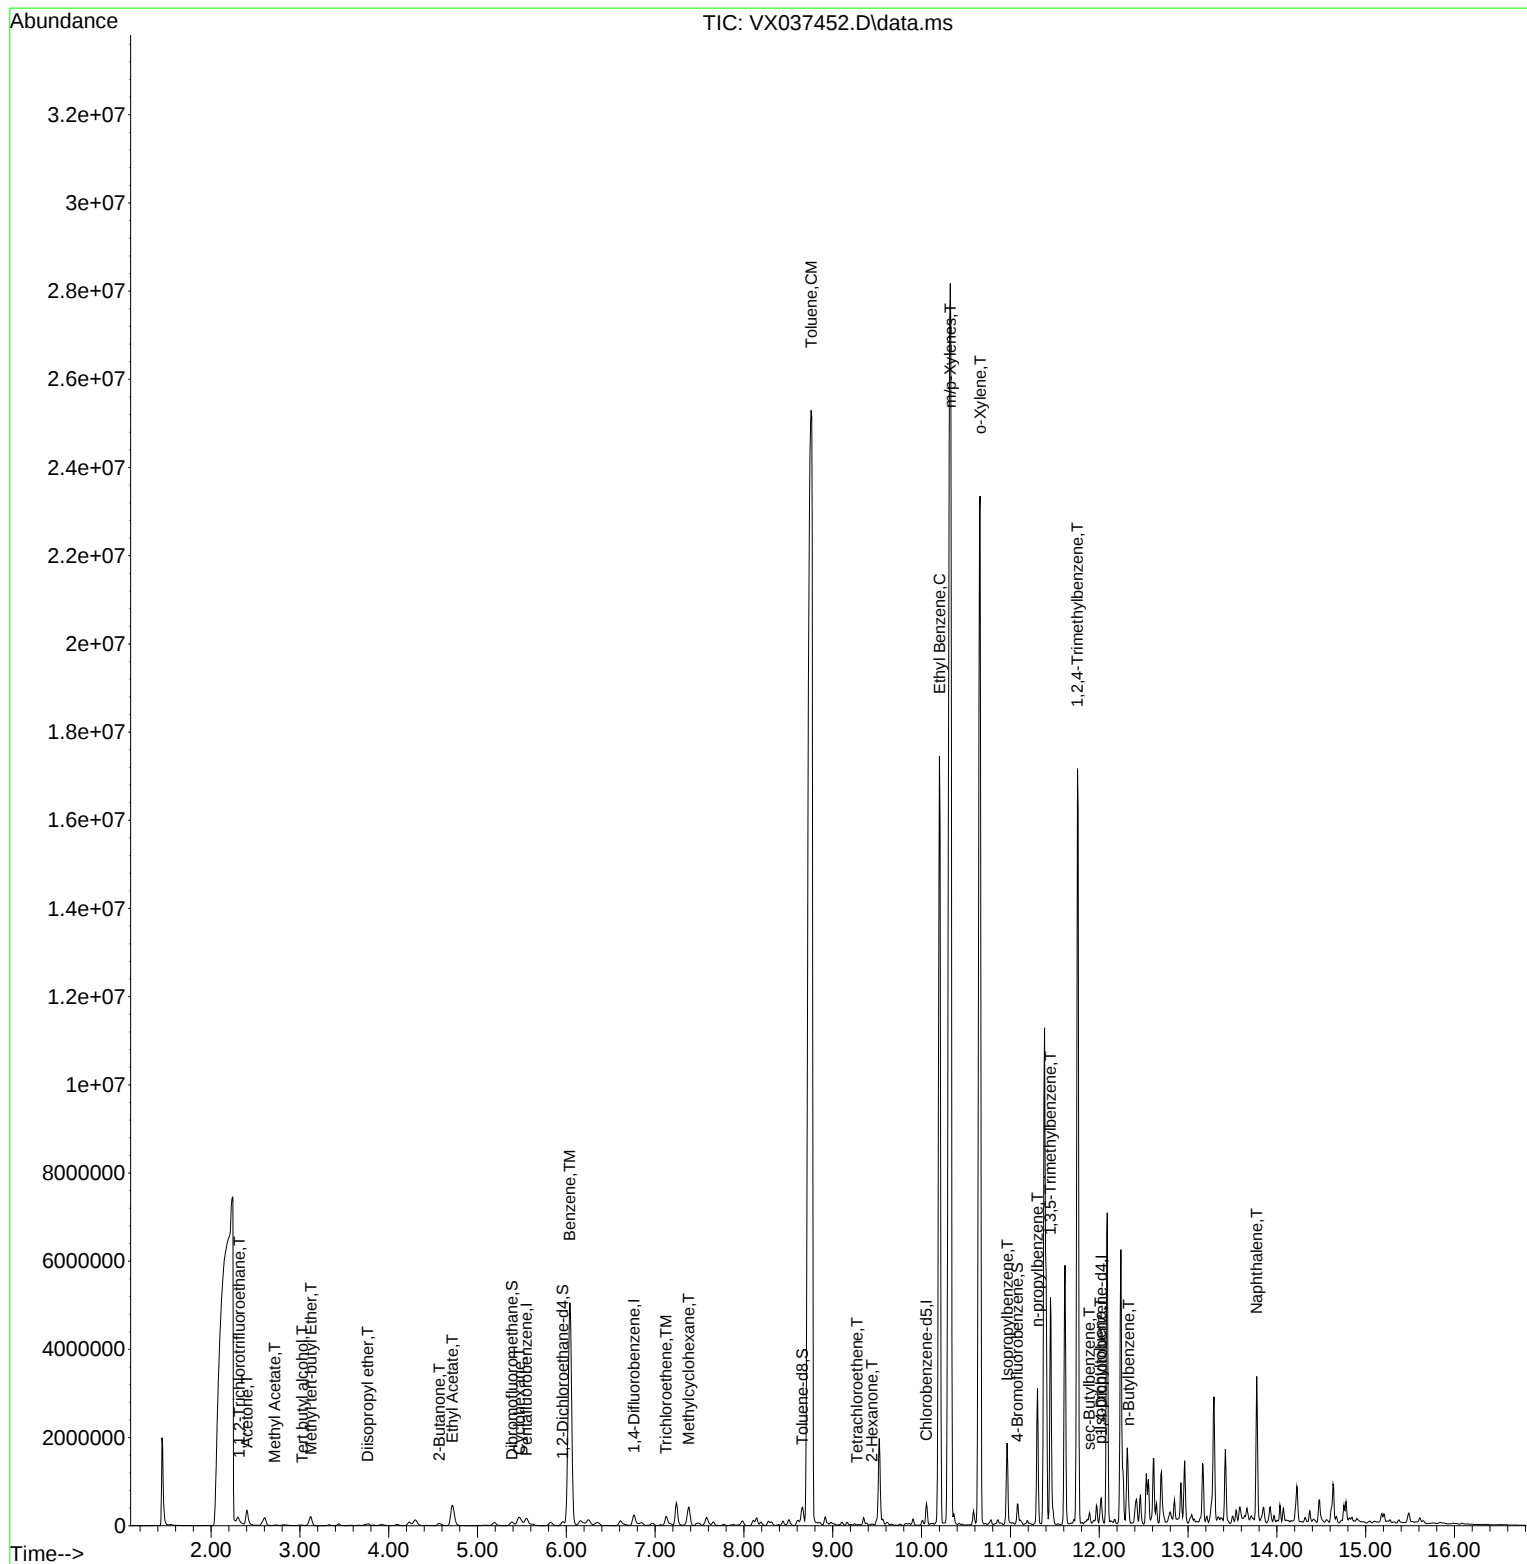



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57




Instrument :
MSVOA_X
ClientSampleId :
50088




Tgt Ion:168 Resp: 15824
Ion Ratio Lower Upper
168 100
99 62.9 56.6 85.0

Manual Integrations
APPROVED



Reviewed By :John Carlone 09/01/2023
Supervised By :Mahesh Dadoda 09/01/2023

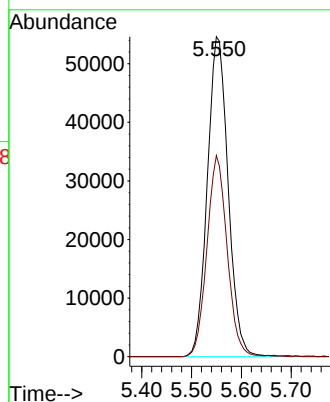


#9
1,1,2-Trichlorotrifluoroethane
Concen: 6.455 ug/l
RT: 2.319 min Scan# 202
Delta R.T. -0.006 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57



Tgt Ion:101 Resp: 10798
Ion Ratio Lower Upper
101 100
85 40.0 37.0 55.6
151 76.5 58.6 87.8

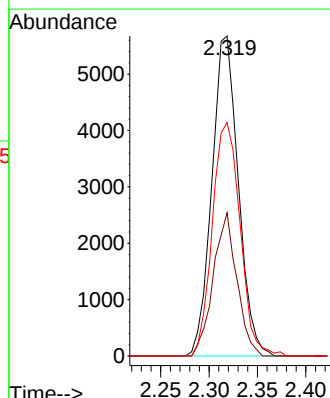







#11
Tert butyl alcohol
Concen: 64.915 ug/l
RT: 3.026 min Scan# 311
Delta R.T. 0.049 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57

Instrument :
MSVOA_X
ClientSampleId :
50088

Tgt Ion: 59 Resp: 34739
Ion Ratio Lower Upper
59 100
57 10.6 6.0 9.0




Manual Integrations
APPROVED


Reviewed By :John Carlone 09/01/2023
Supervised By :Mahesh Dadoda 09/01/2023

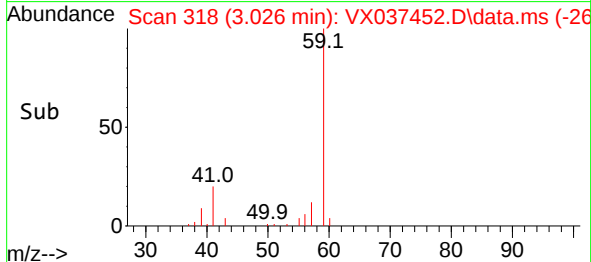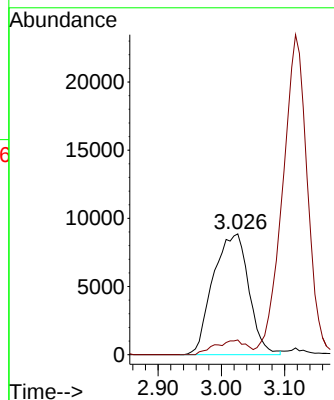

#16
Acetone
Concen: 466.840 ug/l
RT: 2.404 min Scan# 216
Delta R.T. 0.018 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57

Tgt Ion: 43 Resp: 416644
Ion Ratio Lower Upper
43 100
58 35.7 21.9 32.9

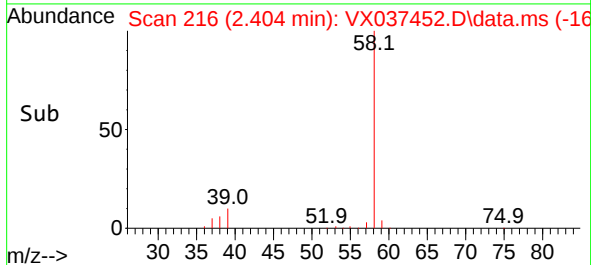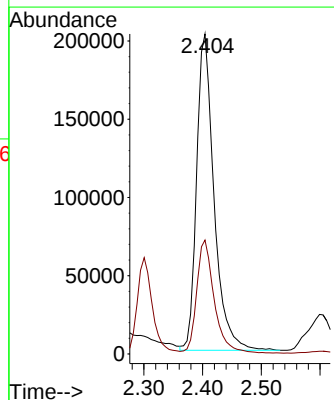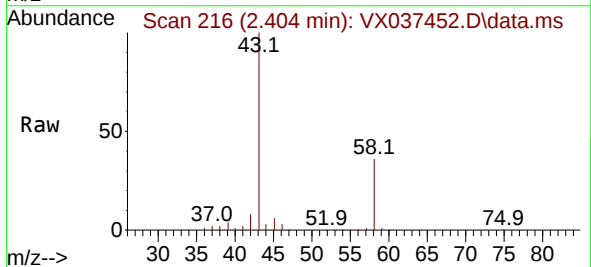



#18

Methyl Acetate

Concen: 3.200 ug/l

RT: 2.715 min Scan# 20

Delta R.T. 0.012 min

Lab File: VX037452.D

Acq: 31 Aug 2023 23:57

Instrument :

MSVOA_X

ClientSampleId :

50088

Tgt Ion: 43 Resp: 10754

Ion Ratio Lower Upper

43 100





74 31.1 17.8 26.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 09/01/2023

Supervised By :Mahesh Dadoda 09/01/2023



#19

Methyl tert-butyl Ether

Concen: 39.339 ug/l

RT: 3.123 min Scan# 334

Delta R.T. 0.006 min

Lab File: VX037452.D




Acq: 31 Aug 2023 23:57


Tgt Ion: 73 Resp: 243031

Ion Ratio Lower Upper

73 100


57 21.2 17.3 25.9

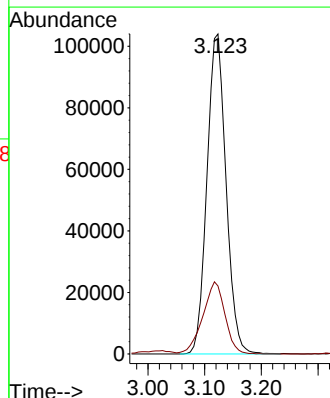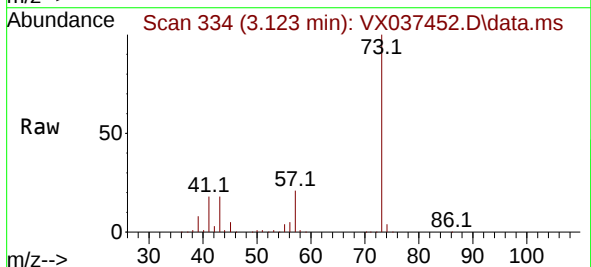



#22
Diisopropyl ether
Concen: 8.992 ug/l
RT: 3.763 min Scan# 41
Delta R.T. 0.000 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57




Instrument :
MSVOA_X
ClientSampleId :
50088




Tgt Ion: 45 Resp: 46520
Ion Ratio Lower Upper
45 100
43 46.9 69.7 104.5
87 33.4 20.8 31.2
59 12.3 9.0 13.4

Manual Integrations
APPROVED



Reviewed By :John Carlone 09/01/2023
Supervised By :Mahesh Dadoda 09/01/2023

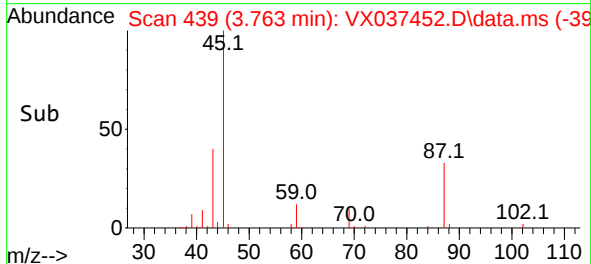


#25
2-Butanone
Concen: 78.066 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.012 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57

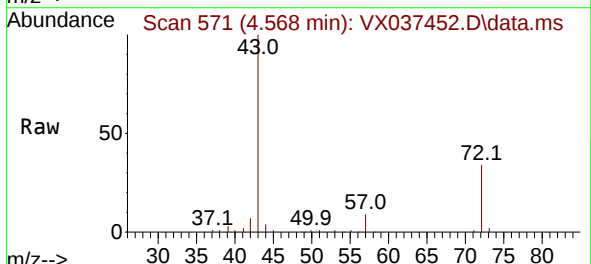


Tgt Ion: 43 Resp: 104905
Ion Ratio Lower Upper
43 100
72 33.8 19.4 29.2

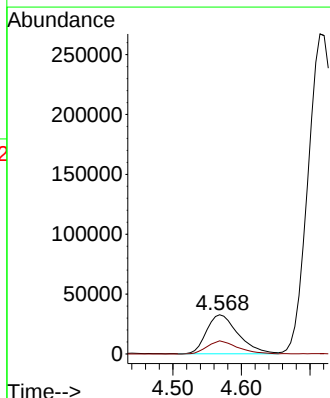



#31
Cyclohexane
Concen: 56.235 ug/l
RT: 5.471 min Scan# 719
Delta R.T. 0.000 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57




Instrument :
MSVOA_X
ClientSampleId :
50088



Tgt Ion: 56 Resp: 14425
Ion Ratio Lower Upper
56 100
69 31.6 23.4 35.2
84 96.9 65.9 98.9




Manual Integrations
APPROVED


Reviewed By :John Carlone 09/01/2023
Supervised By :Mahesh Dadoda 09/01/2023



#33
1,2-Dichloroethane-d4
Concen: 40.565 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57

Tgt Ion: 65 Resp: 92543
Ion Ratio Lower Upper
65 100
67 52.1 0.0 100.2

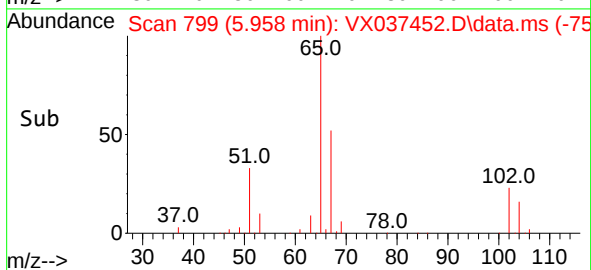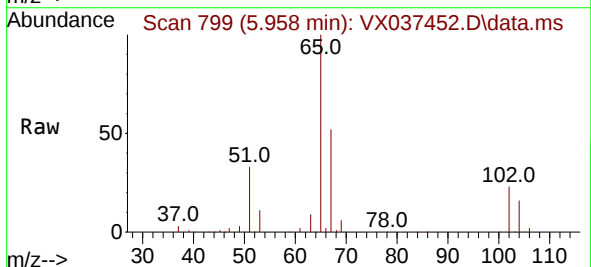







#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57

Instrument :
MSVOA_X
ClientSampleId :
50088

Tgt Ion:114 Resp: 26050
Ion Ratio Lower Upper
114 100
63 18.4 0.0 45.0
88 16.2 0.0 36.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 09/01/2023
Supervised By :Mahesh Dadoda 09/01/2023

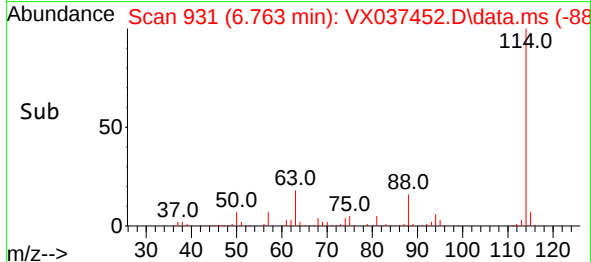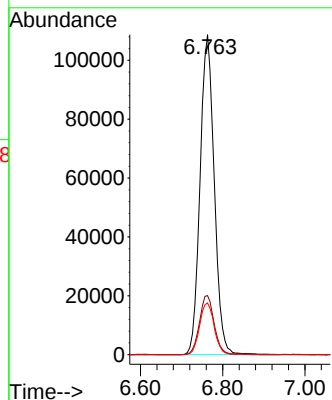

#35
Dibromofluoromethane
Concen: 43.889 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57

Tgt Ion:113 Resp: 75721
Ion Ratio Lower Upper
113 100
111 103.3 82.9 124.3
192 19.1 13.3 19.9

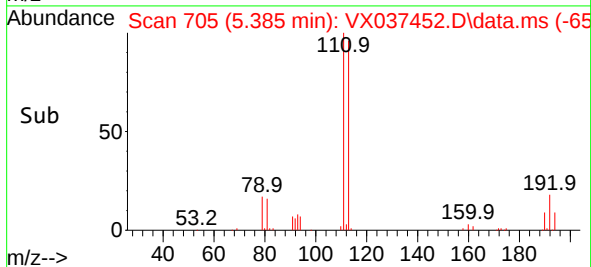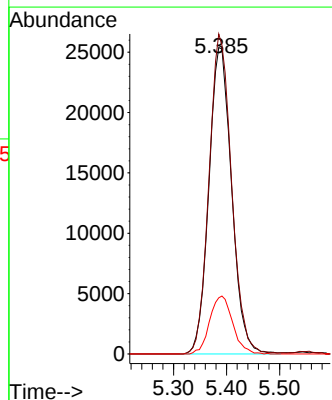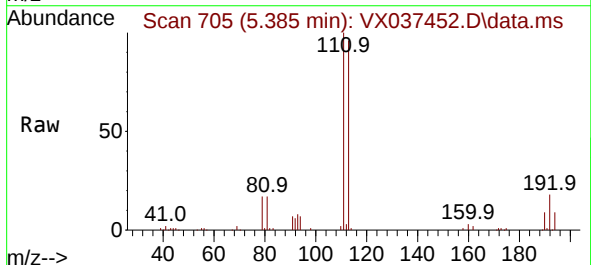



#37

Ethyl Acetate

Concen: 319.685 ug/l

RT: 4.715 min Scan# 595

Delta R.T. 0.000 min

Lab File: VX037452.D

Acq: 31 Aug 2023 23:57

Instrument :

MSVOA_X

ClientSampleId :

50088

Tgt Ion: 43 Resp: 800440





Ion	Ratio	Lower	Upper
43	100		
61	16.6	10.6	16.0
70	14.5	8.3	12.5

Manual Integrations

APPROVED

Reviewed By :John Carlone 09/01/2023

Supervised By :Mahesh Dadoda 09/01/2023

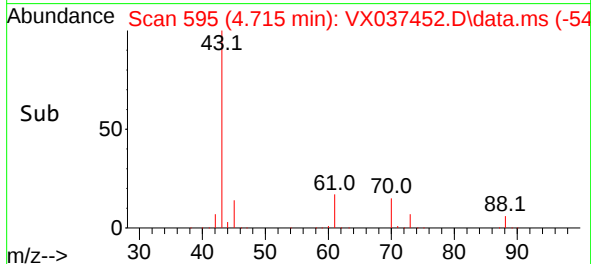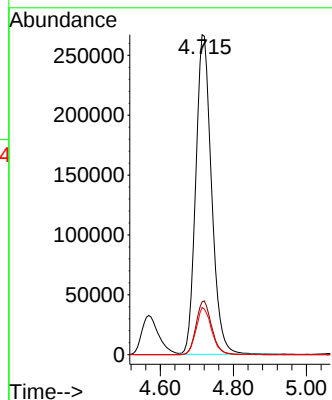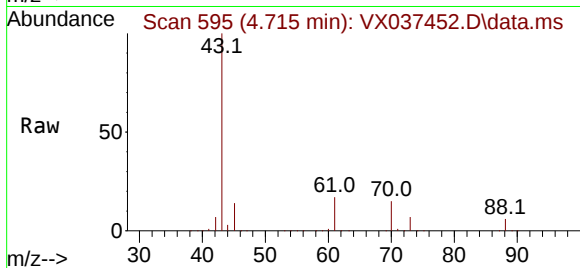

#39

Methylcyclohexane

Concen: 79.363 ug/l

RT: 7.379 min Scan# 1032




Delta R.T. 0.000 min


Lab File: VX037452.D

Acq: 31 Aug 2023 23:57

Tgt Ion: 83 Resp: 204382

Ion	Ratio	Lower	Upper
83	100		
55	73.3	64.6	97.0
98	51.3	36.7	55.1

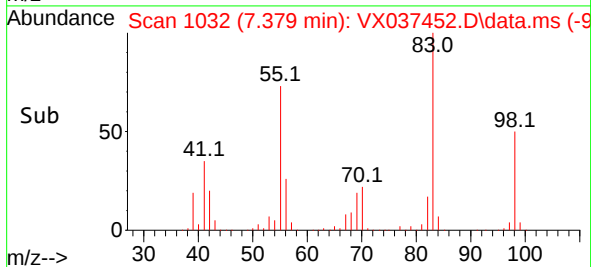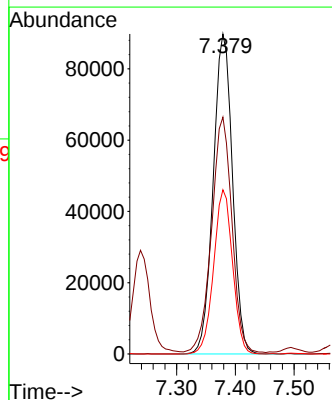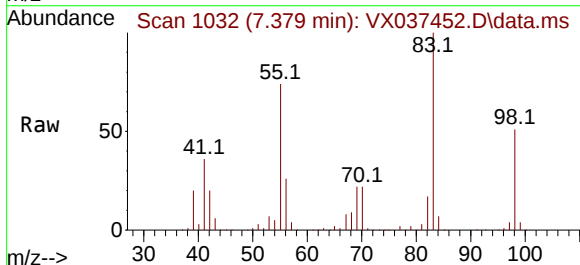

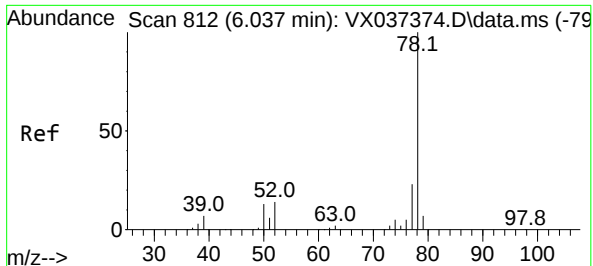





#40
Benzene
Concen: 932.442 ug/l
RT: 6.037 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57

Instrument :
MSVOA_X
ClientSampleId :
50088

Tgt Ion: 78 Resp: 655496
Ion Ratio Lower Upper
78 100
77 25.2 19.3 28.9




Manual Integrations
APPROVED


Reviewed By :John Carlone 09/01/2023
Supervised By :Mahesh Dadoda 09/01/2023

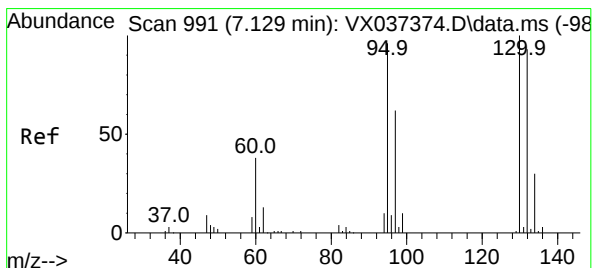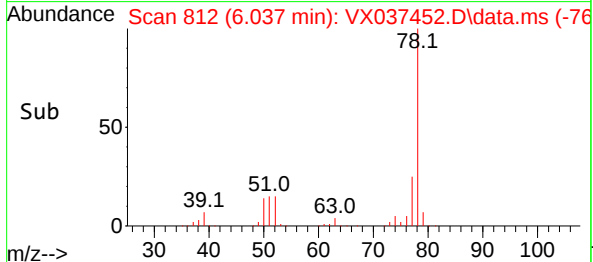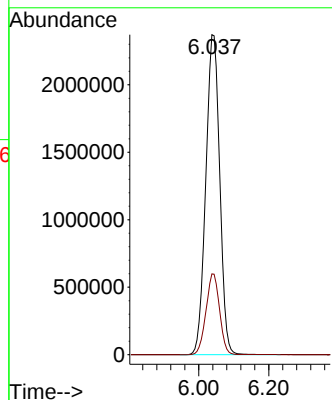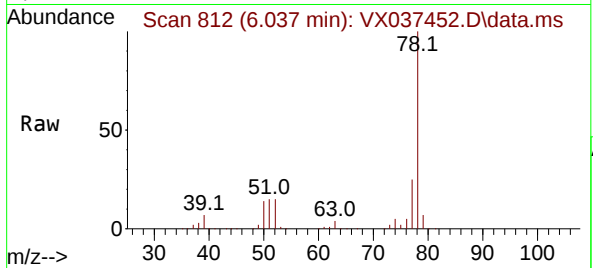

#44
Trichloroethene
Concen: 42.533 ug/l
RT: 7.123 min Scan# 990
Delta R.T. 0.000 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57


Tgt Ion:130 Resp: 84784
Ion Ratio Lower Upper
130 100
95 96.6 0.0 204.4

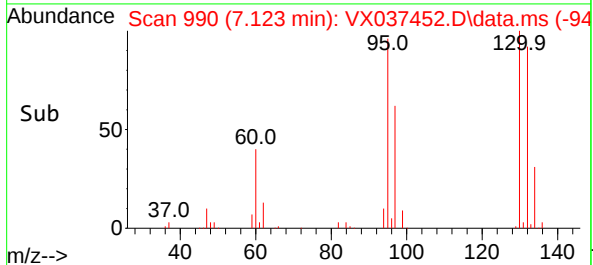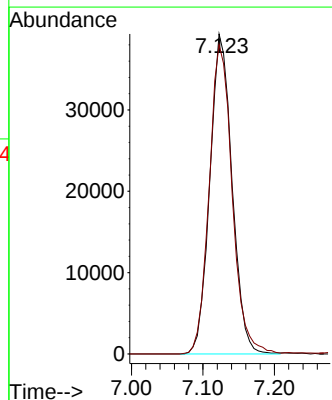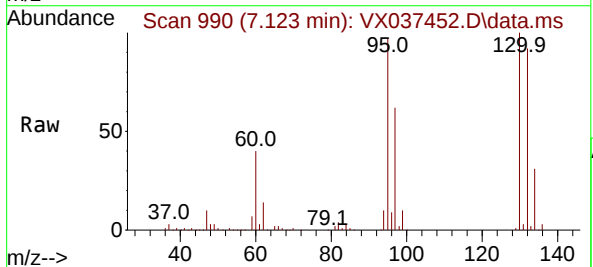

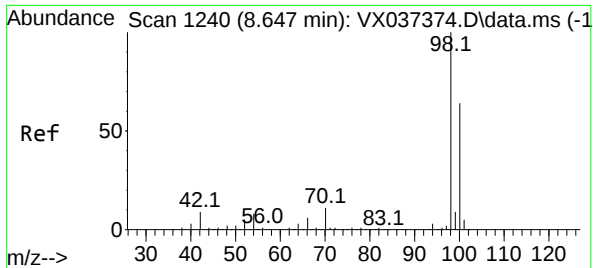

#50
Toluene-d8
Concen: 50.713 ug/l
RT: 8.659 min Scan# 11
Delta R.T. 0.012 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57




Instrument :
MSVOA_X
ClientSampleId :
50088

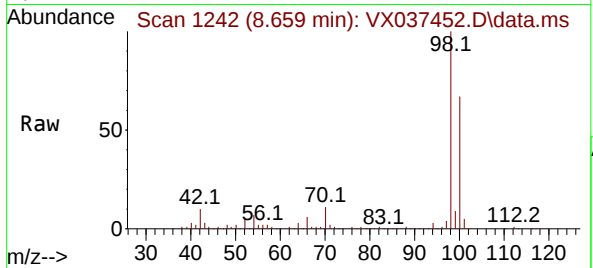


Tgt Ion: 98 Resp: 317374
Ion Ratio Lower Upper
98 100
100 66.8 53.1 79.7

Manual Integrations
APPROVED



Reviewed By :John Carlone 09/01/2023
Supervised By :Mahesh Dadoda 09/01/2023

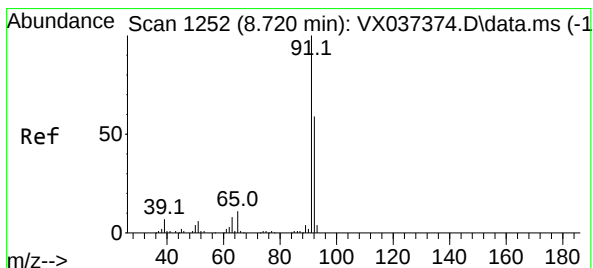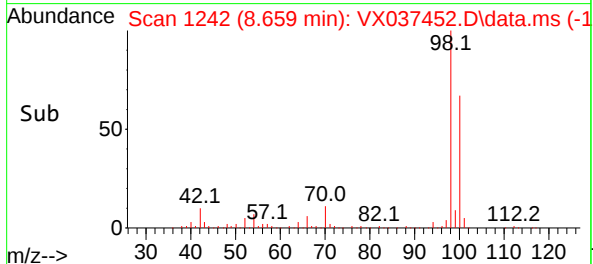


#52
Toluene
Concen: 4743.390 ug/l
RT: 8.756 min Scan# 1258
Delta R.T. 0.037 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57

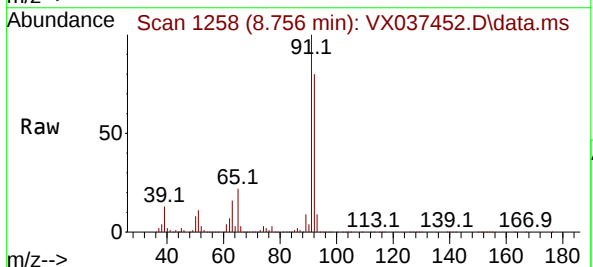


Tgt Ion: 92 Resp:22032073
Ion Ratio Lower Upper
92 100
91 131.1 134.2 201.2#

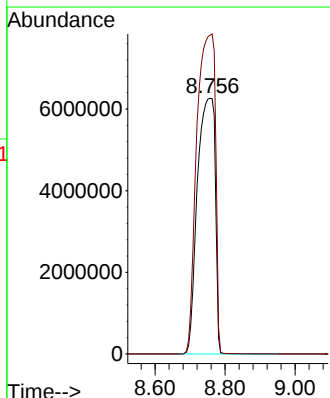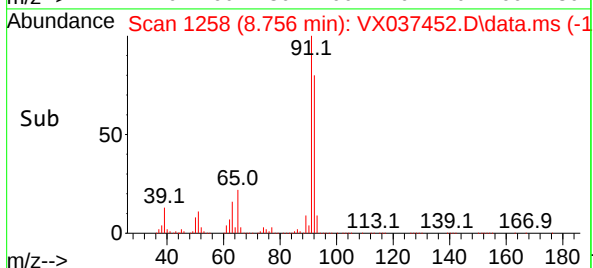



#59
2-Hexanone
Concen: 5.174 ug/l
RT: 9.439 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57




Instrument :
MSVOA_X
ClientSampleId :
50088




Tgt Ion: 43 Resp: 952
Ion Ratio Lower Upper
43 100
58 71.3 26.2 78.5

Manual Integrations
APPROVED



Reviewed By :John Carlone 09/01/2023
Supervised By :Mahesh Dadoda 09/01/2023

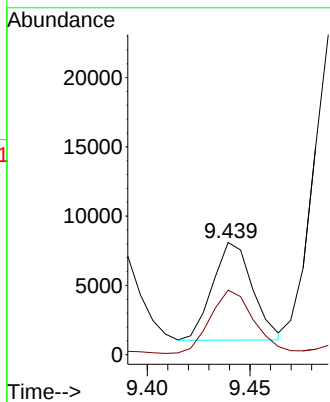


#62
4-Bromofluorobenzene
Concen: 48.875 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57

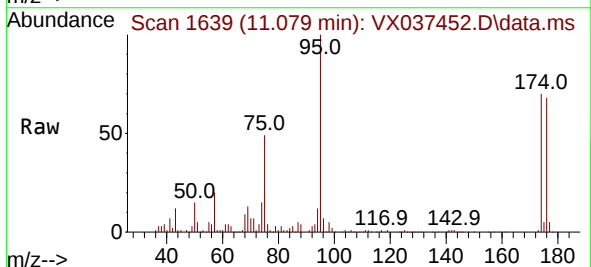


Tgt Ion: 95 Resp: 120203
Ion Ratio Lower Upper
95 100
174 74.3 0.0 135.6
176 72.7 0.0 131.0

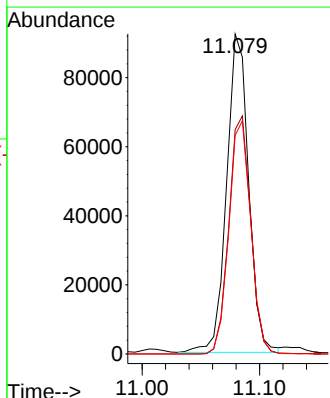



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57




Instrument :
MSVOA_X
ClientSampleId :
50088



Tgt Ion:117 Resp: 241954
Ion Ratio Lower Upper
117 100
82 52.8 46.2 69.4
119 31.8 25.5 38.3




Manual Integrations
APPROVED


Reviewed By :John Carlone 09/01/2023
Supervised By :Mahesh Dadoda 09/01/2023

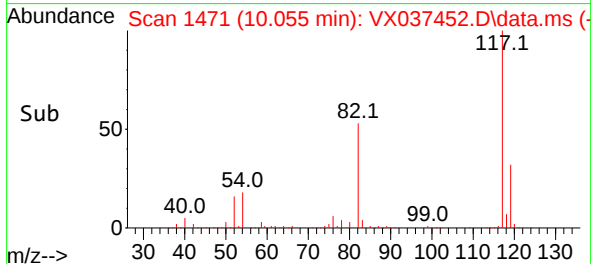

#64
Tetrachloroethene
Concen: 0.377 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. 0.000 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57

Tgt Ion:164 Resp: 666
Ion Ratio Lower Upper
164 100
166 124.2 102.7 154.1
129 115.6 80.4 120.6
131 100.2 76.5 114.7

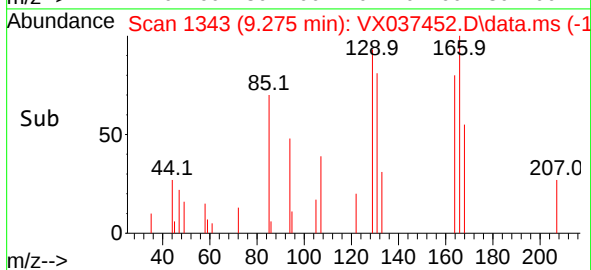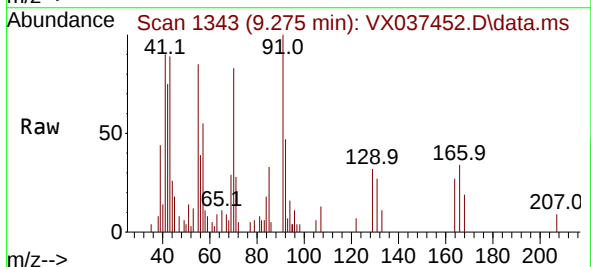

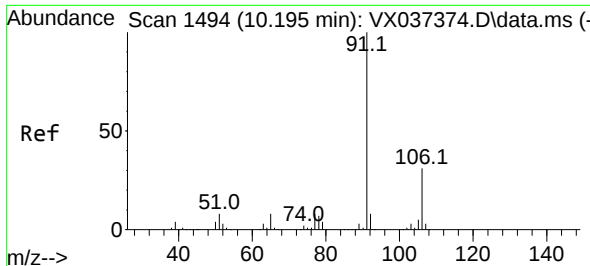

#67

Ethyl Benzene

Concen: 1174.255 ug/l

RT: 10.201 min Scan# 1494

Delta R.T. 0.006 min

Lab File: VX037452.D

Acq: 31 Aug 2023 23:57

Instrument :

MSVOA_X

ClientSampleId :

50088

Tgt Ion: 91 Resp:10566314

Ion Ratio Lower Upper

91 100





106 45.0 24.9 37.3

Manual Integrations

APPROVED

Reviewed By :John Carlone 09/01/2023

Supervised By :Mahesh Dadoda 09/01/2023

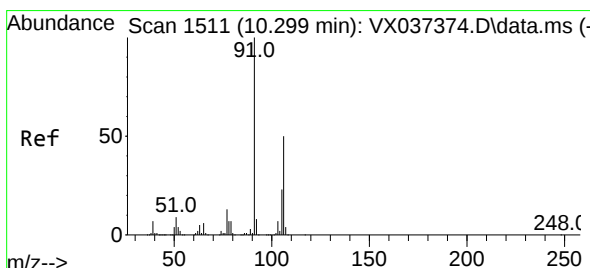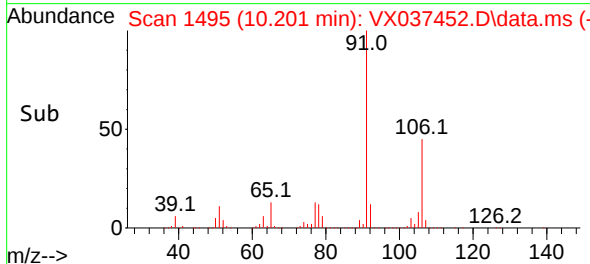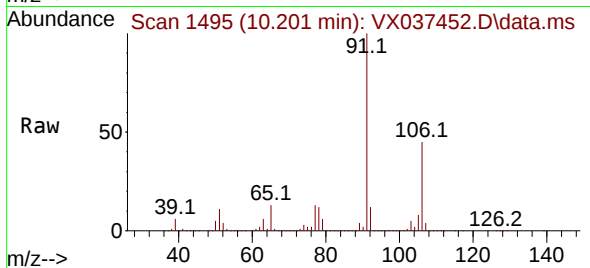

#68

m/p-Xylenes

Concen: 3298.523 ug/l

RT: 10.323 min Scan# 1515

Delta R.T. 0.024 min

Lab File: VX037452.D




Acq: 31 Aug 2023 23:57


Tgt Ion:106 Resp:11462122

Ion Ratio Lower Upper

106 100


91 156.1 165.5 248.3

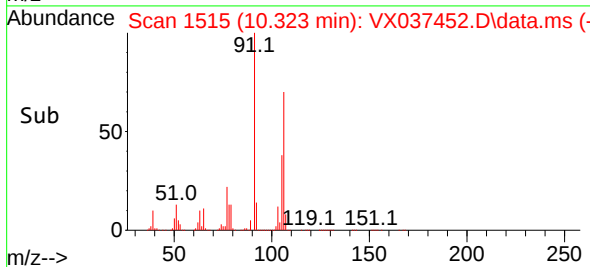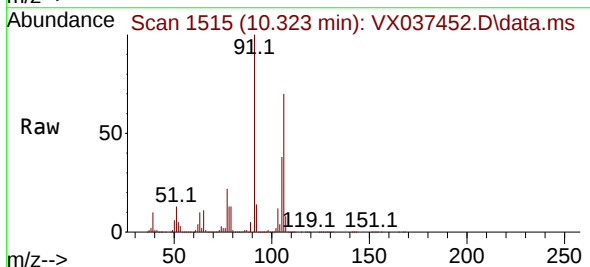

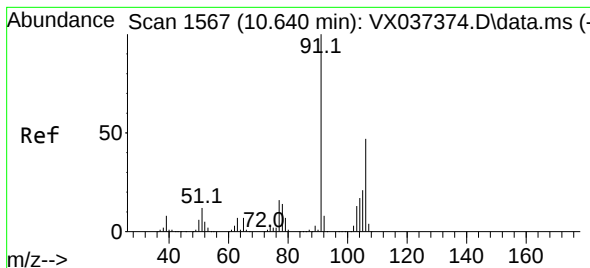

#69
o-Xylene
Concen: 2124.981 ug/l
RT: 10.659 min Scan# 1567
Delta R.T. 0.018 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57




Instrument :
MSVOA_X
ClientSampleId :
50088

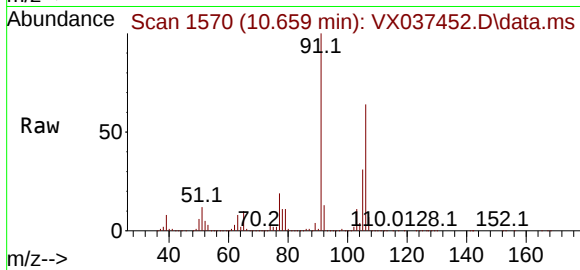

Tgt Ion:106 Resp: 728529
Ion Ratio Lower Upper
106 100
91 170.7 108.9 326.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 09/01/2023
Supervised By :Mahesh Dadoda 09/01/2023

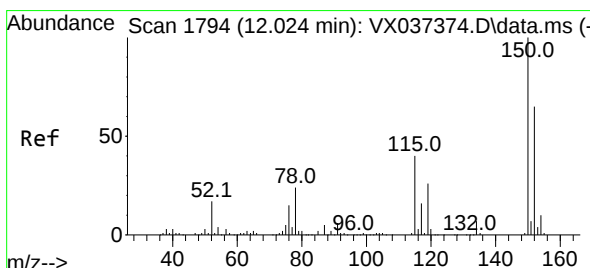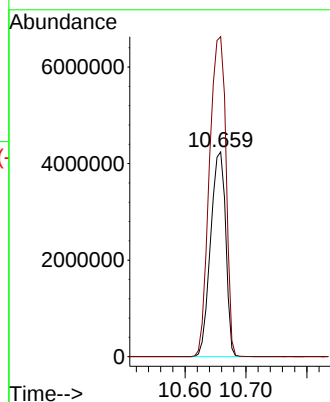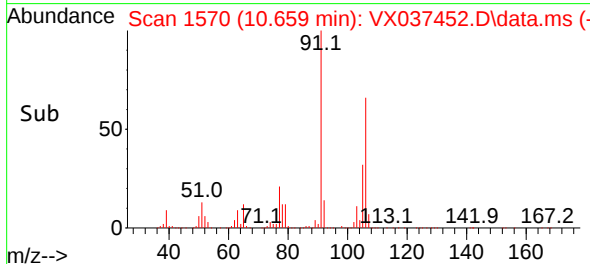

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57

Tgt Ion:152 Resp: 120974
Ion Ratio Lower Upper
152 100
115 64.4 43.3 129.9
150 155.8 0.0 345.0

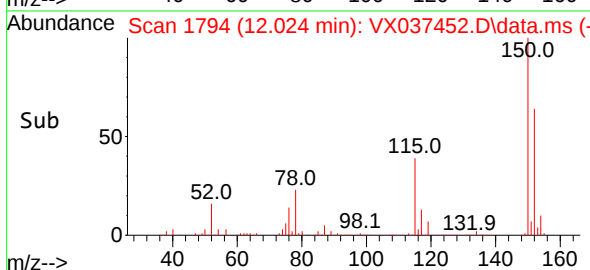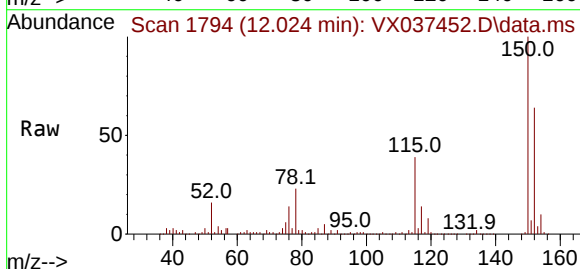



#73

Isopropylbenzene

Concen: 109.531 ug/l

RT: 10.963 min Scan# 1620

Delta R.T. 0.000 min

Lab File: VX037452.D

Acq: 31 Aug 2023 23:57

Instrument :

MSVOA_X

ClientSampleId :

50088

Tgt Ion:105 Resp: 963104

Ion Ratio Lower Upper

105 100





120 27.0 12.9 38.6

Manual Integrations

APPROVED

Reviewed By :John Carlone 09/01/2023

Supervised By :Mahesh Dadoda 09/01/2023

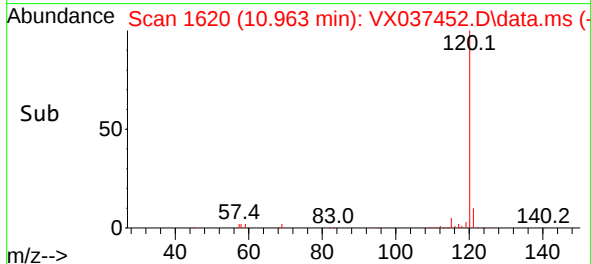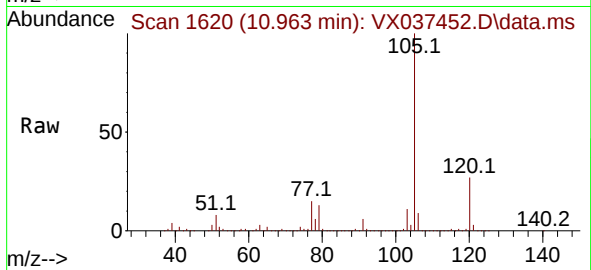

#78

n-propylbenzene

Concen: 191.000 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX037452.D




Acq: 31 Aug 2023 23:57


Tgt Ion: 91 Resp: 1870110

Ion Ratio Lower Upper

91 100

120 24.2 11.5 34.4

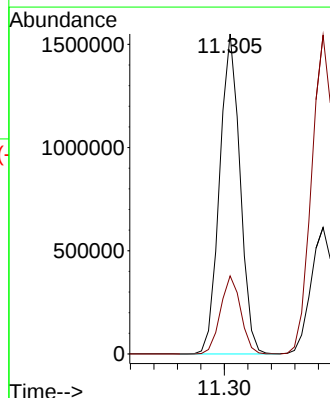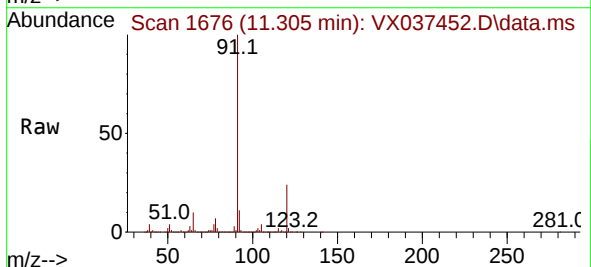



#80

1,3,5-Trimethylbenzene

Concen: 308.393 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX037452.D

Acq: 31 Aug 2023 23:57

Instrument :

MSVOA_X

ClientSampleId :

50088

Tgt Ion:105 Resp: 2262049

Ion Ratio Lower Upper

105 100





120 50.2 24.1 72.3

Manual Integrations

APPROVED

Reviewed By :John Carlone 09/01/2023

Supervised By :Mahesh Dadoda 09/01/2023

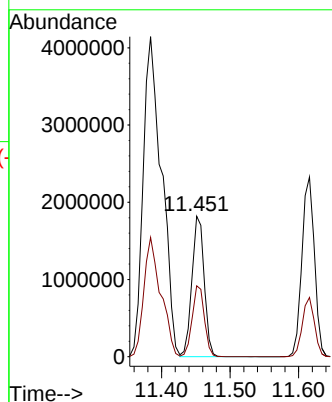

#84

1,2,4-Trimethylbenzene

Concen: 1047.298 ug/l

RT: 11.756 min Scan# 1750

Delta R.T. 0.006 min

Lab File: VX037452.D




Acq: 31 Aug 2023 23:57


Tgt Ion:105 Resp: 7763644

Ion Ratio Lower Upper

105 100


120 52.8 21.2 63.6

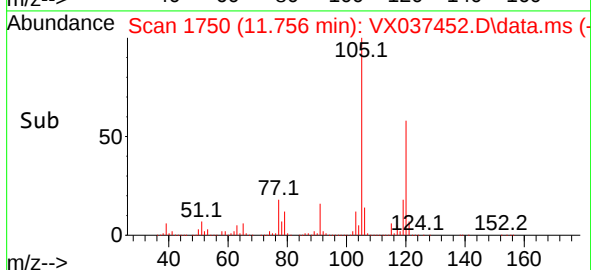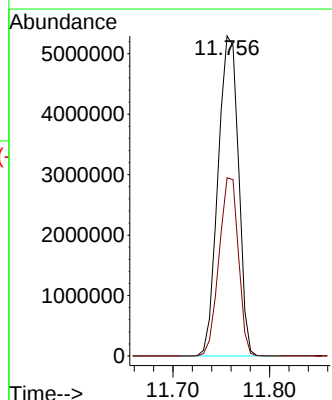



#85
 sec-Butylbenzene
 Concen: 13.574 ug/l m
 RT: 11.890 min Scan# 11891
 Delta R.T. 0.000 min
 Lab File: VX037452.D
 Acq: 31 Aug 2023 23:57




Instrument :
 MSVOA_X
 ClientSampleId :
 50088



Tgt Ion:105 Resp: 11091
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.8 29.4




Manual Integrations
 APPROVED


Reviewed By :John Carlone 09/01/2023
 Supervised By :Mahesh Dadoda 09/01/2023

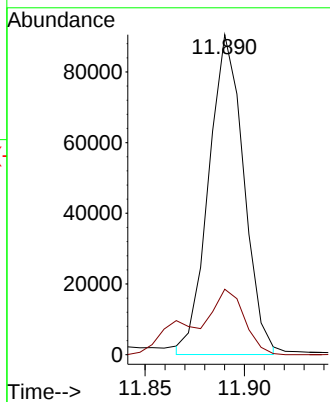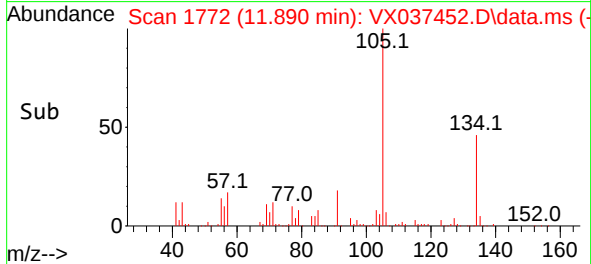

#86
 p-Isopropyltoluene
 Concen: 9.760 ug/l m
 RT: 12.012 min Scan# 1792
 Delta R.T. 0.006 min
 Lab File: VX037452.D
 Acq: 31 Aug 2023 23:57


Tgt Ion:119 Resp: 68647
 Ion Ratio Lower Upper
 119 100
 134 76.4 12.8 38.3#
 91 66.2 13.1 39.3#

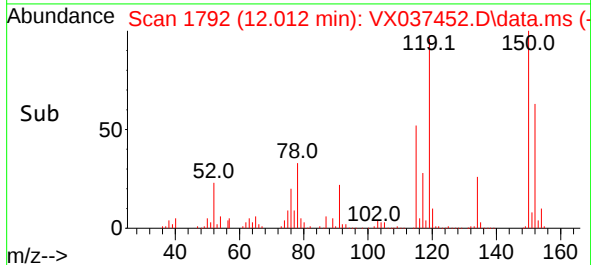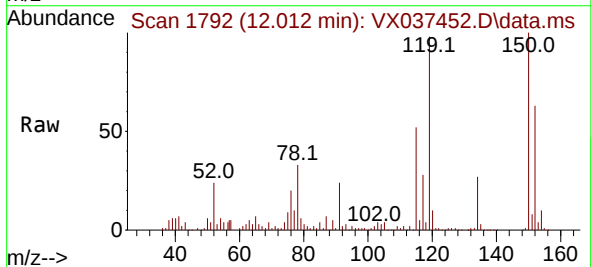

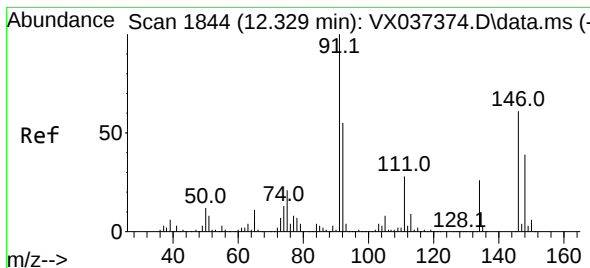

#89
n-Butylbenzene
Concen: 43.499 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. 0.000 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57




Instrument :
MSVOA_X
ClientSampleId :
50088

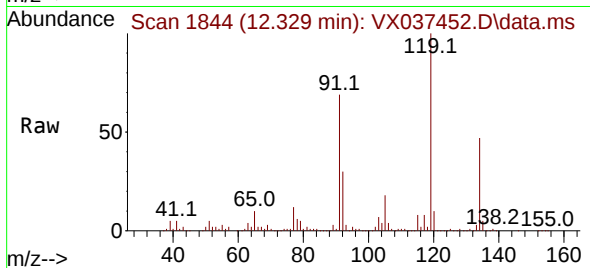


Tgt Ion: 91 Resp: 253670
Ion Ratio Lower Upper
91 100
92 33.0 27.4 82.0
134 106.2 12.6 37.8

Manual Integrations
APPROVED

Reviewed By :John Carlone 09/01/2023
Supervised By :Mahesh Dadoda 09/01/2023

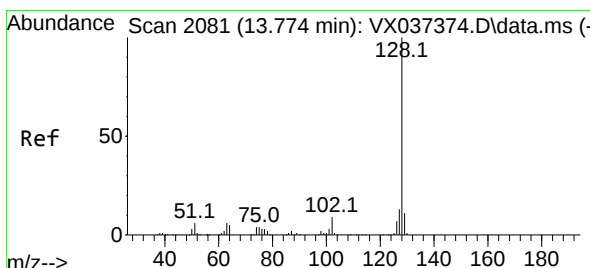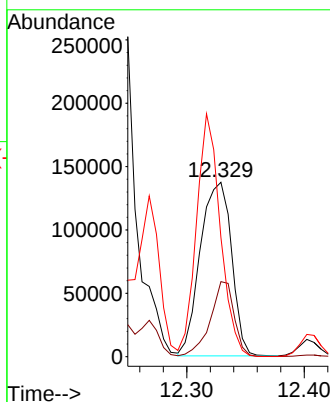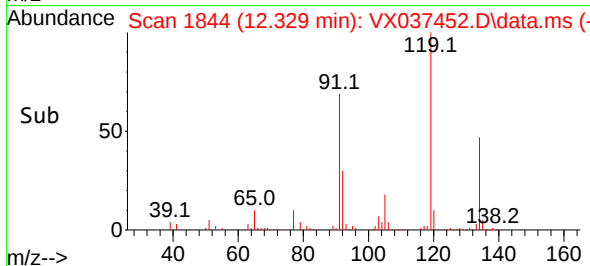

#95
Naphthalene
Concen: 201.954 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. 0.000 min
Lab File: VX037452.D
Acq: 31 Aug 2023 23:57

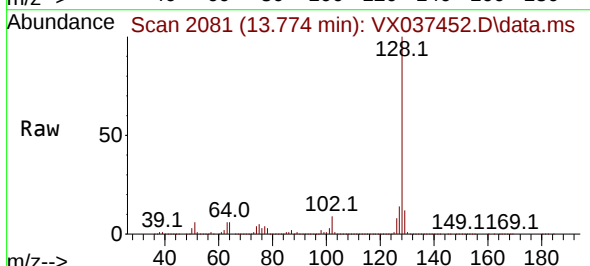

Tgt Ion:128 Resp: 2037879
Ion Ratio Lower Upper
128 100
127 13.2 10.3 15.5
129 11.3 8.8 13.2

