

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083123\
 Data File : VX037436.D
 Acq On : 31 Aug 2023 17:30
 Operator : JC/MD
 Sample : 04128-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP10-20230822

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M

Title : SW846 8260

Signal : TIC: VX037436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.538	228	238	247	rBV	11403	22379	3.06%	0.570%
2	2.941	297	304	313	rVB	3301	7446	1.02%	0.190%
3	4.574	560	572	589	rBV	8292	27691	3.78%	0.705%
4	5.385	694	705	720	rBV	83980	244600	33.40%	6.232%
5	5.550	720	732	748	rVB	157304	442858	60.46%	11.283%
6	5.952	787	798	820	rBV	91473	245782	33.56%	6.262%
7	6.763	920	931	946	rBV	225986	547341	74.73%	13.945%
8	8.647	1233	1240	1256	rBV	472515	732439	100.00%	18.661%
9	10.055	1465	1471	1481	rBV	464381	621459	84.85%	15.833%
10	11.079	1634	1639	1655	rBV	378543	466894	63.75%	11.895%
11	12.024	1788	1794	1806	rBV	430320	566156	77.30%	14.424%




Sum of corrected areas: 3925045

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083123\
Data File : VX037436.D
Acq On : 31 Aug 2023 17:30
Operator : JC/MD
Sample : 04128-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP10-20230822

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

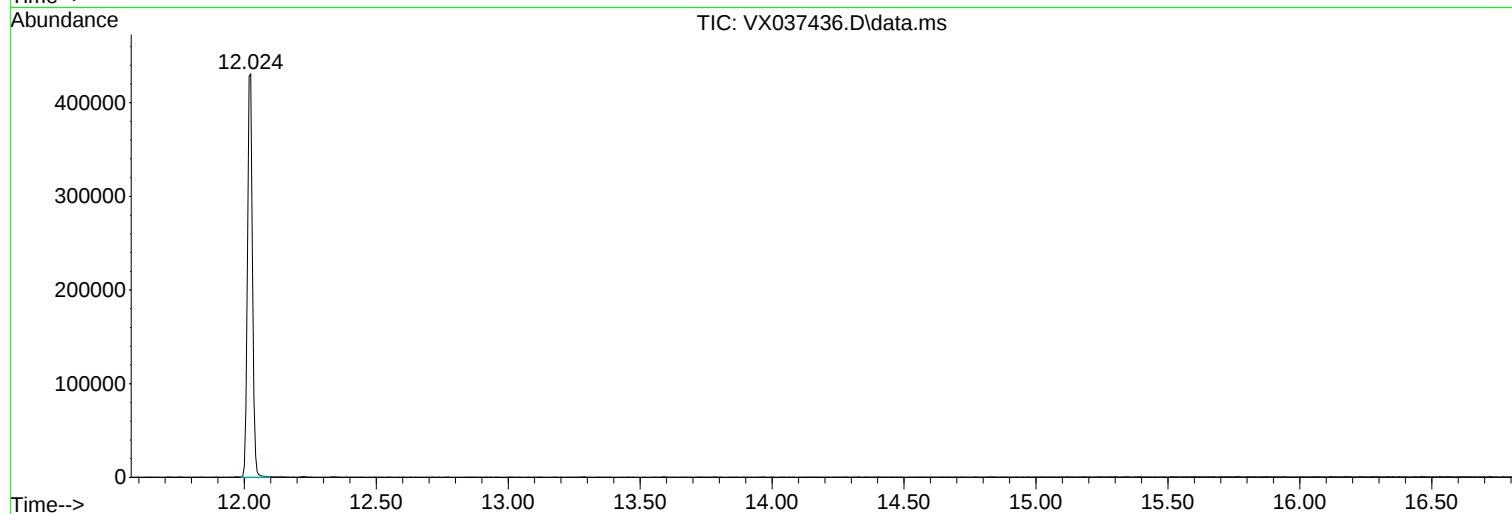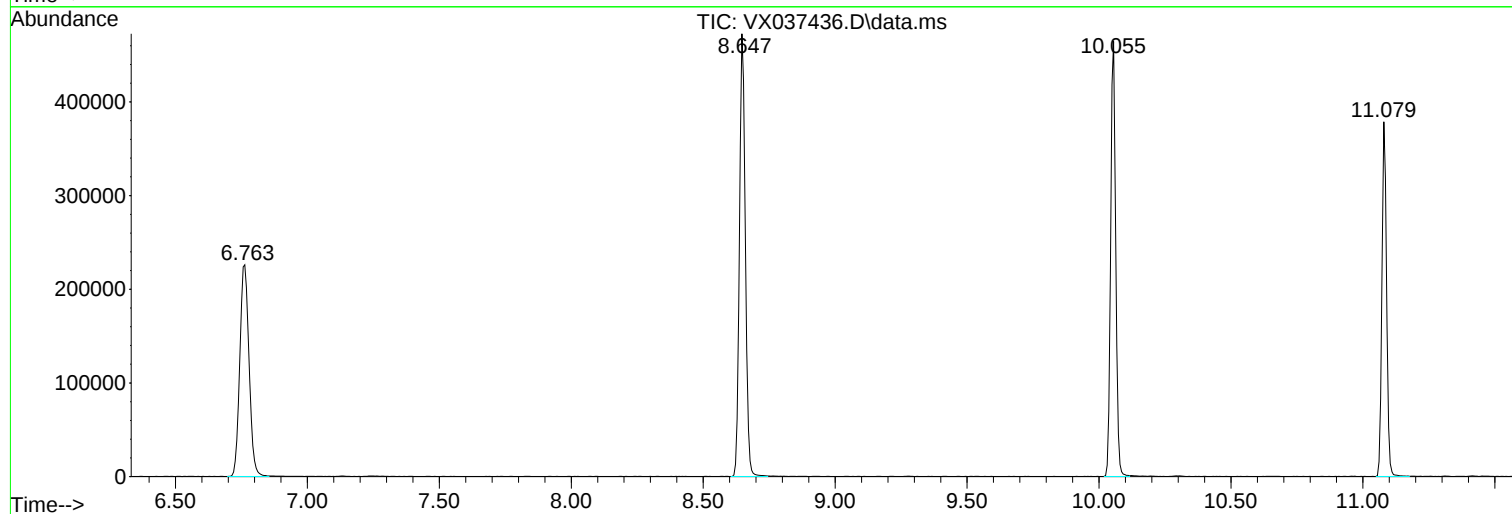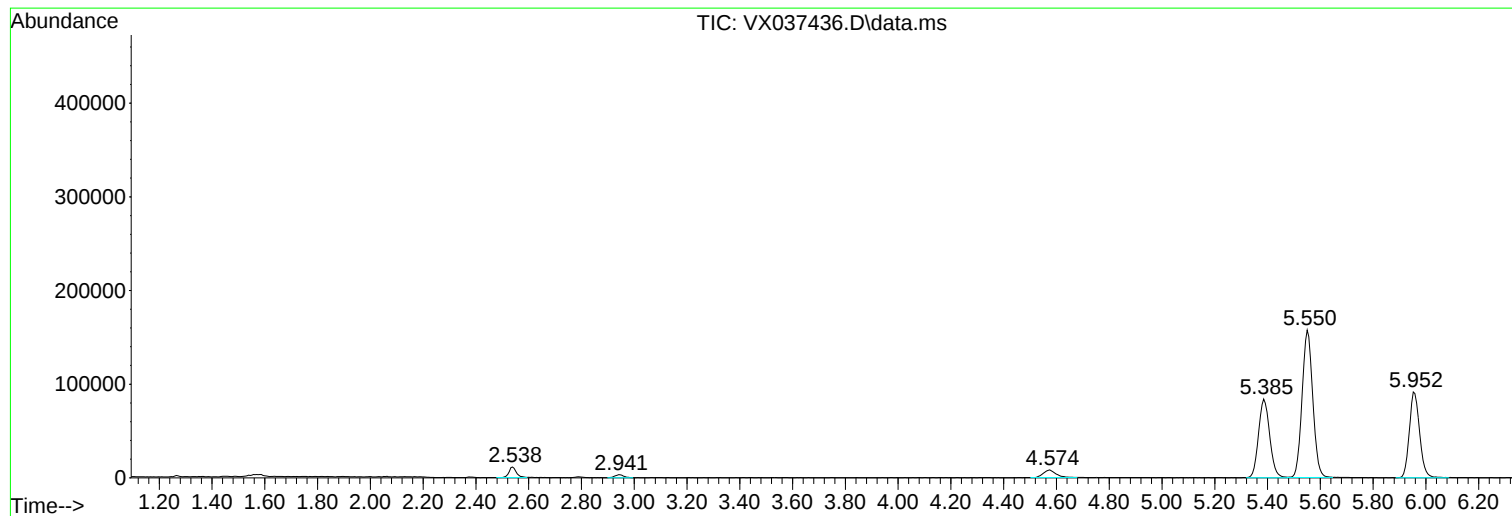

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083123\
Data File : VX037436.D
Acq On : 31 Aug 2023 17:30
Operator : JC/MD
Sample : 04128-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP10-20230822

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX083123\
Data File : VX037436.D
Acq On : 31 Aug 2023 17:30
Operator : JC/MD
Sample : 04128-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP10-20230822

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------