


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX090119\
Data File : VX011986.D
Acq On : 01 Sep 2019 10:06
Operator : SY/SP
Sample : BFB
Misc : 5.00µ/5.0mL/MSVOA X/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082919S.M
Title : SW846 8260
Last Update : Fri Aug 30 01:59:05 2019

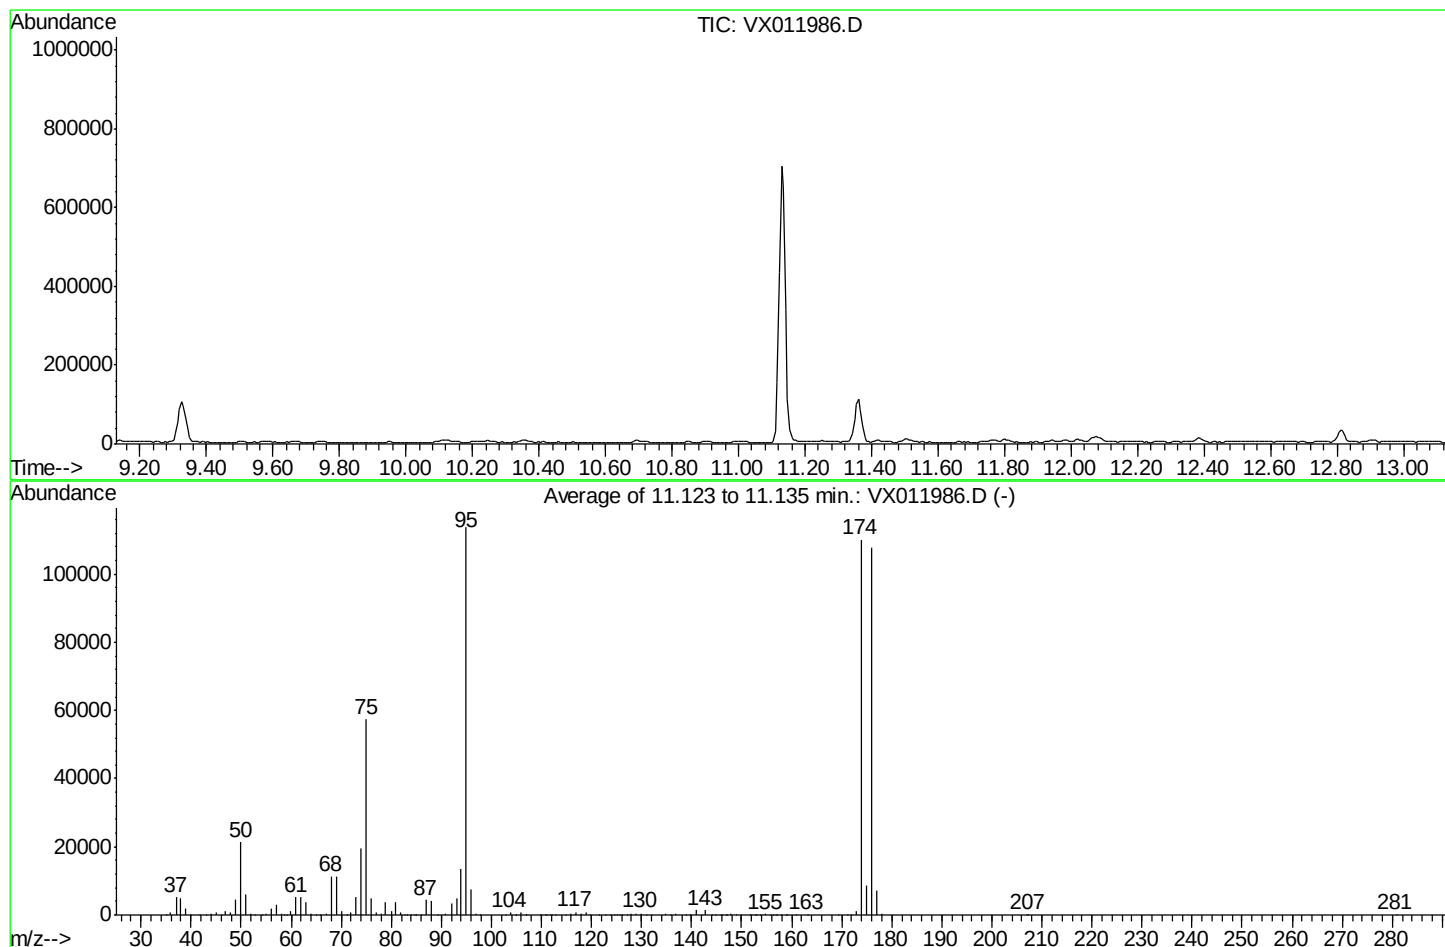

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	21283	PASS
75	95	30	60	50.5	57418	PASS
95	95	100	100	100.0	113693	PASS
96	95	5	9	6.8	7697	PASS
173	174	0.00	2	1.1	1245	PASS
174	95	50	100	96.8	110061	PASS
175	174	5	9	7.7	8469	PASS
176	174	95	101	97.7	107570	PASS
177	176	5	9	6.7	7190	PASS