
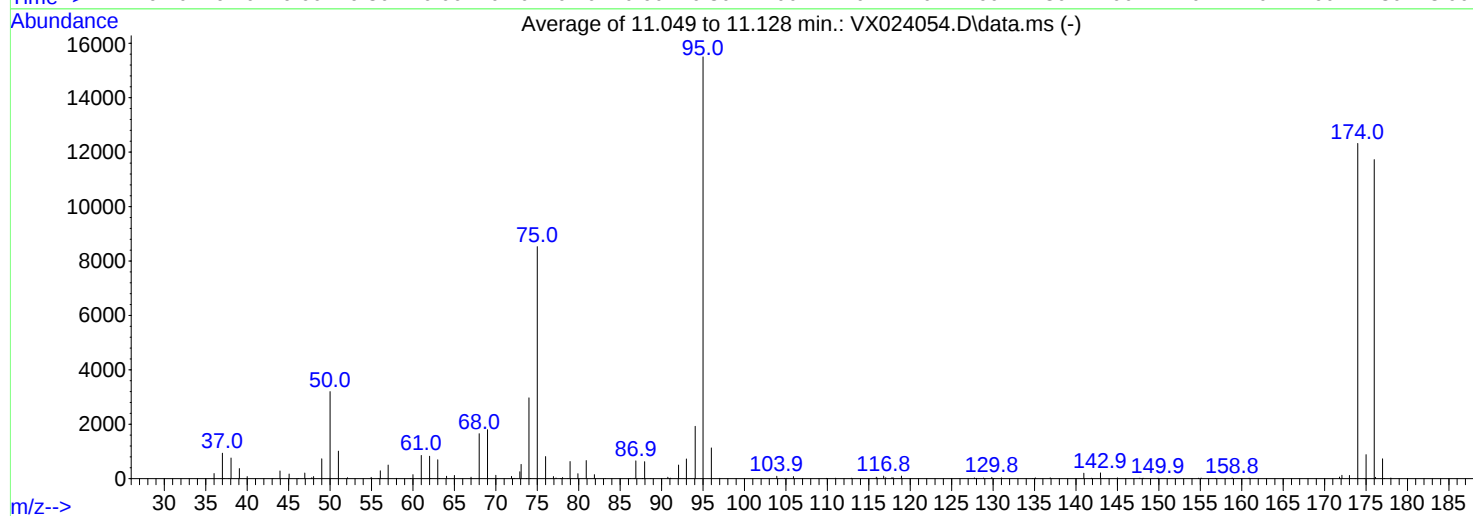


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090121\
 Data File : VX024054.D
 Acq On : 01 Sep 2021 08:26
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080321W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Aug 03 12:05:42 2021

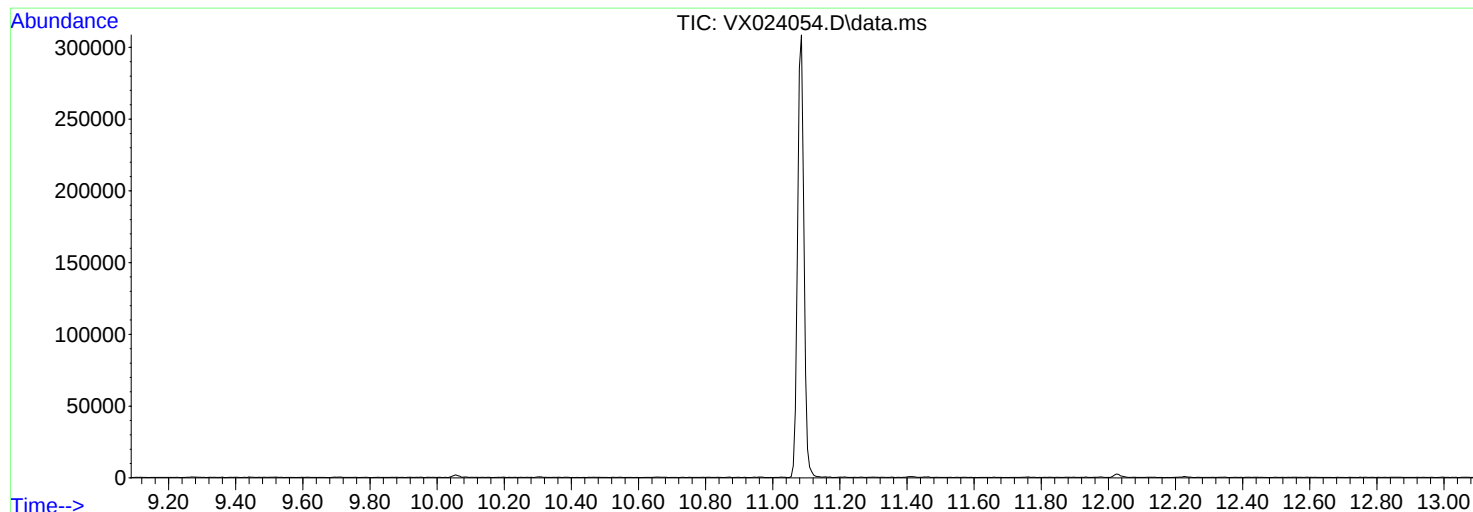

AutoFind: Averaged scan 1634 to 1647; Bkg corrected with scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	3198	PASS
75	95	30	60	55.0	8525	PASS
95	95	100	100	100.0	15503	PASS
96	95	5	9	7.3	1130	PASS
173	174	0.00	2	1.0	118	PASS
174	95	50	100	79.5	12320	PASS
175	174	5	9	7.2	881	PASS
176	174	95	101	95.2	11724	PASS
177	176	5	9	6.2	730	PASS