


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090122\
Data File : VX031027.D
Acq On : 01 Sep 2022 17:14
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Title : SW846 8260
Last Update : Fri Sep 02 02:49:21 2022

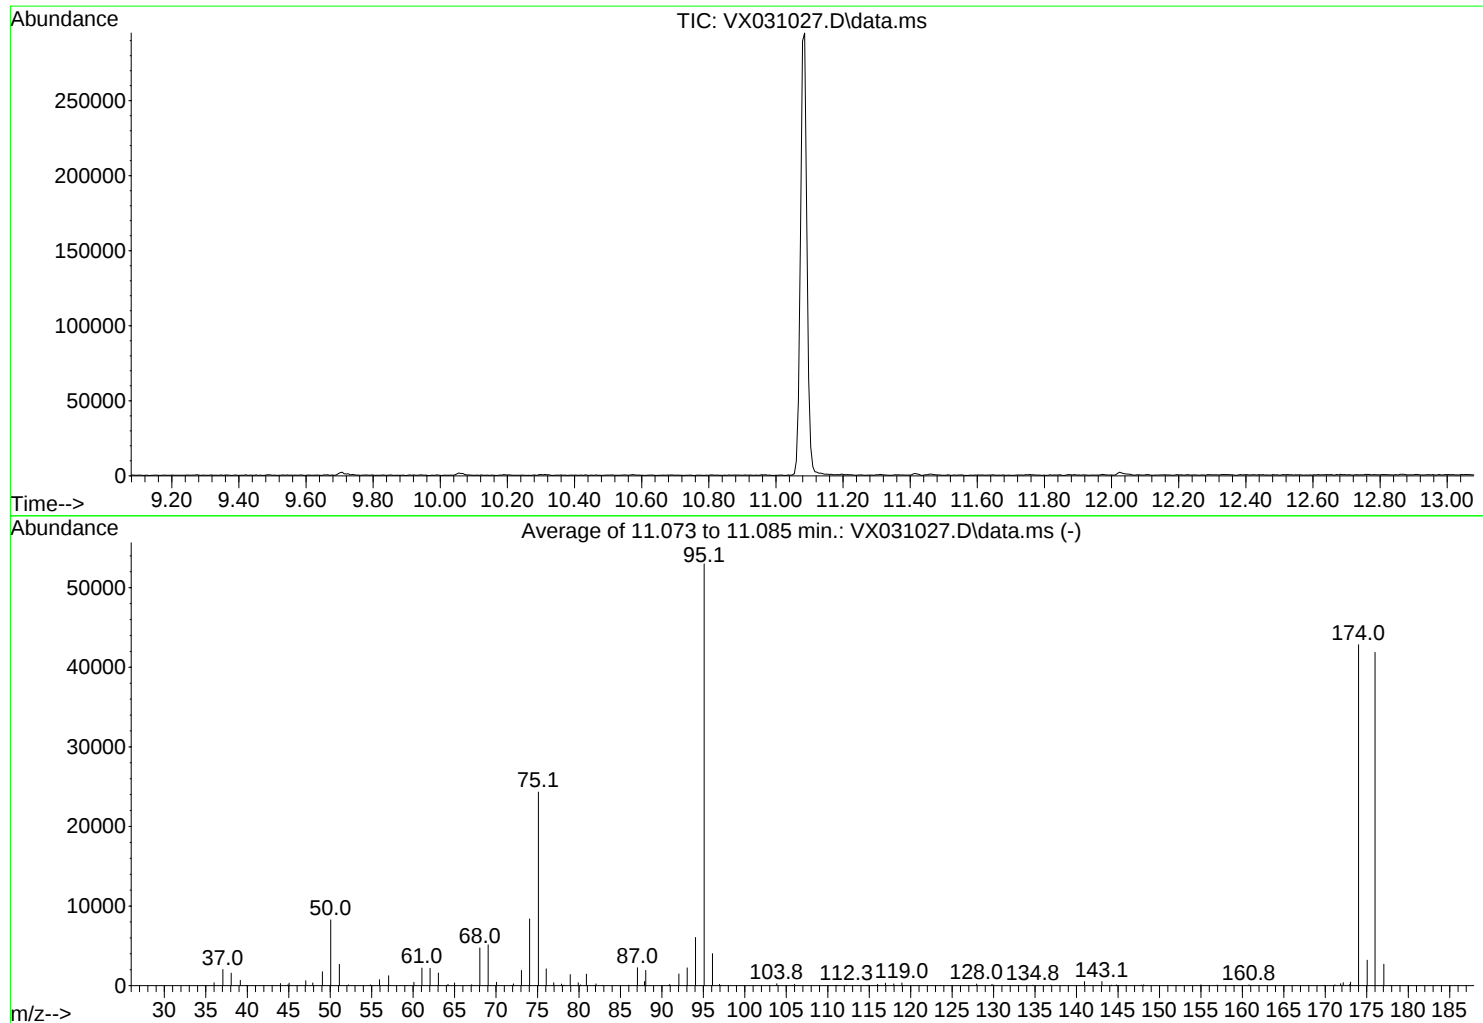

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	8254	PASS
75	95	30	60	45.9	24333	PASS
95	95	100	100	100.0	52989	PASS
96	95	5	9	7.6	4029	PASS
173	174	0.00	2	1.0	434	PASS
174	95	50	100	80.8	42829	PASS
175	174	5	9	7.5	3202	PASS
176	174	95	101	97.8	41875	PASS
177	176	5	9	6.4	2690	PASS