

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090123\
 Data File : VX037460.D
 Acq On : 01 Sep 2023 13:21
 Operator : JC/MD
 Sample : 04189-01
 Misc : 0.90g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-02(22-23)

Quant Time: Sep 01 13:55:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 18 09:30:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	175707	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	285438	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	242368	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	109527	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	99067	39.109	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	78.220%		
35) Dibromofluoromethane	5.385	113	76554	40.496	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	81.000%		
50) Toluene-d8	8.647	98	329172	48.004	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	96.000%		
62) 4-Bromofluorobenzene	11.085	95	115404	42.825	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	85.660%		
Target Compounds						
					Qvalue	
5) Bromomethane	1.618	94	228	0.235	ug/l #	77
9) 1,1,2-Trichlorotrifluo...	2.288	101	505	0.272	ug/l	95
11) Tert butyl alcohol	2.940	59	15915	26.783	ug/l #	81
13) Acrolein	2.245	56	122	0.270	ug/l #	1
16) Acetone	2.422	43	1505	1.519	ug/l #	83
20) Methylene Chloride	2.770	84	1508	0.680	ug/l #	77
29) Tetrahydrofuran	5.068	42	448	0.471	ug/l #	51
31) Cyclohexane	5.538	56	3185	1.118	ug/l #	1
36) 1,1-Dichloropropene	5.544	75	14031	5.224	ug/l #	50
38) Carbon Tetrachloride	5.538	117	18525	6.350	ug/l #	16
44) Trichloroethene	7.123	130	4467	2.045	ug/l	88
52) Toluene	8.714	92	1179	0.232	ug/l	88
59) 2-Hexanone	9.378	43	698	0.346	ug/l #	26
68) m/p-Xylenes	10.305	106	1359	0.390	ug/l	92
73) Isopropylbenzene	10.963	105	1826	0.229	ug/l	93
74) N-amyl acetate	10.854	43	1481	0.479	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.213	83	1230	0.459	ug/l #	26
76) 1,2,3-Trichloropropane	11.079	75	55528	23.806	ug/l #	39
78) n-propylbenzene	11.305	91	3927	0.443	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	55528	66.490	ug/l #	5
82) 4-Chlorotoluene	11.463	91	1352	0.207	ug/l	91
84) 1,2,4-Trimethylbenzene	11.756	105	1946	0.290	ug/l	98
85) sec-Butylbenzene	11.890	105	4028	0.544	ug/l	89
86) p-Isopropyltoluene	12.012	119	1741	0.273	ug/l #	72
87) 1,3-Dichlorobenzene	11.975	146	814	0.224	ug/l #	57
88) 1,4-Dichlorobenzene	12.043	146	818	0.218	ug/l #	1
89) n-Butylbenzene	12.335	91	3982	0.754	ug/l	89
93) 1,2,4-Trichlorobenzene	13.591	180	1334	0.640	ug/l #	73
94) Hexachlorobutadiene	13.719	225	327	0.406	ug/l	89
95) Naphthalene	13.780	128	31031	3.397	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090123\
Data File : VX037460.D
Acq On : 01 Sep 2023 13:21
Operator : JC/MD
Sample : 04189-01
Misc : 0.90g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)

Quant Time: Sep 01 13:55:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 18 09:30:38 2023
Response via : Initial Calibration




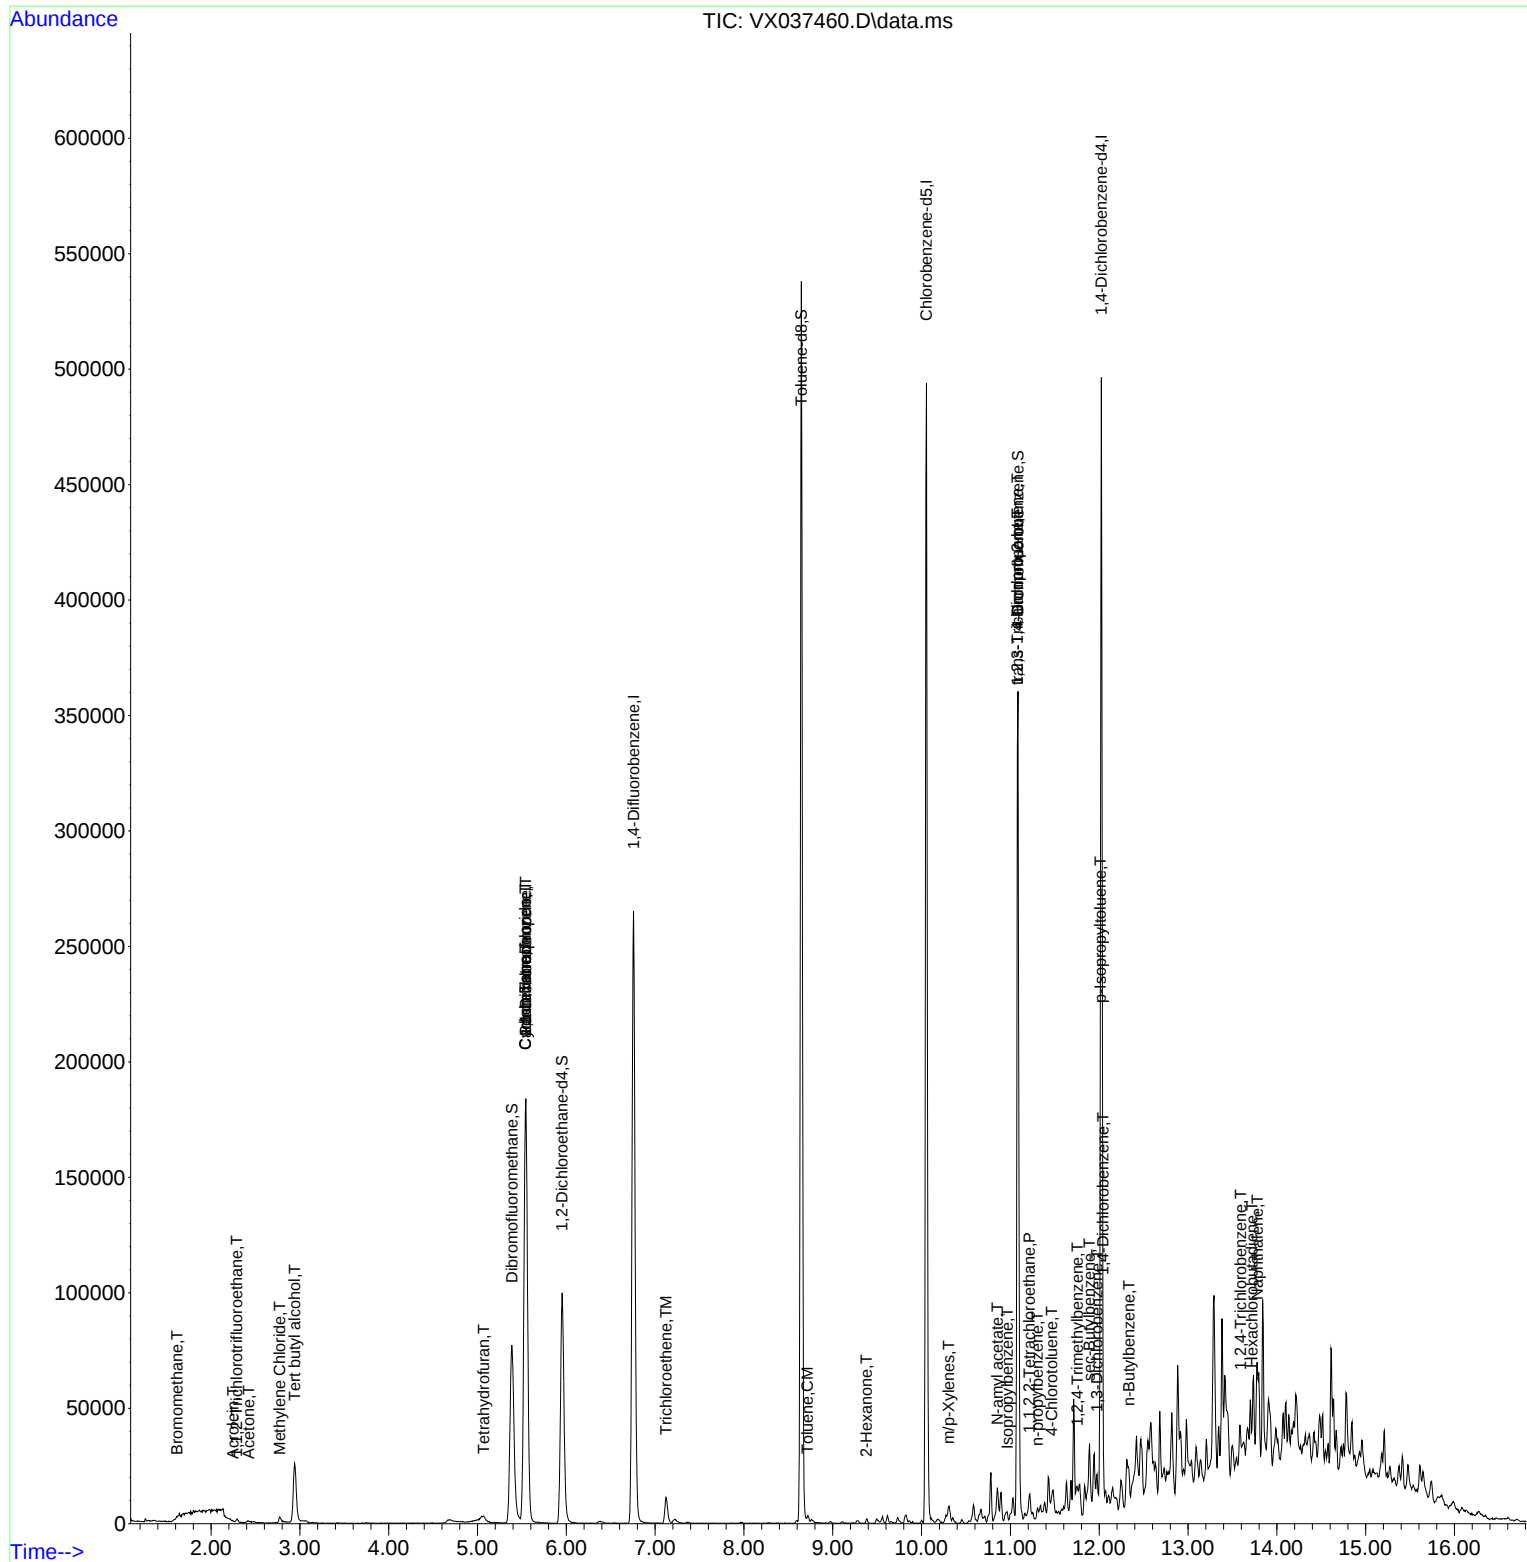


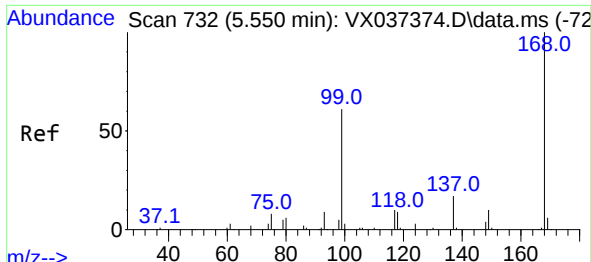

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21




Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)


Tgt Ion:168 Resp: 175707
Ion Ratio Lower Upper
168 100
99 59.6 56.6 85.0

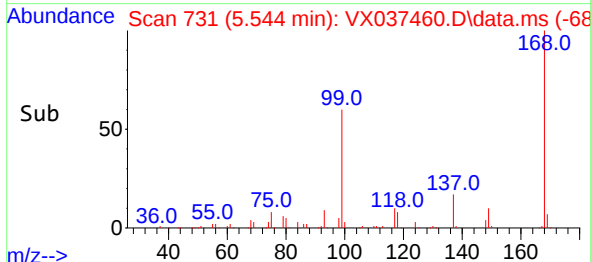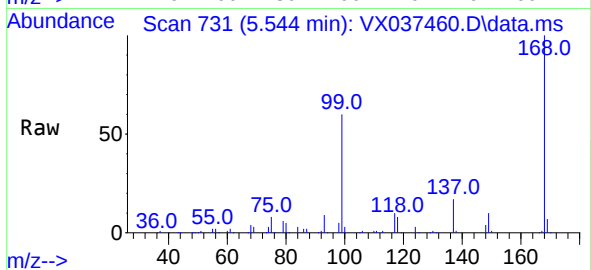

#5
Bromomethane
Concen: 0.235 ug/l
RT: 1.618 min Scan# 87
Delta R.T. 0.019 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Tgt Ion: 94 Resp: 228
Ion Ratio Lower Upper
94 100
96 70.8 74.6 111.8#


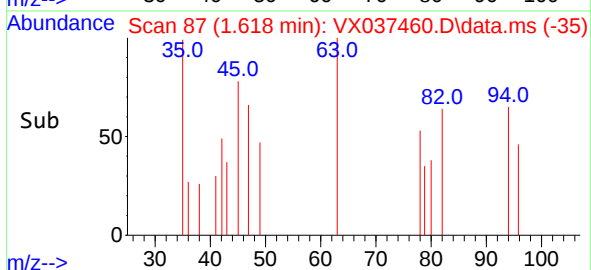






#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.272 ug/l
RT: 2.288 min Scan# 19
Delta R.T. -0.037 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21




Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)


Tgt Ion:101 Resp: 505
Ion Ratio Lower Upper
101 100
85 47.3 37.0 55.6
151 66.5 58.6 87.8

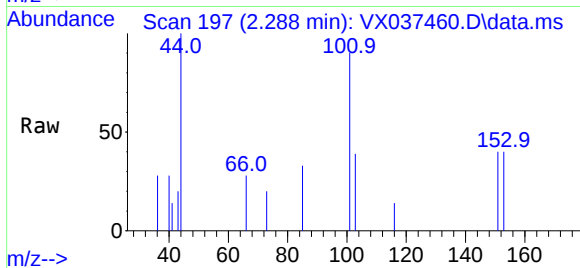

#11
Tert butyl alcohol
Concen: 26.783 ug/l
RT: 2.940 min Scan# 304
Delta R.T. -0.037 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Tgt Ion: 59 Resp: 15915
Ion Ratio Lower Upper
59 100
57 1.0 6.0 9.0#


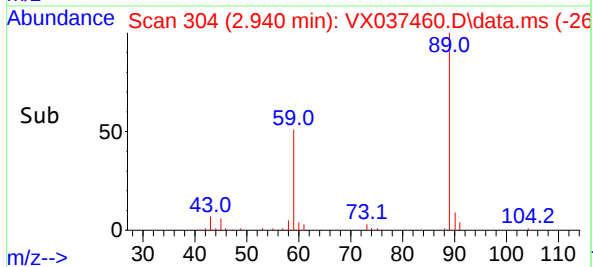

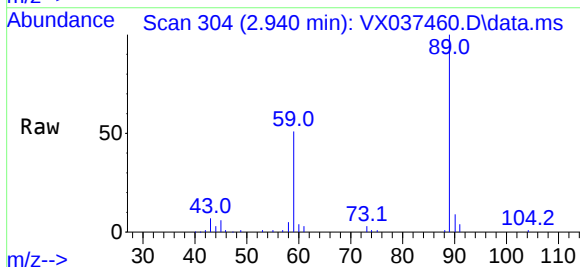




#13
Acrolein
Concen: 0.270 ug/l
RT: 2.245 min Scan# 190
Delta R.T. 0.006 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21




Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)


Tgt Ion: 56 Resp: 122
Ion Ratio Lower Upper
56 100
55 156.6 57.1 85.7#



#16
Acetone
Concen: 1.519 ug/l
RT: 2.422 min Scan# 219
Delta R.T. 0.037 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Tgt Ion: 43 Resp: 1505
Ion Ratio Lower Upper
43 100
58 36.2 21.9 32.9#

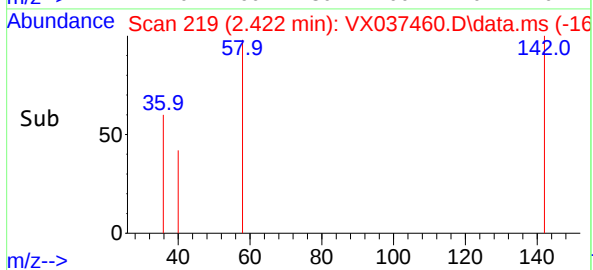



#20

Methylene Chloride

Concen: 0.680 ug/l

RT: 2.770 min Scan# 21

Delta R.T. -0.018 min

Lab File: VX037460.D

Acq: 01 Sep 2023 13:21

Instrument :

MSVOA_X

ClientSampleId :

SB-02(22-23)

Tgt Ion: 84 Resp: 1508





Ion Ratio Lower Upper

84 100

49 91.1 103.6 155.4#

51 31.7 33.8 50.6#

86 55.8 49.4 74.0

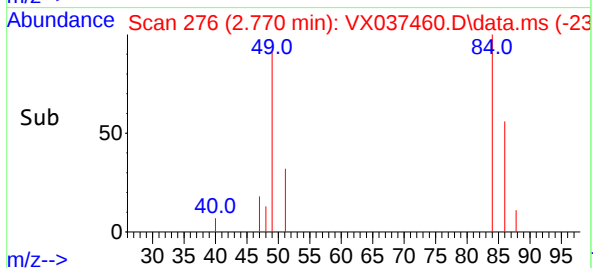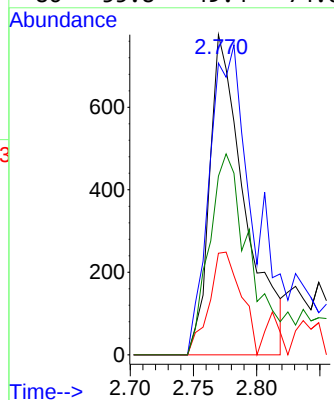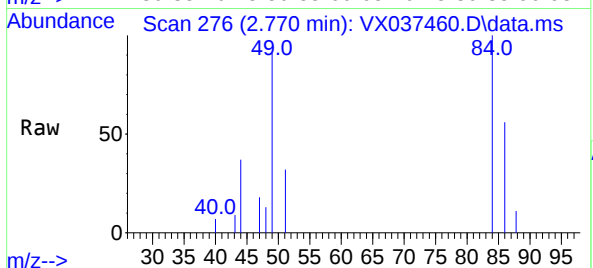

#29

Tetrahydrofuran

Concen: 0.471 ug/l

RT: 5.068 min Scan# 653

Delta R.T. 0.061 min

Lab File: VX037460.D

Acq: 01 Sep 2023 13:21




Tgt Ion: 42 Resp: 448


Ion Ratio Lower Upper

42 100

72 6.7 34.2 51.4#

71 15.4 32.2 48.2#


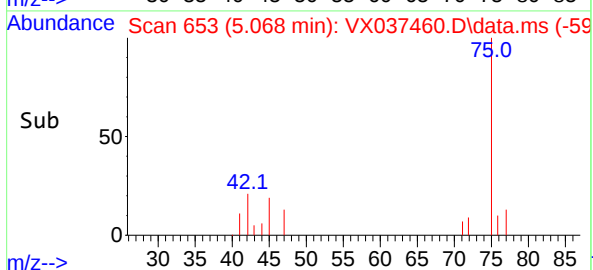
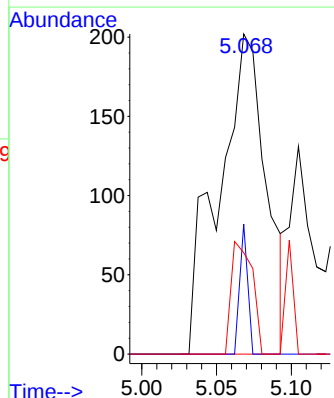





#31
Cyclohexane
Concen: 1.118 ug/l
RT: 5.538 min Scan# 719
Delta R.T. 0.067 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21




Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)


Tgt Ion: 56 Resp: 3185
Ion Ratio Lower Upper
56 100
69 192.4 23.4 35.2#
84 151.5 65.9 98.9#



#33
1,2-Dichloroethane-d4
Concen: 39.109 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Tgt Ion: 65 Resp: 99067
Ion Ratio Lower Upper
65 100
67 52.5 0.0 100.2

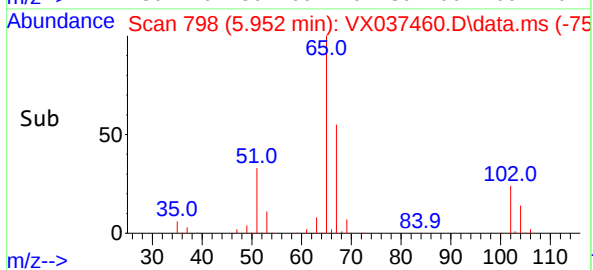



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 91

Delta R.T. -0.006 min

Lab File: VX037460.D

Acq: 01 Sep 2023 13:21

Instrument :

MSVOA_X

ClientSampleId :

SB-02(22-23)





Tgt Ion:114 Resp: 285438

Ion Ratio Lower Upper

114 100

63 19.3 0.0 45.0

88 16.6 0.0 36.6

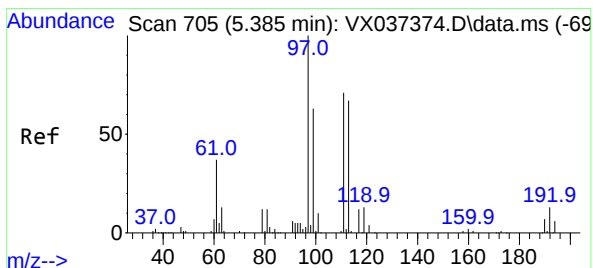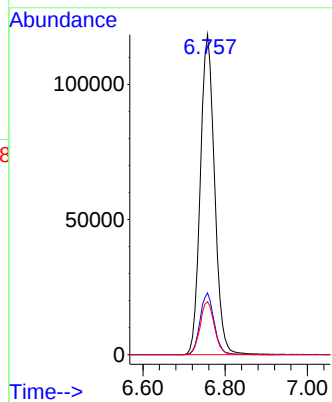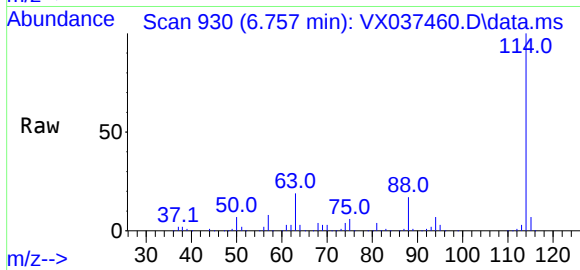

#35

Dibromofluoromethane

Concen: 40.496 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.000 min

Lab File: VX037460.D

Acq: 01 Sep 2023 13:21




Tgt Ion:113 Resp: 76554


Ion Ratio Lower Upper

113 100

111 101.2 82.9 124.3

192 18.9 13.3 19.9


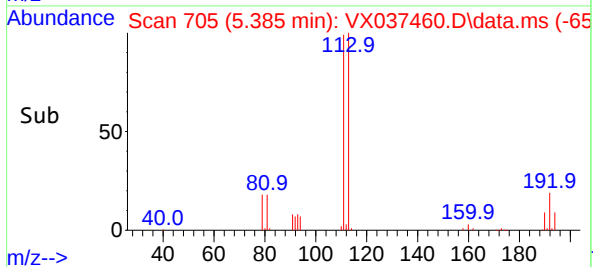

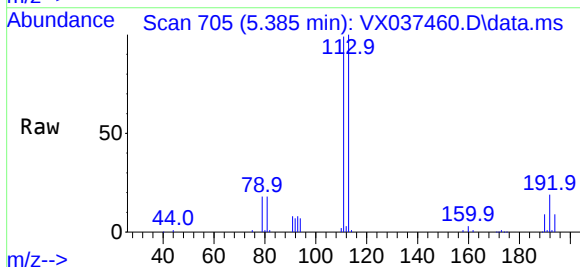


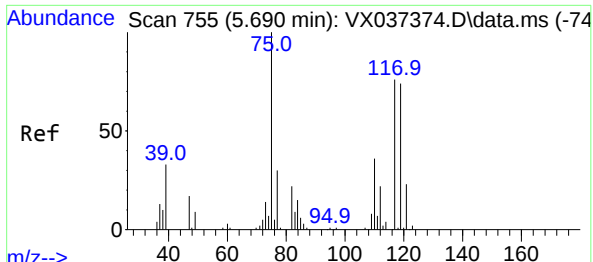

#36
1,1-Dichloropropene
Concen: 5.224 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.152 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21




Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)


Tgt Ion: 75 Resp: 14031
Ion Ratio Lower Upper
75 100
110 9.0 17.0 50.9#
77 0.0 24.7 37.1#

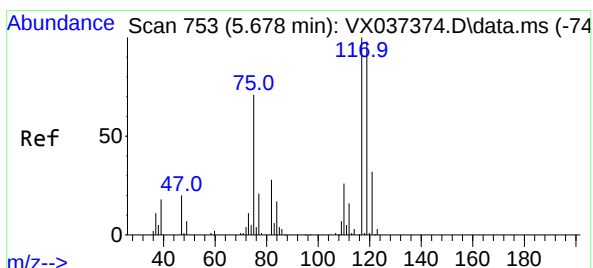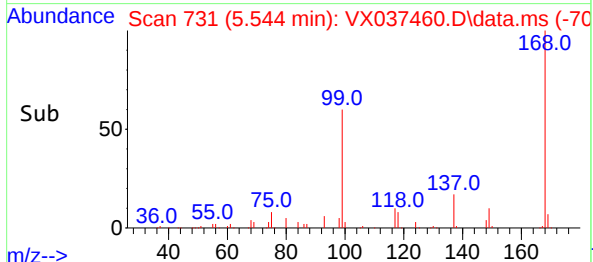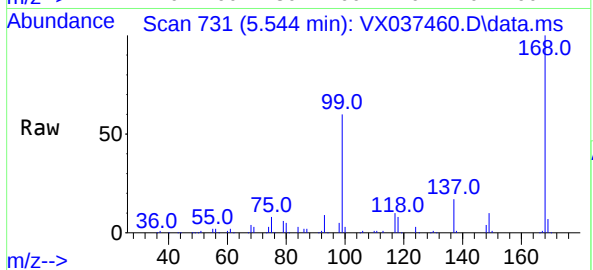

#38
Carbon Tetrachloride
Concen: 6.350 ug/l
RT: 5.538 min Scan# 730
Delta R.T. -0.134 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Tgt Ion: 117 Resp: 18525
Ion Ratio Lower Upper
117 100
119 5.5 78.2 117.2#
121 0.0 24.4 36.6#


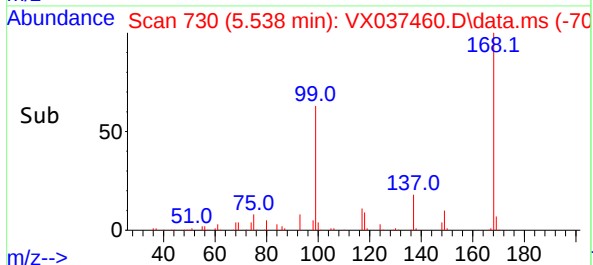

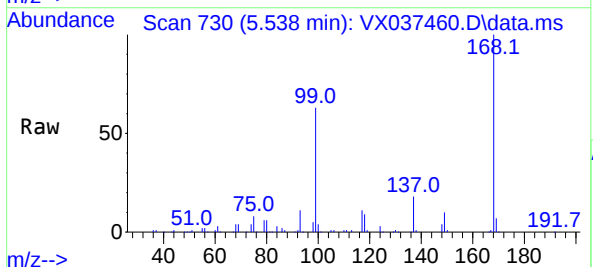




#44
Trichloroethene
Concen: 2.045 ug/l
RT: 7.123 min Scan# 991
Delta R.T. 0.000 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21




Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)


Tgt Ion:130 Resp: 4467
Ion Ratio Lower Upper
130 100
95 89.9 0.0 204.4



#50
Toluene-d8
Concen: 48.004 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Tgt Ion: 98 Resp: 329172
Ion Ratio Lower Upper
98 100
100 66.7 53.1 79.7

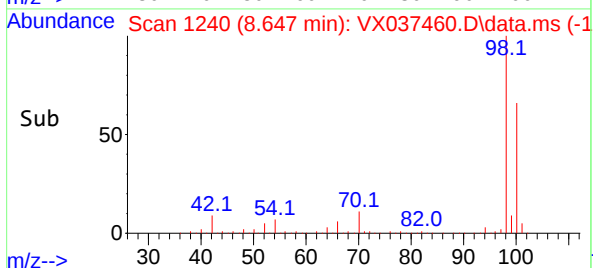



#52

Toluene

Concen: 0.232 ug/l

RT: 8.714 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX037460.D

Acq: 01 Sep 2023 13:21

Instrument :

MSVOA_X

ClientSampleId :





SB-02(22-23)

Tgt Ion: 92 Resp: 1179

Ion Ratio Lower Upper

92 100

91 184.1 134.2 201.2

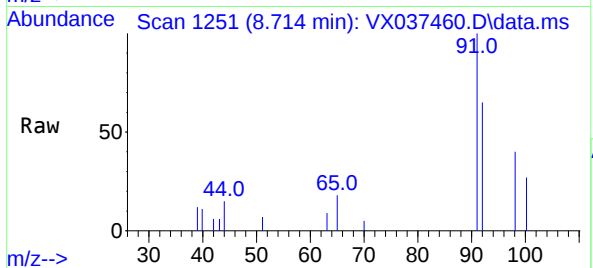

#59

2-Hexanone

Concen: 0.346 ug/l

RT: 9.378 min Scan# 1360

Delta R.T. -0.055 min

Lab File: VX037460.D




Acq: 01 Sep 2023 13:21


Tgt Ion: 43 Resp: 698

Ion Ratio Lower Upper

43 100

58 0.0 26.2 78.5#


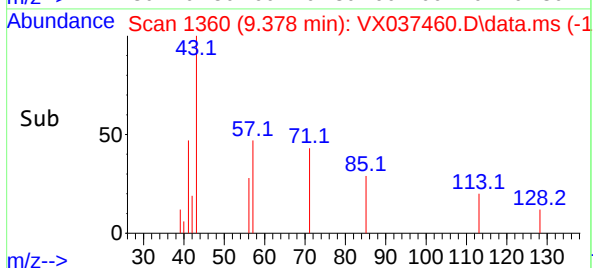
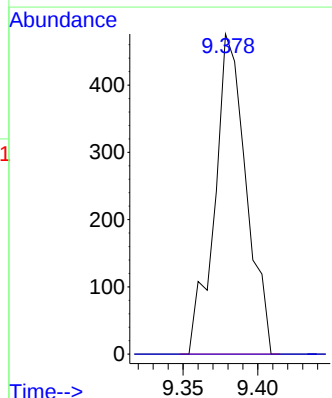





#62
4-Bromofluorobenzene
Concen: 42.825 ug/l
RT: 11.085 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21




Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)


Tgt Ion: 95 Resp: 115404
Ion Ratio Lower Upper
95 100
174 74.1 0.0 135.6
176 70.9 0.0 131.0

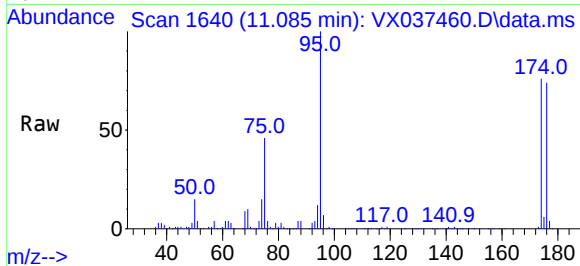

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Tgt Ion: 117 Resp: 242368
Ion Ratio Lower Upper
117 100
82 53.8 46.2 69.4
119 32.1 25.5 38.3


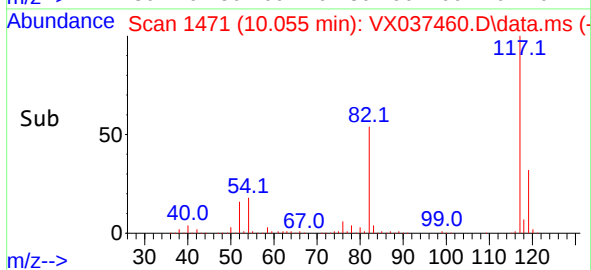

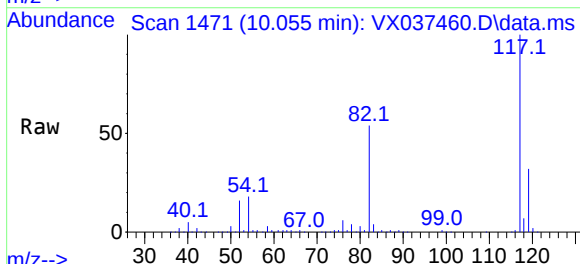




#68
m/p-Xylenes
Concen: 0.390 ug/l
RT: 10.305 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21




Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)


Tgt Ion:106 Resp: 1359
Ion Ratio Lower Upper
106 100
91 218.5 165.5 248.3

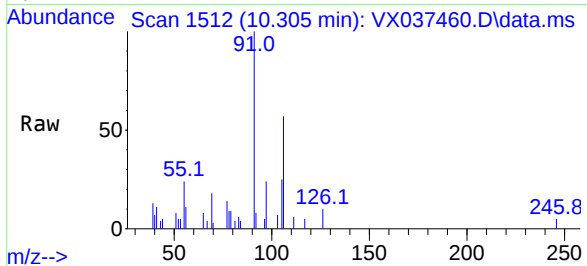

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Tgt Ion:152 Resp: 109527
Ion Ratio Lower Upper
152 100
115 63.0 43.3 129.9
150 159.2 0.0 345.0


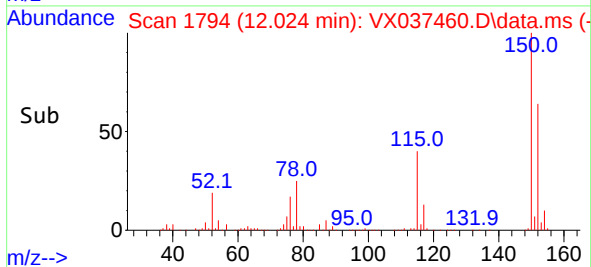

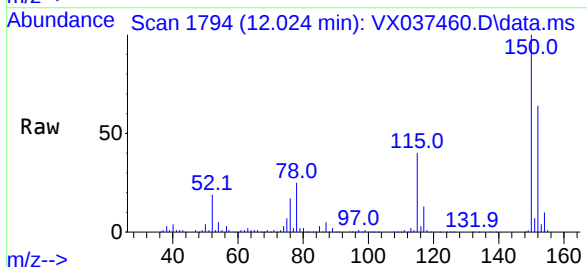




#73
Isopropylbenzene
Concen: 0.229 ug/l
RT: 10.963 min Scan# 110
Delta R.T. 0.000 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21




Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)


Tgt Ion:105 Resp: 1826
Ion Ratio Lower Upper
105 100
120 29.0 12.9 38.6

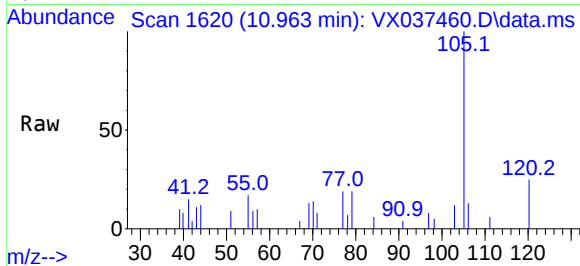

#74
N-ethyl acetate
Concen: 0.479 ug/l
RT: 10.854 min Scan# 1602
Delta R.T. 0.012 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Tgt Ion: 43 Resp: 1481
Ion Ratio Lower Upper
43 100
70 86.2 32.9 49.3#
55 201.3 19.3 28.9#
61 0.0 18.8 28.2#


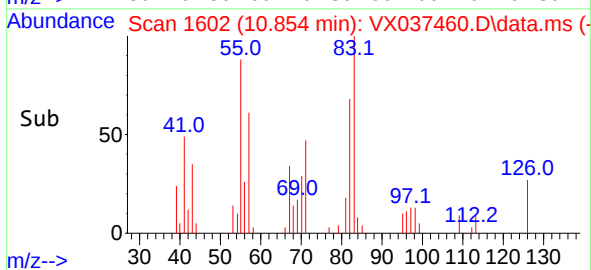

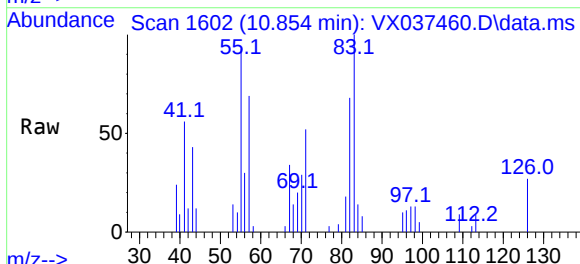




#75
1,1,2,2-Tetrachloroethane
Concen: 0.459 ug/l
RT: 11.213 min Scan# 1661
Delta R.T. 0.000 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21




Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)


Tgt Ion: 83 Resp: 1230
Ion Ratio Lower Upper
83 100
131 0.0 5.3 15.8#
85 0.0 32.0 96.2#

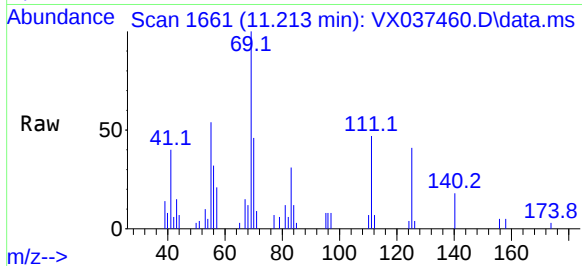

#76
1,2,3-Trichloropropane
Concen: 23.806 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Tgt Ion: 75 Resp: 55528
Ion Ratio Lower Upper
75 100
77 1.3 19.1 57.5#


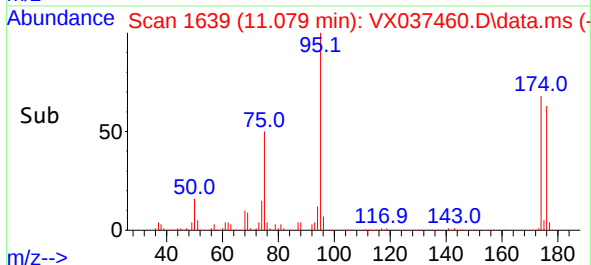

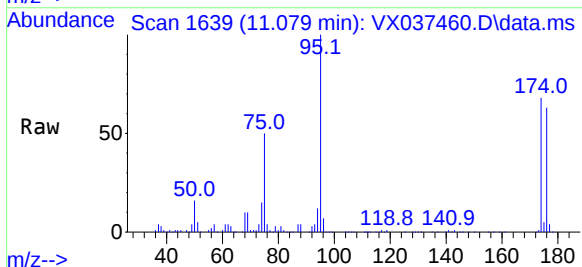




#78
n-propylbenzene
Concen: 0.443 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21




Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)


Tgt Ion: 91 Resp: 3927
Ion Ratio Lower Upper
91 100
120 21.8 11.5 34.4

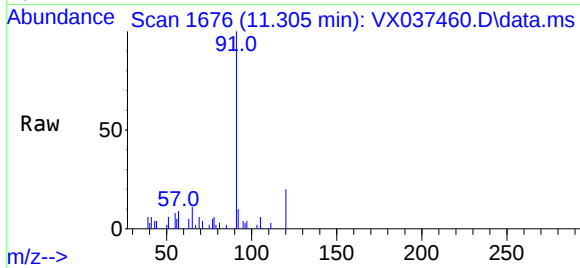

#81
trans-1,4-Dichloro-2-butene
Concen: 66.490 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Tgt Ion: 75 Resp: 55528
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 36.9 55.3#


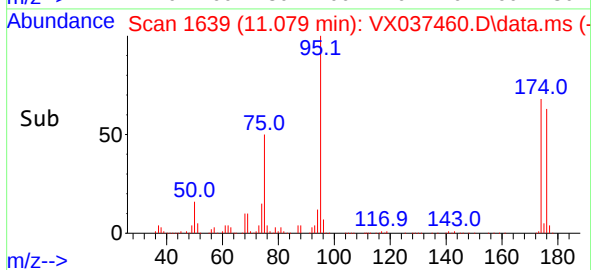

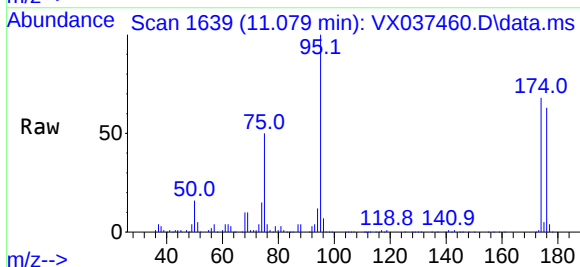




#82
4-Chlorotoluene
Concen: 0.207 ug/l
RT: 11.463 min Scan# 11
Delta R.T. 0.012 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21




Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)


Tgt Ion: 91 Resp: 1352
Ion Ratio Lower Upper
91 100
126 23.7 14.2 42.6

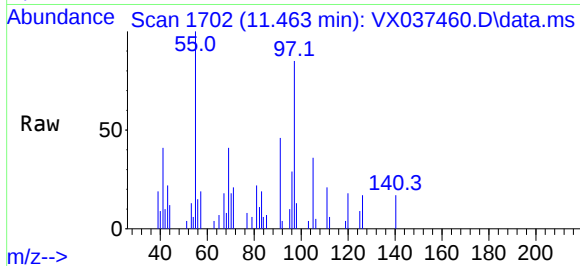

#84
1,2,4-Trimethylbenzene
Concen: 0.290 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Tgt Ion: 105 Resp: 1946
Ion Ratio Lower Upper
105 100
120 41.4 21.2 63.6


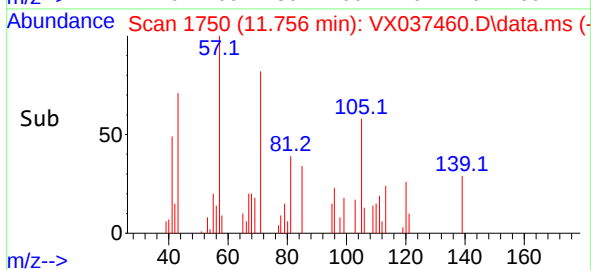

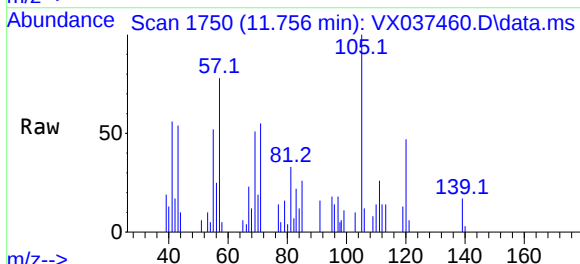




#85
 sec-Butylbenzene
 Concen: 0.544 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. 0.000 min
 Lab File: VX037460.D
 Acq: 01 Sep 2023 13:21




Instrument :
 MSVOA_X
 ClientSampleId :
 SB-02(22-23)


Tgt Ion:105 Resp: 4028
 Ion Ratio Lower Upper
 105 100
 134 24.6 9.8 29.4

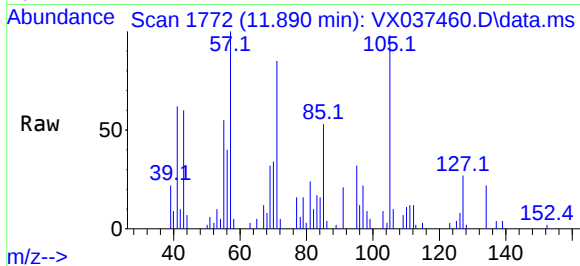

#86
 p-Isopropyltoluene
 Concen: 0.273 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. 0.006 min
 Lab File: VX037460.D
 Acq: 01 Sep 2023 13:21

Tgt Ion:119 Resp: 1741
 Ion Ratio Lower Upper
 119 100
 134 31.1 12.8 38.3
 91 49.0 13.1 39.3#


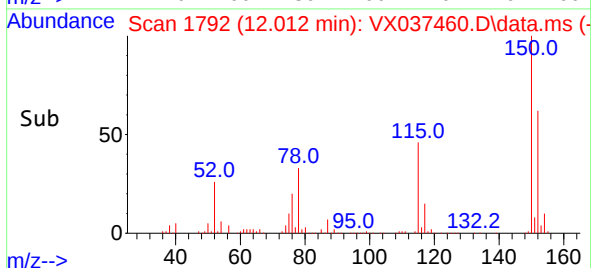
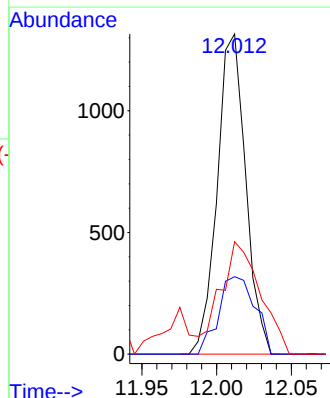
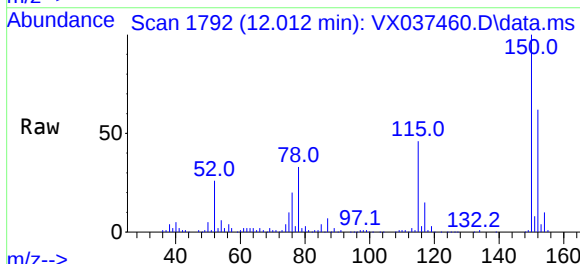




#87
1,3-Dichlorobenzene
Concen: 0.224 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. 0.006 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21




Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)


Tgt Ion:146 Resp: 814
Ion Ratio Lower Upper
146 100
111 106.4 22.1 66.1#
148 59.2 31.8 95.3

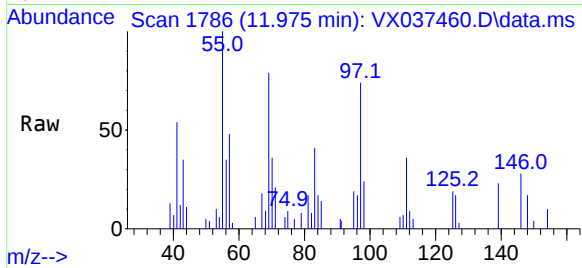

#88
1,4-Dichlorobenzene
Concen: 0.218 ug/l
RT: 12.043 min Scan# 1797
Delta R.T. 0.000 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Tgt Ion:146 Resp: 818
Ion Ratio Lower Upper
146 100
111 272.0 21.3 63.7#
148 98.3 31.8 95.4#

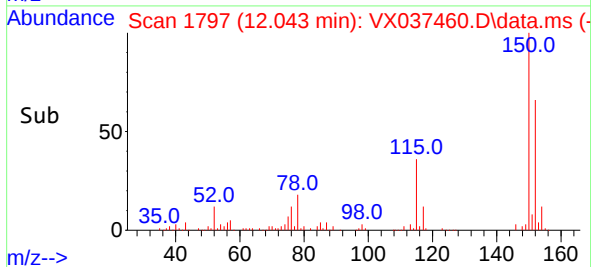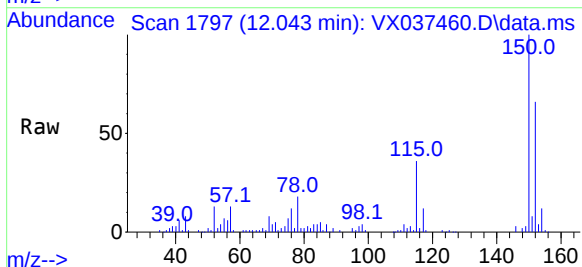



#89

n-Butylbenzene

Concen: 0.754 ug/l

RT: 12.335 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX037460.D

Acq: 01 Sep 2023 13:21

Instrument :

MSVOA_X

ClientSampleId :

SB-02(22-23)





Tgt Ion: 91 Resp: 3982

Ion Ratio Lower Upper

91 100

92 45.0 27.4 82.0

134 28.3 12.6 37.8

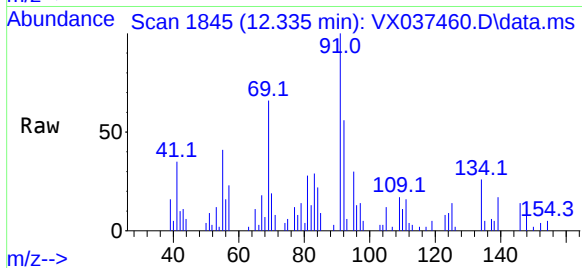

#93

1,2,4-Trichlorobenzene

Concen: 0.640 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. 0.006 min

Lab File: VX037460.D

Acq: 01 Sep 2023 13:21




Tgt Ion:180 Resp: 1334


Ion Ratio Lower Upper

180 100

182 91.8 48.3 144.8

145 86.0 18.0 54.0#


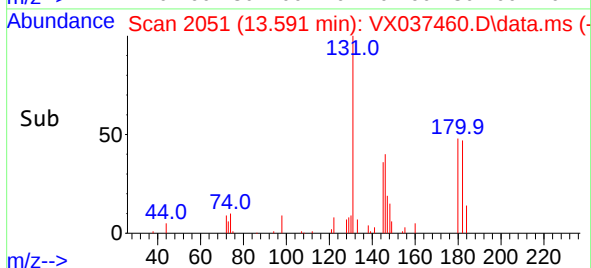
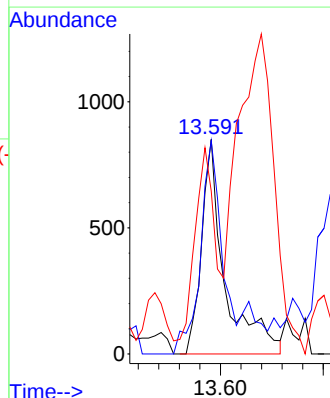
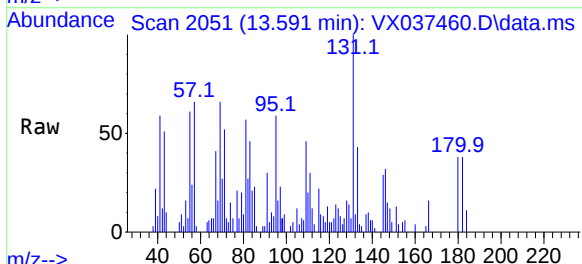




#94
Hexachlorobutadiene
Concen: 0.406 ug/l
RT: 13.719 min Scan# 2072
Delta R.T. -0.006 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Instrument :
MSVOA_X
ClientSampleId :
SB-02(22-23)

Tgt Ion:	225	Resp:	327
Ion	Ratio	Lower	Upper
225	100		
223	62.1	31.1	93.2
227	48.3	32.5	97.5

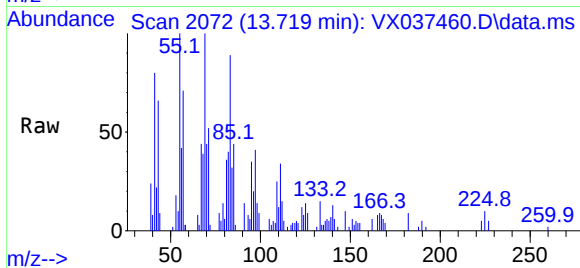

#95
Naphthalene
Concen: 3.397 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX037460.D
Acq: 01 Sep 2023 13:21

Tgt Ion:	128	Resp:	31031
Ion	Ratio	Lower	Upper
128	100		
127	14.2	10.3	15.5
129	12.0	8.8	13.2

