

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090123\
 Data File : VX037462.D
 Acq On : 01 Sep 2023 14:08
 Operator : JC/MD
 Sample : 04189-03 10X
 Misc : 4.91g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-07(14-15)

Quant Time: Sep 01 14:55:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 18 09:30:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	153175	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	253355	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	224978	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	107728	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	90584	41.020	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	82.040%		
35) Dibromofluoromethane	5.385	113	74873	44.623	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	89.240%		
50) Toluene-d8	8.647	98	295766	48.594	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	97.180%		
62) 4-Bromofluorobenzene	11.079	95	110432	46.170	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	92.340%		
Target Compounds						Qvalue
9) 1,1,2-Trichlorotrifluo...	2.319	101	485	0.300	ug/l #	80
11) Tert butyl alcohol	2.941	59	6953	13.422	ug/l #	78
16) Acetone	2.398	43	1218	1.410	ug/l #	73
20) Methylene Chloride	2.788	84	1154	0.597	ug/l	85
25) 2-Butanone	4.587	43	452	0.347	ug/l #	51
31) Cyclohexane	5.556	56	2937	1.183	ug/l #	1
36) 1,1-Dichloropropene	5.544	75	12069	5.063	ug/l #	51
38) Carbon Tetrachloride	5.550	117	16310	6.298	ug/l #	14
44) Trichloroethene	7.129	130	3784	1.952	ug/l	97
52) Toluene	8.720	92	9859	2.183	ug/l	98
67) Ethyl Benzene	10.195	91	30281	3.619	ug/l	100
68) m/p-Xylenes	10.299	106	83513	25.846	ug/l	99
69) o-Xylene	10.640	106	43802	13.740	ug/l	99
70) Styrene	10.647	104	4906	0.934	ug/l #	1
73) Isopropylbenzene	10.964	105	8088	1.033	ug/l	96
76) 1,2,3-Trichloropropane	11.079	75	54795	23.884	ug/l #	38
78) n-propylbenzene	11.305	91	15383	1.764	ug/l	99
79) 2-Chlorotoluene	11.616	91	3950	0.709	ug/l	83
80) 1,3,5-Trimethylbenzene	11.451	105	104510	16.000	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	54795	66.708	ug/l #	5
82) 4-Chlorotoluene	11.451	91	11239	1.747	ug/l #	49
83) tert-Butylbenzene	11.750	119	30841	4.951	ug/l #	62
84) 1,2,4-Trimethylbenzene	11.750	105	257007	38.933	ug/l	96
85) sec-Butylbenzene	11.750	105	257007	35.322	ug/l #	57
86) p-Isopropyltoluene	12.012	119	3151	0.503	ug/l #	64
89) n-Butylbenzene	12.323	91	6551	1.261	ug/l #	19
90) Hexachloroethane	12.603	117	5153	4.929	ug/l #	17
92) 1,2-Dibromo-3-Chloropr...	12.963	75	7860	12.828	ug/l #	9
93) 1,2,4-Trichlorobenzene	13.591	180	470	0.229	ug/l #	77
94) Hexachlorobutadiene	13.725	225	179	0.226	ug/l #	65
95) Naphthalene	13.780	128	8715048	969.858	ug/l #	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090123\
Data File : VX037462.D
Acq On : 01 Sep 2023 14:08
Operator : JC/MD
Sample : 04189-03 10X
Misc : 4.91g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)

Quant Time: Sep 01 14:55:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 18 09:30:38 2023
Response via : Initial Calibration




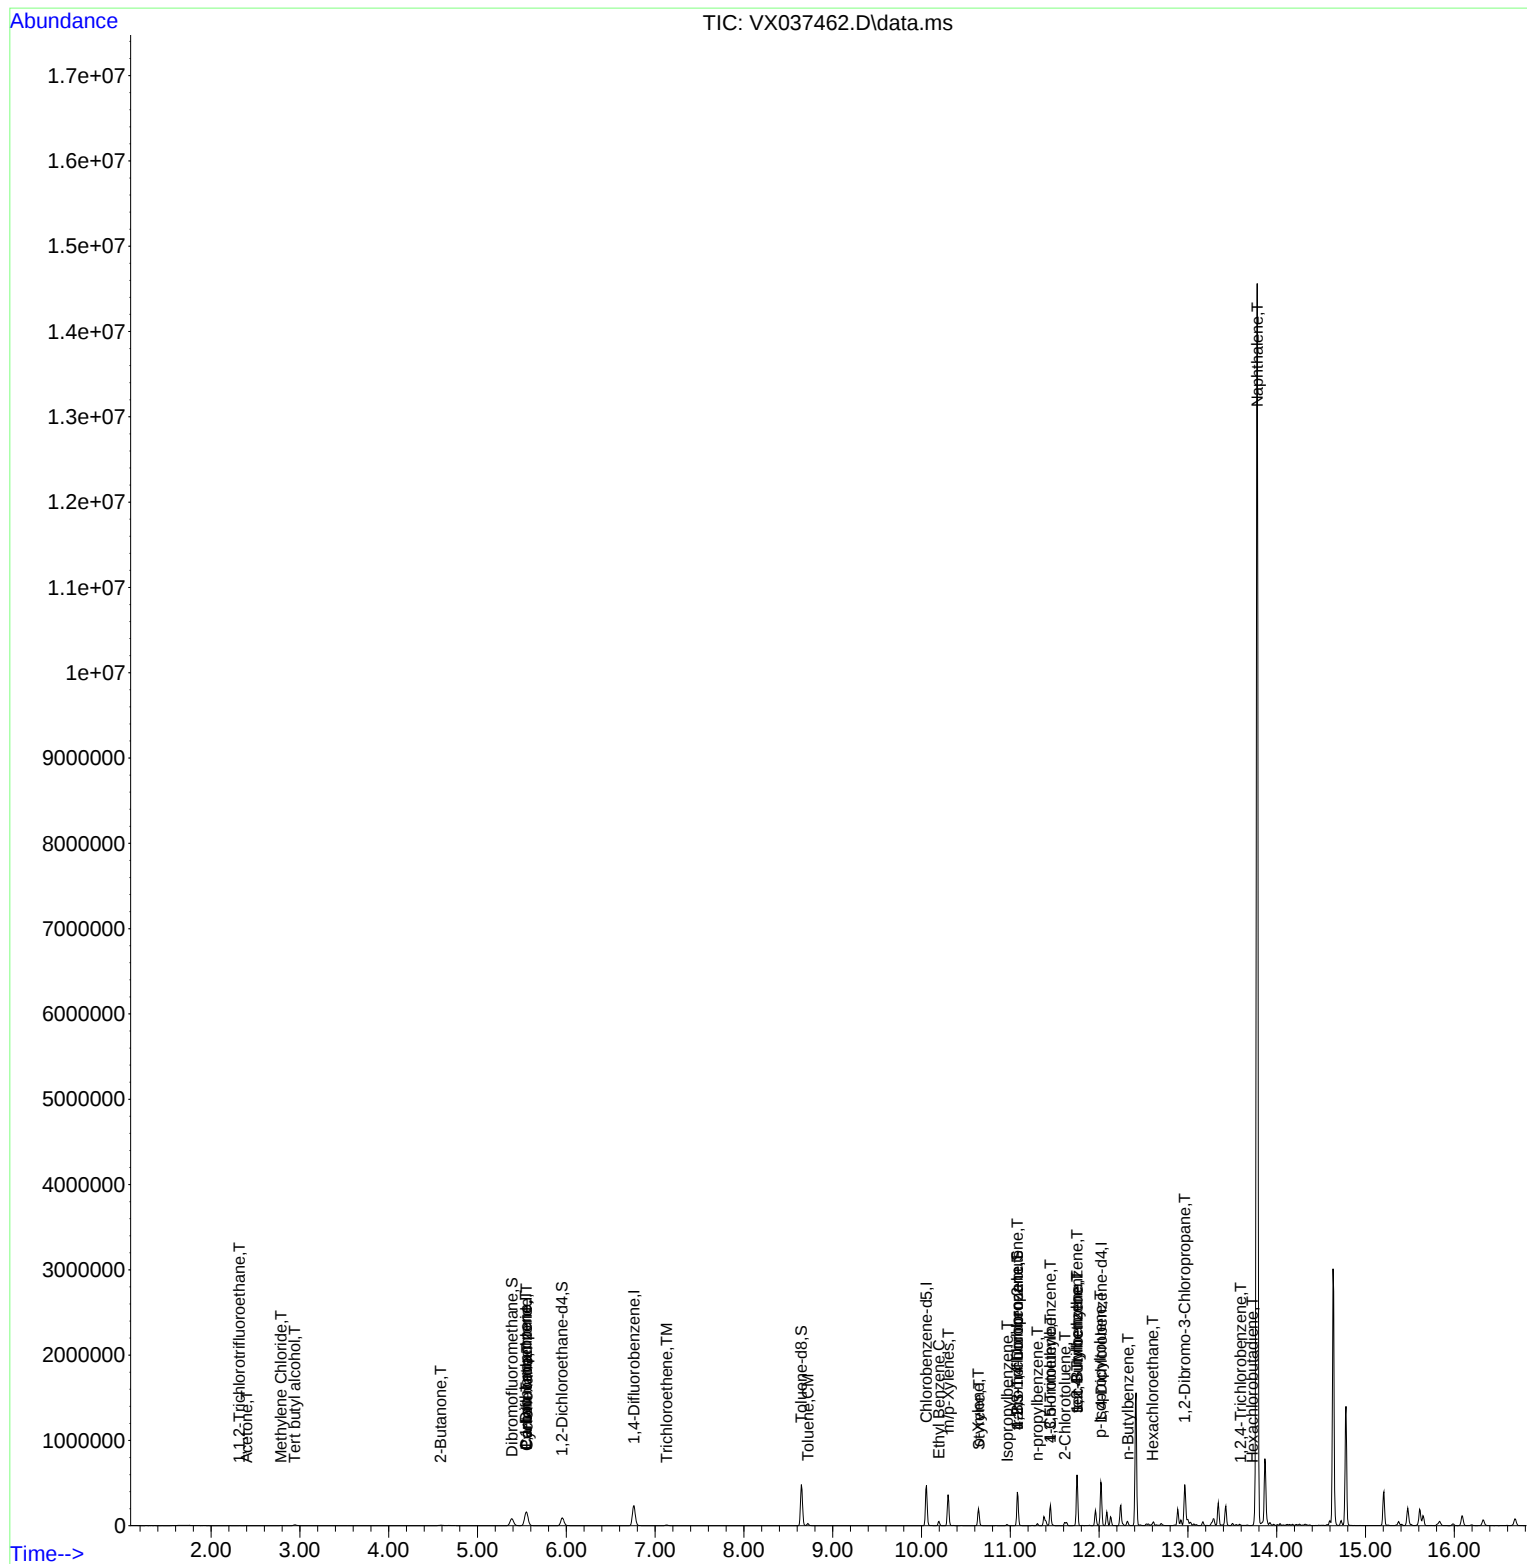


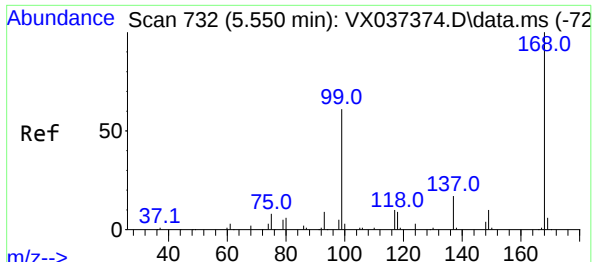

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion:168 Resp: 153175
Ion Ratio Lower Upper
168 100
99 62.0 56.6 85.0

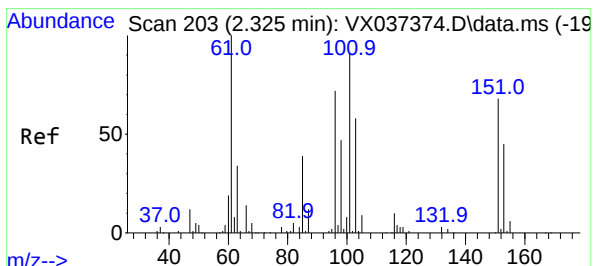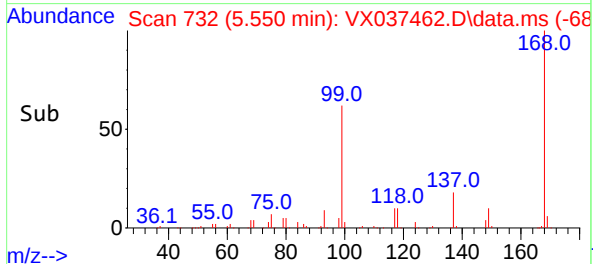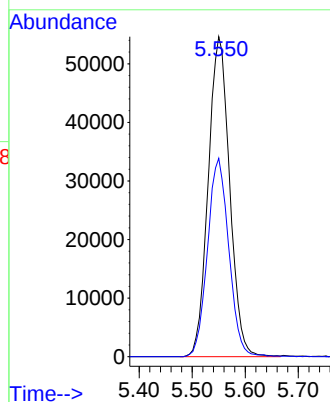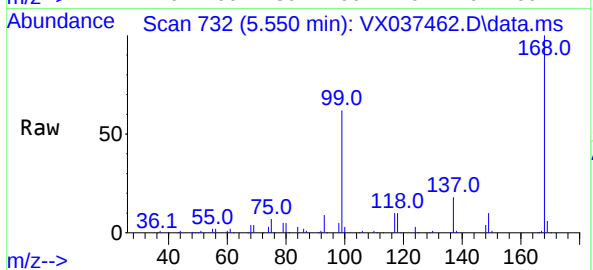

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.300 ug/l
RT: 2.319 min Scan# 202
Delta R.T. -0.006 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion:101 Resp: 485
Ion Ratio Lower Upper
101 100
85 23.1 37.0 55.6#
151 64.3 58.6 87.8

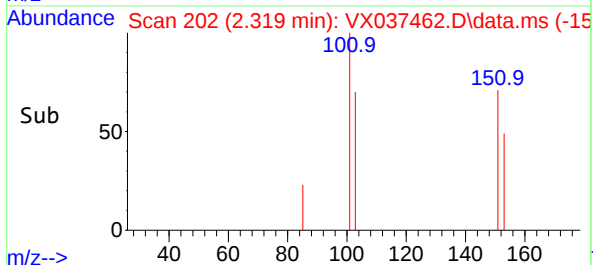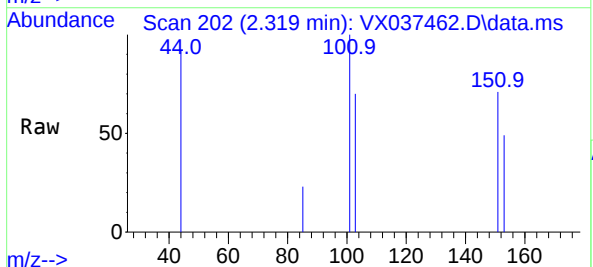

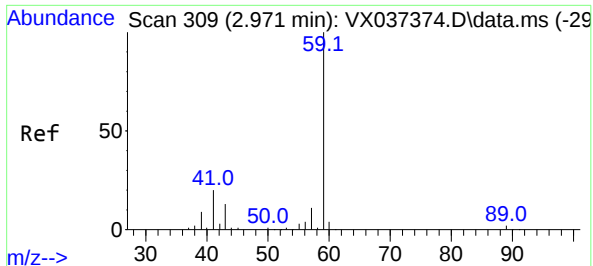

#11

Tert butyl alcohol

Concen: 13.422 ug/l

RT: 2.941 min Scan# 30

Delta R.T. -0.036 min

Lab File: VX037462.D

Acq: 01 Sep 2023 14:08

Instrument :

MSVOA_X

ClientSampleId :





SB-07(14-15)

Tgt Ion: 59 Resp: 6953

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#

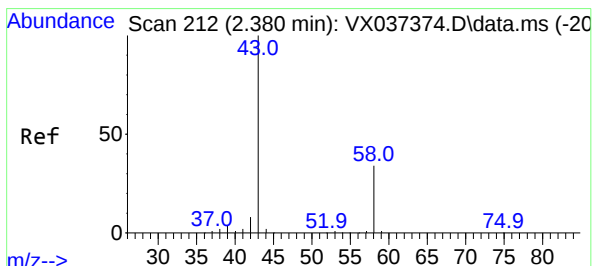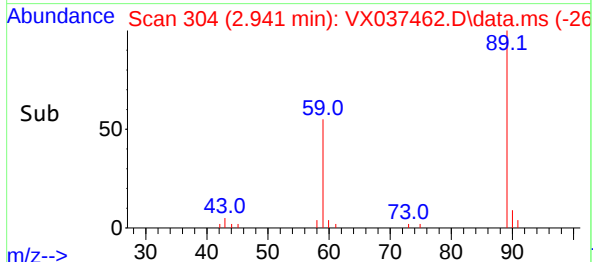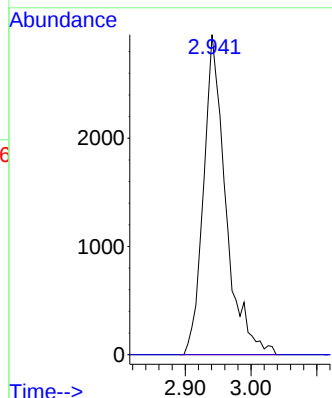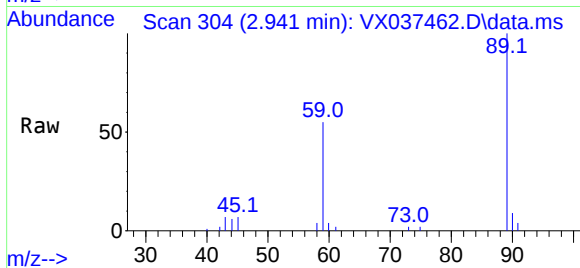

#16

Acetone

Concen: 1.410 ug/l

RT: 2.398 min Scan# 215

Delta R.T. 0.012 min

Lab File: VX037462.D




Acq: 01 Sep 2023 14:08


Tgt Ion: 43 Resp: 1218

Ion Ratio Lower Upper

43 100


58 41.3 21.9 32.9#

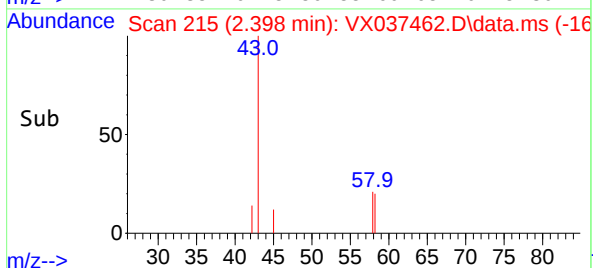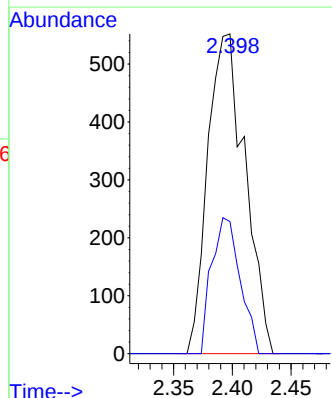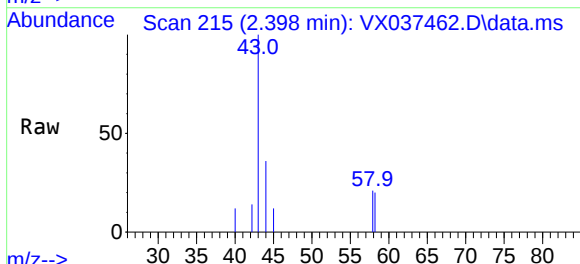





#20
Methylene Chloride
Concen: 0.597 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)

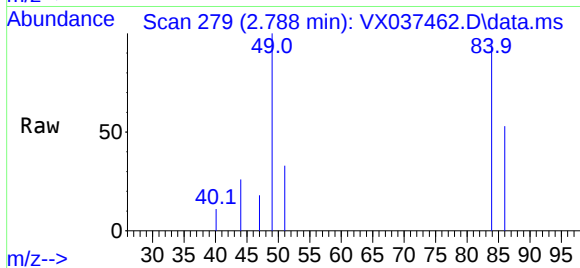

Tgt Ion: 84 Resp: 1154




Ion	Ratio	Lower	Upper
84	100		
49	106.4	103.6	155.4
51	35.0	33.8	50.6
86	56.6	49.4	74.0




#25
2-Butanone
Concen: 0.347 ug/l
RT: 4.587 min Scan# 574
Delta R.T. 0.031 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion: 43 Resp: 452

Ion	Ratio	Lower	Upper
43	100		
72	0.0	19.4	29.2#


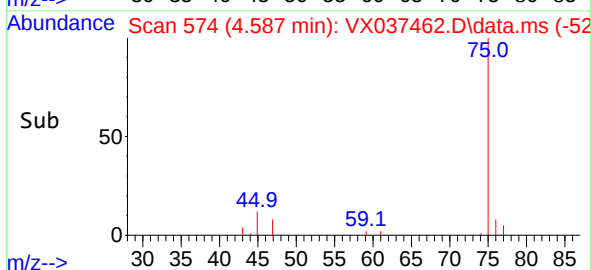
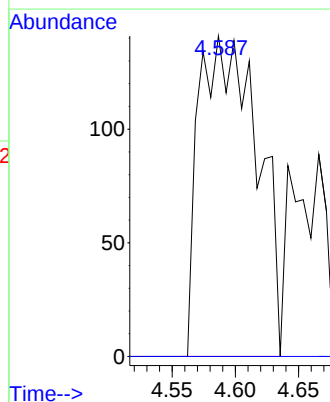
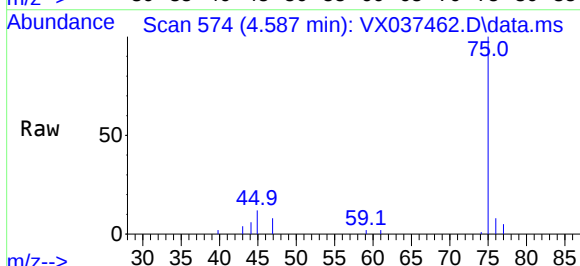


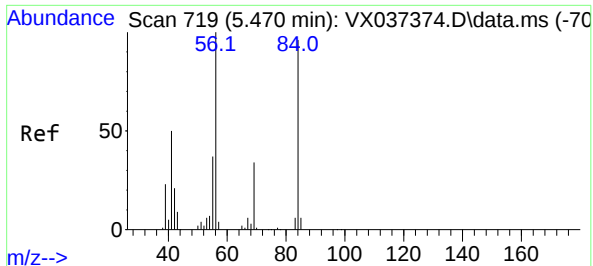

#31
Cyclohexane
Concen: 1.183 ug/l
RT: 5.556 min Scan# 719
Delta R.T. 0.086 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion: 56 Resp: 2937
Ion Ratio Lower Upper
56 100
69 157.6 23.4 35.2#
84 136.9 65.9 98.9#

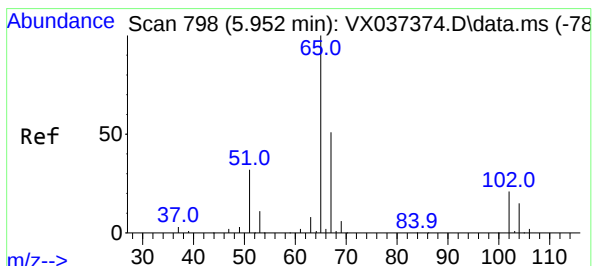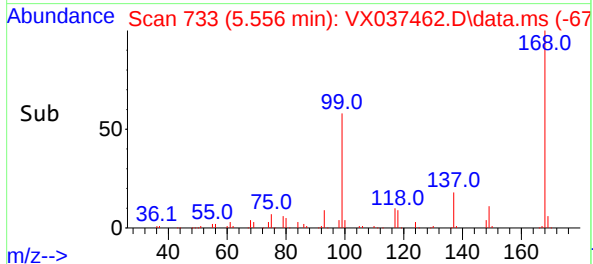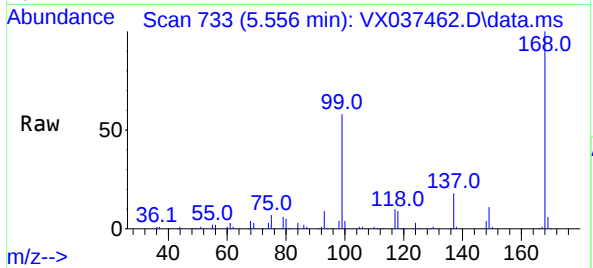

#33
1,2-Dichloroethane-d4
Concen: 41.020 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion: 65 Resp: 90584
Ion Ratio Lower Upper
65 100
67 52.6 0.0 100.2


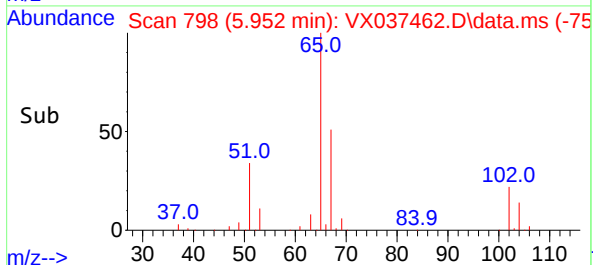
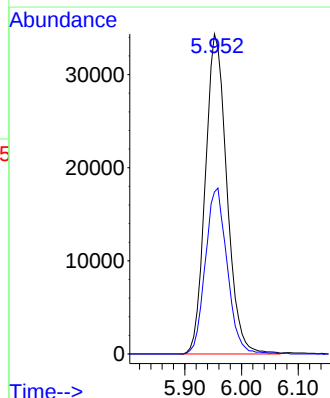
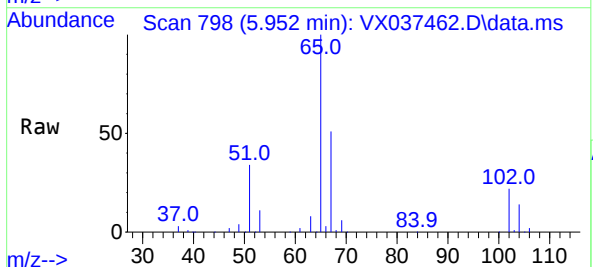


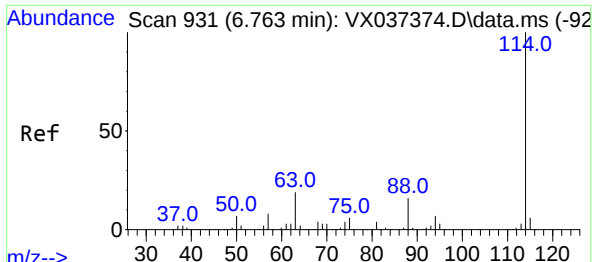

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion:114 Resp: 253355
Ion Ratio Lower Upper
114 100
63 18.2 0.0 45.0
88 16.3 0.0 36.6

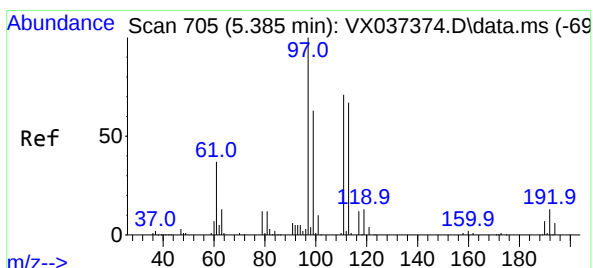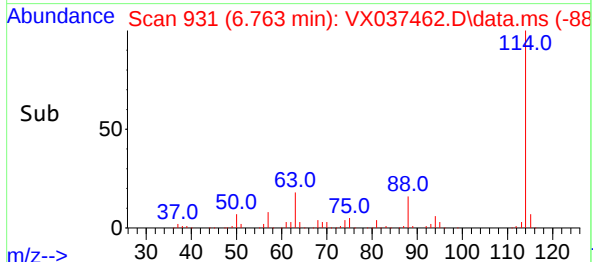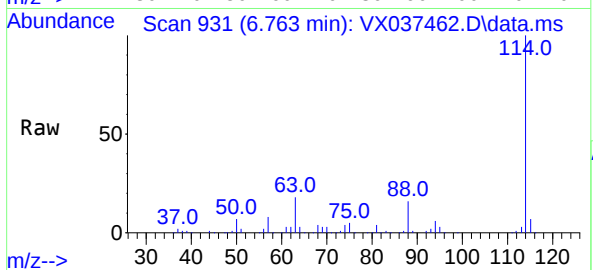

#35
Dibromofluoromethane
Concen: 44.623 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion:113 Resp: 74873
Ion Ratio Lower Upper
113 100
111 101.5 82.9 124.3
192 18.6 13.3 19.9


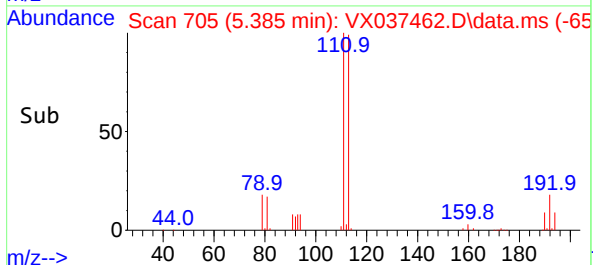

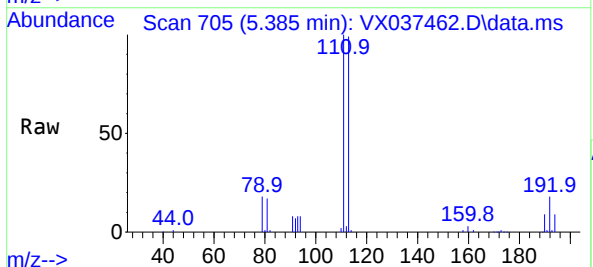


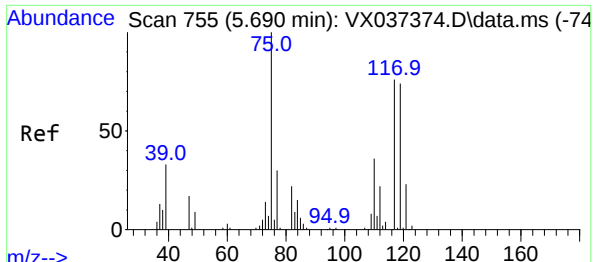

#36
1,1-Dichloropropene
Concen: 5.063 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.152 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion: 75 Resp: 12069
Ion Ratio Lower Upper
75 100
110 9.3 17.0 50.9#
77 0.0 24.7 37.1#

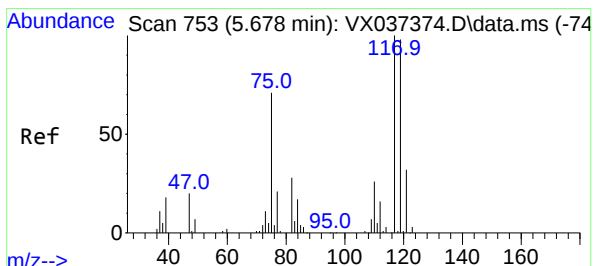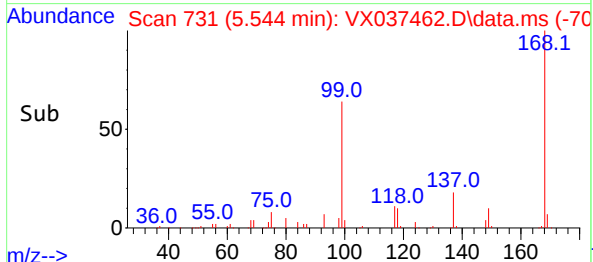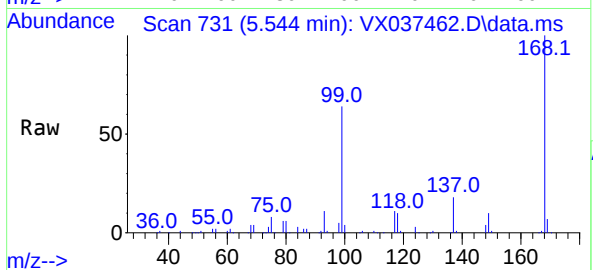

#38
Carbon Tetrachloride
Concen: 6.298 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.122 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion: 117 Resp: 16310
Ion Ratio Lower Upper
117 100
119 3.6 78.2 117.2#
121 0.0 24.4 36.6#


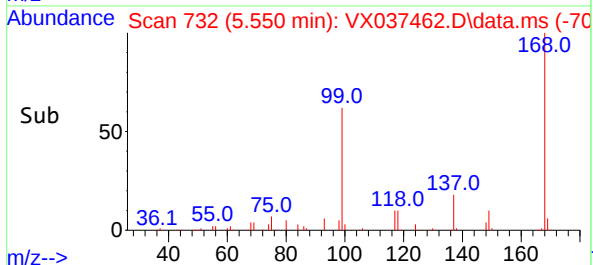

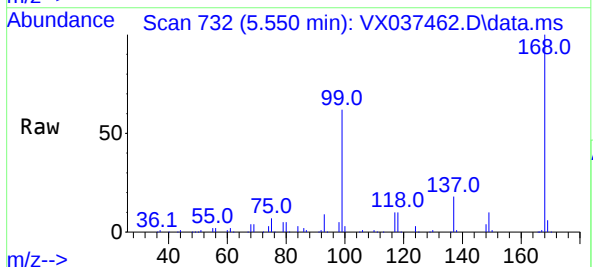


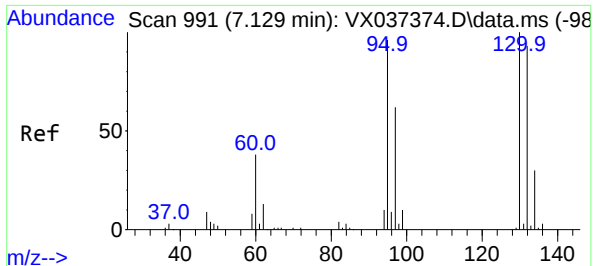

#44
 Trichloroethene
 Concen: 1.952 ug/l
 RT: 7.129 min Scan# 991
 Delta R.T. 0.006 min
 Lab File: VX037462.D
 Acq: 01 Sep 2023 14:08




Instrument :
 MSVOA_X
 ClientSampleId :
 SB-07(14-15)


Tgt Ion:130 Resp: 3784
 Ion Ratio Lower Upper
 130 100
 95 99.5 0.0 204.4

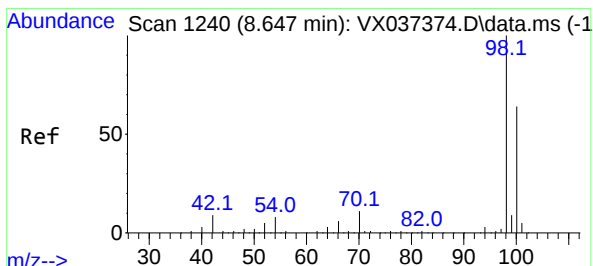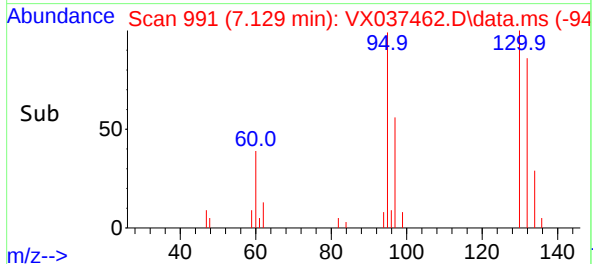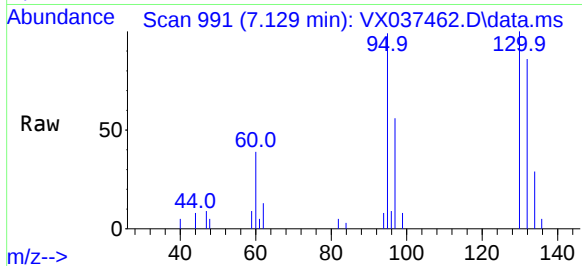

#50
 Toluene-d8
 Concen: 48.594 ug/l
 RT: 8.647 min Scan# 1240
 Delta R.T. 0.000 min
 Lab File: VX037462.D
 Acq: 01 Sep 2023 14:08

Tgt Ion: 98 Resp: 295766
 Ion Ratio Lower Upper
 98 100
 100 66.9 53.1 79.7


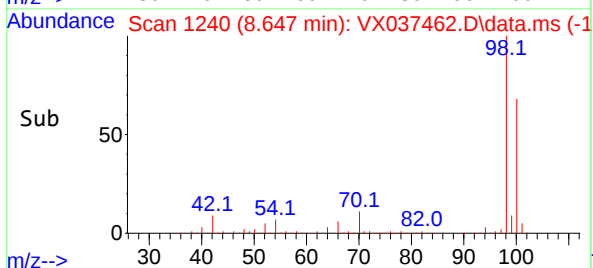
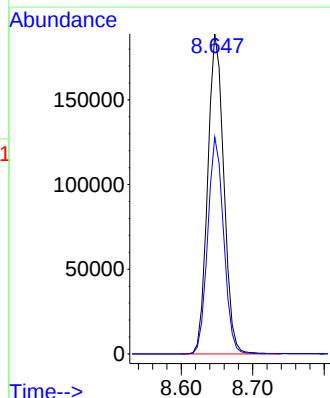
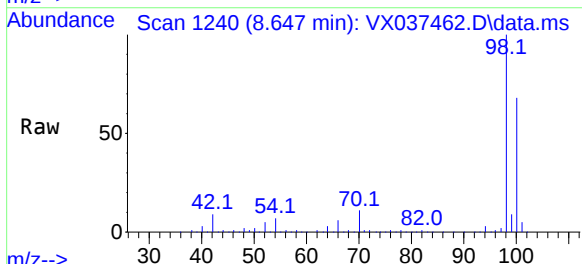


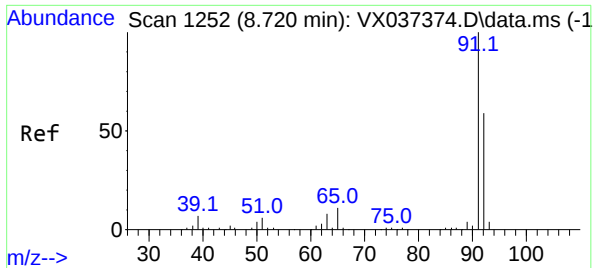

#52
Toluene
Concen: 2.183 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion: 92 Resp: 9859
Ion Ratio Lower Upper
92 100
91 170.0 134.2 201.2

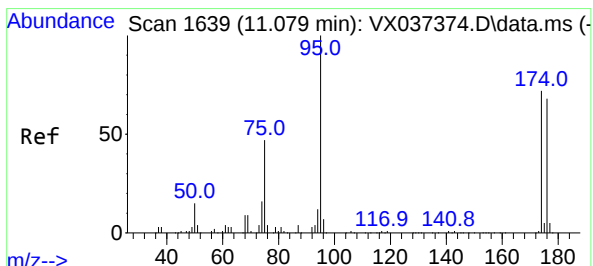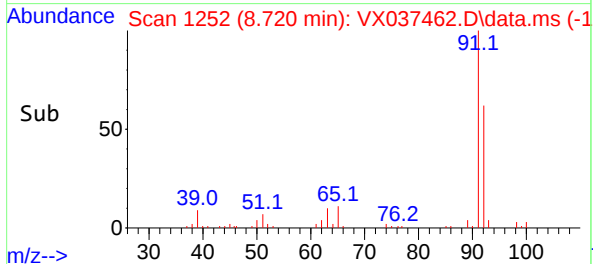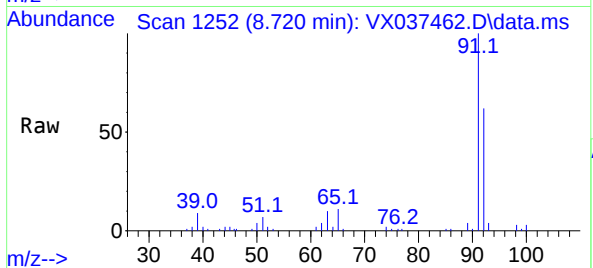

#62
4-Bromofluorobenzene
Concen: 46.170 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion: 95 Resp: 110432
Ion Ratio Lower Upper
95 100
174 74.5 0.0 135.6
176 71.1 0.0 131.0


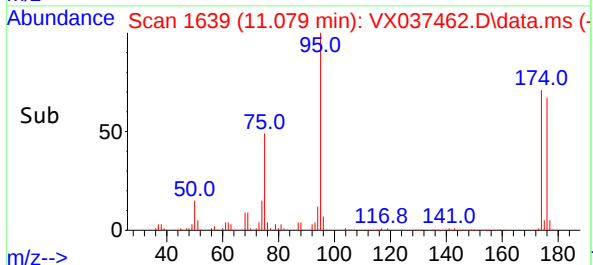
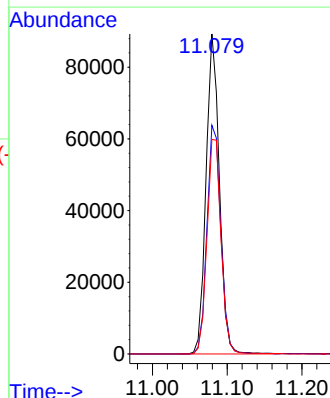
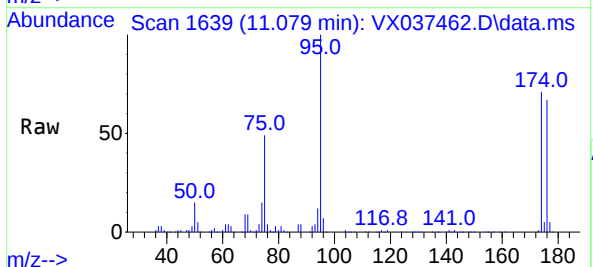




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion:117 Resp: 224978
Ion Ratio Lower Upper
117 100
82 54.2 46.2 69.4
119 32.6 25.5 38.3

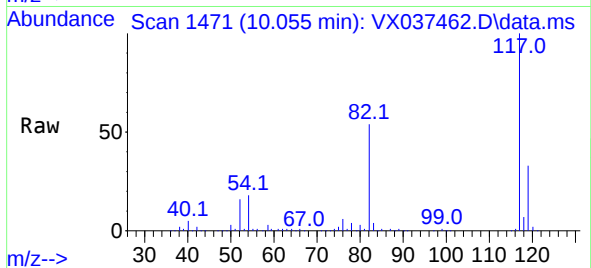

#67
Ethyl Benzene
Concen: 3.619 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion: 91 Resp: 30281
Ion Ratio Lower Upper
91 100
106 31.0 24.9 37.3


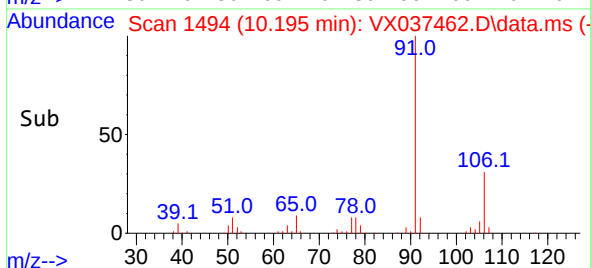
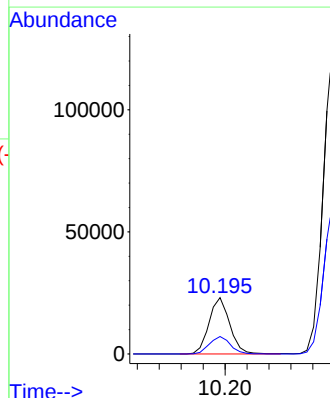





#68
m/p-Xylenes
Concen: 25.846 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion:106 Resp: 83513
Ion Ratio Lower Upper
106 100
91 204.8 165.5 248.3

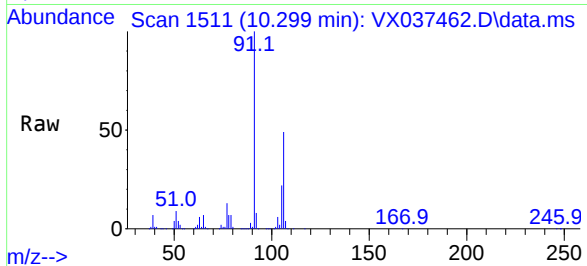

#69
o-Xylene
Concen: 13.740 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion:106 Resp: 43802
Ion Ratio Lower Upper
106 100
91 216.5 108.9 326.8


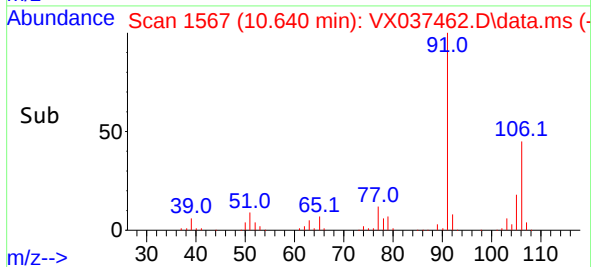

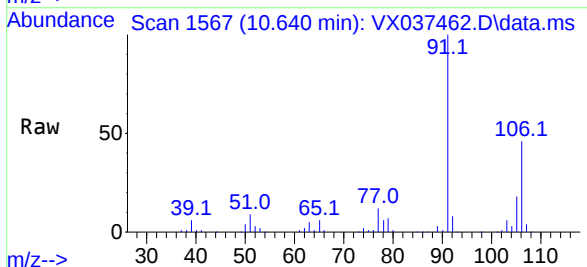




#70
Styrene
Concen: 0.934 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. -0.005 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion:104 Resp: 4906
Ion Ratio Lower Upper
104 100
78 146.7 43.6 65.4#
103 142.2 43.6 65.4#

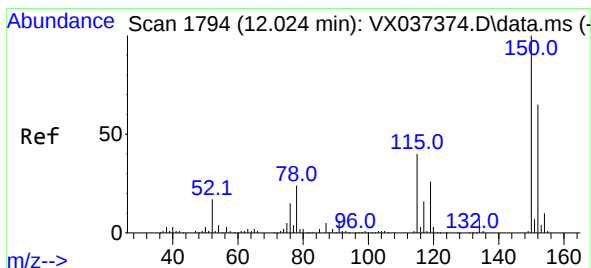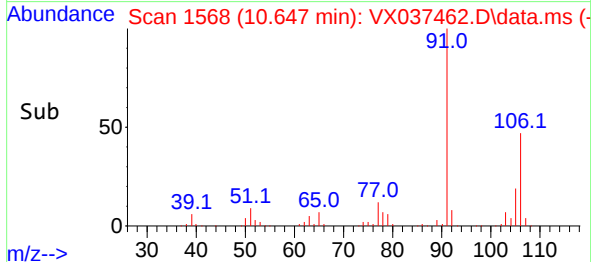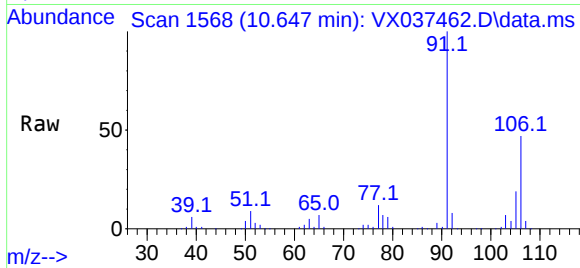

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion:152 Resp: 107728
Ion Ratio Lower Upper
152 100
115 62.6 43.3 129.9
150 157.4 0.0 345.0


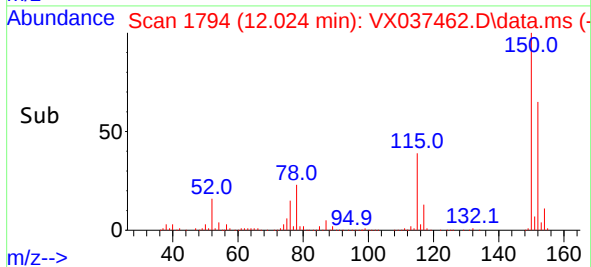

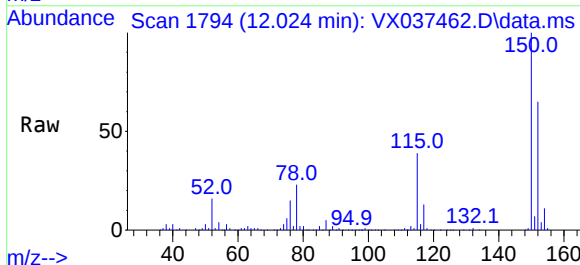




#73
Isopropylbenzene
Concen: 1.033 ug/l
RT: 10.964 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion:105 Resp: 8088
Ion Ratio Lower Upper
105 100
120 23.9 12.9 38.6

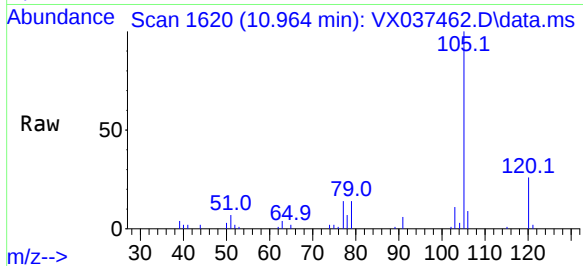

#76
1,2,3-Trichloropropane
Concen: 23.884 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion: 75 Resp: 54795
Ion Ratio Lower Upper
75 100
77 0.9 19.1 57.5#


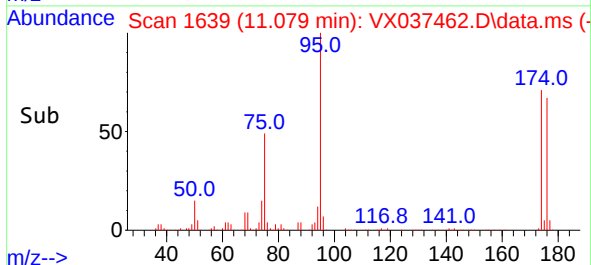

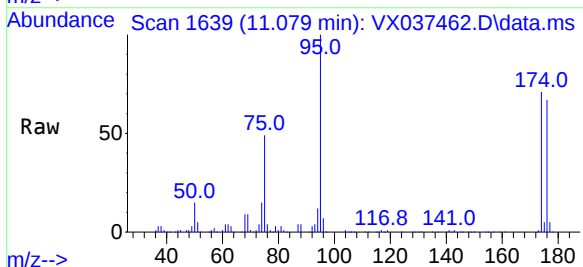




#78
n-propylbenzene
Concen: 1.764 ug/l
RT: 11.305 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion: 91 Resp: 15383
Ion Ratio Lower Upper
91 100
120 23.4 11.5 34.4

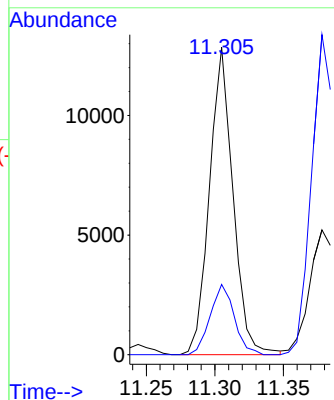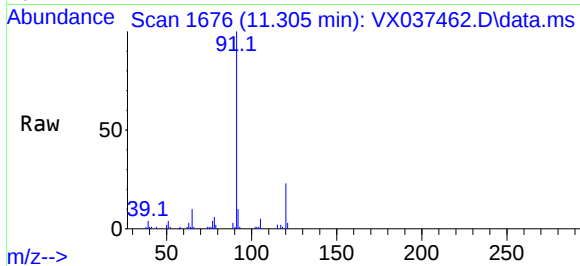

#79
2-Chlorotoluene
Concen: 0.709 ug/l
RT: 11.616 min Scan# 1727
Delta R.T. 0.250 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion: 91 Resp: 3950
Ion Ratio Lower Upper
91 100
126 42.2 16.3 48.8


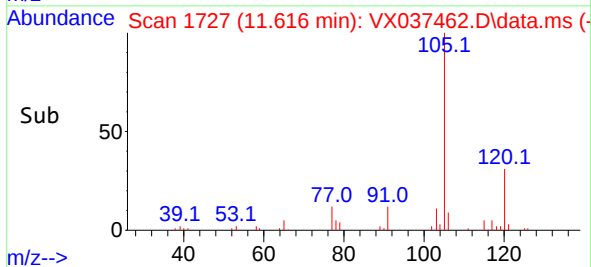
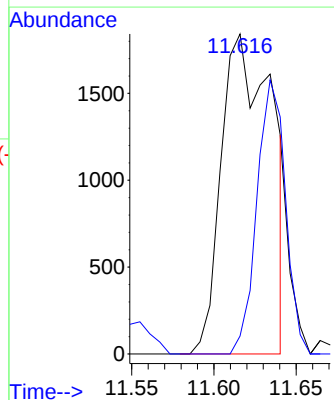
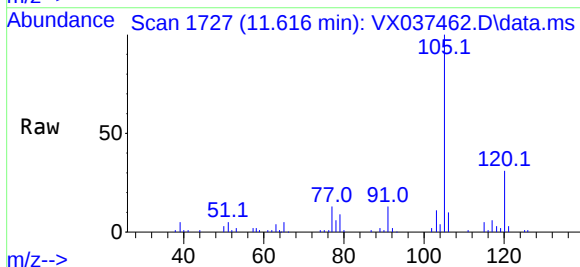




#80
1,3,5-Trimethylbenzene
Concen: 16.000 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion:105 Resp: 104510
Ion Ratio Lower Upper
105 100
120 48.5 24.1 72.3



#81
trans-1,4-Dichloro-2-butene
Concen: 66.708 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion: 75 Resp: 54795
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#


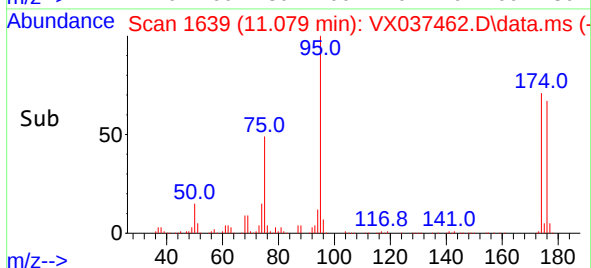
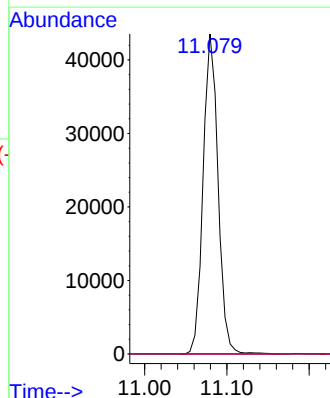





#82
4-Chlorotoluene
Concen: 1.747 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion: 91 Resp: 11239
Ion Ratio Lower Upper
91 100
126 1.1 14.2 42.6#

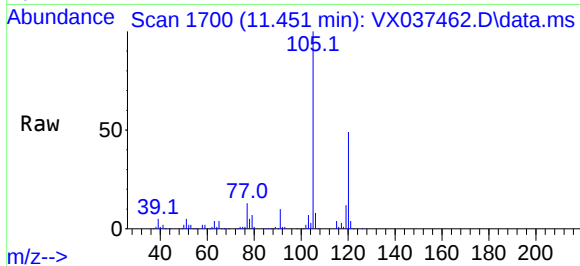

#83
tert-Butylbenzene
Concen: 4.951 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.037 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion: 119 Resp: 30841
Ion Ratio Lower Upper
119 100
91 89.2 31.2 93.6
134 0.0 11.7 35.0#


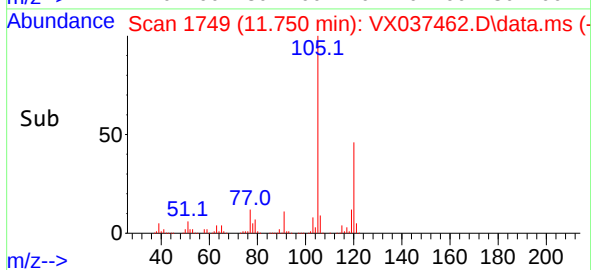

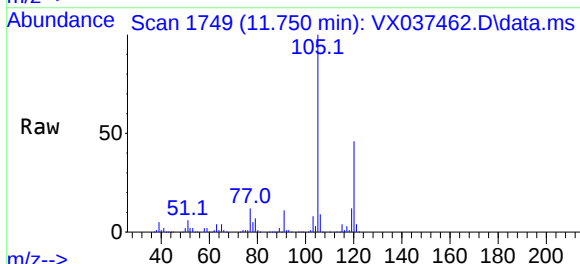




#84
1,2,4-Trimethylbenzene
Concen: 38.933 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion:105 Resp: 257007
Ion Ratio Lower Upper
105 100
120 45.1 21.2 63.6

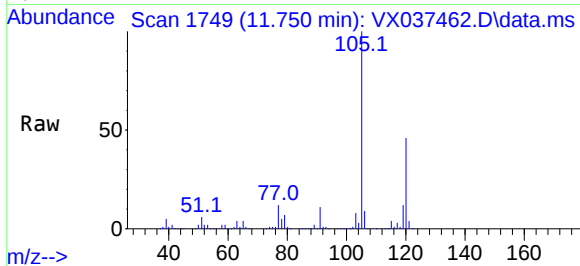

#85
sec-Butylbenzene
Concen: 35.322 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.140 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion:105 Resp: 257007
Ion Ratio Lower Upper
105 100
134 0.0 9.8 29.4#


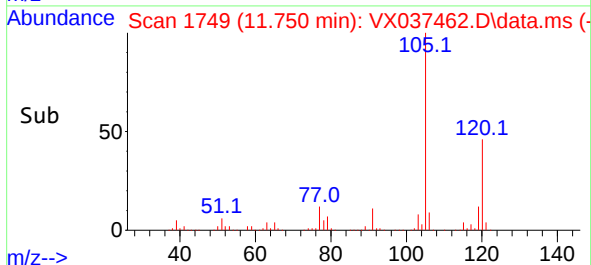

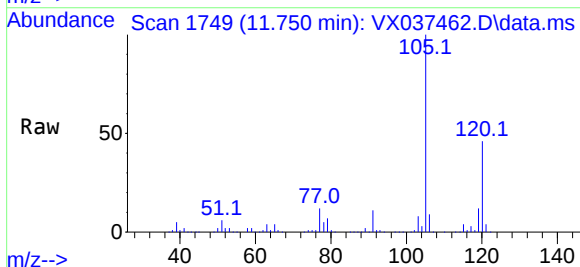




#86
p-Isopropyltoluene
Concen: 0.503 ug/l
RT: 12.012 min Scan# 119
Delta R.T. 0.006 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion:119 Resp: 3151
Ion Ratio Lower Upper
119 100
134 24.7 12.8 38.3
91 62.2 13.1 39.3#

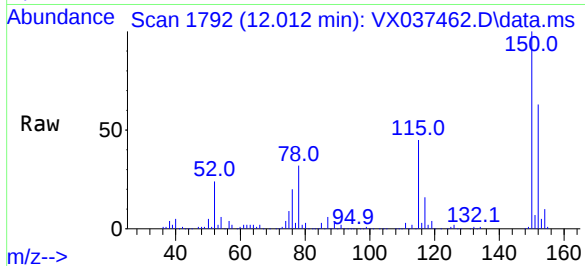

#89
n-Butylbenzene
Concen: 1.261 ug/l
RT: 12.323 min Scan# 1843
Delta R.T. -0.006 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion: 91 Resp: 6551
Ion Ratio Lower Upper
91 100
92 31.8 27.4 82.0
134 120.0 12.6 37.8#


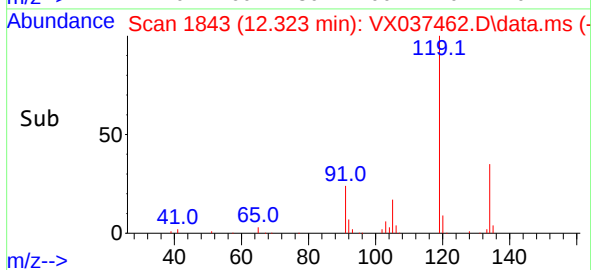

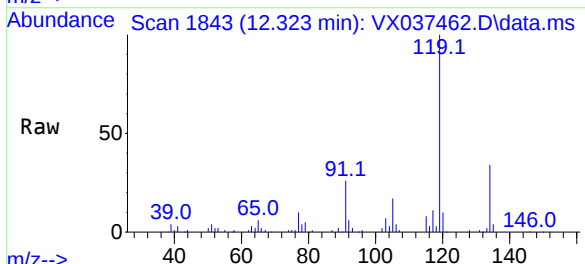




#90
Hexachloroethane
Concen: 4.929 ug/l
RT: 12.603 min Scan# 117
Delta R.T. 0.067 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion:117 Resp: 5153
Ion Ratio Lower Upper
117 100
201 0.0 32.9 98.6#

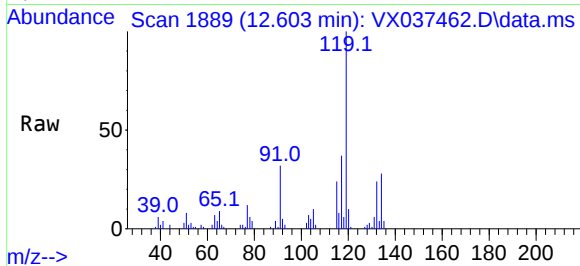

#92
1,2-Dibromo-3-Chloropropane
Concen: 12.828 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.018 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion: 75 Resp: 7860
Ion Ratio Lower Upper
75 100
155 0.0 36.1 108.5#
157 0.0 44.9 134.7#


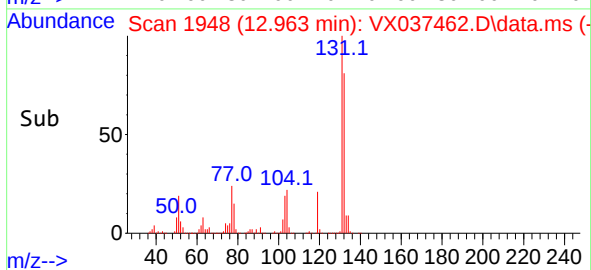






#93
1,2,4-Trichlorobenzene
Concen: 0.229 ug/l
RT: 13.591 min Scan# 2050
Delta R.T. 0.006 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08




Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)


Tgt Ion:	180	Resp:	470
Ion	Ratio	Lower	Upper
180	100		
182	105.1	48.3	144.8
145	0.0	18.0	54.0#

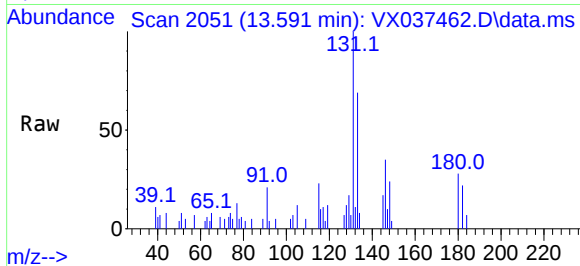

#94
Hexachlorobutadiene
Concen: 0.226 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. 0.000 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Tgt Ion:	225	Resp:	179
Ion	Ratio	Lower	Upper
225	100		
223	24.6	31.1	93.2#
227	48.0	32.5	97.5

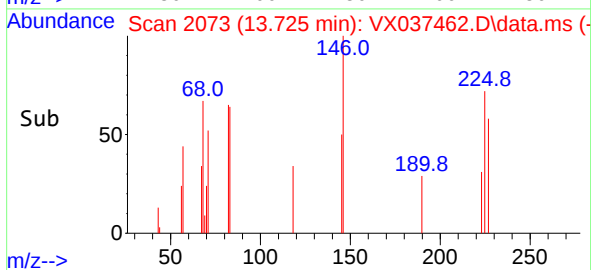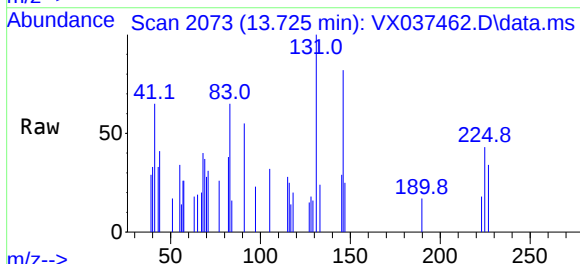



#95
Naphthalene
Concen: 969.858 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX037462.D
Acq: 01 Sep 2023 14:08

Instrument :
MSVOA_X
ClientSampleId :
SB-07(14-15)

Tgt Ion:128 Resp: 8715048
Ion Ratio Lower Upper
128 100
127 16.5 10.3 15.5#
129 14.4 8.8 13.2#

