


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX090219\
Data File : VX012008.D
Acq On : 02 Sep 2019 08:32
Operator : SY/SP
Sample : BFB
Misc : 5.00µ/5.0mL/MSVOA X/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X090219S.M
Title : SW846 8260
Last Update : Tue Sep 03 05:18:49 2019

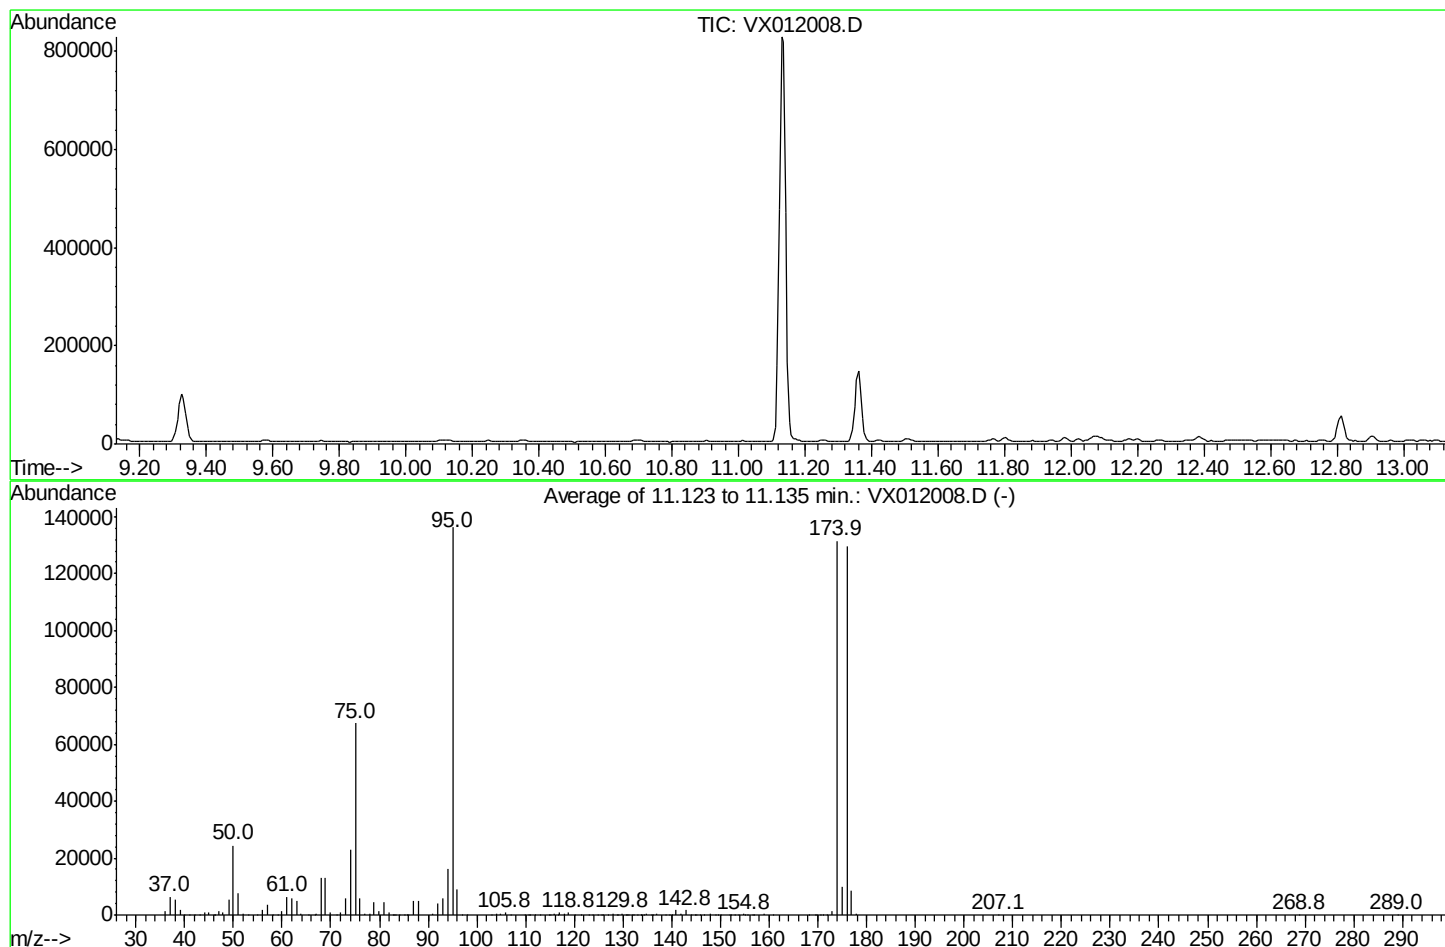

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	24533	PASS
75	95	30	60	49.4	67376	PASS
95	95	100	100	100.0	136272	PASS
96	95	5	9	6.8	9212	PASS
173	174	0.00	2	1.1	1494	PASS
174	95	50	100	96.6	131589	PASS
175	174	5	9	7.5	9812	PASS
176	174	95	101	98.3	129381	PASS
177	176	5	9	6.6	8511	PASS