

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090221\
 Data File : VX024081.D
 Acq On : 02 Sep 2021 19:32
 Operator : JC/MD
 Sample : M3621-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PILOT-PLANT-PROCESS-BLEED

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Title : SW846 8260

Signal : TIC: VX024081.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	56	60	69	rVB	73468	89770	13.57%	1.851%
2	2.300	193	199	207	rVB2	3002	6777	1.02%	0.140%
3	2.392	207	214	221	rBV	9416	15808	2.39%	0.326%
4	2.550	232	240	246	rBV2	4086	7493	1.13%	0.155%
5	2.648	249	256	265	rBV	12494	23607	3.57%	0.487%
6	4.690	582	591	608	rVB2	19172	56585	8.55%	1.167%
7	5.105	647	659	675	rVB2	78903	244781	36.99%	5.048%
8	5.397	696	707	723	rBV2	79154	229450	34.68%	4.732%
9	5.562	723	734	751	rVB2	135902	376450	56.89%	7.763%
10	5.964	789	800	812	rBV	85023	225461	34.07%	4.649%
11	6.099	812	822	838	rVB	238042	613901	92.78%	12.660%
12	6.769	921	932	943	rBV	210017	496016	74.96%	10.229%
13	7.830	1094	1106	1118	rBV	47023	99120	14.98%	2.044%
14	8.171	1156	1162	1170	rVB	27718	45278	6.84%	0.934%
15	8.568	1220	1227	1233	rBV	4001	7049	1.07%	0.145%
16	8.653	1233	1241	1249	rBV	426911	661697	100.00%	13.645%
17	9.000	1291	1298	1303	rBV2	6397	10067	1.52%	0.208%
18	9.525	1379	1384	1390	rBV	23816	33829	5.11%	0.698%
19	10.055	1464	1471	1480	rBV	445727	610740	92.30%	12.594%
20	10.860	1597	1603	1606	rBV2	6694	7951	1.20%	0.164%
21	10.945	1613	1617	1628	rVB	14869	20019	3.03%	0.413%
22	11.085	1634	1640	1653	rVB	358166	445447	67.32%	9.186%
23	12.024	1789	1794	1804	rVB	428627	522028	78.89%	10.765%




Sum of corrected areas: 4849324

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090221\
Data File : VX024081.D
Acq On : 02 Sep 2021 19:32
Operator : JC/MD
Sample : M3621-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PILOT-PLANT-PROCESS-BLEED

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

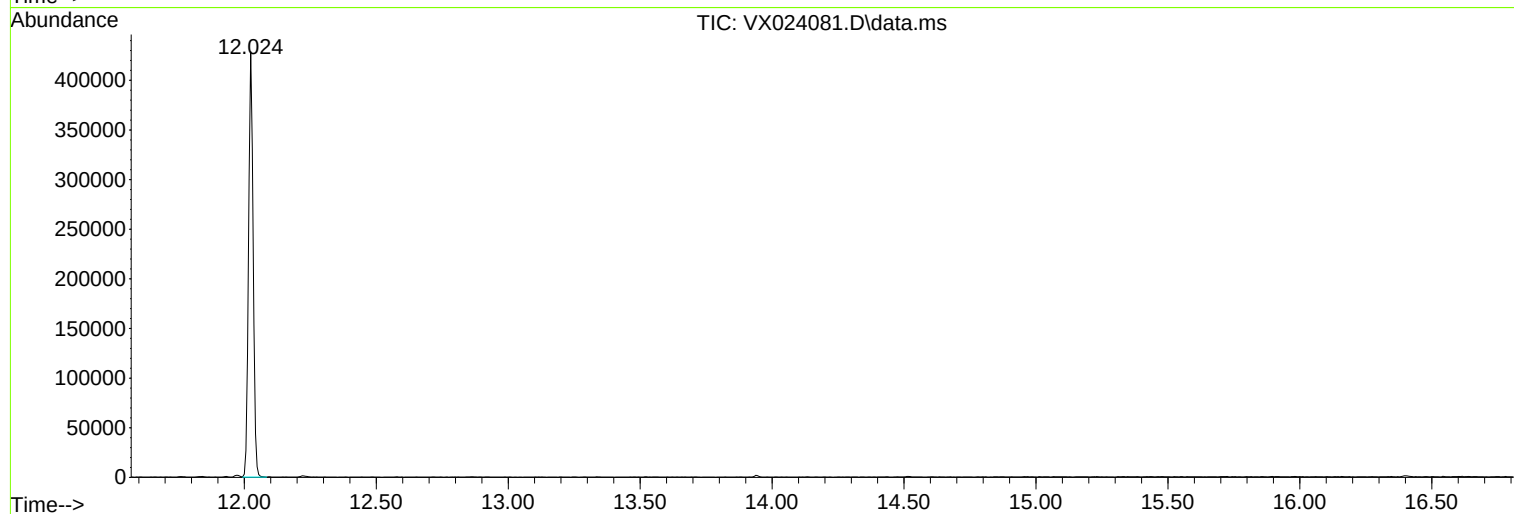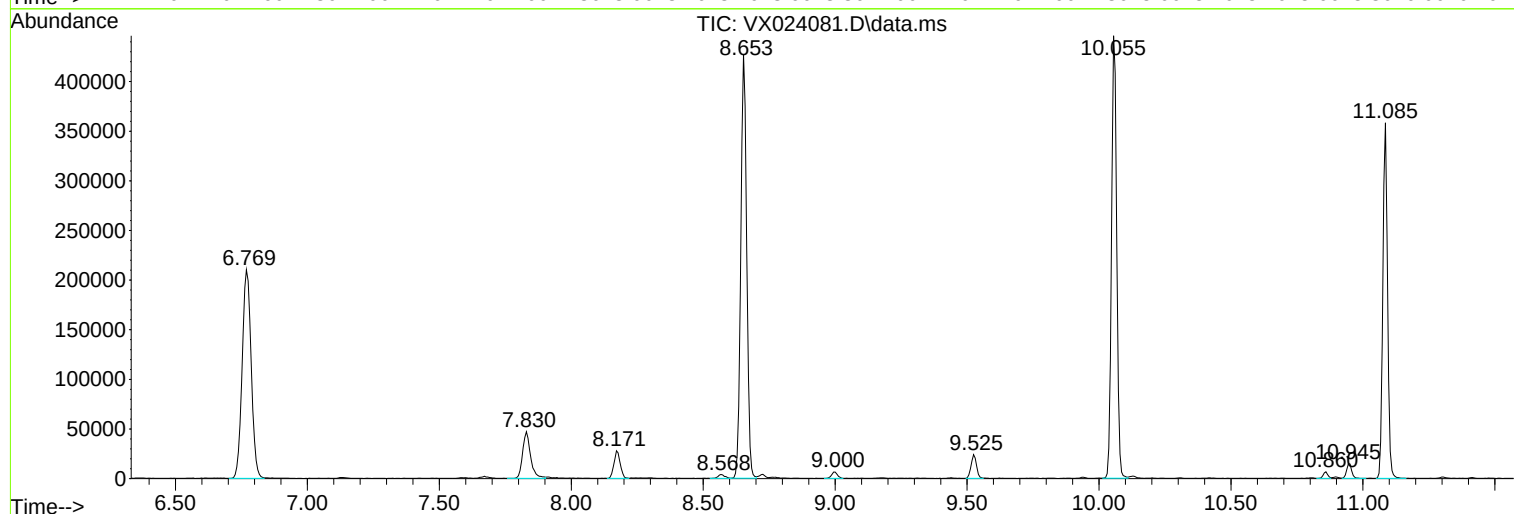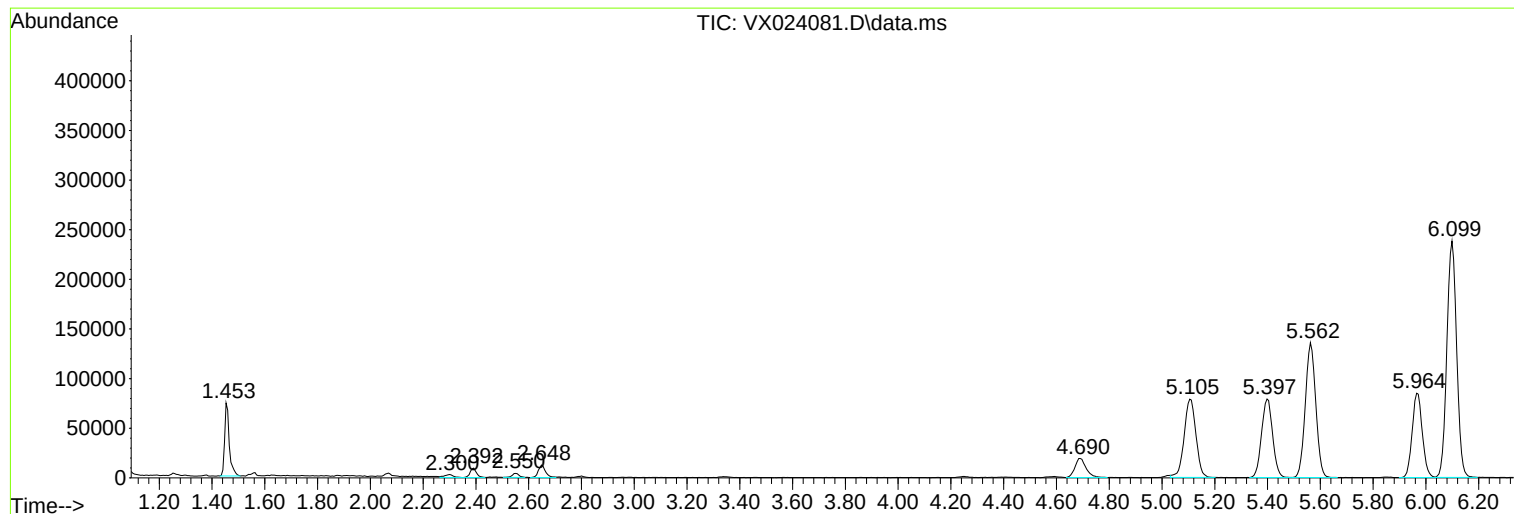

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090221\
Data File : VX024081.D
Acq On : 02 Sep 2021 19:32
Operator : JC/MD
Sample : M3621-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PILOT-PLANT-PROCESS-BLEED

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1,3-Dioxolane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.690	7.52 ug/l	56585	Pentafluorobenzene	5.568

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Dioxolane	74	C3H6O2	000646-06-0	90
2			Dimethylamine	45	C2H7N	000124-40-3	7
3			N-Ethylformamide	73	C3H7NO	000627-45-2	5
4			Thiocyanic acid, methyl ester	73	C2H3NS	000556-64-9	5
5			Methane, isothiocyanato-	73	C2H3NS	000556-61-6	5

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090221\
Data File : VX024081.D
Acq On : 02 Sep 2021 19:32
Operator : JC/MD
Sample : M3621-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PILOT-PLANT-PROCESS-BLEED

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1,3-Dioxolane	4.690	7.5	ug/l	56585	1	5.568	376450	50.0