

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090221\
 Data File : VX024082.D
 Acq On : 02 Sep 2021 19:56
 Operator : JC/MD
 Sample : M3621-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PILOT-PLANT-PROCESS-BLEED

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M

Title : SW846 8260

Signal : TIC: VX024082.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	56	60	73	rBV	118819	149058	21.56%	2.953%
2	2.391	207	214	220	rVB	9739	16178	2.34%	0.320%
3	2.550	233	240	248	rVB	4875	9241	1.34%	0.183%
4	2.647	250	256	265	rBV	15887	28468	4.12%	0.564%
5	4.690	582	591	606	rVB2	20474	59132	8.55%	1.171%
6	5.104	638	659	674	rBV2	85726	269709	39.00%	5.343%
7	5.397	694	707	722	rBV2	83000	239364	34.61%	4.742%
8	5.562	722	734	747	rVB	143435	395421	57.18%	7.833%
9	5.970	790	801	811	rBV	89935	237154	34.30%	4.698%
10	6.098	811	822	839	rVB	210211	539615	78.03%	10.690%
11	6.769	922	932	948	rBV	219622	523515	75.71%	10.371%
12	7.829	1098	1106	1119	rBV	48244	102529	14.83%	2.031%
13	8.171	1155	1162	1170	rBV	28146	49524	7.16%	0.981%
14	8.652	1232	1241	1249	rVV	446367	691508	100.00%	13.699%
15	9.000	1292	1298	1303	rBV2	6676	10479	1.52%	0.208%
16	9.524	1379	1384	1392	rBV	26572	38187	5.52%	0.756%
17	10.055	1463	1471	1480	rBV	463311	647577	93.65%	12.829%
18	10.859	1598	1603	1606	rBV2	5591	7050	1.02%	0.140%
19	10.951	1612	1618	1624	rVB	14607	19464	2.81%	0.386%
20	11.085	1634	1640	1650	rBV	382088	467542	67.61%	9.262%
21	12.024	1789	1794	1807	rBV	435496	547137	79.12%	10.839%


Sum of corrected areas: 5047852

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090221\
Data File : VX024082.D
Acq On : 02 Sep 2021 19:56
Operator : JC/MD
Sample : M3621-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PILOT-PLANT-PROCESS-BLEED

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

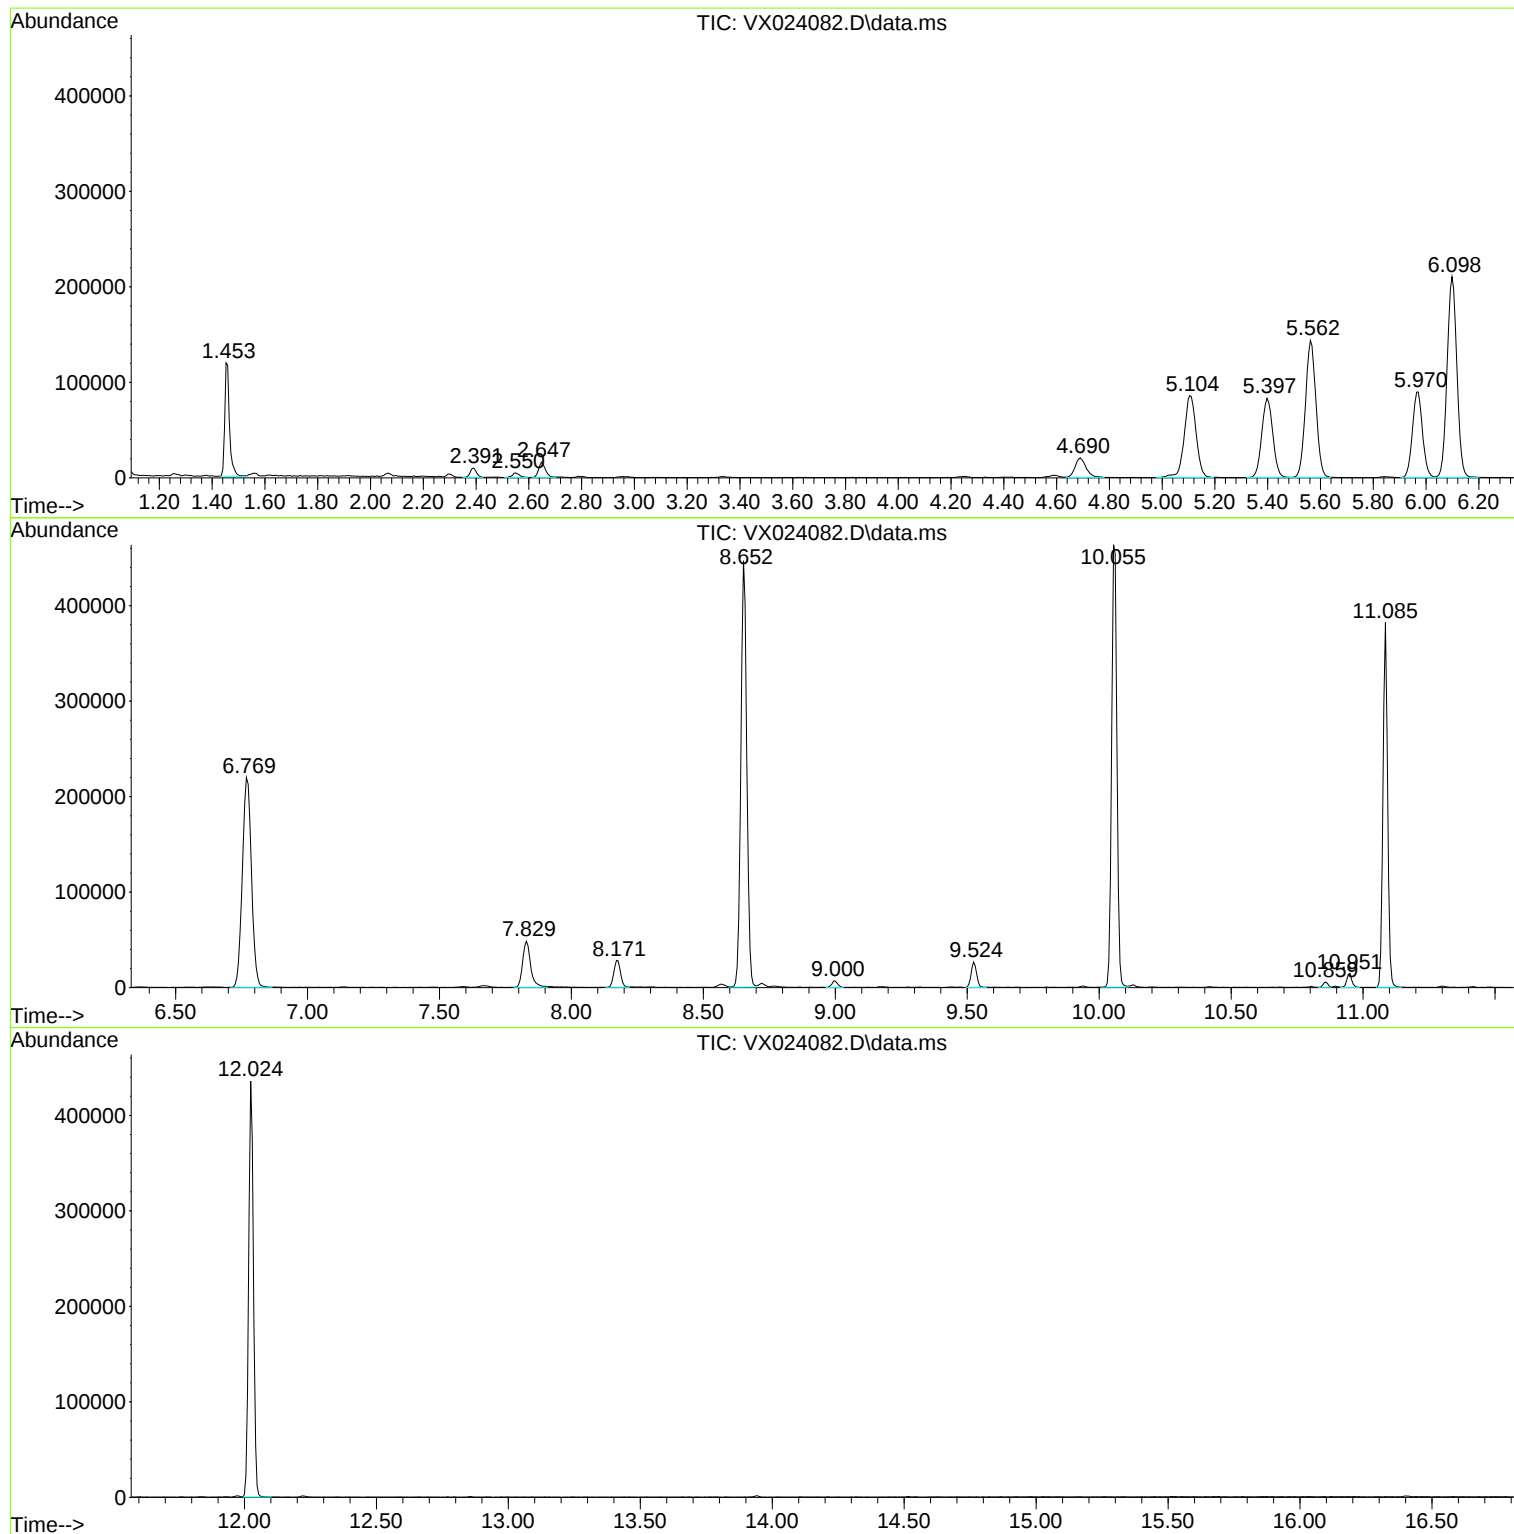

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090221\
Data File : VX024082.D
Acq On : 02 Sep 2021 19:56
Operator : JC/MD
Sample : M3621-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PILOT-PLANT-PROCESS-BLEED










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1,3-Dioxolane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.690	7.48 ug/l	59132	Pentafluorobenzene	5.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Dioxolane	74	C3H6O2	000646-06-0	90
2			Dimethylamine	45	C2H7N	000124-40-3	9
3			N-Ethylformamide	73	C3H7NO	000627-45-2	5
4			1,2-Ethanediamine, N-methyl-	74	C3H10N2	000109-81-9	5
5			Guanidine, methyl-	73	C2H7N3	000471-29-4	5

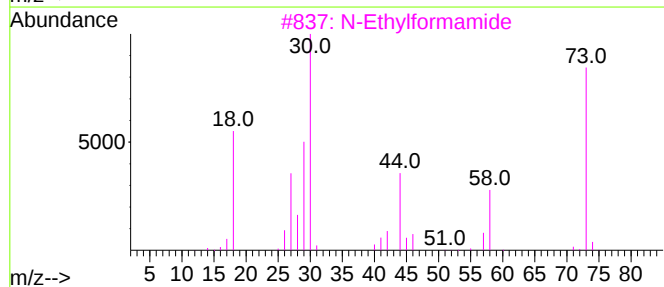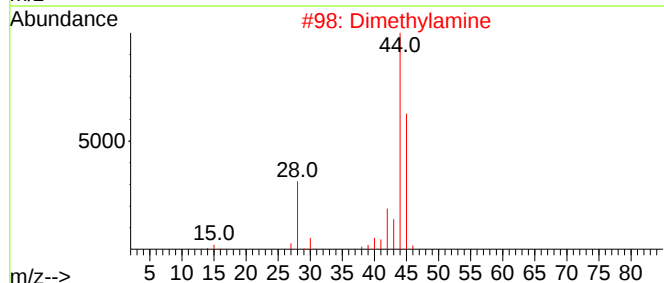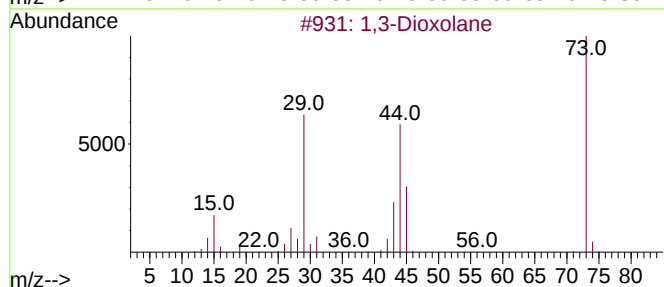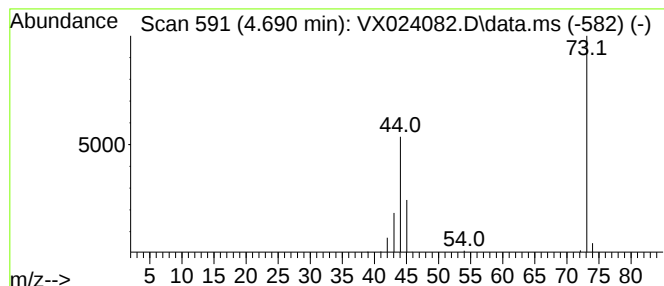

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090221\
Data File : VX024082.D
Acq On : 02 Sep 2021 19:56
Operator : JC/MD
Sample : M3621-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PILOT-PLANT-PROCESS-BLEED

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1,3-Dioxolane	4.690	7.5	ug/l	59132	1	5.562	395421	50.0