

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090223\
 Data File : VX037487.D
 Acq On : 02 Sep 2023 16:51
 Operator : JC/MD
 Sample : 04269-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-13B-47-083123

Quant Time: Sep 04 04:30:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 18 09:30:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	170564	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	283113	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	250212	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	107879	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	100627	40.922	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	81.840%
35) Dibromofluoromethane	5.385	113	85171	45.425	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.840%
50) Toluene-d8	8.647	98	331686	48.768	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.540%
62) 4-Bromofluorobenzene	11.079	95	115302	43.139	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	86.280%
Target Compounds						
44) Trichloroethene	7.123	130	1566	0.723	ug/l	Qvalue 69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090223\
Data File : VX037487.D
Acq On : 02 Sep 2023 16:51
Operator : JC/MD
Sample : 04269-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-13B-47-083123

Quant Time: Sep 04 04:30:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 18 09:30:38 2023
Response via : Initial Calibration




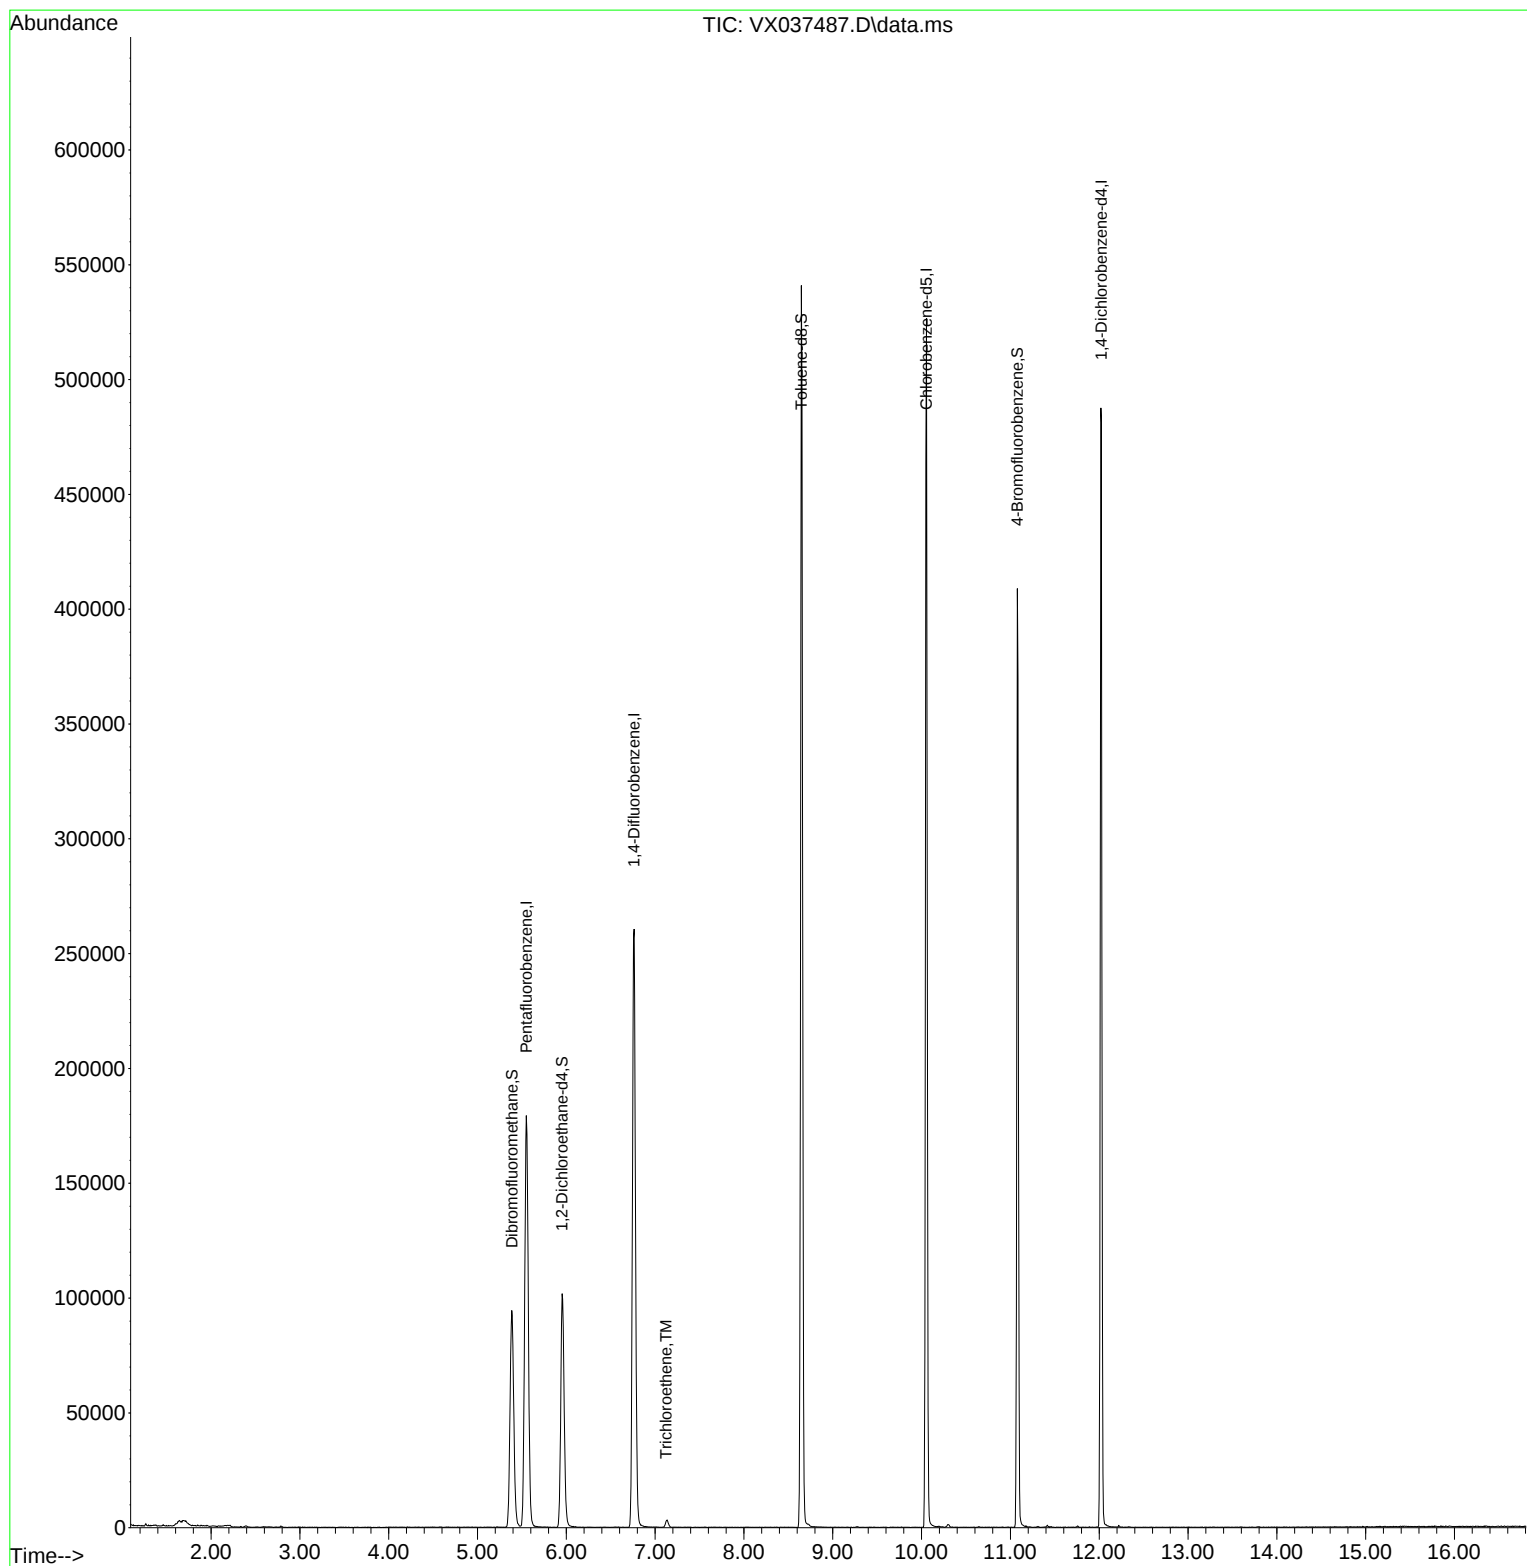




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX037487.D
Acq: 02 Sep 2023 16:51




Instrument :
MSVOA_X
ClientSampleId :
MW-13B-47-083123


Tgt Ion:168 Resp: 170564
Ion Ratio Lower Upper
168 100
99 62.0 56.6 85.0

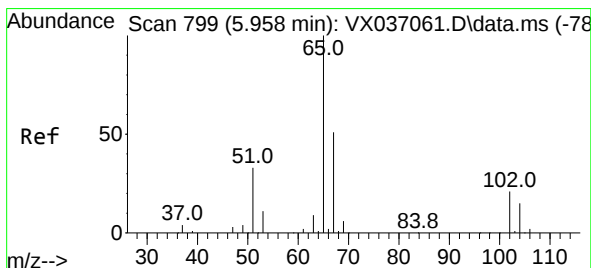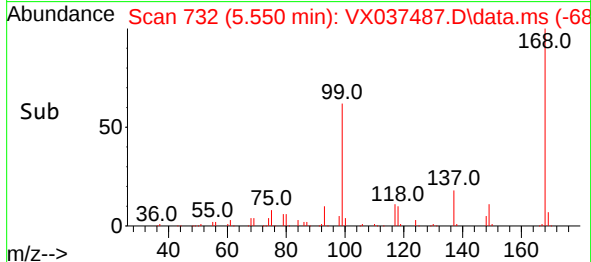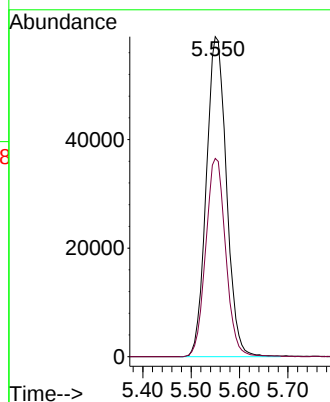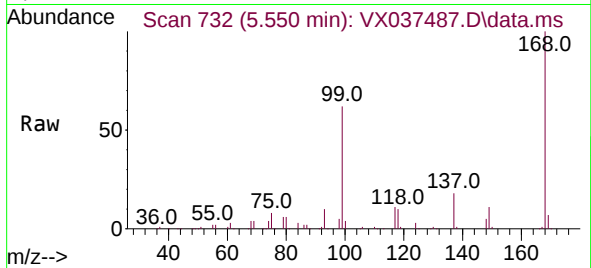

#33
1,2-Dichloroethane-d4
Concen: 40.922 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX037487.D
Acq: 02 Sep 2023 16:51

Tgt Ion: 65 Resp: 100627
Ion Ratio Lower Upper
65 100
67 51.6 0.0 100.2


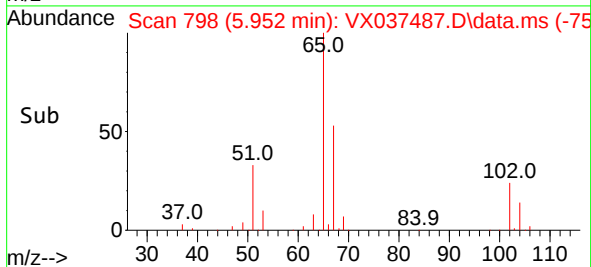
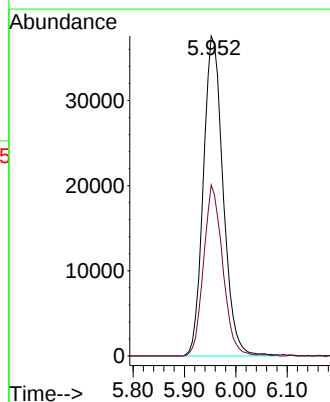
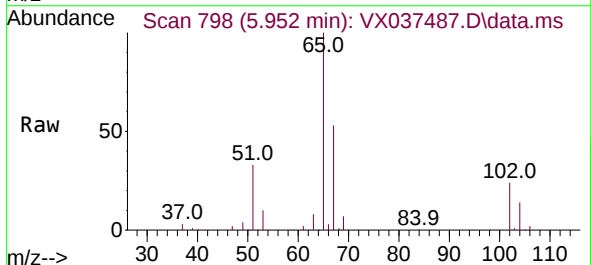


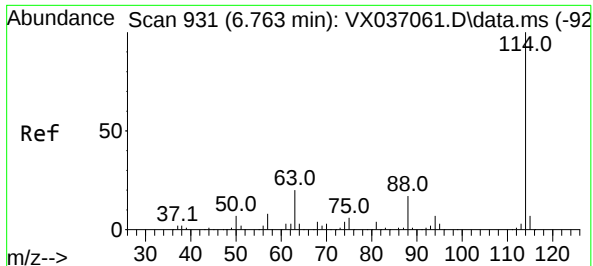

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX037487.D
Acq: 02 Sep 2023 16:51




Instrument :
MSVOA_X
ClientSampleId :
MW-13B-47-083123


Tgt Ion:114 Resp: 283113
Ion Ratio Lower Upper
114 100
63 18.6 0.0 45.0
88 16.2 0.0 36.6

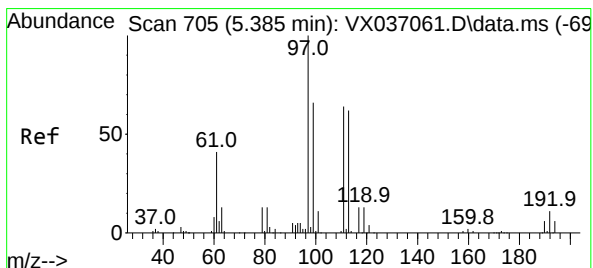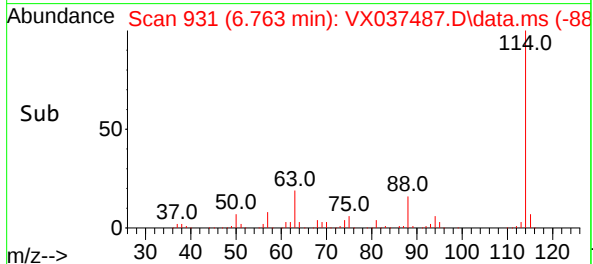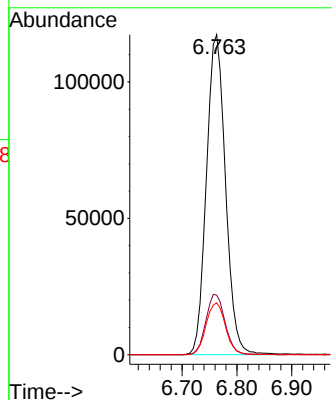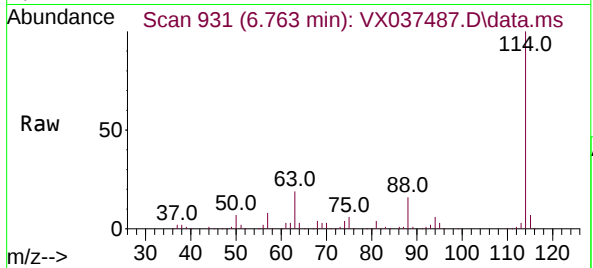

#35
Dibromofluoromethane
Concen: 45.425 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX037487.D
Acq: 02 Sep 2023 16:51

Tgt Ion:113 Resp: 85171
Ion Ratio Lower Upper
113 100
111 102.6 82.9 124.3
192 18.7 13.3 19.9


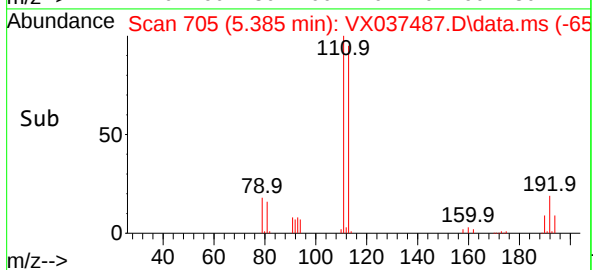
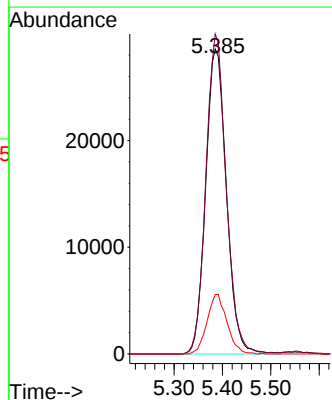
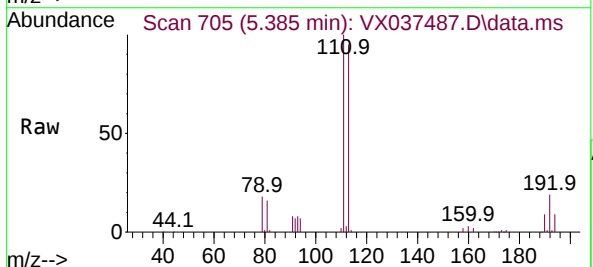


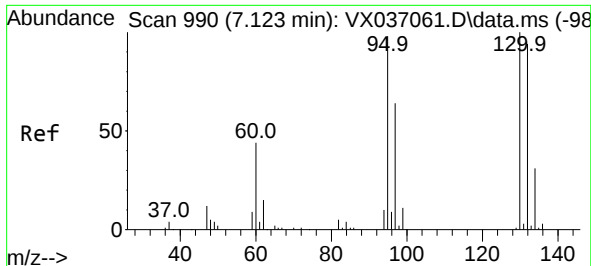

#44
Trichloroethene
Concen: 0.723 ug/l
RT: 7.123 min Scan# 990
Delta R.T. 0.000 min
Lab File: VX037487.D
Acq: 02 Sep 2023 16:51




Instrument :
MSVOA_X
ClientSampleId :
MW-13B-47-083123


Tgt Ion:130 Resp: 1566
Ion Ratio Lower Upper
130 100
95 70.8 0.0 204.4

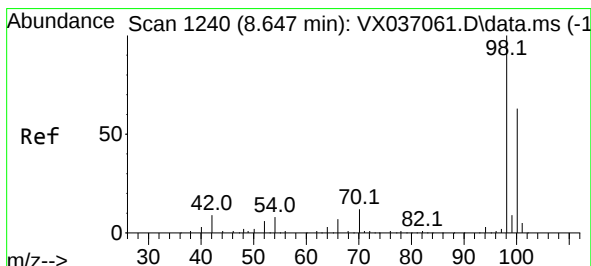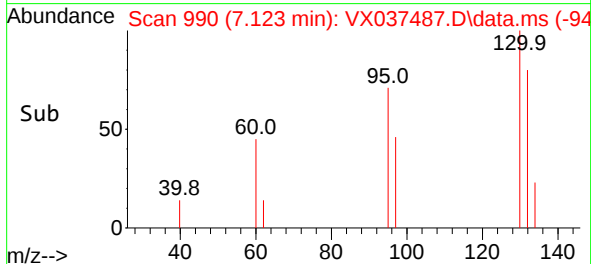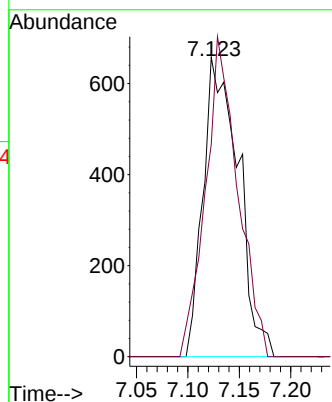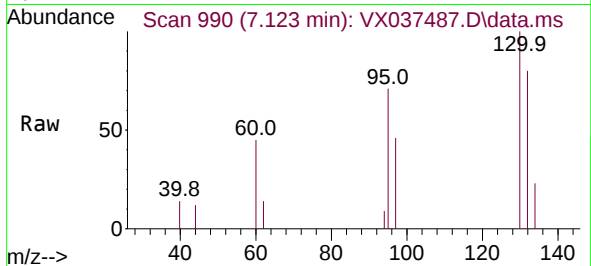

#50
Toluene-d8
Concen: 48.768 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX037487.D
Acq: 02 Sep 2023 16:51

Tgt Ion: 98 Resp: 331686
Ion Ratio Lower Upper
98 100
100 66.3 53.1 79.7


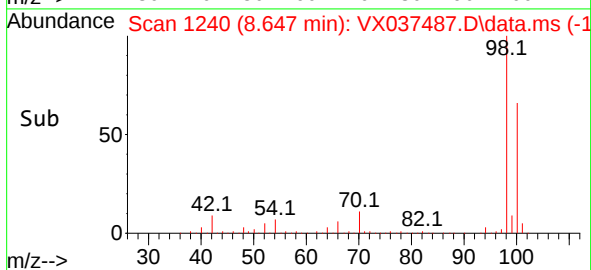
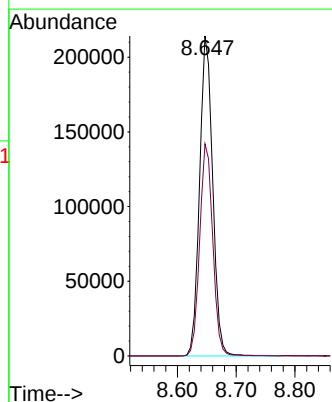
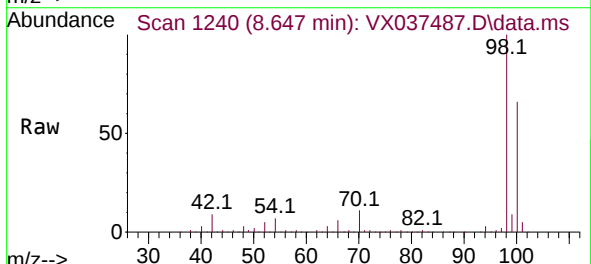


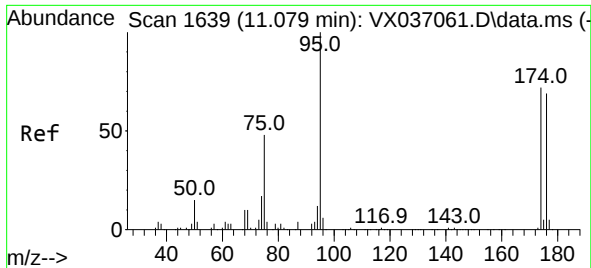

#62
4-Bromofluorobenzene
Concen: 43.139 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX037487.D
Acq: 02 Sep 2023 16:51




Instrument :
MSVOA_X
ClientSampleId :
MW-13B-47-083123


Tgt Ion: 95 Resp: 115302
Ion Ratio Lower Upper
95 100
174 76.4 0.0 135.6
176 71.6 0.0 131.0

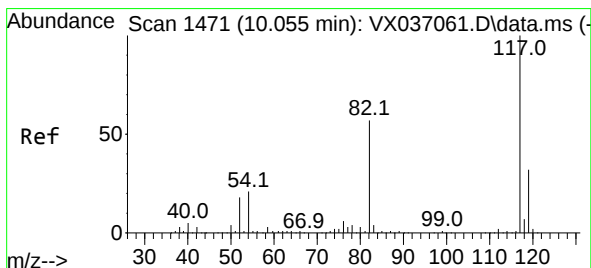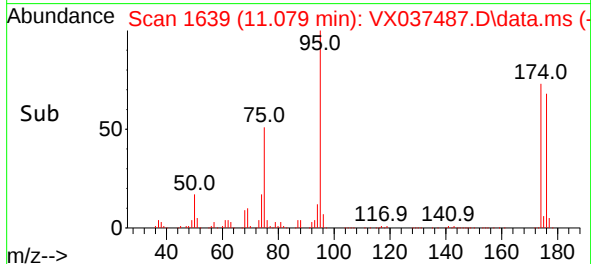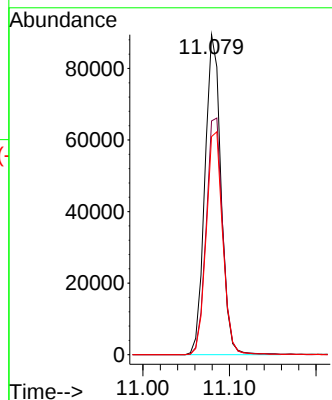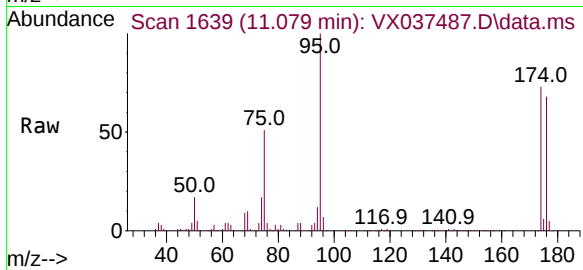

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX037487.D
Acq: 02 Sep 2023 16:51

Tgt Ion: 117 Resp: 250212
Ion Ratio Lower Upper
117 100
82 54.3 46.2 69.4
119 32.1 25.5 38.3

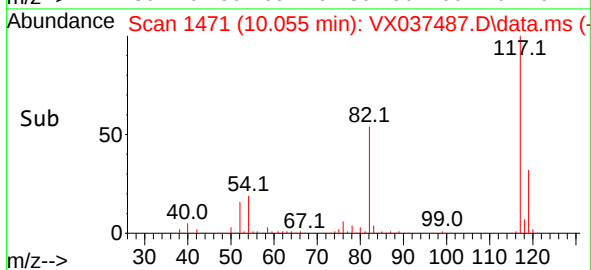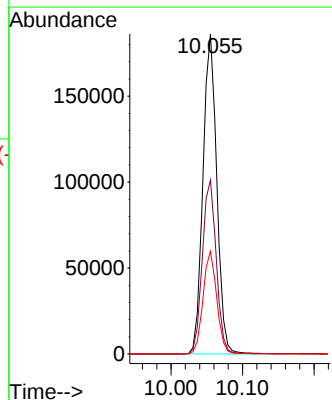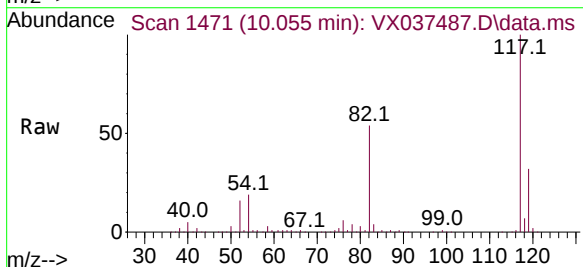

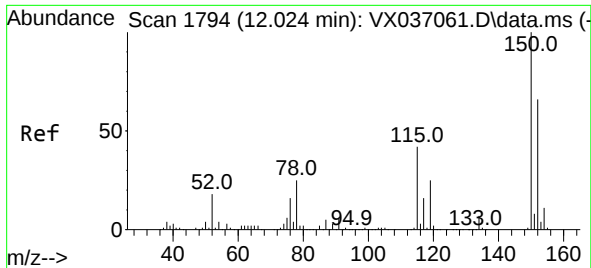

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX037487.D


Acq: 02 Sep 2023 16:51

Instrument :

MSVOA_X

ClientSampleId :

MW-13B-47-083123

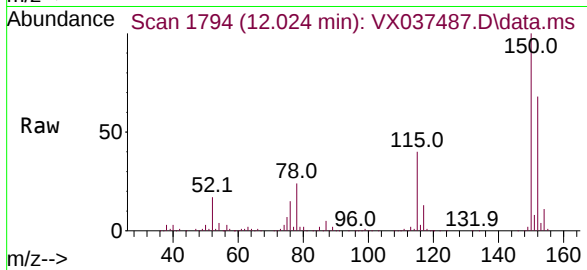

Tgt Ion:152 Resp: 107879

Ion Ratio Lower Upper

152 100

115 62.6 43.3 129.9

150 154.1 0.0 345.0

