

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090223\  
 Data File : VX037493.D  
 Acq On : 02 Sep 2023 19:14  
 Operator : JC/MD  
 Sample : 04272-03  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 OW-01B-67-083123

Quant Time: Sep 04 04:32:33 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081723W.M  
 Quant Title : SW846 8260  
 QLast Update : Fri Aug 18 09:30:38 2023  
 Response via : Initial Calibration


| Compound                     | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|------------------------------|--------|-------|----------|----------|--------|----------|
| -----                        |        |       |          |          |        |          |
| Internal Standards           |        |       |          |          |        |          |
| 1) Pentafluorobenzene        | 5.550  | 168   | 158126   | 50.000   | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene      | 6.763  | 114   | 262107   | 50.000   | ug/l   | 0.00     |
| 63) Chlorobenzene-d5         | 10.055 | 117   | 232304   | 50.000   | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4   | 12.024 | 152   | 102984   | 50.000   | ug/l   | 0.00     |
| System Monitoring Compounds  |        |       |          |          |        |          |
| 33) 1,2-Dichloroethane-d4    | 5.952  | 65    | 94203    | 41.323   | ug/l   | 0.00     |
| Spiked Amount                | 50.000 | Range | 78 - 117 | Recovery | =      | 82.640%  |
| 35) Dibromofluoromethane     | 5.385  | 113   | 78529    | 45.239   | ug/l   | 0.00     |
| Spiked Amount                | 50.000 | Range | 75 - 124 | Recovery | =      | 90.480%  |
| 50) Toluene-d8               | 8.647  | 98    | 304187   | 48.309   | ug/l   | 0.00     |
| Spiked Amount                | 50.000 | Range | 92 - 112 | Recovery | =      | 96.620%  |
| 62) 4-Bromofluorobenzene     | 11.079 | 95    | 109170   | 44.118   | ug/l   | 0.00     |
| Spiked Amount                | 50.000 | Range | 83 - 123 | Recovery | =      | 88.240%  |
| Target Compounds             |        |       |          |          |        |          |
|                              |        |       |          |          | Qvalue |          |
| 9) 1,1,2-Trichlorotrifluo... | 2.331  | 101   | 422      | 0.252    | ug/l   | 95       |
| 12) 1,1-Dichloroethene       | 2.319  | 96    | 600      | 0.369    | ug/l # | 62       |
| 27) cis-1,2-Dichloroethene   | 4.501  | 96    | 1747     | 0.801    | ug/l   | 77       |
| 44) Trichloroethene          | 7.129  | 130   | 8685     | 4.330    | ug/l   | 94       |
| 64) Tetrachloroethene        | 9.275  | 164   | 822      | 0.485    | ug/l # | 76       |
| -----                        |        |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090223\  
Data File : VX037493.D  
Acq On : 02 Sep 2023 19:14  
Operator : JC/MD  
Sample : 04272-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
OW-01B-67-083123

Quant Time: Sep 04 04:32:33 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081723W.M  
Quant Title : SW846 8260  
QLast Update : Fri Aug 18 09:30:38 2023  
Response via : Initial Calibration




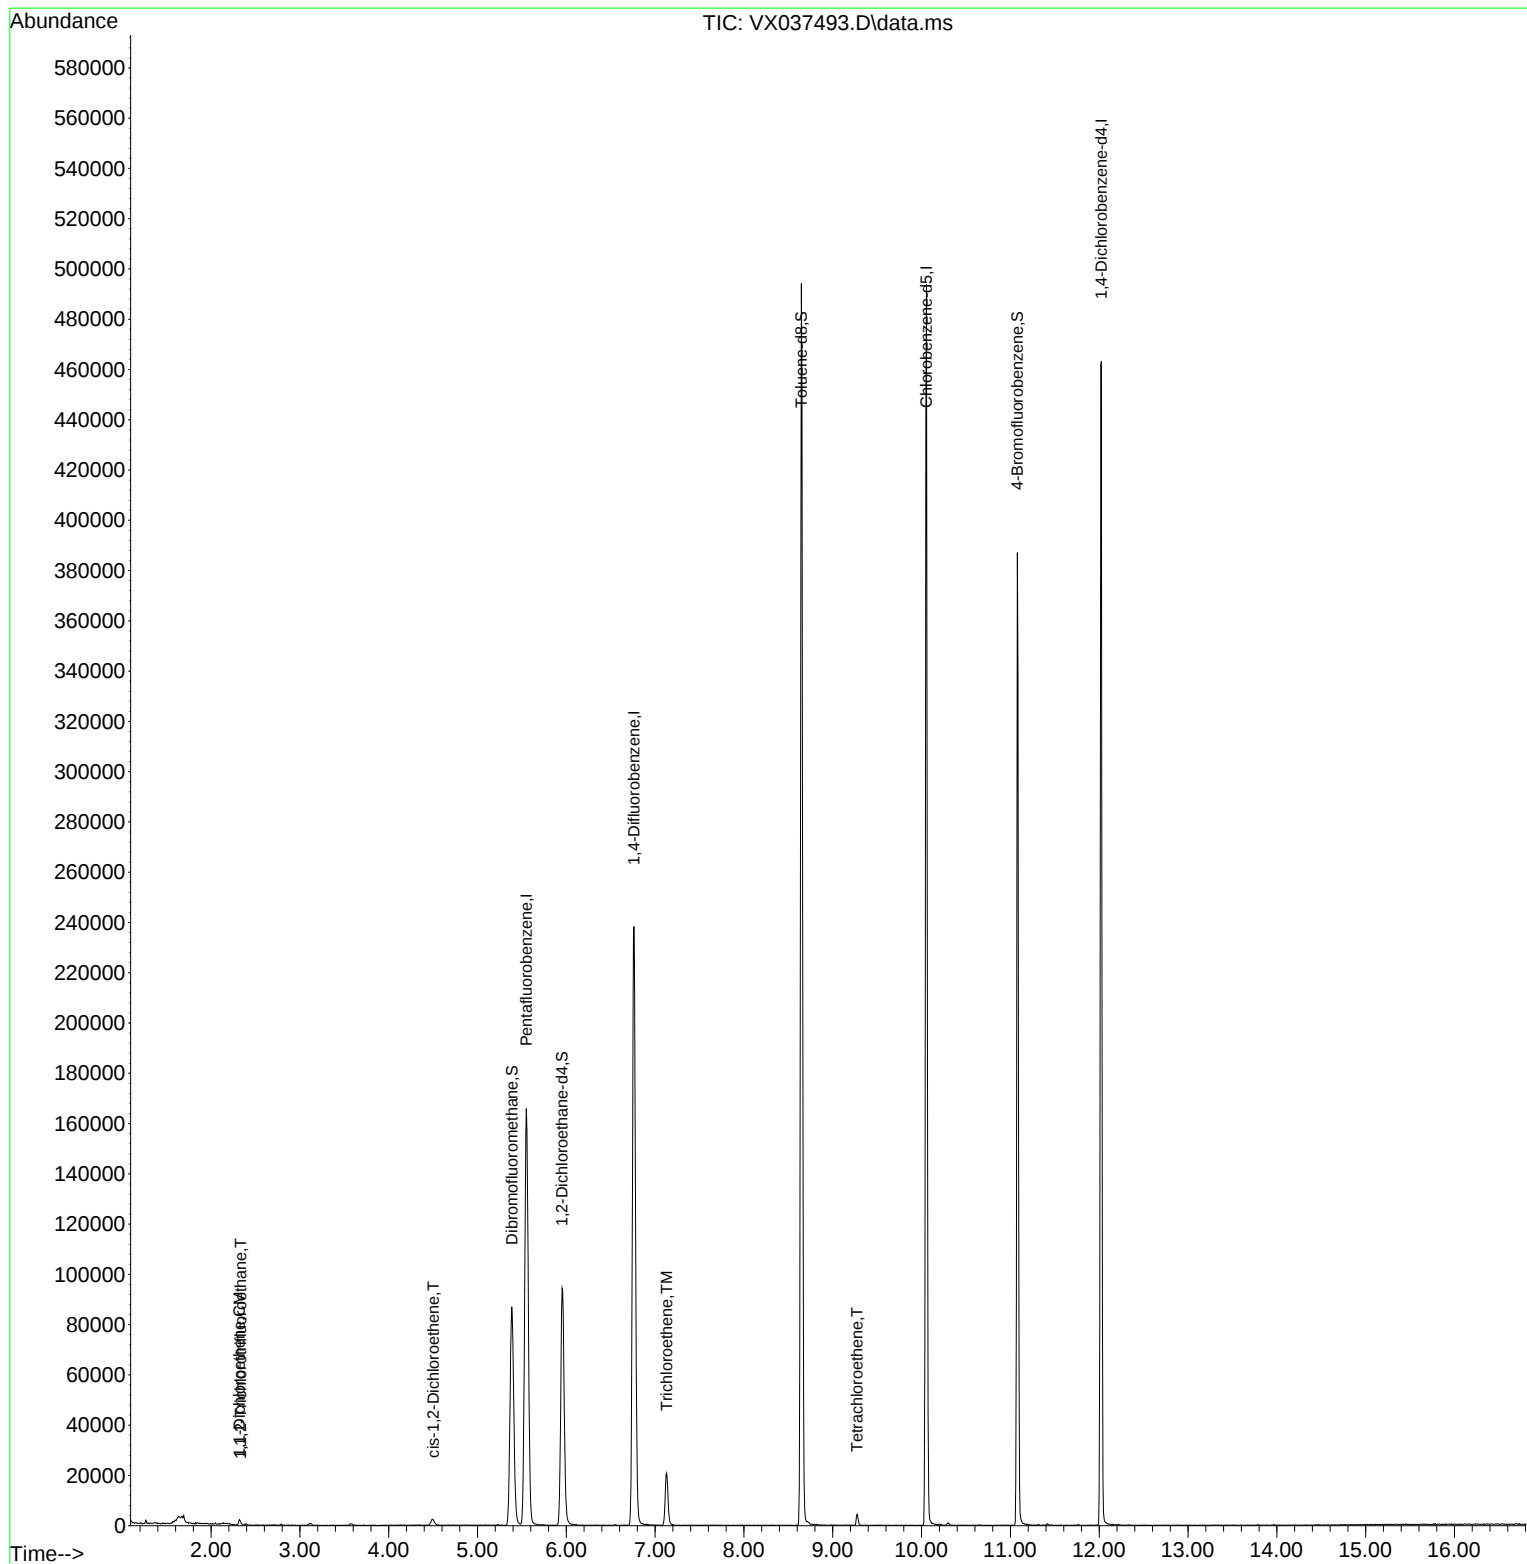


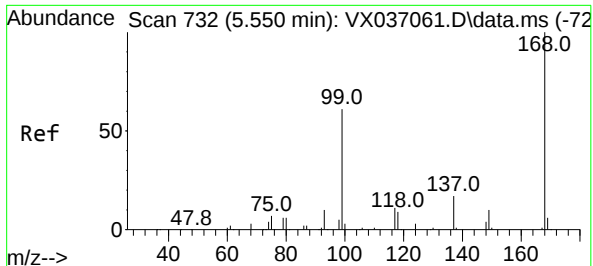

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 71  
Delta R.T. -0.000 min  
Lab File: VX037493.D  
Acq: 02 Sep 2023 19:14




Instrument :  
MSVOA\_X  
ClientSampleId :  
OW-01B-67-083123


Tgt Ion:168 Resp: 158126  
Ion Ratio Lower Upper  
168 100  
99 60.9 56.6 85.0

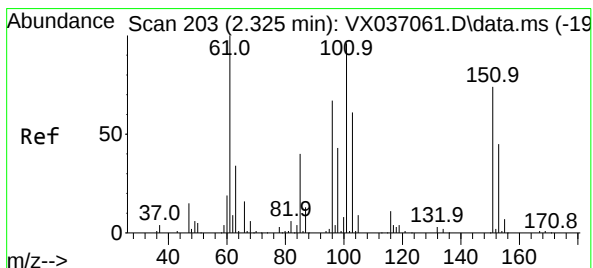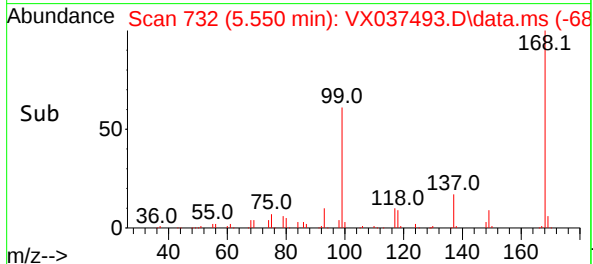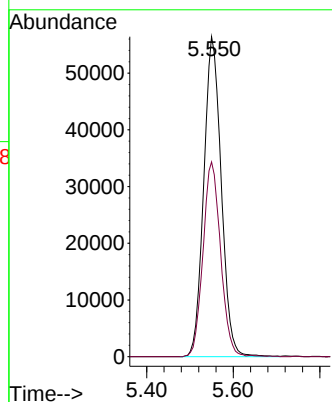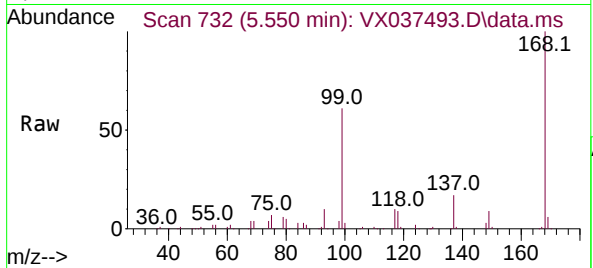

#9  
1,1,2-Trichlorotrifluoroethane  
Concen: 0.252 ug/l  
RT: 2.331 min Scan# 204  
Delta R.T. 0.006 min  
Lab File: VX037493.D  
Acq: 02 Sep 2023 19:14

Tgt Ion:101 Resp: 422  
Ion Ratio Lower Upper  
101 100  
85 38.6 37.0 55.6  
151 73.9 58.6 87.8


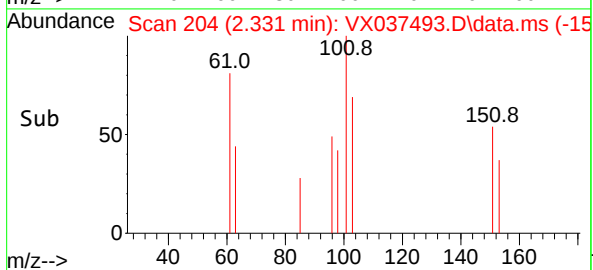
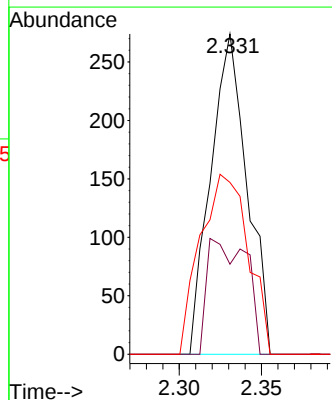
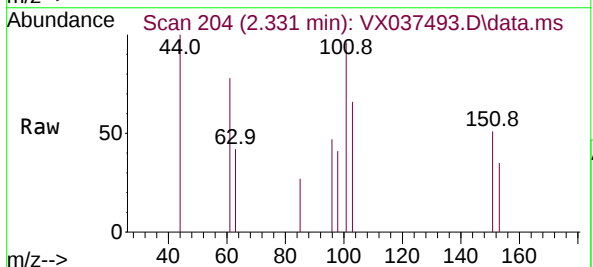


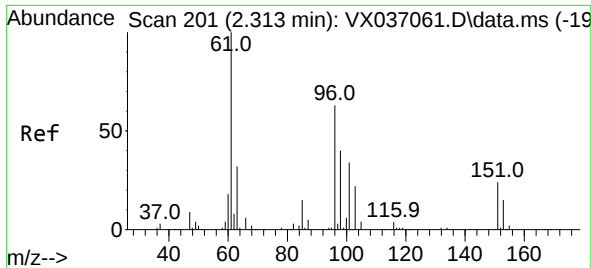

#12  
 1,1-Dichloroethene  
 Concen: 0.369 ug/l  
 RT: 2.319 min Scan# 201  
 Delta R.T. 0.006 min  
 Lab File: VX037493.D  
 Acq: 02 Sep 2023 19:14




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 OW-01B-67-083123


Tgt Ion: 96 Resp: 600  
 Ion Ratio Lower Upper  
 96 100  
 61 113.9 144.6 216.8#  
 98 52.4 50.4 75.6

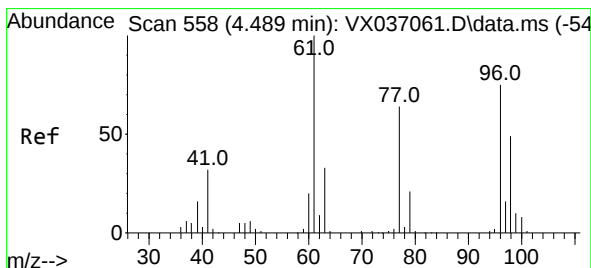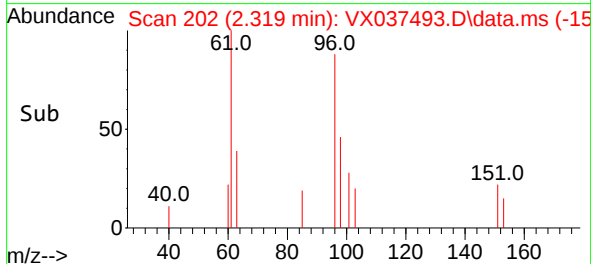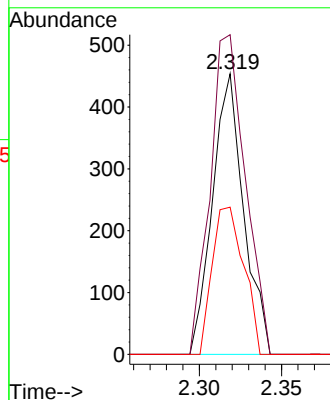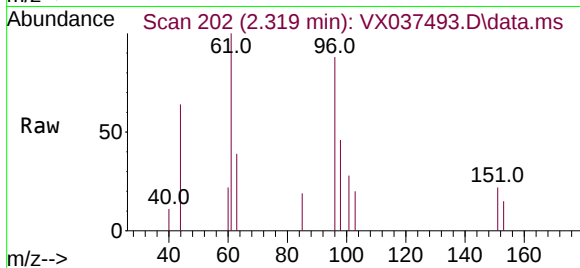

#27  
 cis-1,2-Dichloroethene  
 Concen: 0.801 ug/l  
 RT: 4.501 min Scan# 560  
 Delta R.T. 0.012 min  
 Lab File: VX037493.D  
 Acq: 02 Sep 2023 19:14

Tgt Ion: 96 Resp: 1747  
 Ion Ratio Lower Upper  
 96 100  
 61 118.3 0.0 312.2  
 98 70.7 0.0 129.0

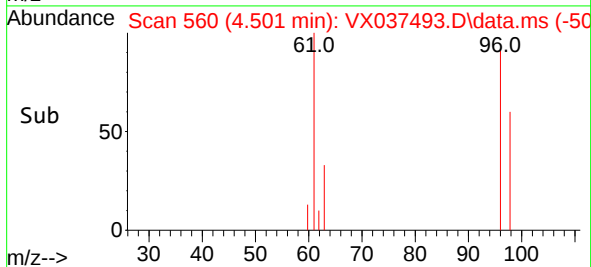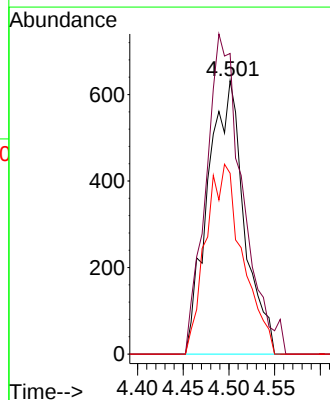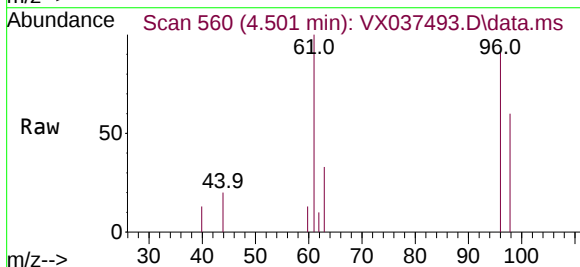

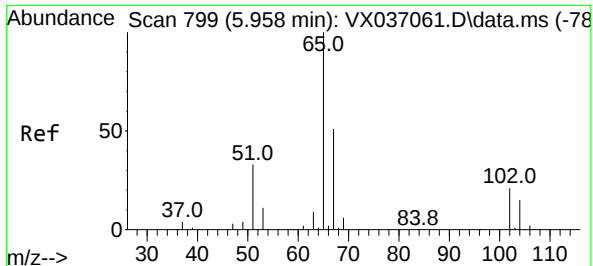

#33

1,2-Dichloroethane-d4

Concen: 41.323 ug/l

RT: 5.952 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX037493.D

Acq: 02 Sep 2023 19:14

Instrument :

MSVOA\_X

ClientSampleId :





OW-01B-67-083123

Tgt Ion: 65 Resp: 94203

Ion Ratio Lower Upper

65 100

67 52.3 0.0 100.2

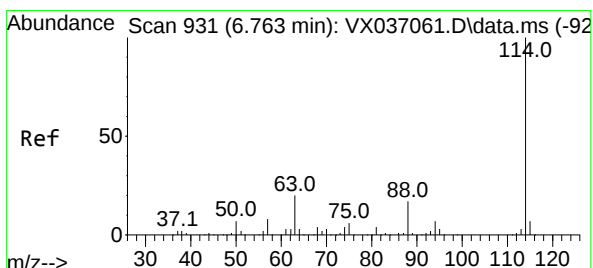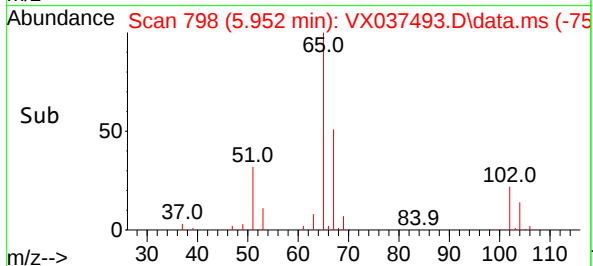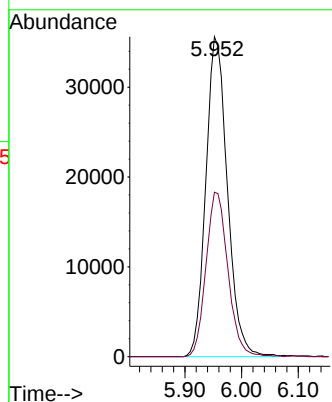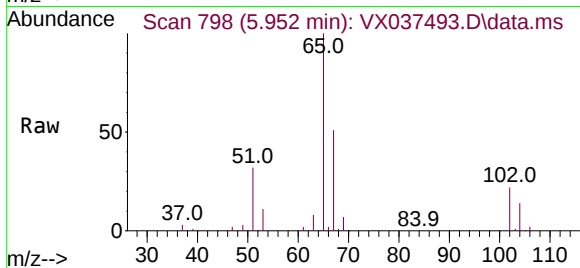

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX037493.D

Acq: 02 Sep 2023 19:14




Tgt Ion: 114 Resp: 262107


Ion Ratio Lower Upper

114 100

63 18.4 0.0 45.0


88 17.1 0.0 36.6

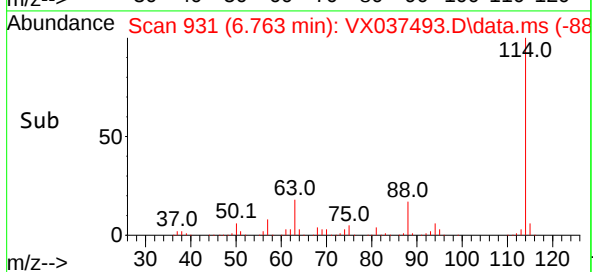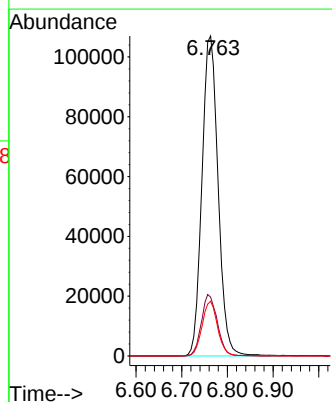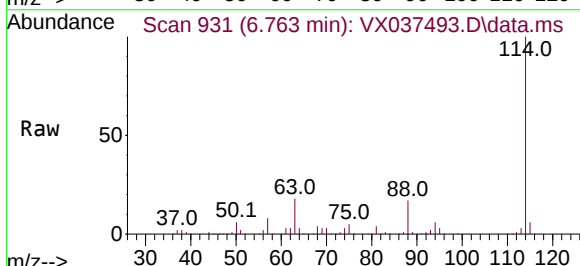



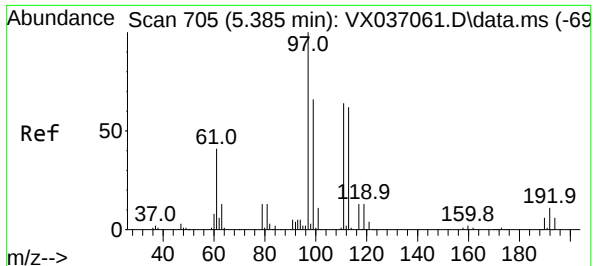


#35  
Dibromofluoromethane  
Concen: 45.239 ug/l  
RT: 5.385 min Scan# 705  
Delta R.T. 0.000 min  
Lab File: VX037493.D  
Acq: 02 Sep 2023 19:14

Instrument :  
MSVOA\_X  
ClientSampleId :  
OW-01B-67-083123



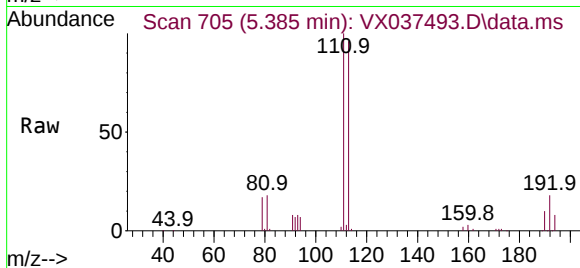



Tgt Ion:113 Resp: 78529  
Ion Ratio Lower Upper  
113 100  
111 102.8 82.9 124.3  
192 18.7 13.3 19.9

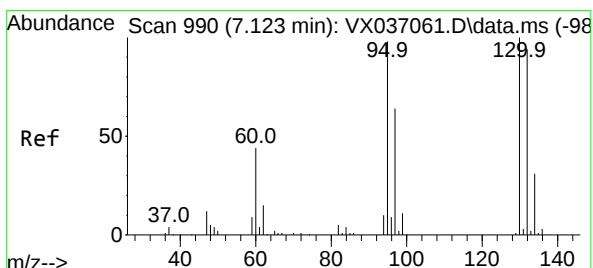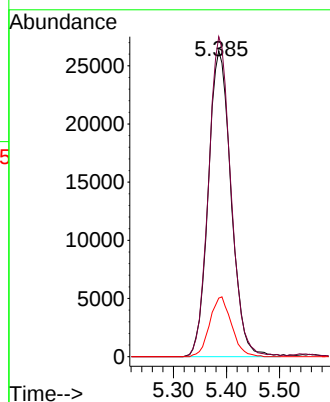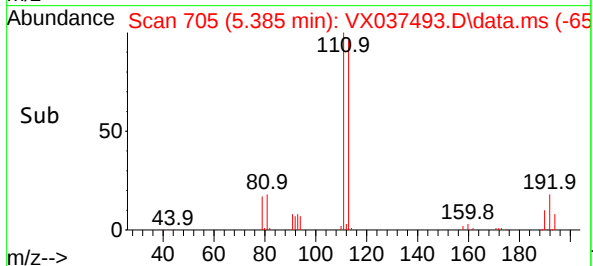

#44  
Trichloroethene  
Concen: 4.330 ug/l  
RT: 7.129 min Scan# 991  
Delta R.T. 0.006 min  
Lab File: VX037493.D  
Acq: 02 Sep 2023 19:14

Tgt Ion:130 Resp: 8685  
Ion Ratio Lower Upper  
130 100  
95 95.6 0.0 204.4


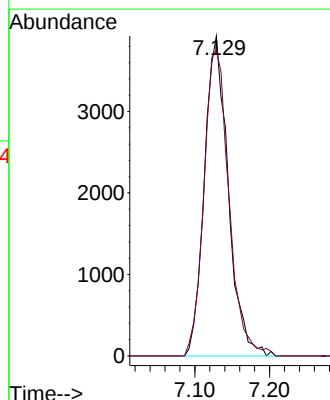
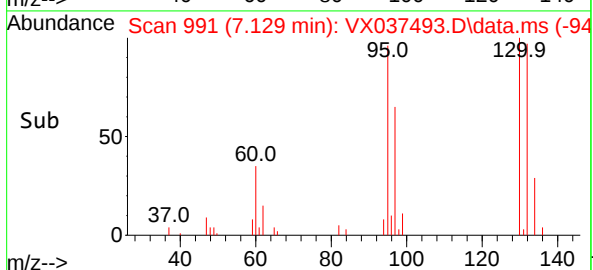
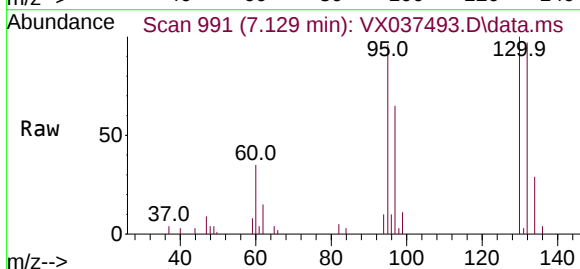


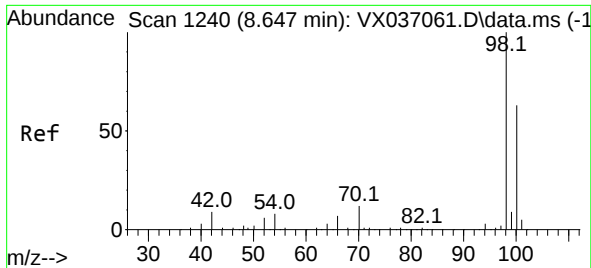

#50  
Toluene-d8  
Concen: 48.309 ug/l  
RT: 8.647 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VX037493.D  
Acq: 02 Sep 2023 19:14




Instrument :  
MSVOA\_X  
ClientSampleId :  
OW-01B-67-083123


Tgt Ion: 98 Resp: 304187  
Ion Ratio Lower Upper  
98 100  
100 67.2 53.1 79.7

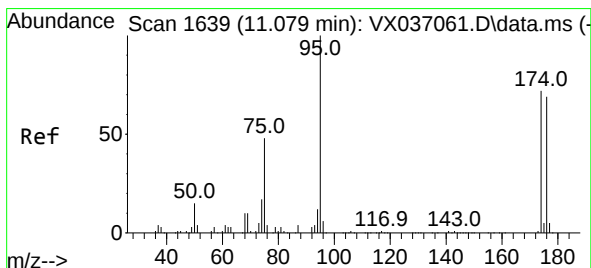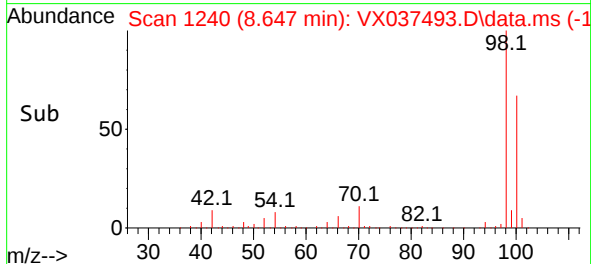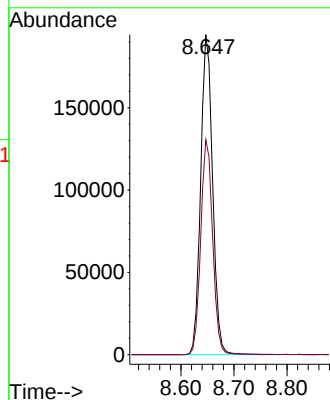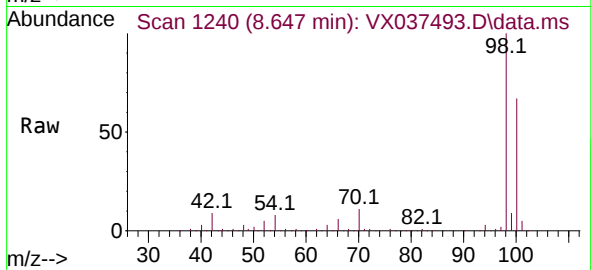

#62  
4-Bromofluorobenzene  
Concen: 44.118 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. 0.000 min  
Lab File: VX037493.D  
Acq: 02 Sep 2023 19:14

Tgt Ion: 95 Resp: 109170  
Ion Ratio Lower Upper  
95 100  
174 75.6 0.0 135.6  
176 71.9 0.0 131.0


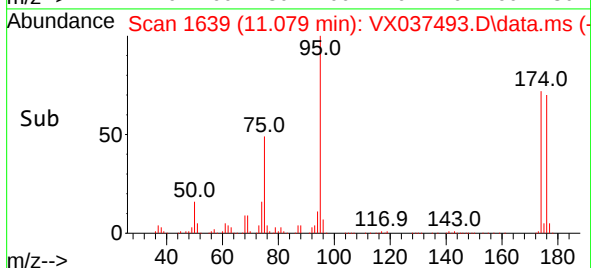
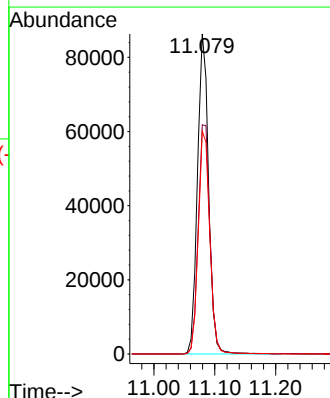
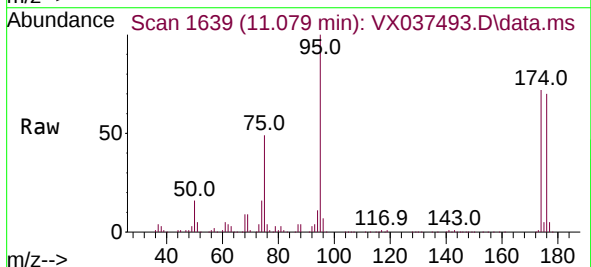


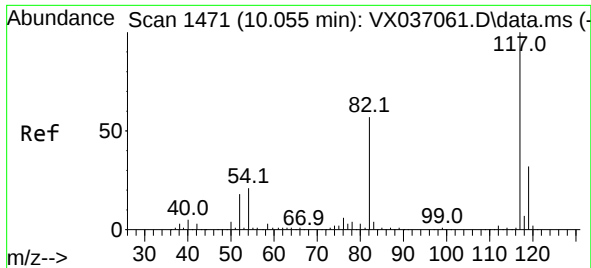

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. 0.000 min  
Lab File: VX037493.D  
Acq: 02 Sep 2023 19:14




Instrument :  
MSVOA\_X  
ClientSampleId :  
OW-01B-67-083123


Tgt Ion:117 Resp: 232304  
Ion Ratio Lower Upper  
117 100  
82 53.6 46.2 69.4  
119 31.6 25.5 38.3

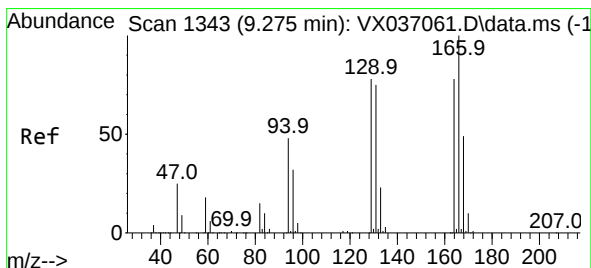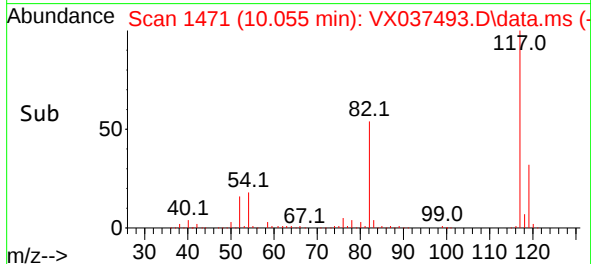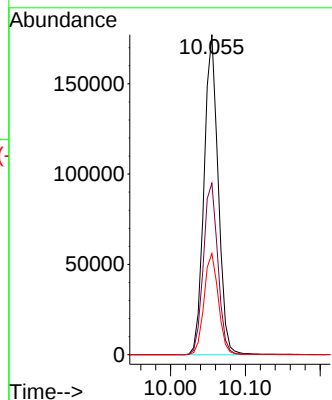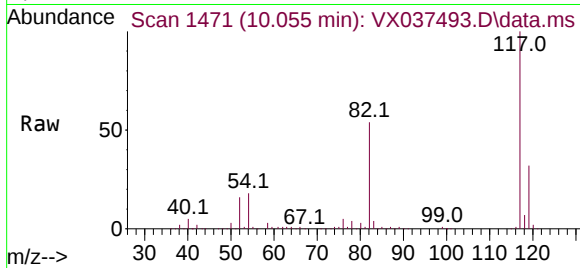

#64  
Tetrachloroethene  
Concen: 0.485 ug/l  
RT: 9.275 min Scan# 1343  
Delta R.T. 0.000 min  
Lab File: VX037493.D  
Acq: 02 Sep 2023 19:14

Tgt Ion:164 Resp: 822  
Ion Ratio Lower Upper  
164 100  
166 138.3 102.7 154.1  
129 142.2 80.4 120.6#  
131 120.5 76.5 114.7#

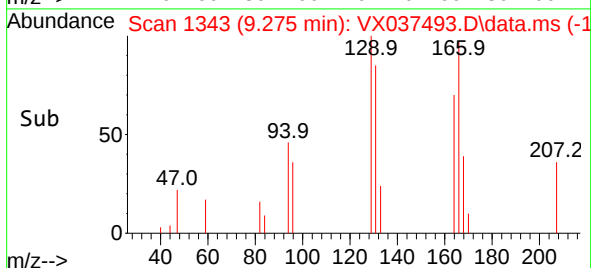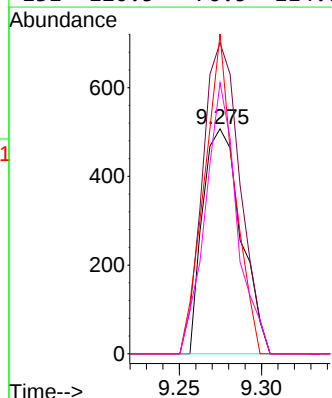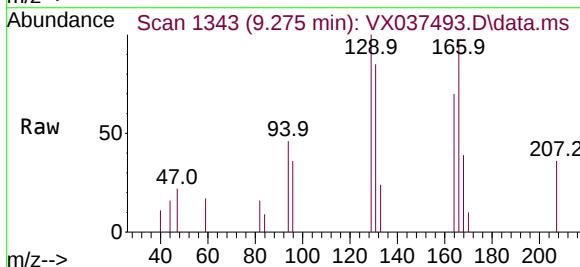

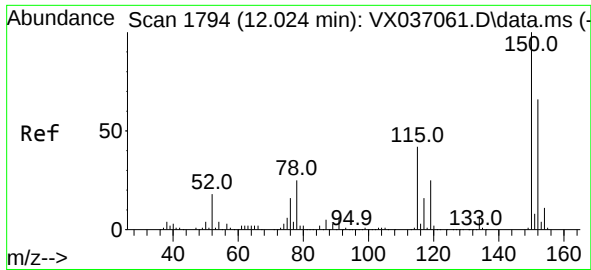

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX037493.D


Acq: 02 Sep 2023 19:14

Instrument :

MSVOA\_X

ClientSampleId :

OW-01B-67-083123

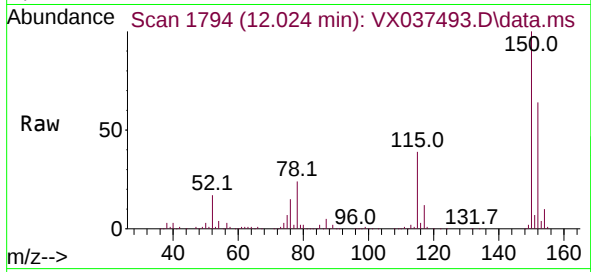

Tgt Ion:152 Resp: 102984

Ion Ratio Lower Upper

152 100

115 62.5 43.3 129.9

150 156.0 0.0 345.0

