

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090223\
 Data File : VX037481.D
 Acq On : 02 Sep 2023 14:28
 Operator : JC/MD
 Sample : 04270-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-033123

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M

Title : SW846 8260

Signal : TIC: VX037481.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.392	208	214	226	rVB2	4108	8400	1.09%	0.207%
2	2.794	273	280	288	rBV	5234	10388	1.35%	0.256%
3	5.385	693	705	721	rBV	87449	256675	33.30%	6.336%
4	5.550	721	732	748	rVV	166301	469580	60.92%	11.591%
5	5.958	785	799	815	rBV	94974	253682	32.91%	6.262%
6	6.763	920	931	949	rBV	244214	584188	75.79%	14.420%
7	8.580	1223	1229	1234	rBV	12609	20992	2.72%	0.518%
8	8.647	1234	1240	1249	rVV	499609	770811	100.00%	19.026%
9	10.055	1465	1471	1482	rBV	479612	645661	83.76%	15.937%
10	11.079	1634	1639	1653	rBV	375382	470235	61.01%	11.607%
11	12.024	1788	1794	1805	rBV	435966	560732	72.75%	13.841%




Sum of corrected areas: 4051344

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090223\
Data File : VX037481.D
Acq On : 02 Sep 2023 14:28
Operator : JC/MD
Sample : 04270-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-033123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

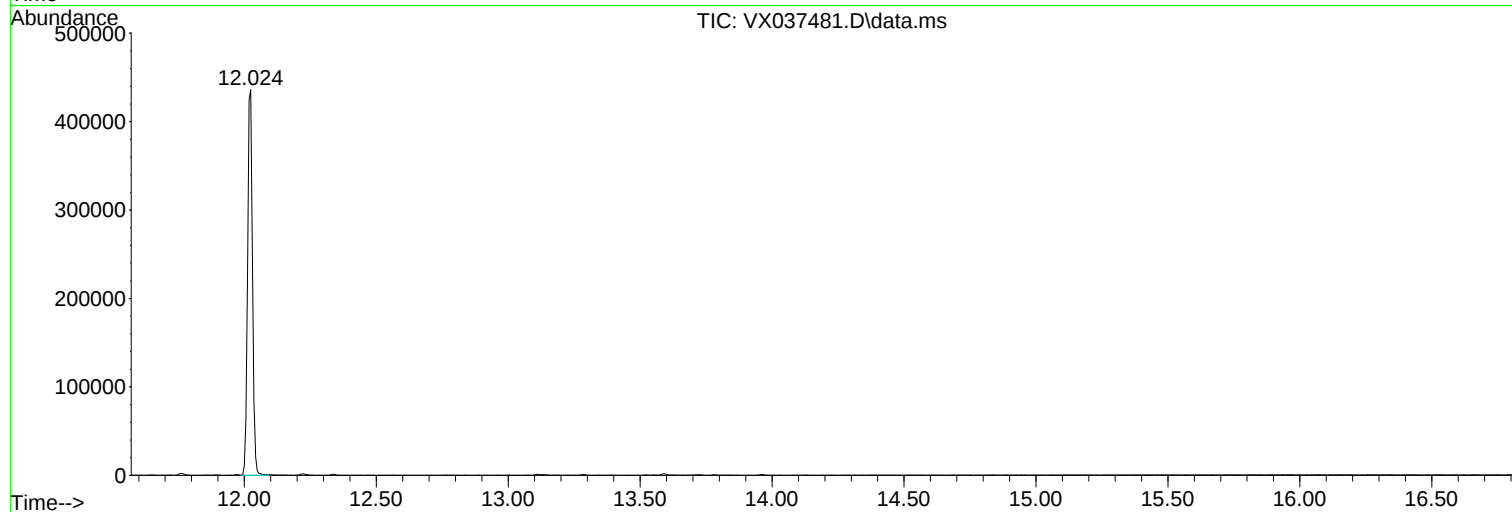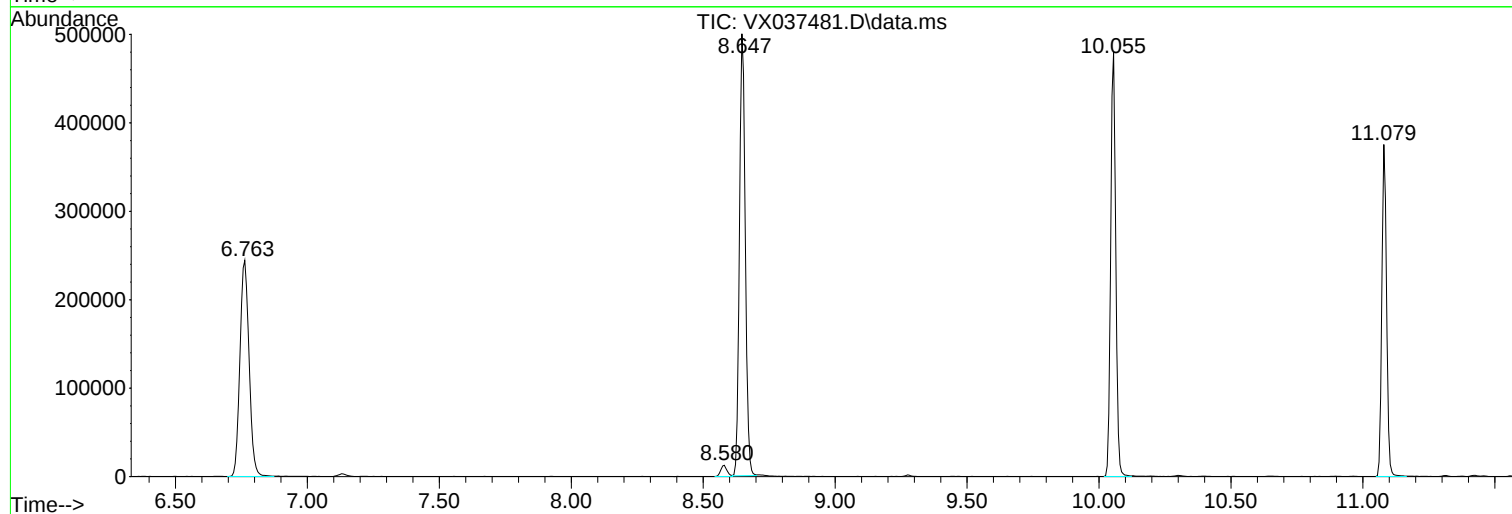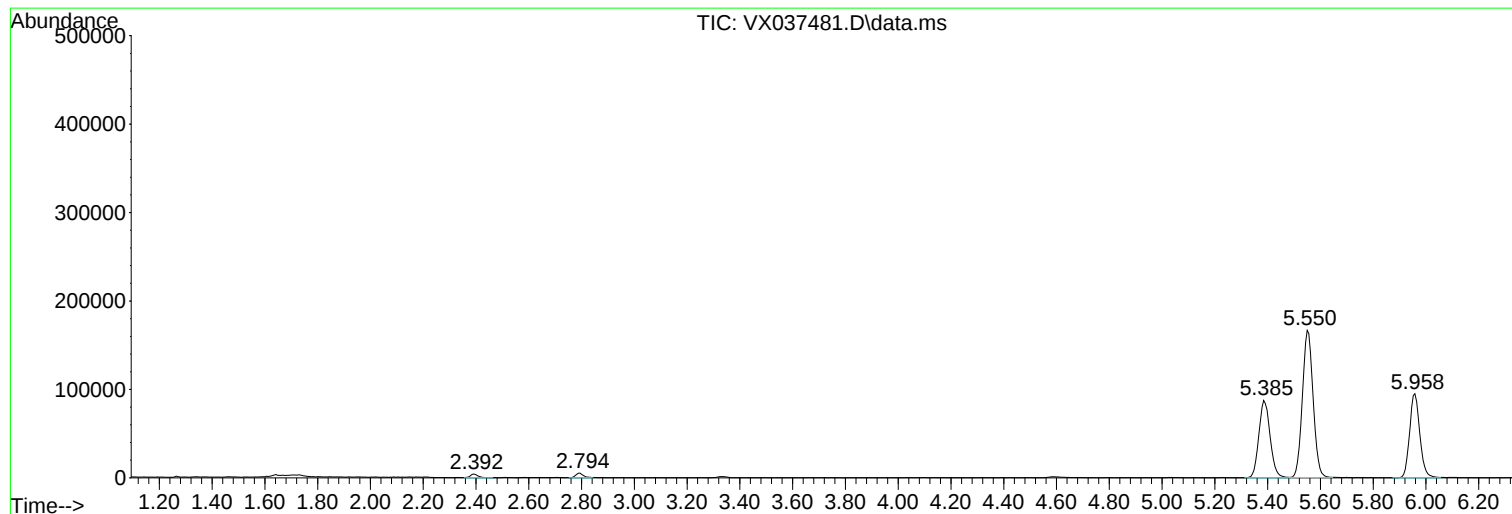

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090223\
Data File : VX037481.D
Acq On : 02 Sep 2023 14:28
Operator : JC/MD
Sample : 04270-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-033123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090223\
Data File : VX037481.D
Acq On : 02 Sep 2023 14:28
Operator : JC/MD
Sample : 04270-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-033123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------