


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090319\
Data File : VX012017.D
Acq On : 03 Sep 2019 11:09
Operator : SY/SP
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_X/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X090319S.M
Title : SW846 8260
Last Update : Tue Sep 03 12:11:35 2019

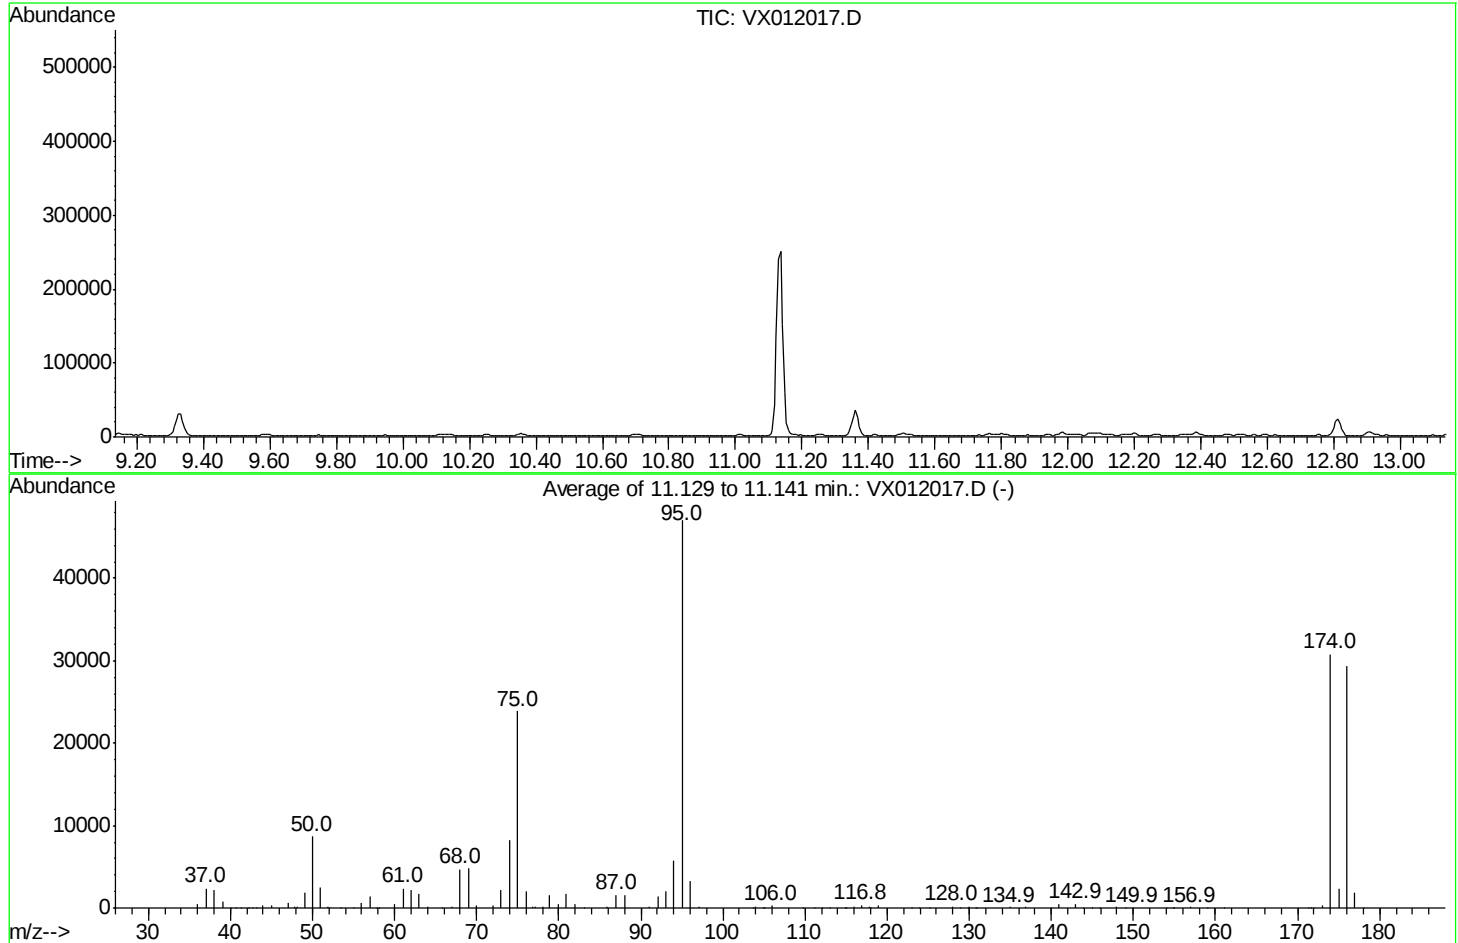

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	8645	PASS
75	95	30	60	50.8	23901	PASS
95	95	100	100	100.0	47034	PASS
96	95	5	9	7.0	3270	PASS
173	174	0.00	2	1.0	313	PASS
174	95	50	100	65.4	30757	PASS
175	174	5	9	7.7	2374	PASS
176	174	95	101	95.6	29392	PASS
177	176	5	9	6.2	1811	PASS