

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
 Data File : VX031118.D
 Acq On : 04 Sep 2022 05:55
 Operator : JC/MD
 Sample : N4479-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-11

Quant Time: Sep 06 01:32:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 02 02:49:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	213500	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	333346	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	310007	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	142265	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	132381	48.190	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	96.380%
35) Dibromofluoromethane	5.391	113	126287	51.913	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.820%
50) Toluene-d8	8.653	98	442984	49.479	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	98.960%
62) 4-Bromofluorobenzene	11.079	95	160428	50.733	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	101.460%


Target Compounds						Qvalue
3) Chloromethane	1.295	50	497	0.934	ug/l #	78
6) Chloroethane	1.709	64	429	1.985	ug/l #	41
10) Methyl Iodide	2.453	142	327	3.033	ug/l #	76
11) Tert butyl alcohol	2.941	59	5555	Below Cal	#	74
13) Acrolein	2.252	56	334	0.664	ug/l	90
16) Acetone	2.392	43	23970	22.602	ug/l	93
18) Methyl Acetate	2.709	43	2417	0.793	ug/l	95
20) Methylene Chloride	2.788	84	14737	3.681	ug/l #	82
25) 2-Butanone	4.574	43	7985	4.877	ug/l #	66
29) Tetrahydrofuran	5.032	42	923	0.874	ug/l #	72
31) Cyclohexane	5.550	56	3287	0.876	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	13299	3.903	ug/l #	48
37) Ethyl Acetate	4.715	43	23788	8.035	ug/l #	90
38) Carbon Tetrachloride	5.550	117	20725	5.860	ug/l #	17
40) Benzene	6.044	78	4164	0.426	ug/l #	65
43) Isopropyl Acetate	6.342	43	104794	22.648	ug/l #	92
48) Methyl methacrylate	7.800	41	94642	40.515	ug/l #	42
49) 1,4-Dioxane	7.806	88	155	2.182	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	79745	26.810	ug/l #	51
52) Toluene	8.720	92	4872	0.768	ug/l	90
53) t-1,3-Dichloropropene	8.958	75	887	0.255	ug/l #	42
54) cis-1,3-Dichloropropene	8.549	75	46893	12.079	ug/l #	56
57) 1,3-Dichloropropane	9.482	76	5680	1.332	ug/l #	42
59) 2-Hexanone	9.379	43	89870	39.953	ug/l #	24
68) m/p-Xylenes	10.305	106	2242	0.451	ug/l	98
69) o-Xylene	10.640	106	1548	0.317	ug/l	95
70) Styrene	10.659	104	2194	0.278	ug/l #	83
74) N-amyl acetate	10.775	43	892	0.258	ug/l #	49
76) 1,2,3-Trichloropropane	11.079	75	74093	22.032	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	74093	69.240	ug/l #	13
85) sec-Butylbenzene	11.756	105	4636	0.368	ug/l #	56
95) Naphthalene	13.774	128	49574	3.844	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031118.D
Acq On : 04 Sep 2022 05:55
Operator : JC/MD
Sample : N4479-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-11

Quant Time: Sep 06 01:32:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 02 02:49:21 2022
Response via : Initial Calibration




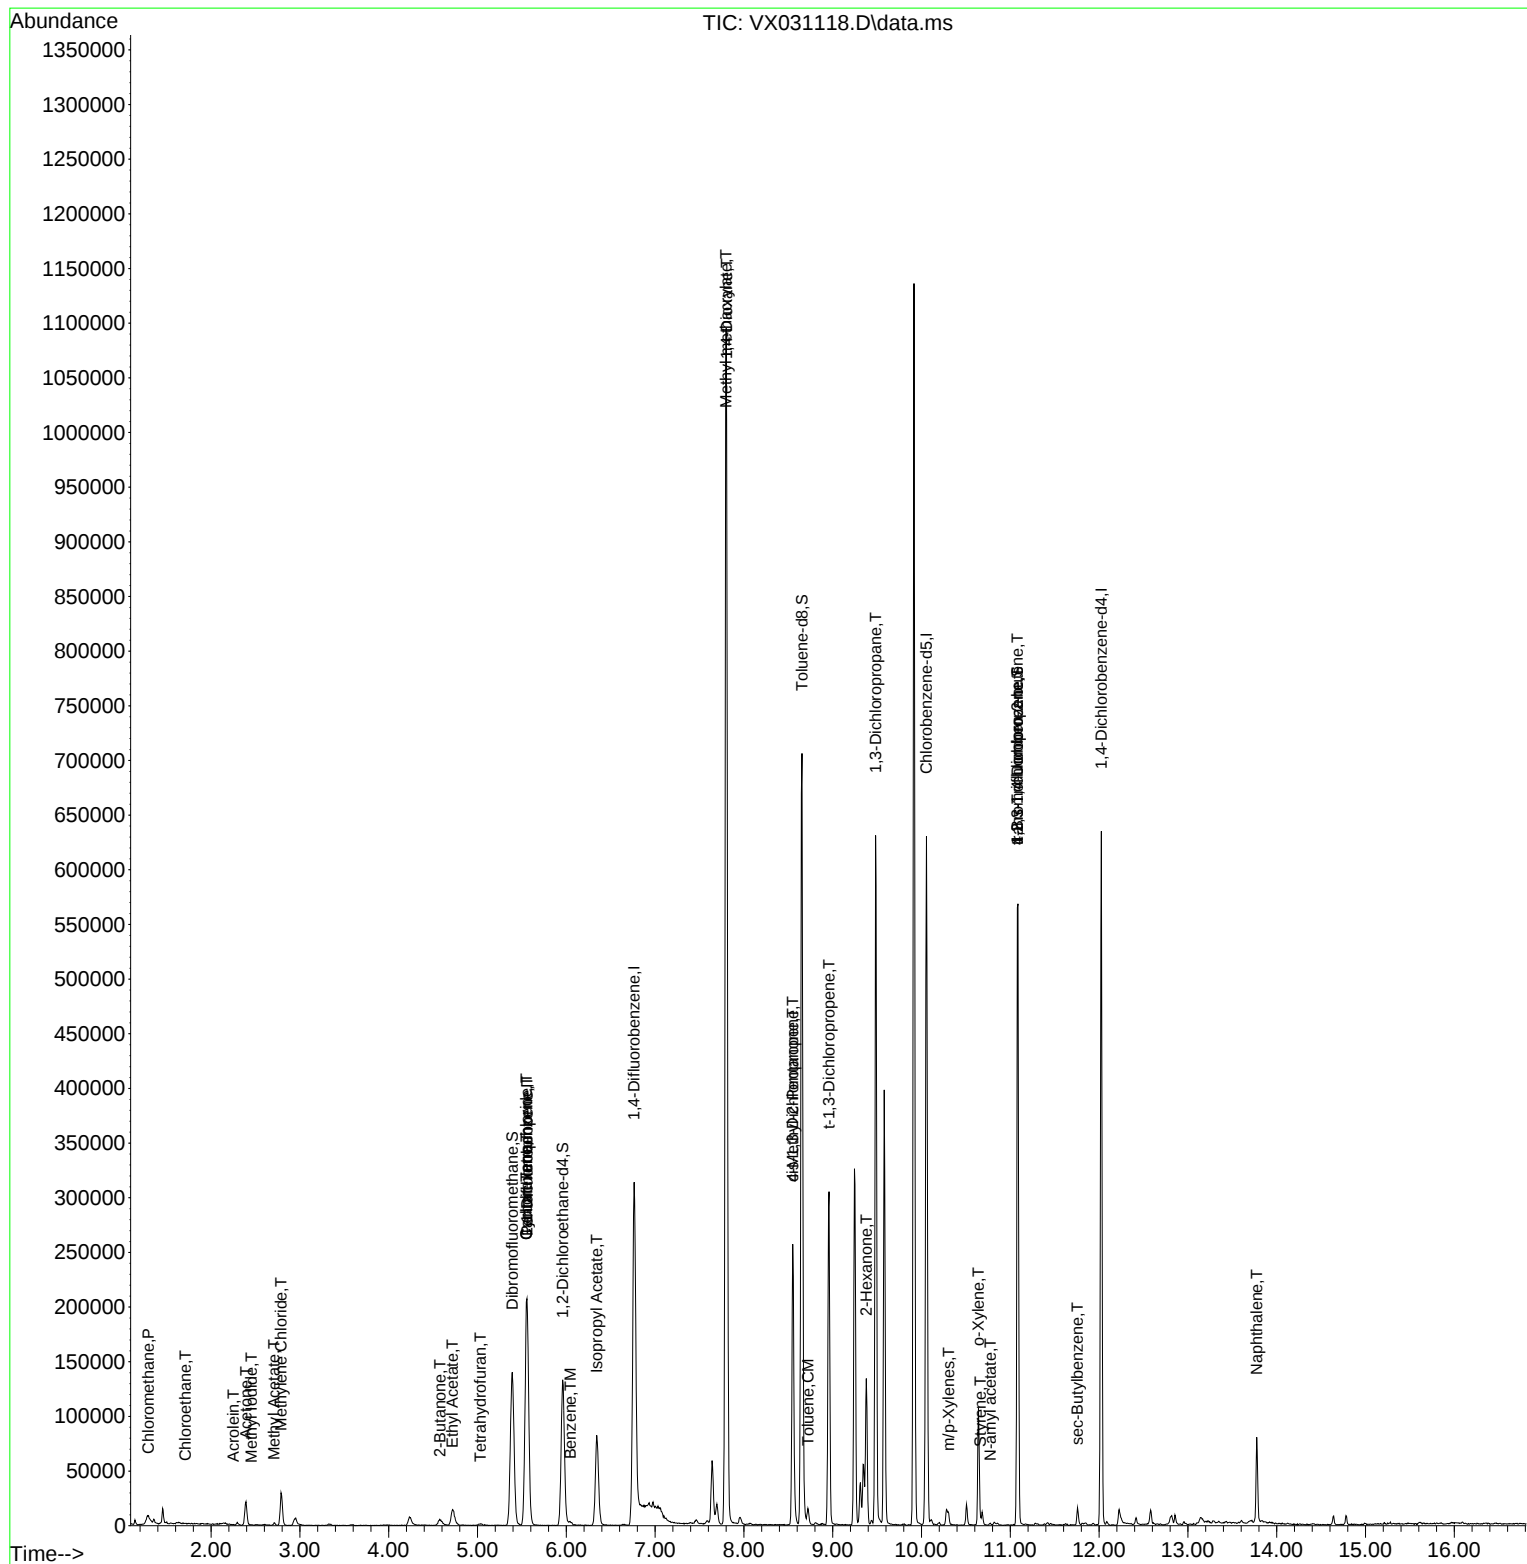




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.000 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55




Instrument :
MSVOA_X
ClientSampleId :
SB-11


Tgt Ion:168 Resp: 213500
Ion Ratio Lower Upper
168 100
99 52.6 44.0 66.0

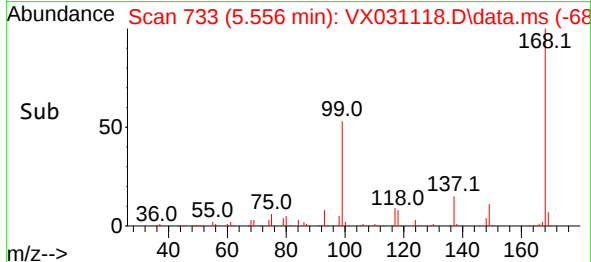

#3
Chloromethane
Concen: 0.934 ug/l
RT: 1.295 min Scan# 34
Delta R.T. 0.007 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55

Tgt Ion: 50 Resp: 497
Ion Ratio Lower Upper
50 100
52 20.2 26.3 39.5#


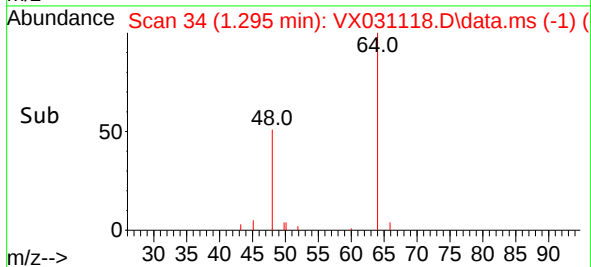

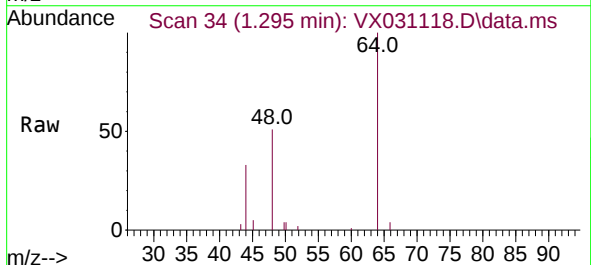


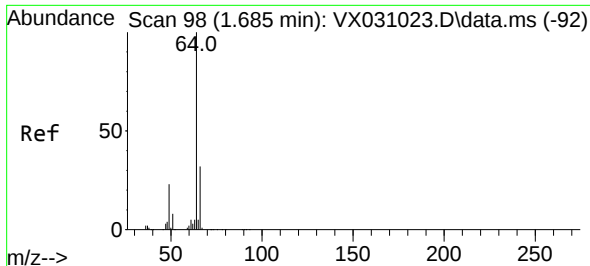

#6
Chloroethane
Concen: 1.985 ug/l
RT: 1.709 min Scan# 102
Delta R.T. 0.024 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55




Instrument :
MSVOA_X
ClientSampleId :
SB-11


Tgt Ion: 64 Resp: 429
Ion Ratio Lower Upper
64 100
66 0.0 27.2 40.8#

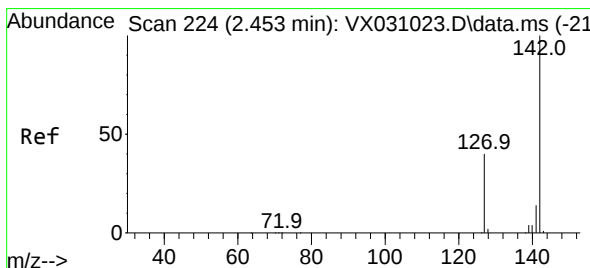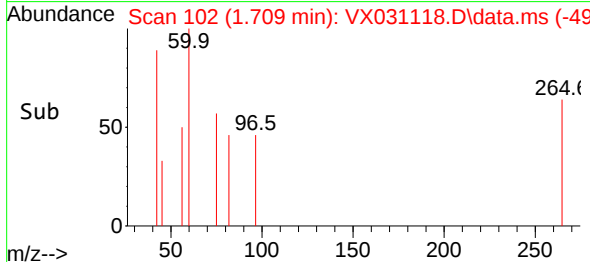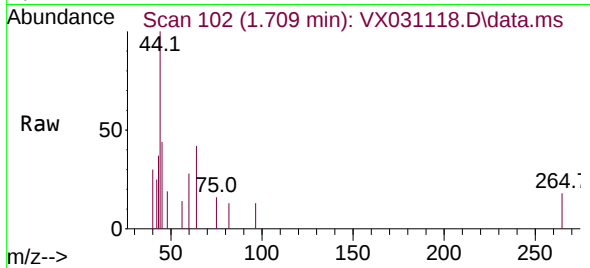

#10
Methyl Iodide
Concen: 3.033 ug/l
RT: 2.453 min Scan# 224
Delta R.T. -0.000 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55

Tgt Ion: 142 Resp: 327
Ion Ratio Lower Upper
142 100
127 26.0 30.2 45.2#
141 0.0 11.3 16.9#


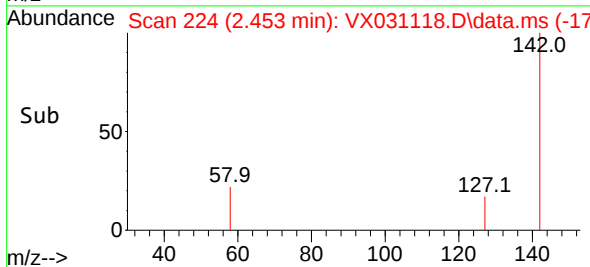

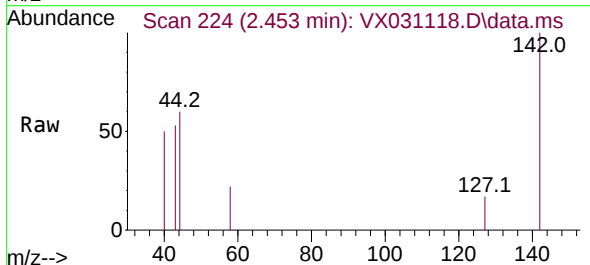


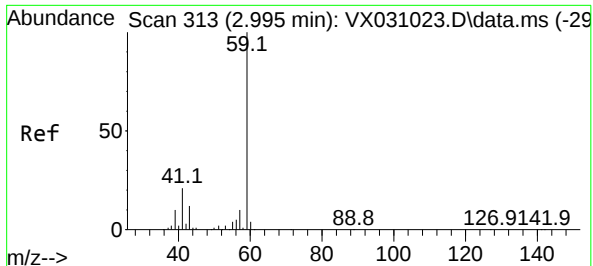

#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.941 min Scan# 30
Delta R.T. -0.048 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55




Instrument :
MSVOA_X
ClientSampleId :
SB-11


Tgt Ion: 59 Resp: 5555
Ion Ratio Lower Upper
59 100
57 0.0 7.4 11.2#

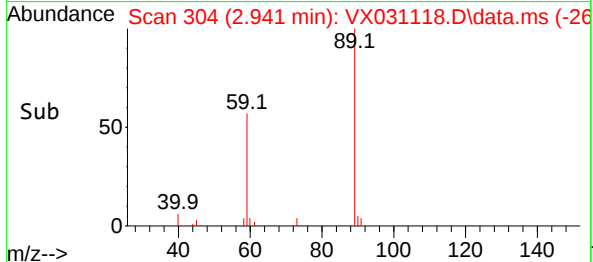

#13
Acrolein
Concen: 0.664 ug/l
RT: 2.252 min Scan# 191
Delta R.T. 0.013 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55

Tgt Ion: 56 Resp: 334
Ion Ratio Lower Upper
56 100
55 79.0 56.6 84.8


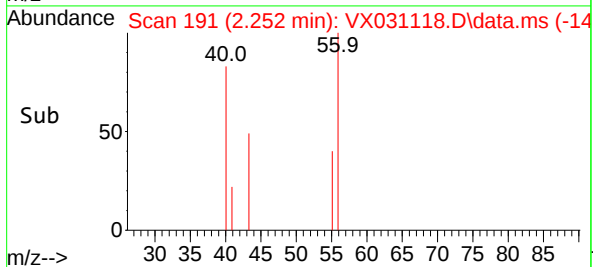

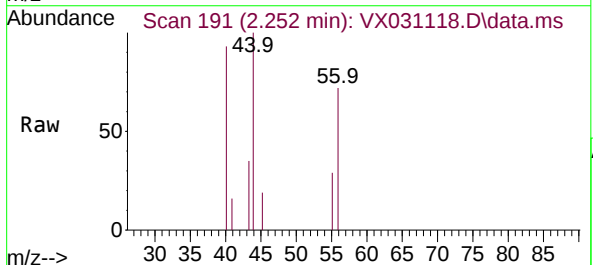




#16
Acetone
Concen: 22.602 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55




Instrument :
MSVOA_X
ClientSampleId :
SB-11


Tgt Ion: 43 Resp: 23970
Ion Ratio Lower Upper
43 100
58 30.6 27.7 41.5

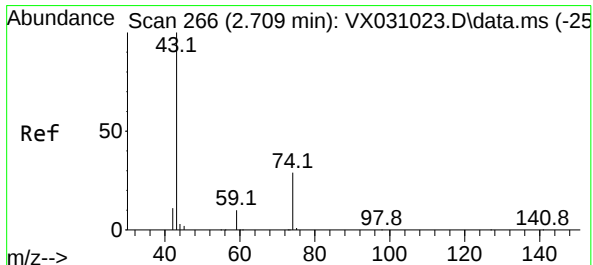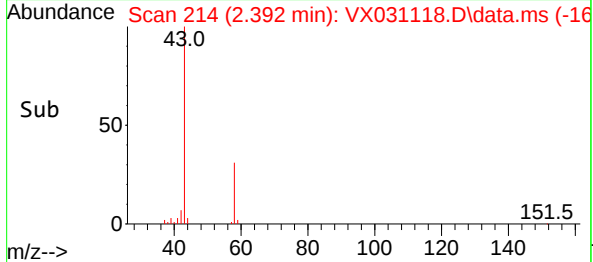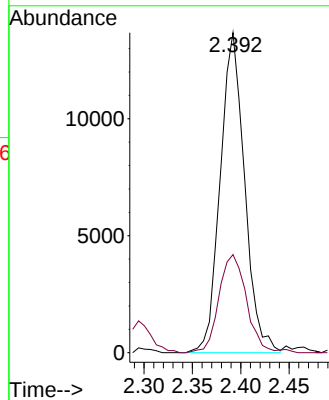

#18
Methyl Acetate
Concen: 0.793 ug/l
RT: 2.709 min Scan# 266
Delta R.T. -0.000 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55

Tgt Ion: 43 Resp: 2417
Ion Ratio Lower Upper
43 100
74 26.7 19.4 29.2


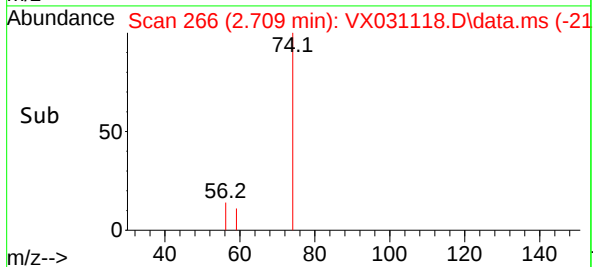
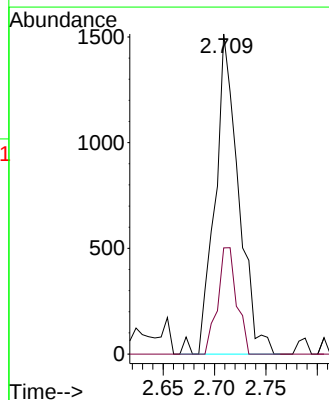
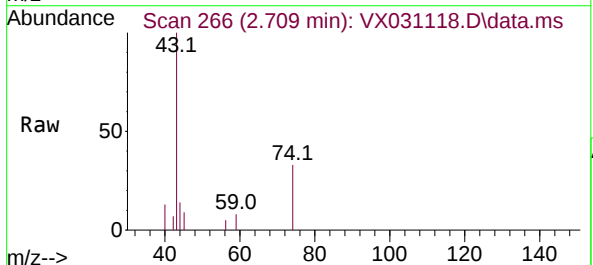


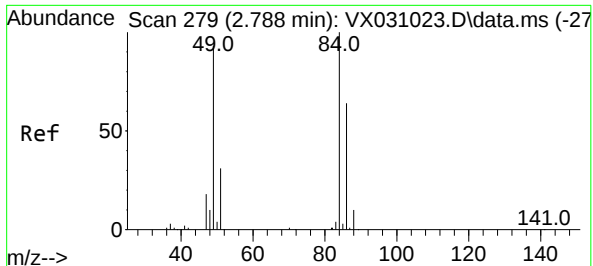

#20
Methylene Chloride
Concen: 3.681 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55




Instrument :
MSVOA_X
ClientSampleId :
SB-11


Tgt Ion:	84	Resp:	14737
Ion	Ratio	Lower	Upper
84	100		
49	91.2	93.8	140.6#
51	27.5	29.4	44.0#
86	71.7	51.0	76.4

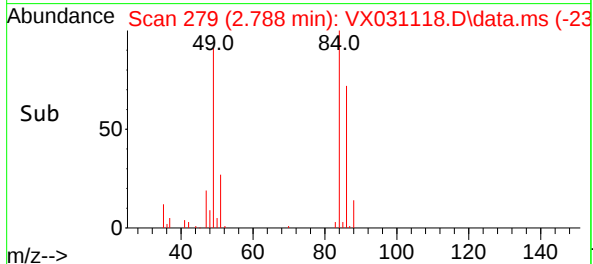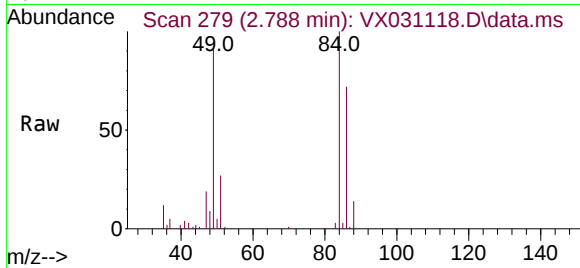

#25
2-Butanone
Concen: 4.877 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.006 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55

Tgt Ion:	43	Resp:	7985
Ion	Ratio	Lower	Upper
43	100		
72	44.5	21.7	32.5#

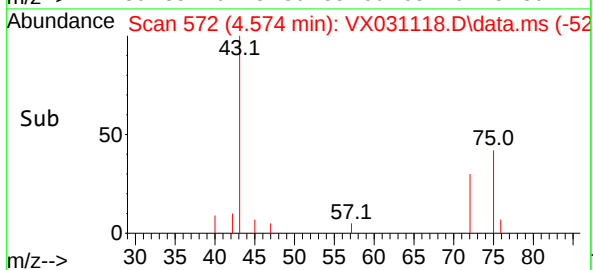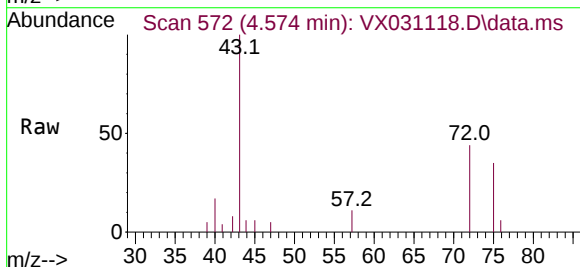

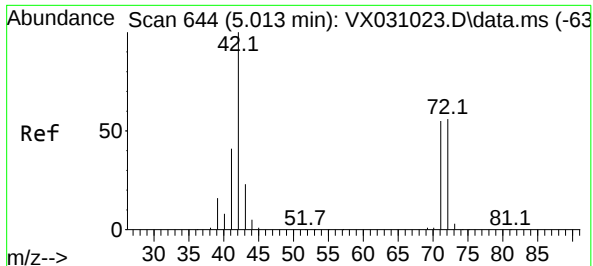

#29

Tetrahydrofuran

Concen: 0.874 ug/l

RT: 5.032 min Scan# 644

Delta R.T. 0.019 min

Lab File: VX031118.D

Acq: 04 Sep 2022 05:55

Instrument :

MSVOA_X

ClientSampleId :

SB-11





Tgt Ion: 42 Resp: 923

Ion Ratio Lower Upper

42 100

72 77.8 36.5 54.7#

71 39.4 33.9 50.9

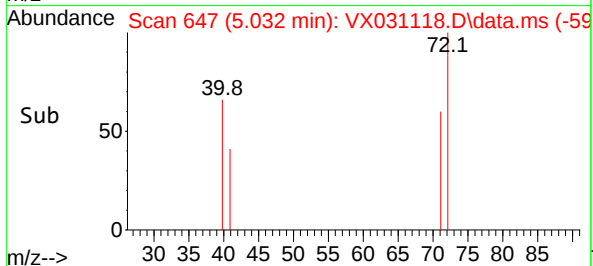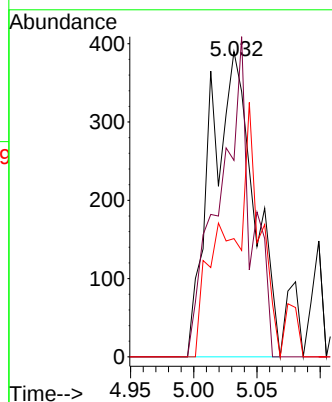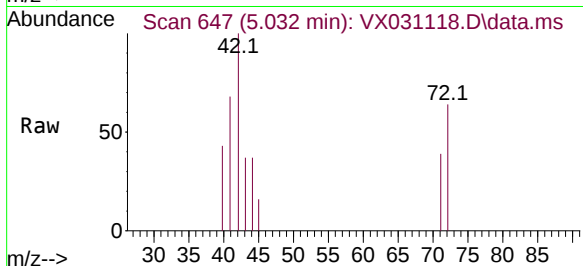

#31

Cyclohexane

Concen: 0.876 ug/l

RT: 5.550 min Scan# 732

Delta R.T. 0.073 min

Lab File: VX031118.D

Acq: 04 Sep 2022 05:55




Tgt Ion: 56 Resp: 3287


Ion Ratio Lower Upper

56 100

69 209.4 25.4 38.0#

84 143.0 68.9 103.3#

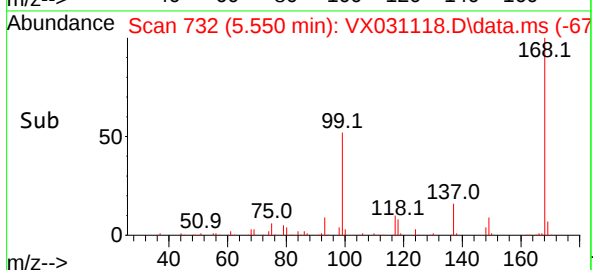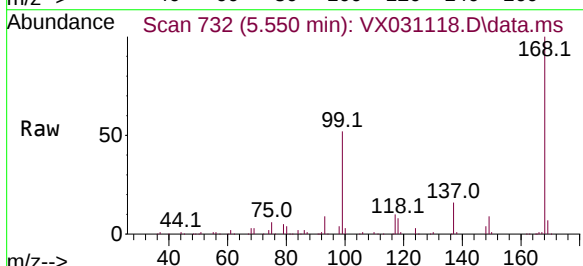



#33

1,2-Dichloroethane-d4

Concen: 48.190 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX031118.D

Acq: 04 Sep 2022 05:55

Instrument :

MSVOA_X

ClientSampleId :





SB-11

Tgt Ion: 65 Resp: 132381

Ion Ratio Lower Upper

65 100

67 52.3 0.0 109.6

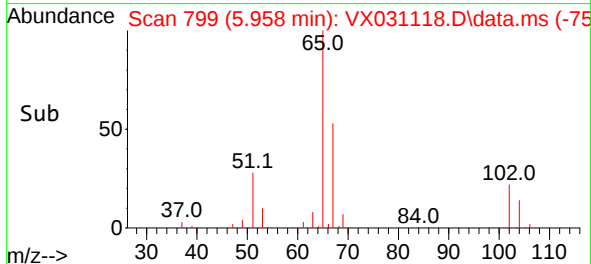

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.006 min

Lab File: VX031118.D

Acq: 04 Sep 2022 05:55




Tgt Ion: 114 Resp: 333346


Ion Ratio Lower Upper

114 100

63 16.4 0.0 38.4

88 15.7 0.0 31.8

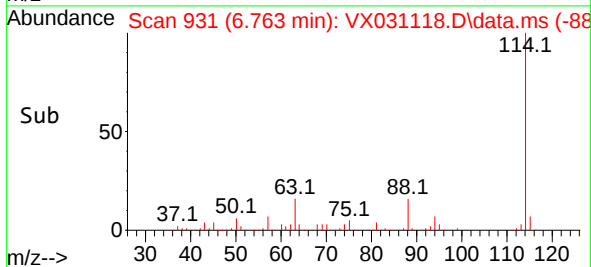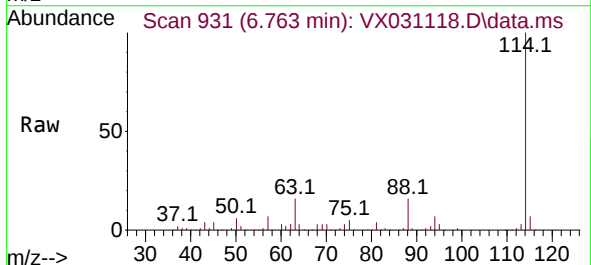

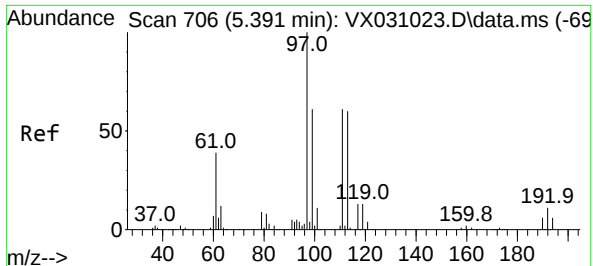

#35

Dibromofluoromethane

Concen: 51.913 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX031118.D

Acq: 04 Sep 2022 05:55

Instrument :

MSVOA_X

ClientSampleId :

SB-11





Tgt Ion:113 Resp: 126287

Ion Ratio Lower Upper

113 100

111 102.7 83.2 124.8

192 21.1 14.8 22.2

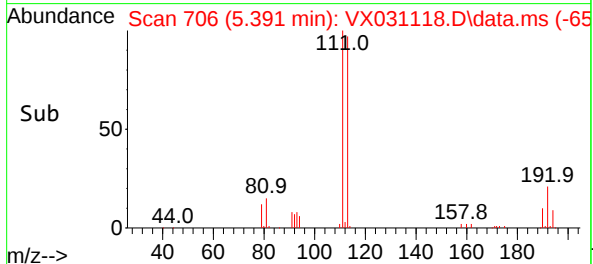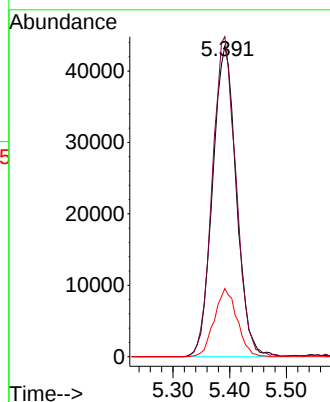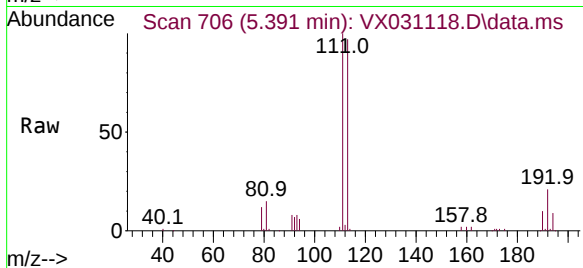

#36

1,1-Dichloropropene

Concen: 3.903 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX031118.D

Acq: 04 Sep 2022 05:55




Tgt Ion: 75 Resp: 13299


Ion Ratio Lower Upper

75 100

110 9.3 19.3 57.9#

77 0.0 24.4 36.6#

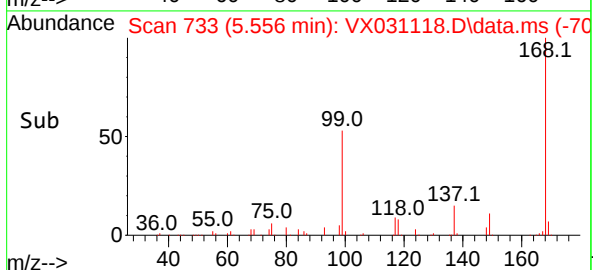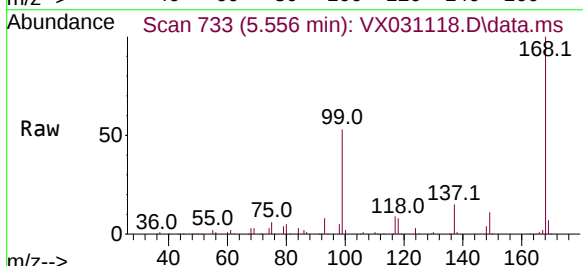



#37

Ethyl Acetate

Concen: 8.035 ug/l

RT: 4.715 min Scan# 51

Delta R.T. -0.006 min

Lab File: VX031118.D

Acq: 04 Sep 2022 05:55

Instrument :

MSVOA_X

ClientSampleId :

SB-11





Tgt Ion: 43 Resp: 23788

Ion Ratio Lower Upper

43 100

61 19.4 11.7 17.5#

70 14.5 9.3 13.9#

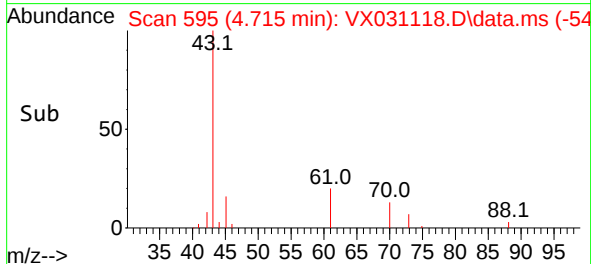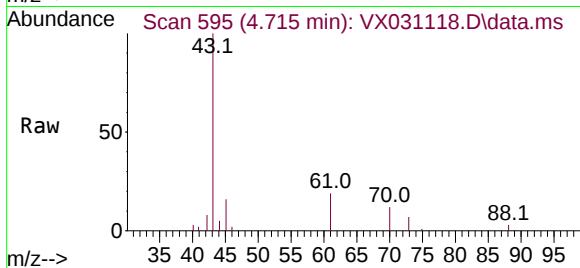

#38

Carbon Tetrachloride

Concen: 5.860 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.134 min

Lab File: VX031118.D

Acq: 04 Sep 2022 05:55




Tgt Ion: 117 Resp: 20725


Ion Ratio Lower Upper

117 100

119 5.1 74.1 111.1#

121 0.0 25.8 38.8#

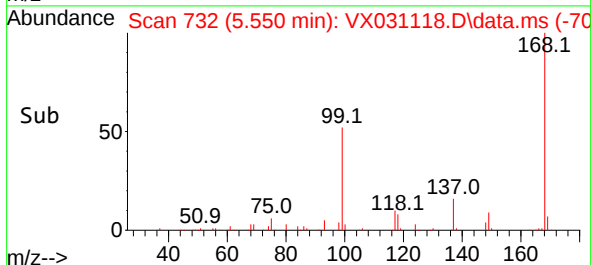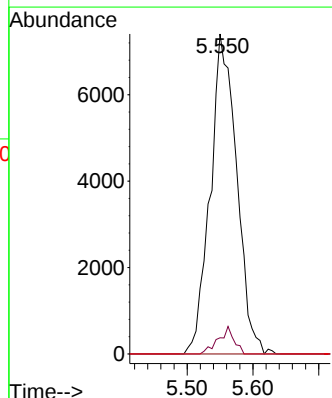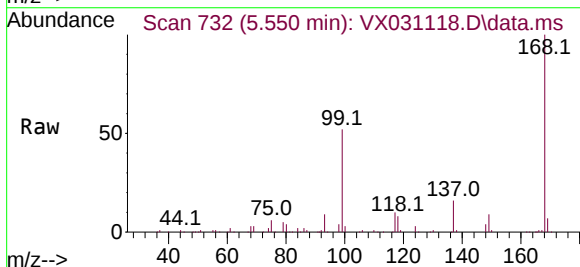



#40

Benzene

Concen: 0.426 ug/l

RT: 6.044 min Scan# 813

Delta R.T. -0.000 min

Lab File: VX031118.D

Acq: 04 Sep 2022 05:55

Instrument :

MSVOA_X

ClientSampleId :





SB-11

Tgt Ion: 78 Resp: 4164

Ion Ratio Lower Upper

78 100

77 39.3 18.0 27.0#

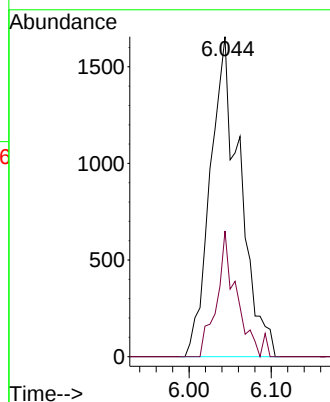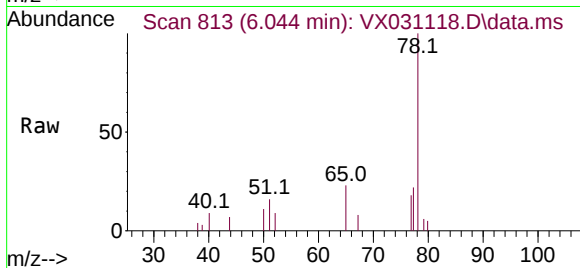

#43

Isopropyl Acetate

Concen: 22.648 ug/l

RT: 6.342 min Scan# 862

Delta R.T. -0.006 min

Lab File: VX031118.D

Acq: 04 Sep 2022 05:55




Tgt Ion: 43 Resp: 104794


Ion Ratio Lower Upper

43 100

61 23.3 16.5 24.7

87 18.4 11.1 16.7#


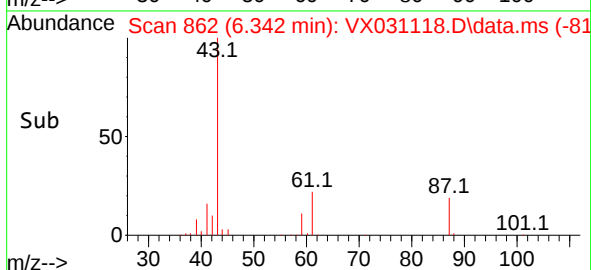

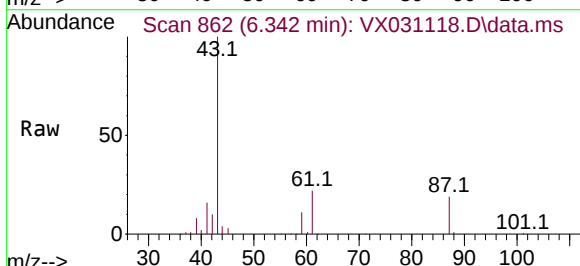


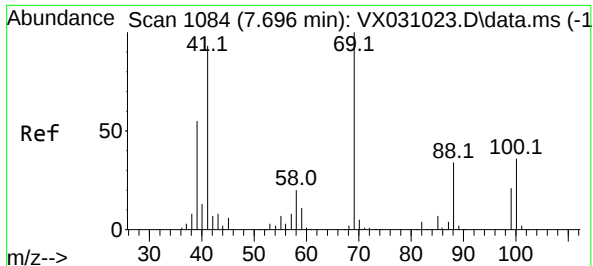

#48
Methyl methacrylate
Concen: 40.515 ug/l
RT: 7.800 min Scan# 1101
Delta R.T. 0.104 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55




Instrument :
MSVOA_X
ClientSampleId :
SB-11


Tgt Ion: 41 Resp: 94642
Ion Ratio Lower Upper
41 100
69 0.2 68.8 103.2#
39 53.0 44.6 66.8

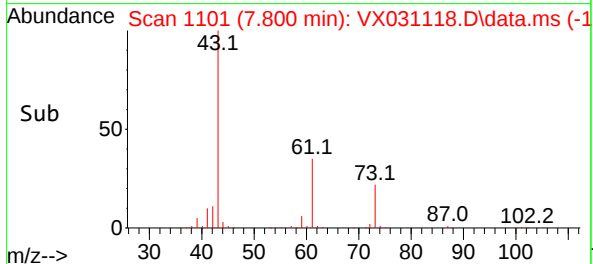

#49
1,4-Dioxane
Concen: 2.182 ug/l
RT: 7.806 min Scan# 1102
Delta R.T. 0.129 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55

Tgt Ion: 88 Resp: 155
Ion Ratio Lower Upper
88 100
43 636221.3 23.8 35.8#
58 2838.7 53.8 80.6#


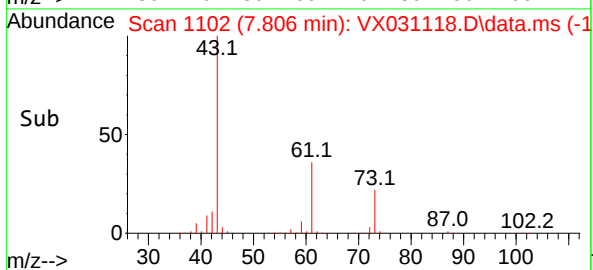

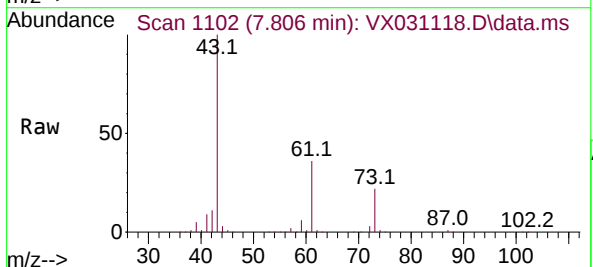




#50
Toluene-d8
Concen: 49.479 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55




Instrument :
MSVOA_X
ClientSampleId :
SB-11


Tgt Ion: 98 Resp: 442984
Ion Ratio Lower Upper
98 100
100 64.7 52.3 78.5

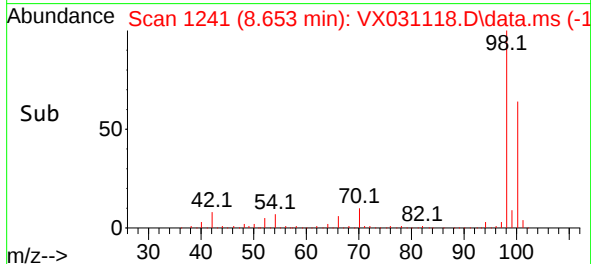

#51
4-Methyl-2-Pentanone
Concen: 26.810 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.031 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55

Tgt Ion: 43 Resp: 79745
Ion Ratio Lower Upper
43 100
58 9.0 31.4 47.2#


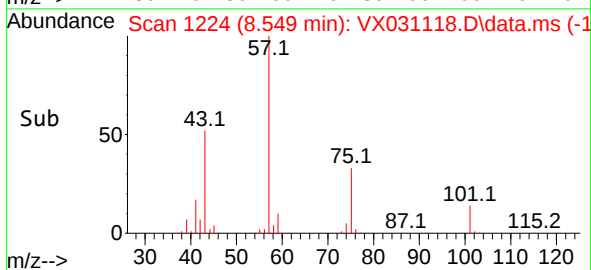

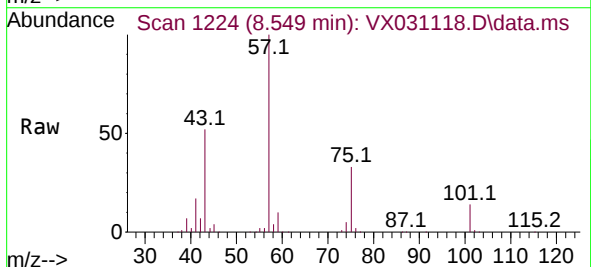




#52
Toluene
Concen: 0.768 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55




Instrument :
MSVOA_X
ClientSampleId :
SB-11


Tgt Ion: 92 Resp: 4872
Ion Ratio Lower Upper
92 100
91 188.4 139.2 208.8

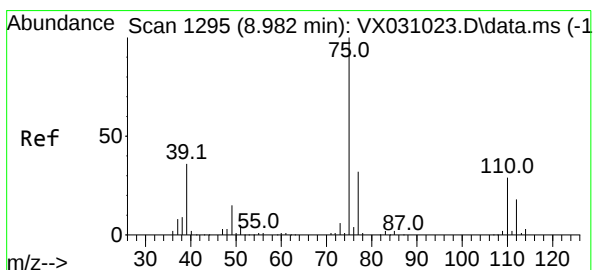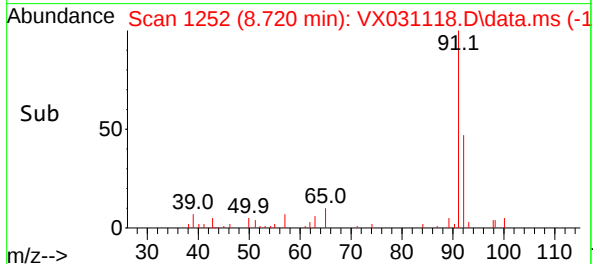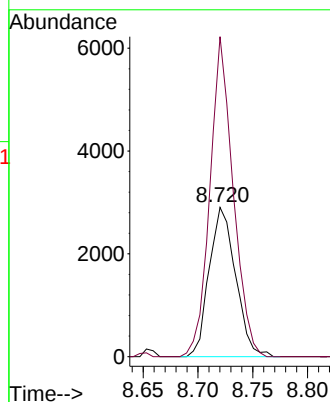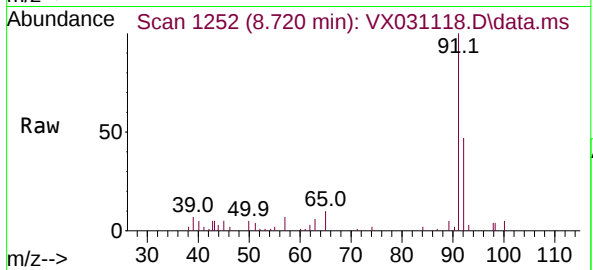

#53
t-1,3-Dichloropropene
Concen: 0.255 ug/l
RT: 8.958 min Scan# 1291
Delta R.T. -0.024 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55

Tgt Ion: 75 Resp: 887
Ion Ratio Lower Upper
75 100
77 0.0 26.3 39.5#

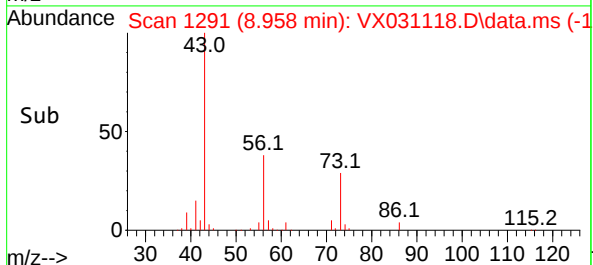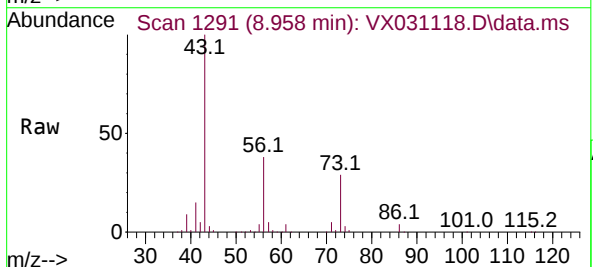

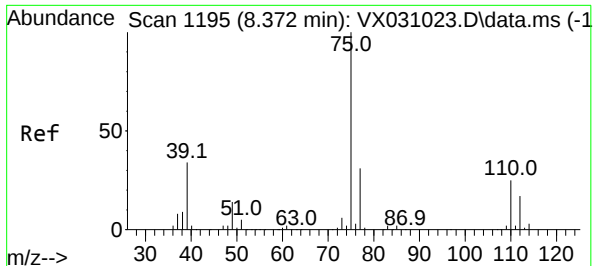

#54

cis-1,3-Dichloropropene

Concen: 12.079 ug/l

RT: 8.549 min Scan# 1195

Delta R.T. 0.177 min

Lab File: VX031118.D

Acq: 04 Sep 2022 05:55

Instrument :

MSVOA_X

ClientSampleId :

SB-11





Tgt Ion: 75 Resp: 46893

Ion Ratio Lower Upper

75 100

77 0.8 25.0 37.4#

39 22.5 37.5 56.3#

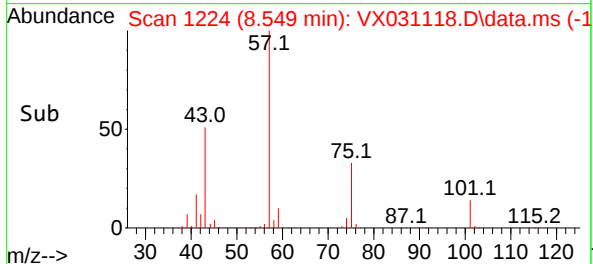

#57

1,3-Dichloropropane

Concen: 1.332 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.171 min

Lab File: VX031118.D




Acq: 04 Sep 2022 05:55


Tgt Ion: 76 Resp: 5680

Ion Ratio Lower Upper

76 100

78 0.0 25.9 38.9#

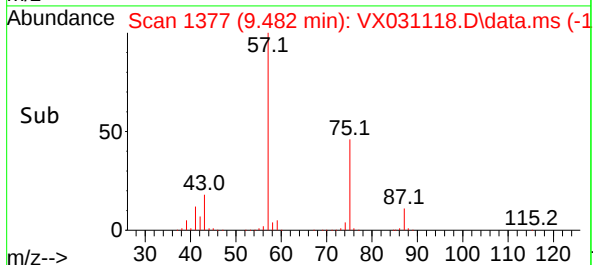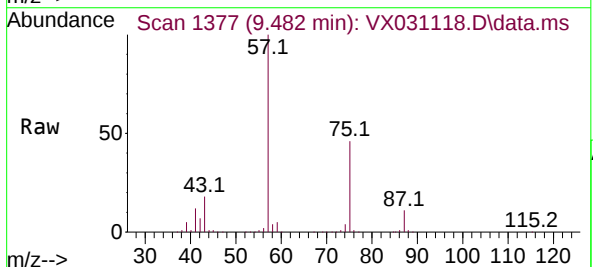



#59

2-Hexanone

Concen: 39.953 ug/l

RT: 9.379 min Scan# 11

Delta R.T. -0.054 min

Lab File: VX031118.D

Acq: 04 Sep 2022 05:55

Instrument :

MSVOA_X

ClientSampleId :





SB-11

Tgt Ion: 43 Resp: 89870

Ion Ratio Lower Upper

43 100

58 0.0 27.6 82.8#

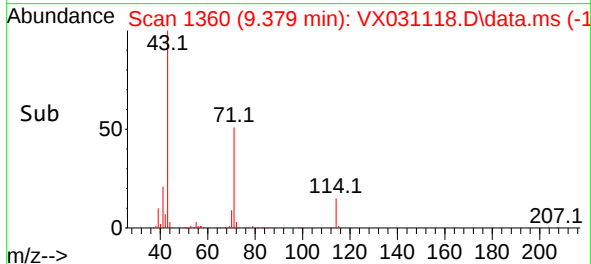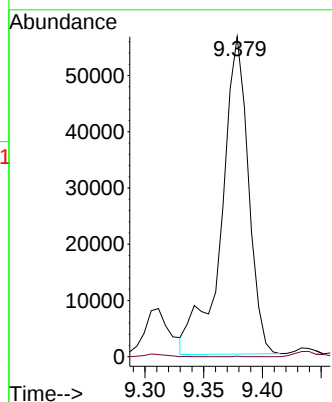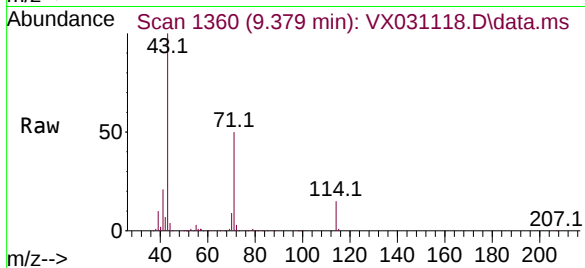

#62

4-Bromofluorobenzene

Concen: 50.733 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.006 min

Lab File: VX031118.D

Acq: 04 Sep 2022 05:55




Tgt Ion: 95 Resp: 160428


Ion Ratio Lower Upper

95 100

174 87.2 0.0 149.0

176 82.8 0.0 146.0


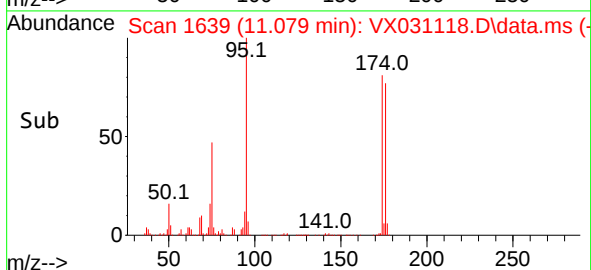

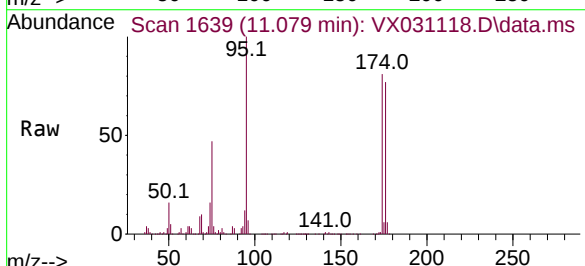




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55




Instrument :
MSVOA_X
ClientSampleId :
SB-11


Tgt Ion:117 Resp: 310007
Ion Ratio Lower Upper
117 100
82 48.5 42.7 64.1
119 31.6 25.4 38.2

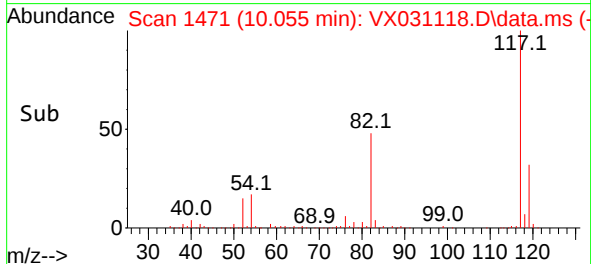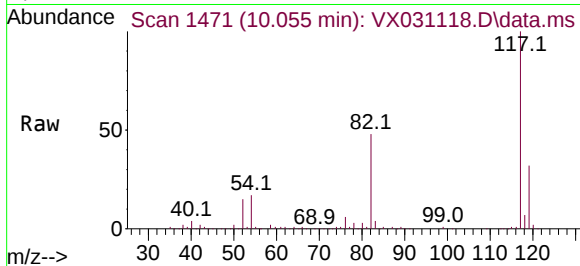

#68
m/p-Xylenes
Concen: 0.451 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55

Tgt Ion:106 Resp: 2242
Ion Ratio Lower Upper
106 100
91 201.3 158.2 237.4


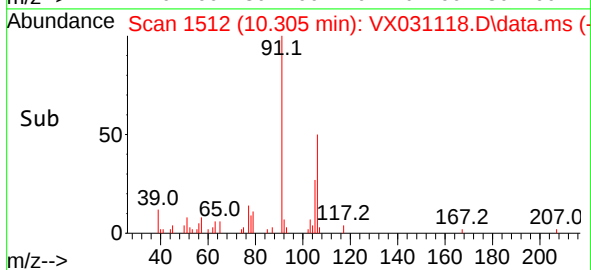

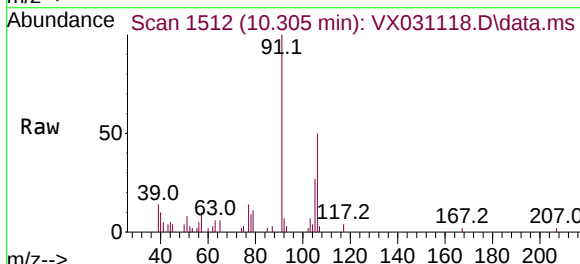




#69
o-Xylene
Concen: 0.317 ug/l
RT: 10.640 min Scan# 1568
Delta R.T. -0.006 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55




Instrument :
MSVOA_X
ClientSampleId :
SB-11


Tgt Ion:106 Resp: 1548
Ion Ratio Lower Upper
106 100
91 215.8 103.8 311.6

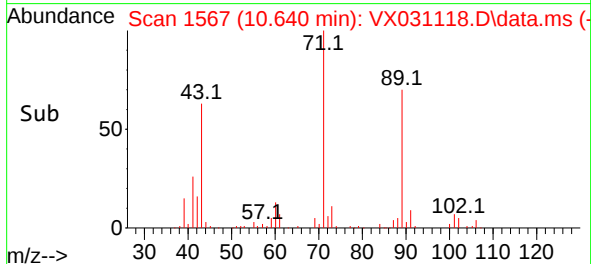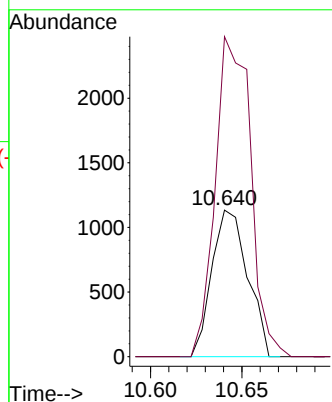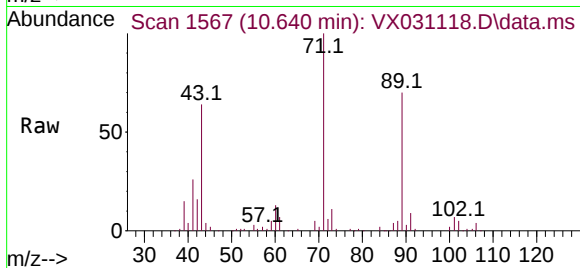

#70
Styrene
Concen: 0.278 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. -0.000 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55

Tgt Ion:104 Resp: 2194
Ion Ratio Lower Upper
104 100
78 36.1 37.8 56.8#
103 43.2 44.5 66.7#


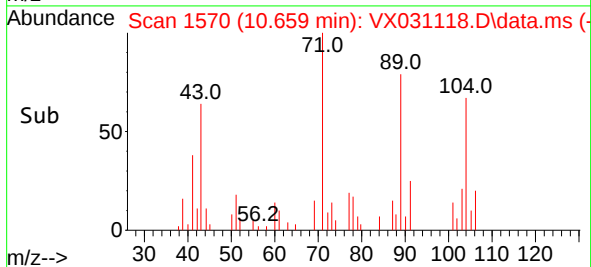

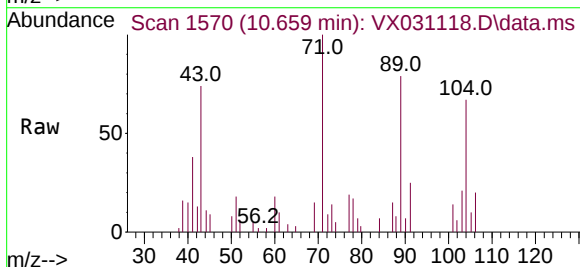




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55




Instrument :
MSVOA_X
ClientSampleId :
SB-11


Tgt Ion:152 Resp: 142265
Ion Ratio Lower Upper
152 100
115 57.5 40.5 121.5
150 156.5 0.0 347.0

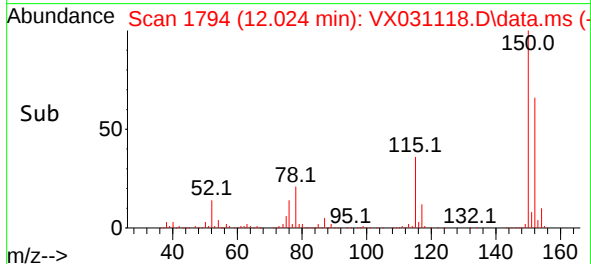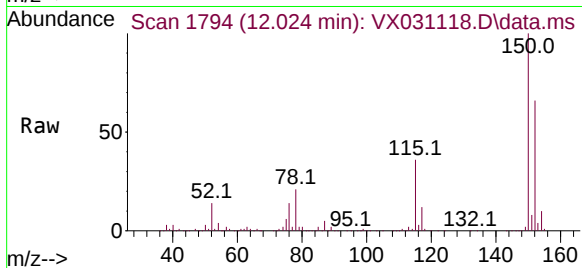

#74
N-ethyl acetate
Concen: 0.258 ug/l
RT: 10.775 min Scan# 1589
Delta R.T. -0.073 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55

Tgt Ion: 43 Resp: 892
Ion Ratio Lower Upper
43 100
70 0.0 32.3 48.5#
55 9.9 18.4 27.6#
61 0.0 19.2 28.8#


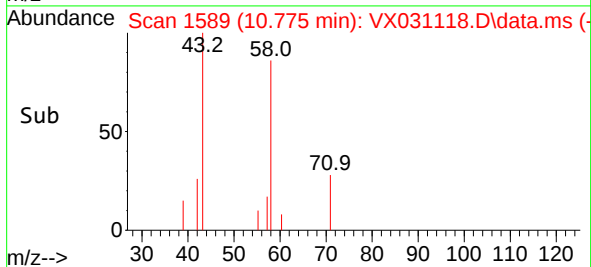

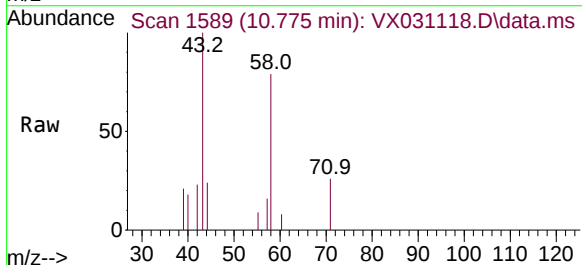




#76
1,2,3-Trichloropropane
Concen: 22.032 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55




Instrument :
MSVOA_X
ClientSampleId :
SB-11


Tgt Ion: 75 Resp: 74093
Ion Ratio Lower Upper
75 100
77 1.3 19.8 59.3#

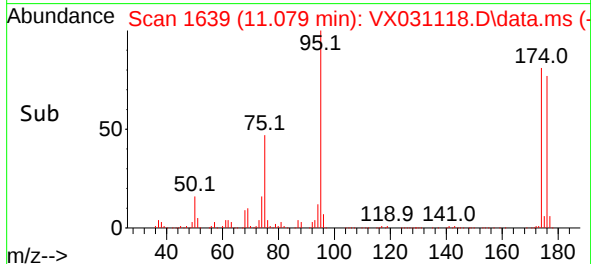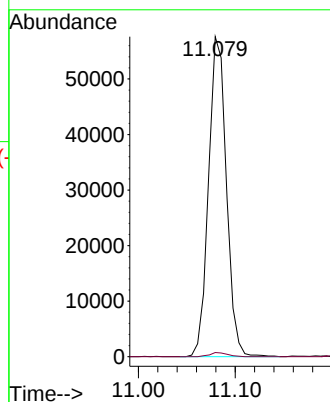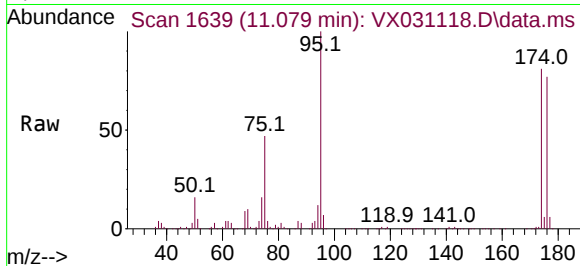

#81
trans-1,4-Dichloro-2-butene
Concen: 69.240 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.055 min
Lab File: VX031118.D
Acq: 04 Sep 2022 05:55

Tgt Ion: 75 Resp: 74093
Ion Ratio Lower Upper
75 100
53 0.0 74.2 111.4#
89 0.0 34.8 52.2#


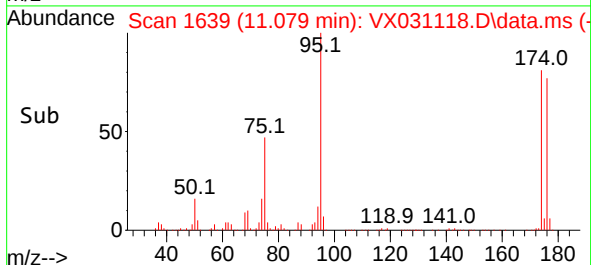

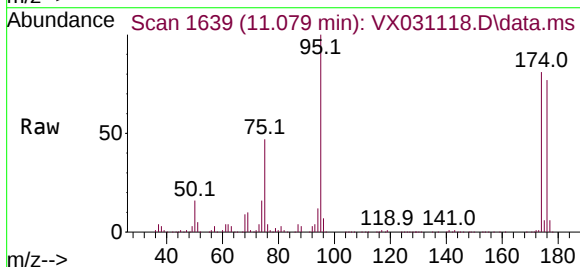




#85
 sec-Butylbenzene
 Concen: 0.368 ug/l
 RT: 11.756 min Scan# 11
 Delta R.T. -0.140 min
 Lab File: VX031118.D
 Acq: 04 Sep 2022 05:55

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-11

Tgt Ion:105 Resp: 4636
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.0 30.0#

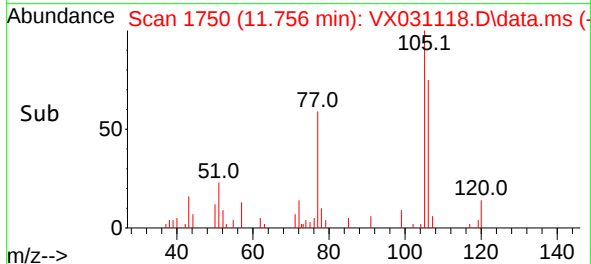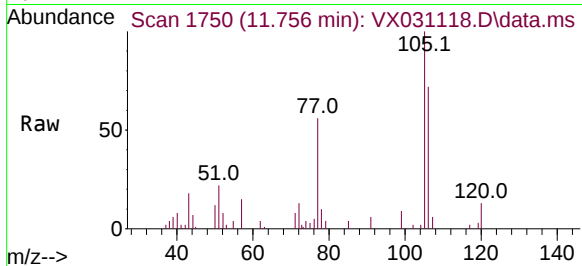

#95
 Naphthalene
 Concen: 3.844 ug/l
 RT: 13.774 min Scan# 2081
 Delta R.T. 0.000 min
 Lab File: VX031118.D
 Acq: 04 Sep 2022 05:55

Tgt Ion:128 Resp: 49574
 Ion Ratio Lower Upper
 128 100
 127 12.7 10.2 15.2
 129 11.6 8.6 13.0

