

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
 Data File : VX031119.D
 Acq On : 04 Sep 2022 06:18
 Operator : JC/MD
 Sample : N4479-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-12

Quant Time: Sep 06 01:32:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 02 02:49:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	227889	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	361184	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	338109	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	155091	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	140154	47.798	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	95.600%
35) Dibromofluoromethane	5.385	113	133521	50.657	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.320%
50) Toluene-d8	8.653	98	478225	49.298	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	98.600%
62) 4-Bromofluorobenzene	11.085	95	170371	49.725	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.460%
Target Compounds						
					Qvalue	
3) Chloromethane	1.288	50	315	0.839	ug/l #	42
6) Chloroethane	1.678	64	188	1.841	ug/l #	41
10) Methyl Iodide	2.459	142	228	2.990	ug/l #	54
11) Tert butyl alcohol	2.946	59	7368	Below Cal	#	74
13) Acrolein	2.245	56	683	1.273	ug/l	94
16) Acetone	2.392	43	28080	24.806	ug/l	90
17) Carbon Disulfide	2.514	76	1637	0.238	ug/l #	74
18) Methyl Acetate	2.703	43	2695	0.829	ug/l #	90
20) Methylene Chloride	2.788	84	15333	3.530	ug/l #	83
25) 2-Butanone	4.568	43	8063	4.614	ug/l	98
29) Tetrahydrofuran	5.013	42	1115	0.990	ug/l #	91
31) Cyclohexane	5.556	56	3427	0.856	ug/l #	1
36) 1,1-Dichloropropene	5.562	75	15397	4.170	ug/l #	49
37) Ethyl Acetate	4.727	43	26002	8.106	ug/l #	92
38) Carbon Tetrachloride	5.556	117	22212	5.796	ug/l #	17
40) Benzene	6.043	78	43666	4.119	ug/l	99
41) Methacrylonitrile	5.044	41	762	0.446	ug/l #	43
43) Isopropyl Acetate	6.342	43	107931	21.528	ug/l #	93
48) Methyl methacrylate	7.799	41	93367	36.889	ug/l #	43
49) 1,4-Dioxane	7.702	88	29	0.377	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	79958	24.809	ug/l #	52
52) Toluene	8.720	92	20584	2.994	ug/l	92
53) t-1,3-Dichloropropene	8.951	75	788	0.209	ug/l #	61
54) cis-1,3-Dichloropropene	8.549	75	45519	10.822	ug/l #	57
56) Ethyl methacrylate	9.250	69	928	0.232	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	6385	1.382	ug/l #	42
59) 2-Hexanone	9.378	43	88035	36.121	ug/l #	24
67) Ethyl Benzene	10.201	91	2969	0.215	ug/l	97
68) m/p-Xylenes	10.305	106	5594	1.031	ug/l	99
69) o-Xylene	10.646	106	3783	0.711	ug/l	95
70) Styrene	10.659	104	5997	0.696	ug/l	96
74) N-amyl acetate	10.774	43	1008	0.267	ug/l #	56
76) 1,2,3-Trichloropropane	11.079	75	77106	21.031	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	77106	66.096	ug/l #	13
85) sec-Butylbenzene	11.756	105	9081	0.662	ug/l #	56
95) Naphthalene	13.780	128	308154	21.921	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031119.D
Acq On : 04 Sep 2022 06:18
Operator : JC/MD
Sample : N4479-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-12

Quant Time: Sep 06 01:32:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 02 02:49:21 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031119.D
Acq On : 04 Sep 2022 06:18
Operator : JC/MD
Sample : N4479-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-12

Quant Time: Sep 06 01:32:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 02 02:49:21 2022
Response via : Initial Calibration




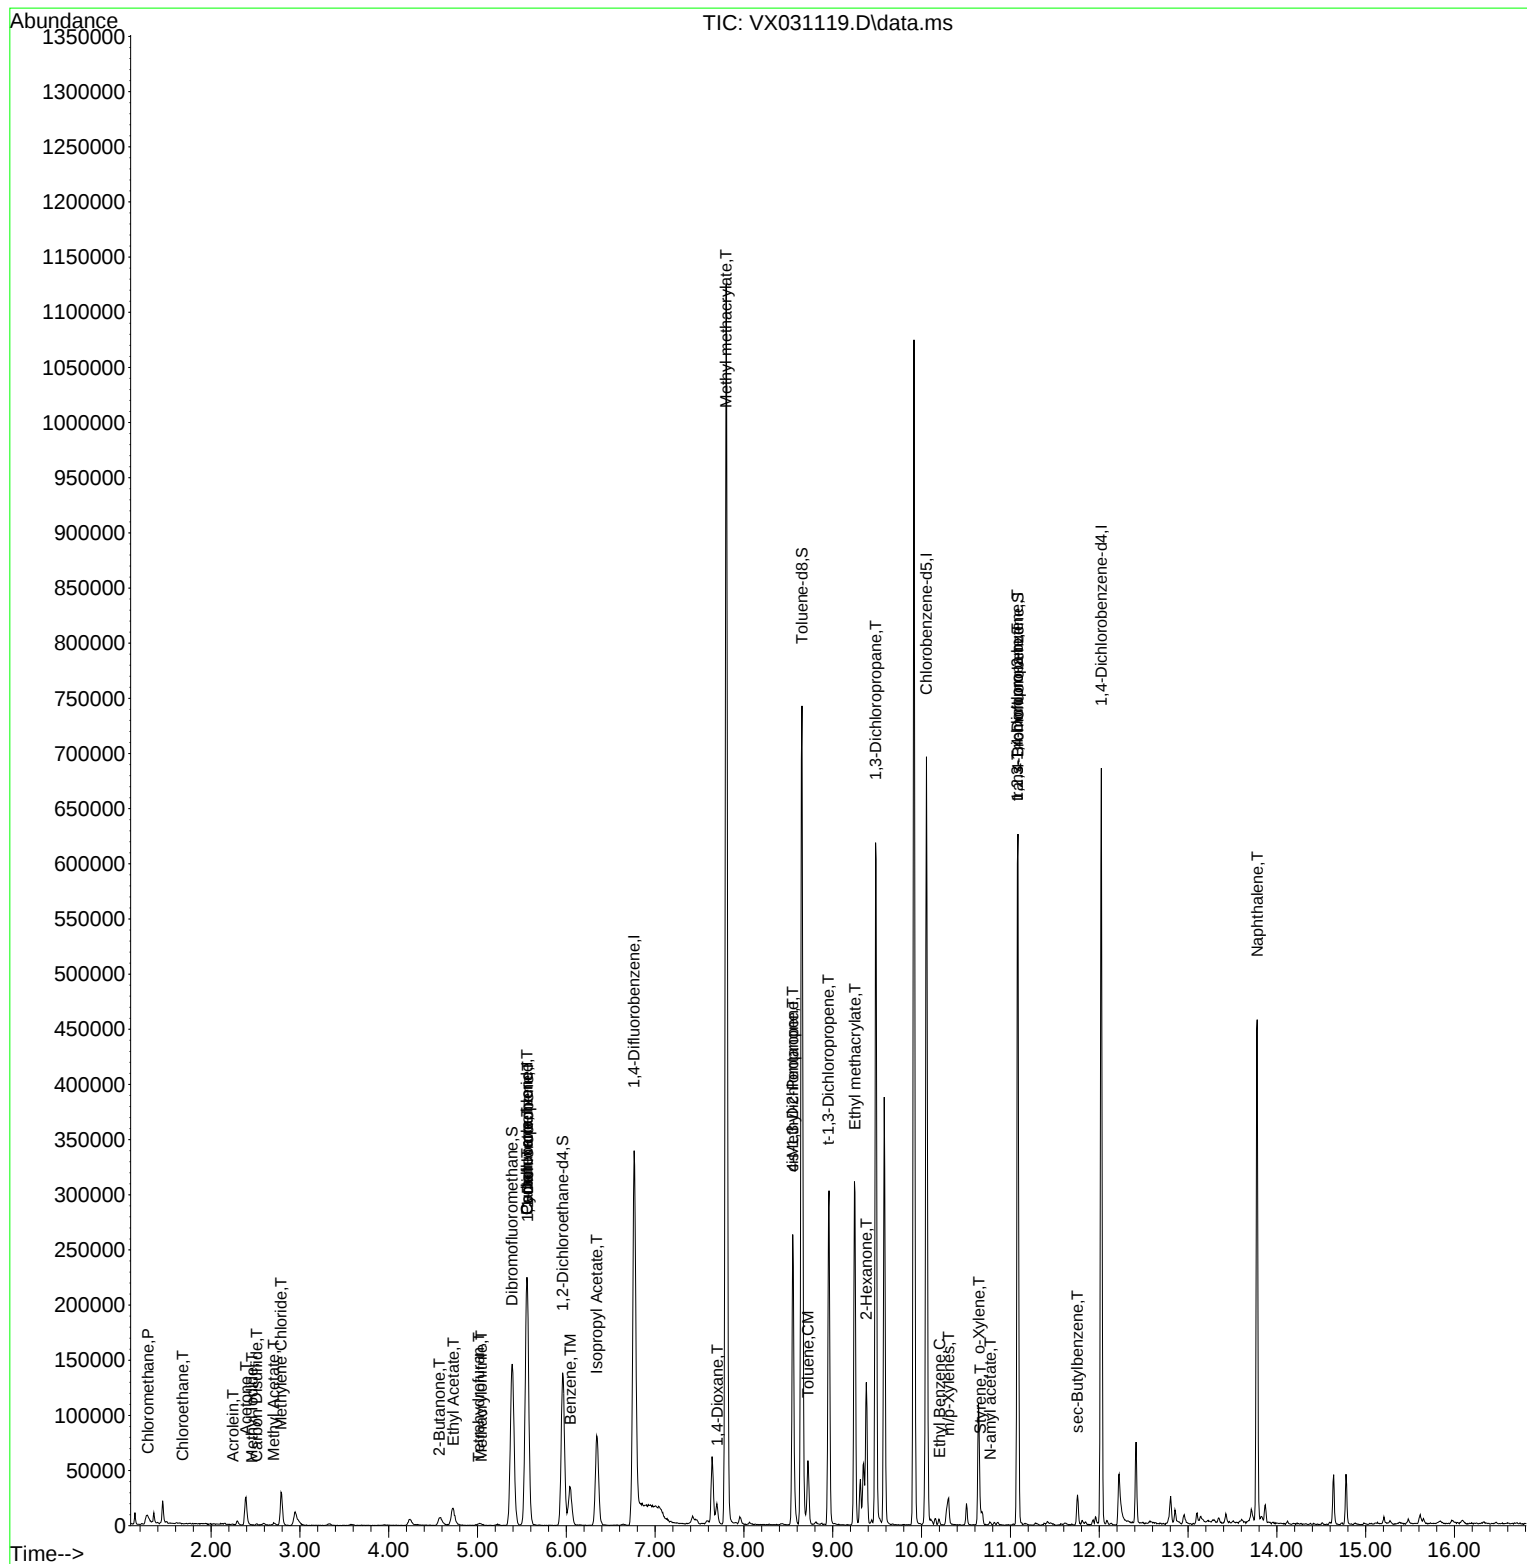


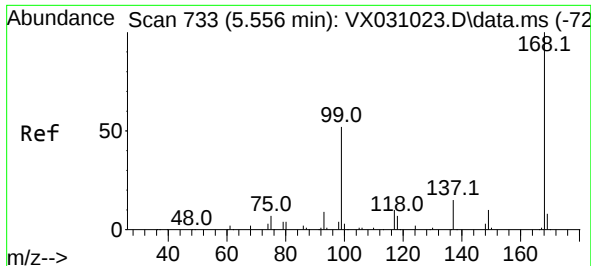

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion:168 Resp: 227889
Ion Ratio Lower Upper
168 100
99 51.7 44.0 66.0

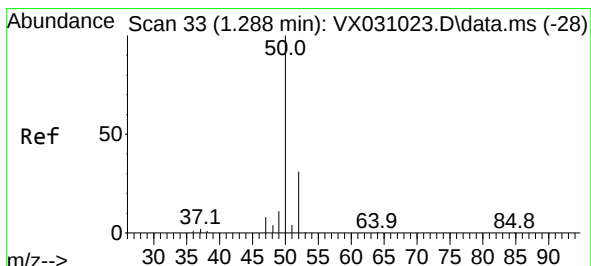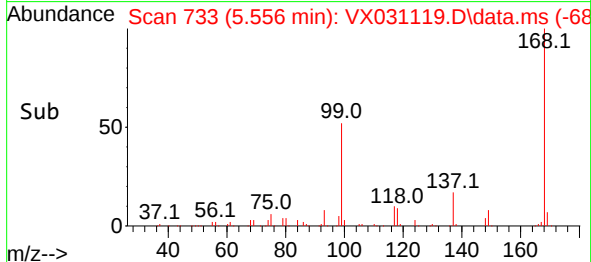

#3
Chloromethane
Concen: 0.839 ug/l
RT: 1.288 min Scan# 33
Delta R.T. 0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 50 Resp: 315
Ion Ratio Lower Upper
50 100
52 0.0 26.3 39.5#


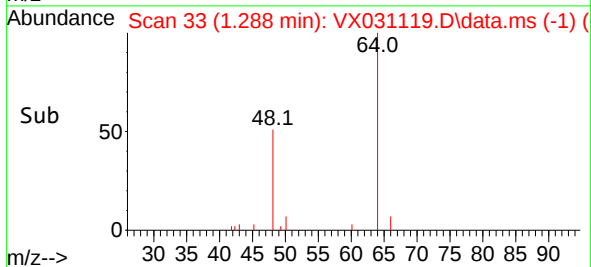

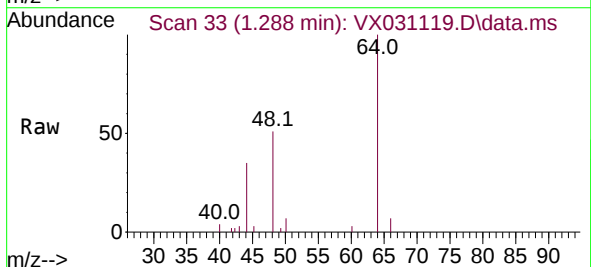


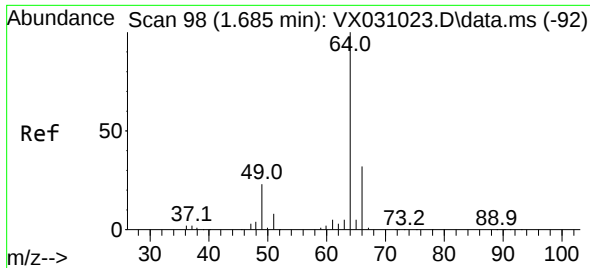

#6
Chloroethane
Concen: 1.841 ug/l
RT: 1.678 min Scan# 91
Delta R.T. -0.007 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion: 64 Resp: 188
Ion Ratio Lower Upper
64 100
66 0.0 27.2 40.8#

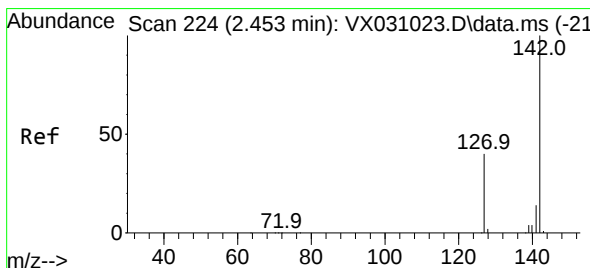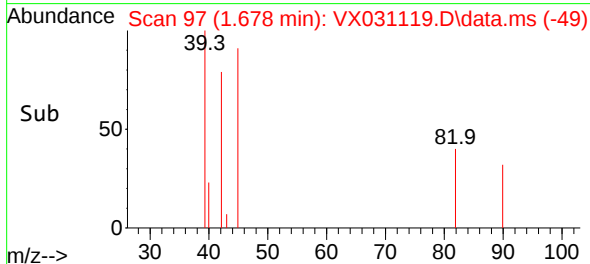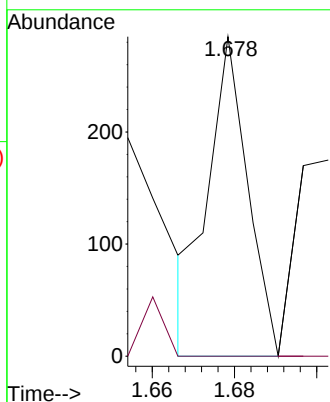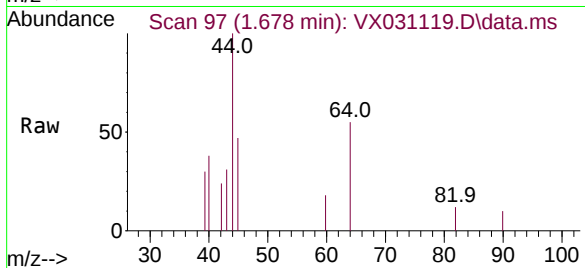

#10
Methyl Iodide
Concen: 2.990 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion:142 Resp: 228
Ion Ratio Lower Upper
142 100
127 68.0 30.2 45.2#
141 0.0 11.3 16.9#


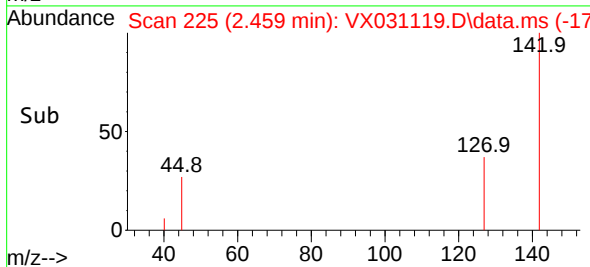

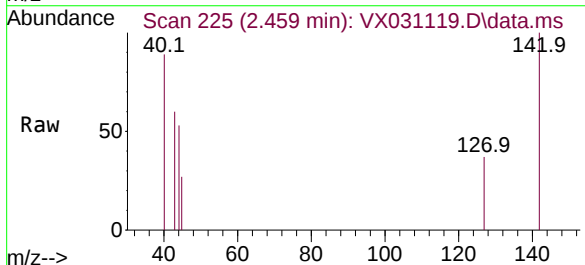




#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.946 min Scan# 305
Delta R.T. -0.043 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion: 59 Resp: 7368
Ion Ratio Lower Upper
59 100
57 0.0 7.4 11.2#

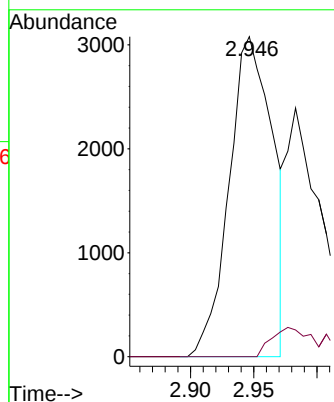

#13
Acrolein
Concen: 1.273 ug/l
RT: 2.245 min Scan# 190
Delta R.T. 0.006 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 56 Resp: 683
Ion Ratio Lower Upper
56 100
55 75.5 56.6 84.8


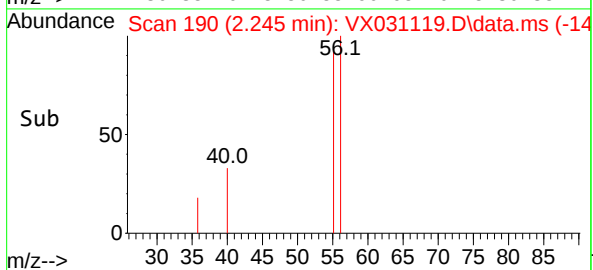
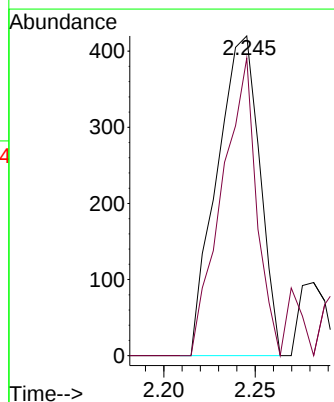





#16
Acetone
Concen: 24.806 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion: 43 Resp: 28080
Ion Ratio Lower Upper
43 100
58 40.1 27.7 41.5



#17
Carbon Disulfide
Concen: 0.238 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 76 Resp: 1637
Ion Ratio Lower Upper
76 100
78 0.0 7.8 11.6#


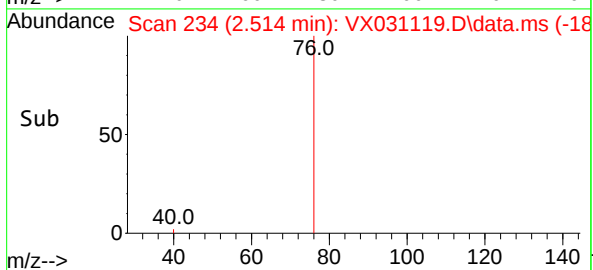




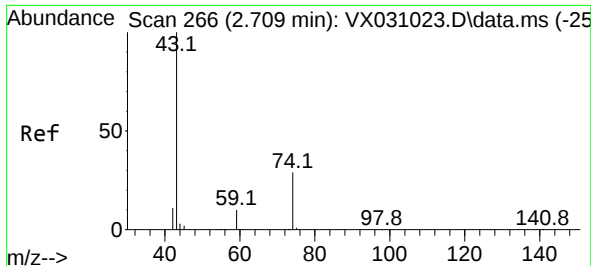

#18
Methyl Acetate
Concen: 0.829 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.006 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion: 43 Resp: 2695
Ion Ratio Lower Upper
43 100
74 29.2 19.4 29.2#

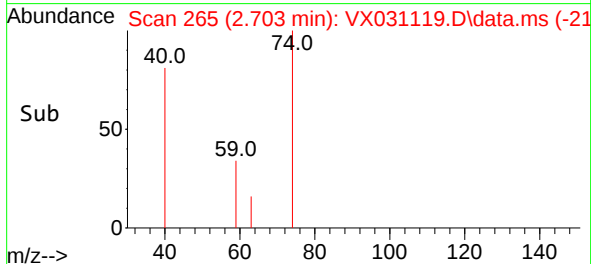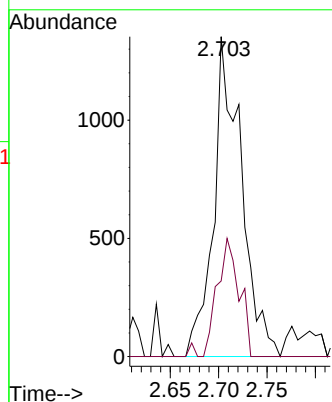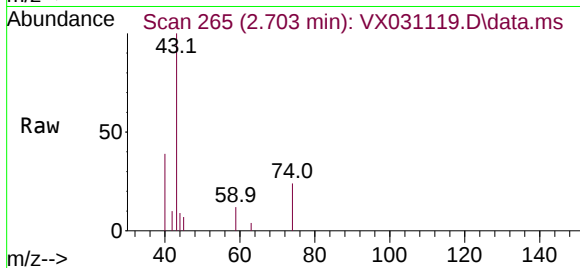

#20
Methylene Chloride
Concen: 3.530 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 84 Resp: 15333
Ion Ratio Lower Upper
84 100
49 90.3 93.8 140.6#
51 29.1 29.4 44.0#
86 67.3 51.0 76.4


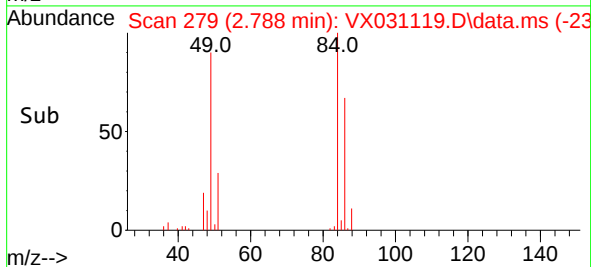

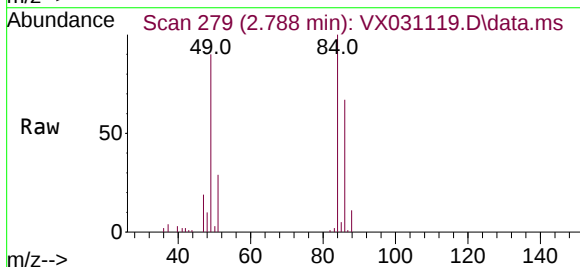




#25
2-Butanone
Concen: 4.614 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion: 43 Resp: 8063
Ion Ratio Lower Upper
43 100
72 25.9 21.7 32.5

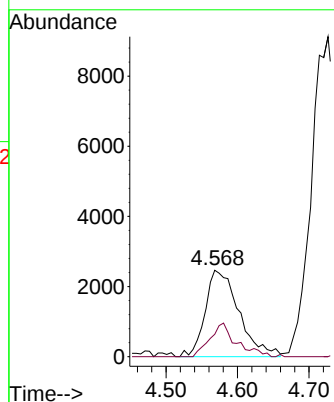

#29
Tetrahydrofuran
Concen: 0.990 ug/l
RT: 5.013 min Scan# 644
Delta R.T. 0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 42 Resp: 1115
Ion Ratio Lower Upper
42 100
72 54.9 36.5 54.7#
71 39.7 33.9 50.9


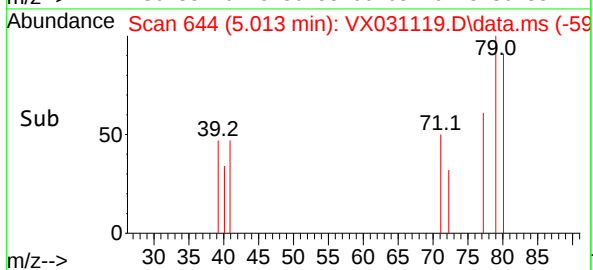
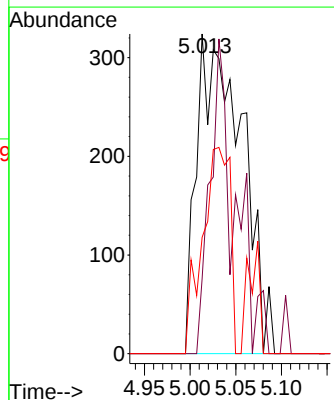





#31
Cyclohexane
Concen: 0.856 ug/l
RT: 5.556 min Scan# 711
Delta R.T. 0.079 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion: 56 Resp: 3427
Ion Ratio Lower Upper
56 100
69 145.1 25.4 38.0#
84 143.5 68.9 103.3#



#33
1,2-Dichloroethane-d4
Concen: 47.798 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 65 Resp: 140154
Ion Ratio Lower Upper
65 100
67 51.3 0.0 109.6


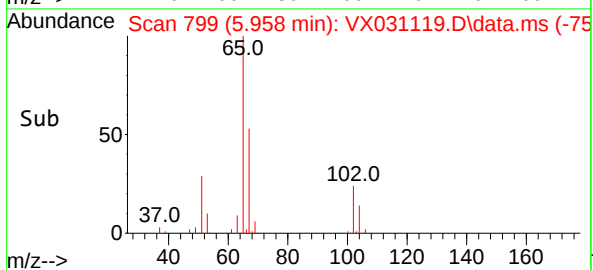




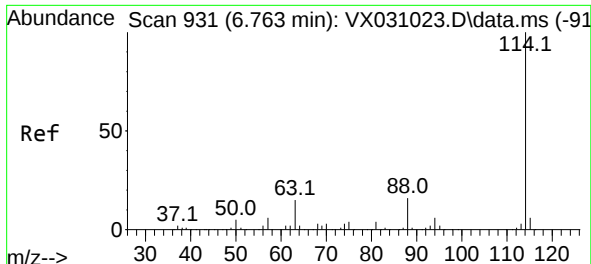

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion:114 Resp: 361184
Ion Ratio Lower Upper
114 100
63 17.4 0.0 38.4
88 14.5 0.0 31.8

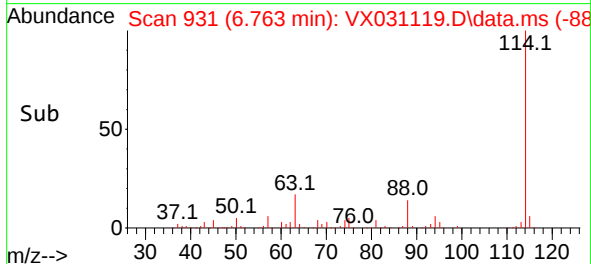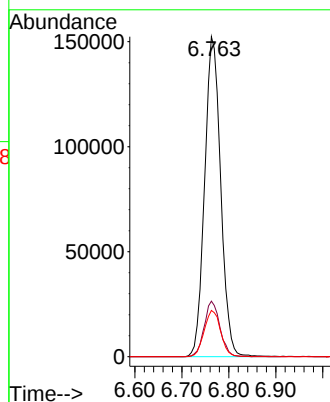

#35
Dibromofluoromethane
Concen: 50.657 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion:113 Resp: 133521
Ion Ratio Lower Upper
113 100
111 102.5 83.2 124.8
192 20.4 14.8 22.2


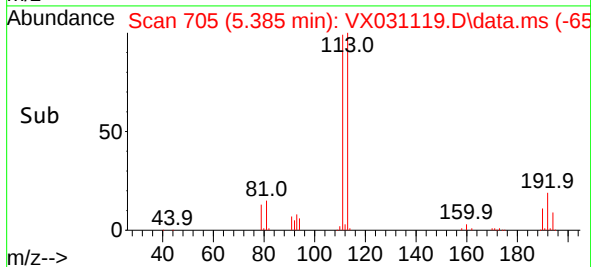
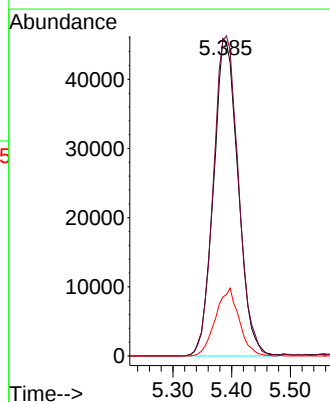
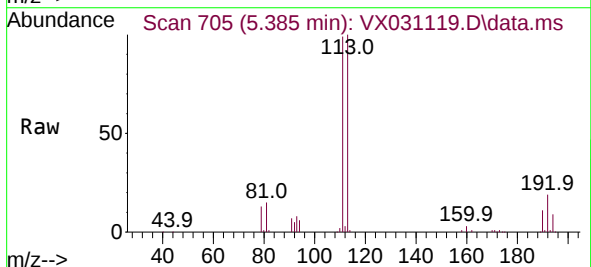


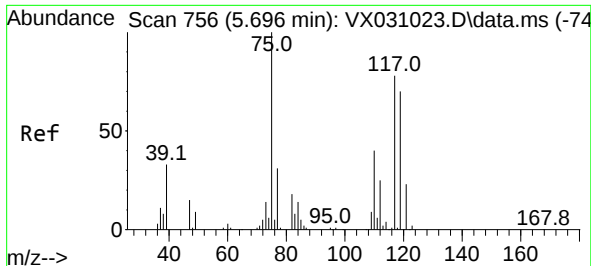

#36
1,1-Dichloropropene
Concen: 4.170 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion: 75 Resp: 15397
Ion Ratio Lower Upper
75 100
110 10.2 19.3 57.9#
77 0.0 24.4 36.6#

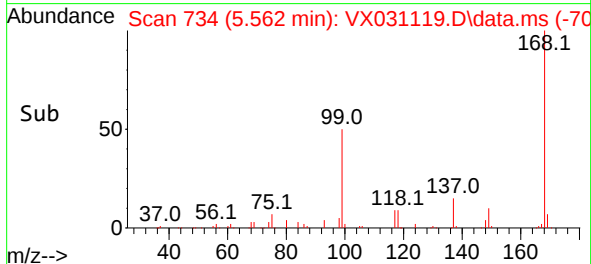

#37
Ethyl Acetate
Concen: 8.106 ug/l
RT: 4.727 min Scan# 597
Delta R.T. 0.006 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 43 Resp: 26002
Ion Ratio Lower Upper
43 100
61 18.3 11.7 17.5#
70 14.6 9.3 13.9#


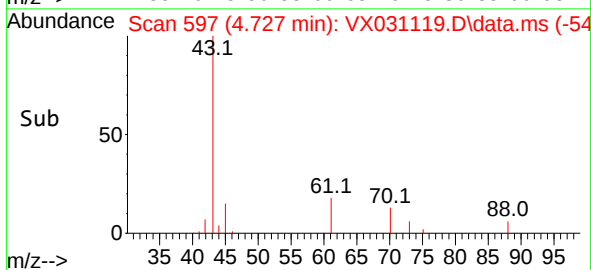

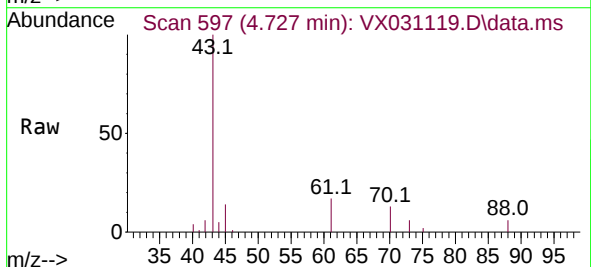




#38
Carbon Tetrachloride
Concen: 5.796 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.128 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion:117 Resp: 22212
Ion Ratio Lower Upper
117 100
119 5.3 74.1 111.1#
121 0.0 25.8 38.8#



#40
Benzene
Concen: 4.119 ug/l
RT: 6.043 min Scan# 813
Delta R.T. -0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 78 Resp: 43666
Ion Ratio Lower Upper
78 100
77 23.1 18.0 27.0









#41
Methacrylonitrile
Concen: 0.446 ug/l
RT: 5.044 min Scan# 649
Delta R.T. 0.116 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion: 41 Resp: 762
Ion Ratio Lower Upper
41 100
39 38.7 42.9 64.3#
67 3.3 60.1 90.1#
52 0.0 22.6 34.0#

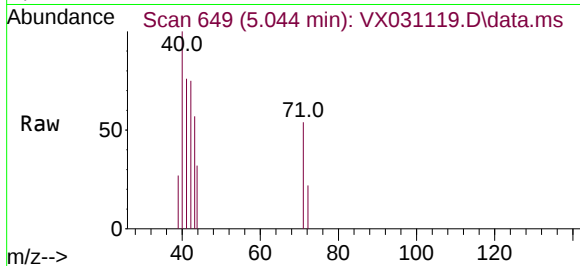

#43
Isopropyl Acetate
Concen: 21.528 ug/l
RT: 6.342 min Scan# 862
Delta R.T. -0.006 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 43 Resp: 107931
Ion Ratio Lower Upper
43 100
61 22.4 16.5 24.7
87 18.6 11.1 16.7#




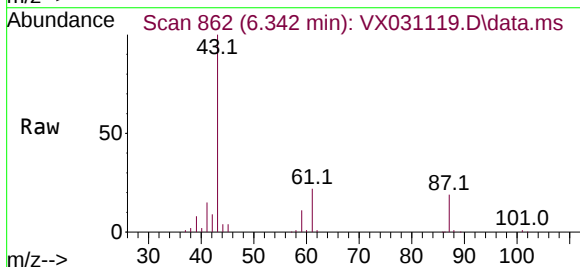




#48
Methyl methacrylate
Concen: 36.889 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.103 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion: 41 Resp: 93367
Ion Ratio Lower Upper
41 100
69 0.3 68.8 103.2#
39 55.0 44.6 66.8

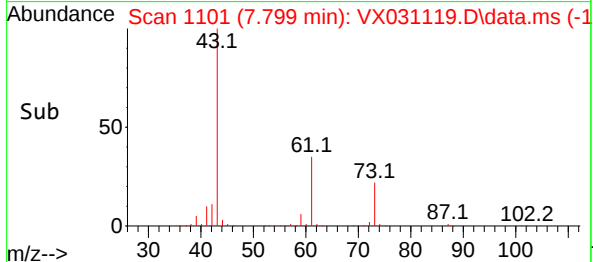

#49
1,4-Dioxane
Concen: 0.377 ug/l
RT: 7.702 min Scan# 1085
Delta R.T. 0.025 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 88 Resp: 29
Ion Ratio Lower Upper
88 100
43 0.0 23.8 35.8#
58 3089.7 53.8 80.6#

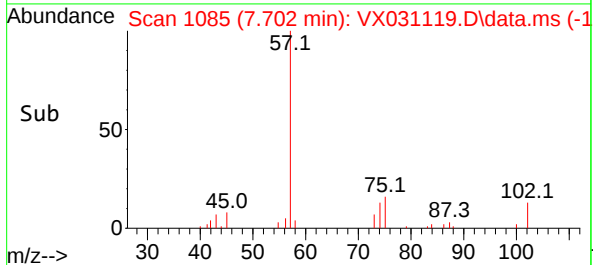



#50

Toluene-d8

Concen: 49.298 ug/l

RT: 8.653 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX031119.D

Acq: 04 Sep 2022 06:18

Instrument :

MSVOA_X

ClientSampleId :





SB-12

Tgt Ion: 98 Resp: 478225

Ion Ratio Lower Upper

98 100

100 63.3 52.3 78.5



#51

4-Methyl-2-Pentanone

Concen: 24.809 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. -0.031 min

Lab File: VX031119.D




Acq: 04 Sep 2022 06:18


Tgt Ion: 43 Resp: 79958

Ion Ratio Lower Upper

43 100

58 10.1 31.4 47.2#









#52
Toluene
Concen: 2.994 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion: 92 Resp: 20584
Ion Ratio Lower Upper
92 100
91 185.7 139.2 208.8

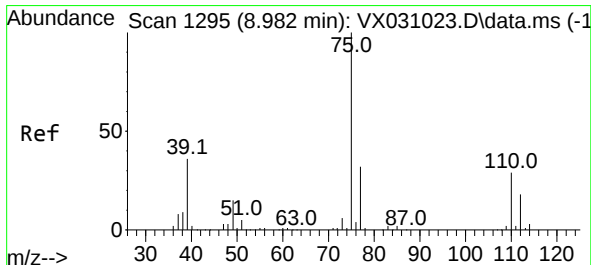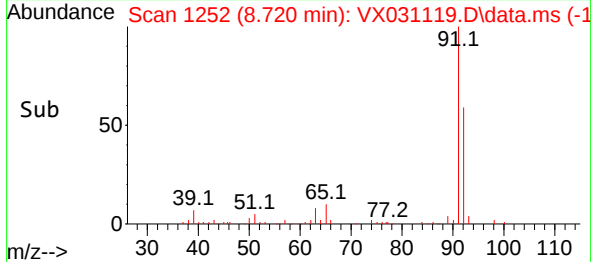

#53
t-1,3-Dichloropropene
Concen: 0.209 ug/l
RT: 8.951 min Scan# 1290
Delta R.T. -0.030 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 75 Resp: 788
Ion Ratio Lower Upper
75 100
77 10.8 26.3 39.5#


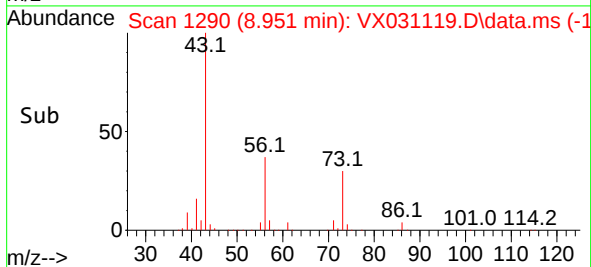

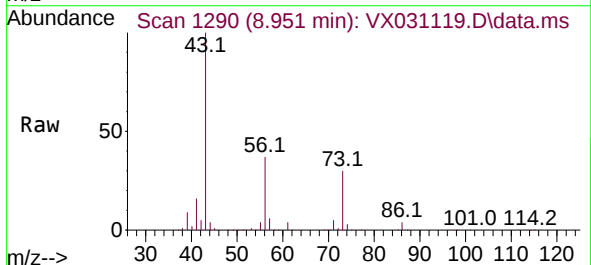




#54
 cis-1,3-Dichloropropene
 Concen: 10.822 ug/l
 RT: 8.549 min Scan# 1195
 Delta R.T. 0.177 min
 Lab File: VX031119.D
 Acq: 04 Sep 2022 06:18




Instrument :
 MSVOA_X
 ClientSampleId :
 SB-12


Tgt Ion: 75 Resp: 45519
 Ion Ratio Lower Upper
 75 100
 77 0.8 25.0 37.4#
 39 23.9 37.5 56.3#

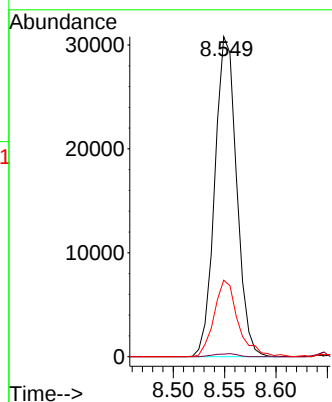

#56
 Ethyl methacrylate
 Concen: 0.232 ug/l
 RT: 9.250 min Scan# 1339
 Delta R.T. 0.128 min
 Lab File: VX031119.D
 Acq: 04 Sep 2022 06:18

Tgt Ion: 69 Resp: 928
 Ion Ratio Lower Upper
 69 100
 41 4743.0 52.3 78.5#
 39 1932.2 28.2 42.4#

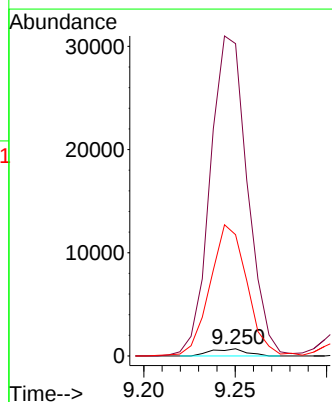



#57

1,3-Dichloropropane

Concen: 1.382 ug/l

RT: 9.482 min Scan# 1

Delta R.T. 0.171 min

Lab File: VX031119.D

Acq: 04 Sep 2022 06:18

Instrument :

MSVOA_X

ClientSampleId :





SB-12

Tgt Ion: 76 Resp: 6385

Ion Ratio Lower Upper

76 100

78 0.0 25.9 38.9#



#59

2-Hexanone

Concen: 36.121 ug/l

RT: 9.378 min Scan# 1360

Delta R.T. -0.055 min

Lab File: VX031119.D




Acq: 04 Sep 2022 06:18


Tgt Ion: 43 Resp: 88035

Ion Ratio Lower Upper

43 100

58 0.0 27.6 82.8#


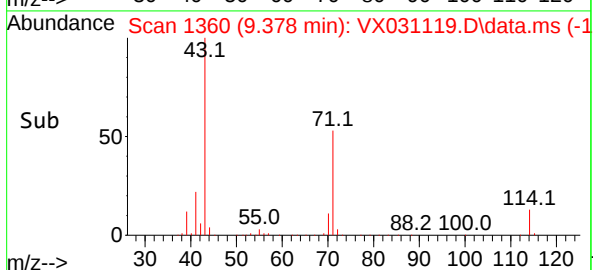




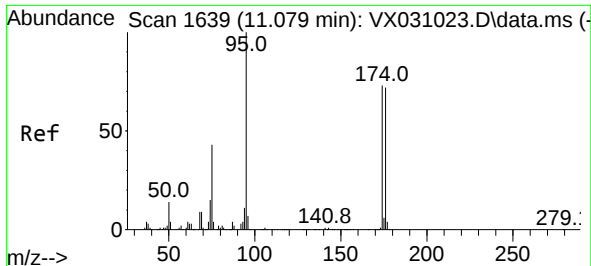

#62
4-Bromofluorobenzene
Concen: 49.725 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion: 95 Resp: 170371
Ion Ratio Lower Upper
95 100
174 88.4 0.0 149.0
176 84.2 0.0 146.0

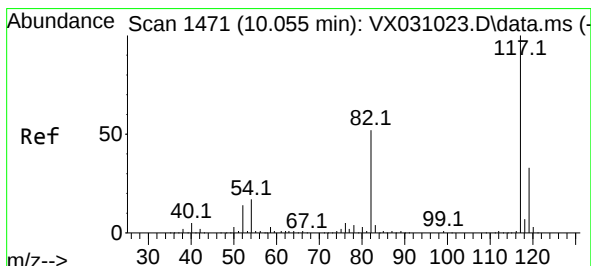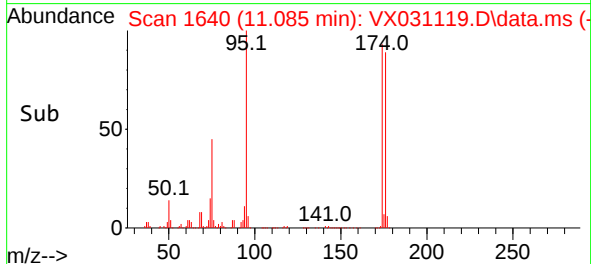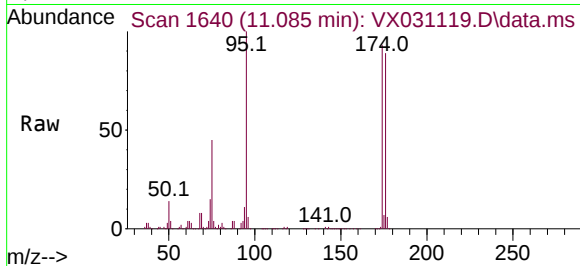

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 117 Resp: 338109
Ion Ratio Lower Upper
117 100
82 48.8 42.7 64.1
119 33.2 25.4 38.2


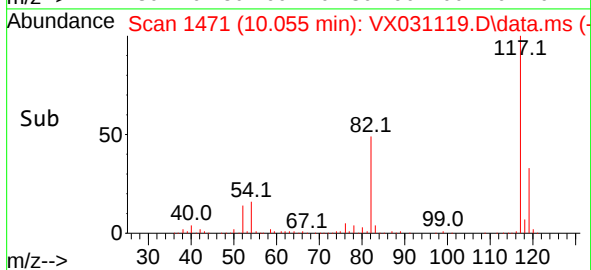

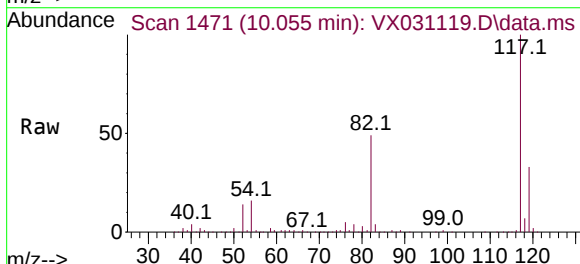




#67
Ethyl Benzene
Concen: 0.215 ug/l
RT: 10.201 min Scan# 1494
Delta R.T. 0.006 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion: 91 Resp: 2969
Ion Ratio Lower Upper
91 100
106 33.4 25.5 38.3

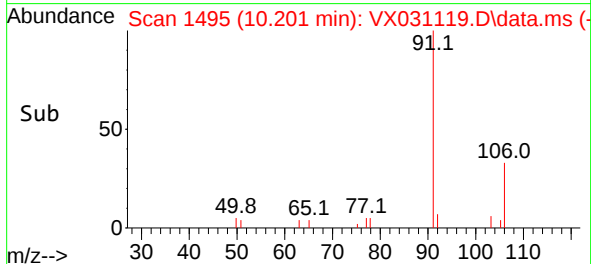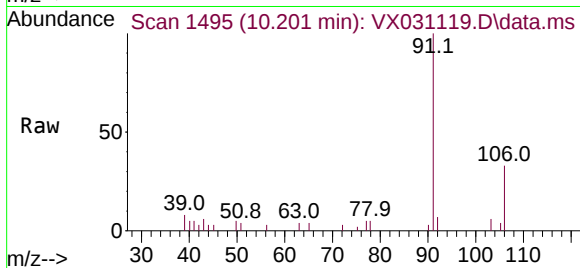

#68
m/p-Xylenes
Concen: 1.031 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 106 Resp: 5594
Ion Ratio Lower Upper
106 100
91 199.3 158.2 237.4


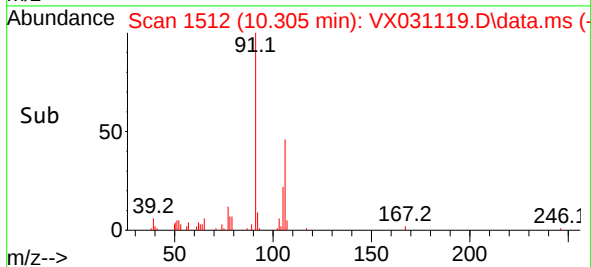

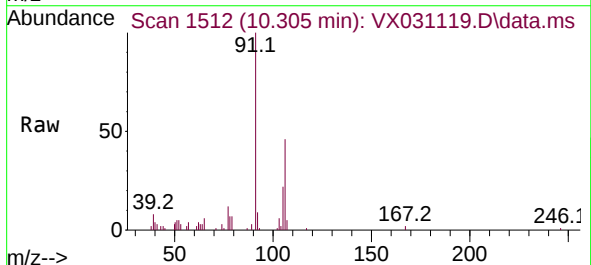




#69
o-Xylene
Concen: 0.711 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion:106 Resp: 3783
Ion Ratio Lower Upper
106 100
91 200.7 103.8 311.6

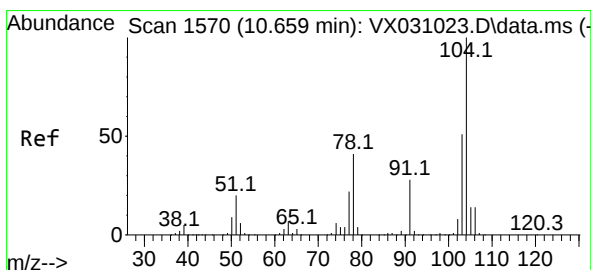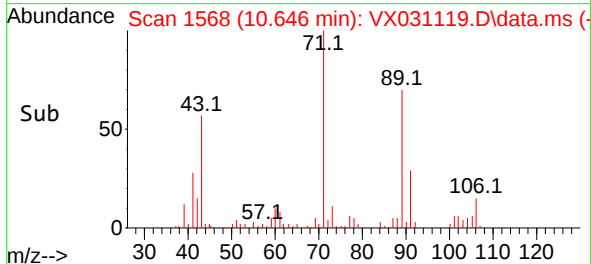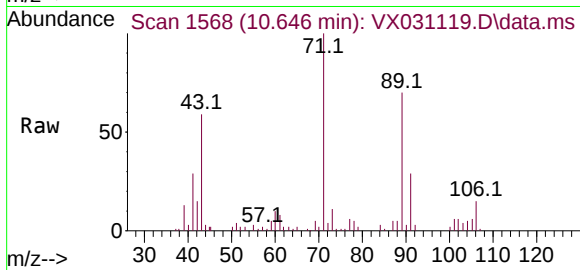

#70
Styrene
Concen: 0.696 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. -0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion:104 Resp: 5997
Ion Ratio Lower Upper
104 100
78 43.2 37.8 56.8
103 56.7 44.5 66.7




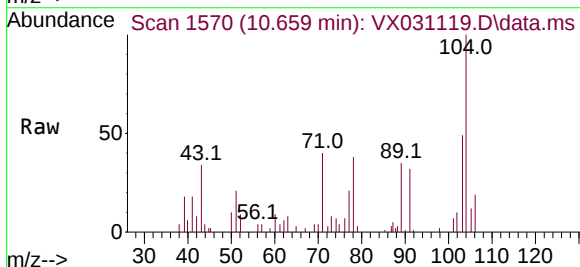




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion:152 Resp: 155091
Ion Ratio Lower Upper
152 100
115 57.0 40.5 121.5
150 154.4 0.0 347.0

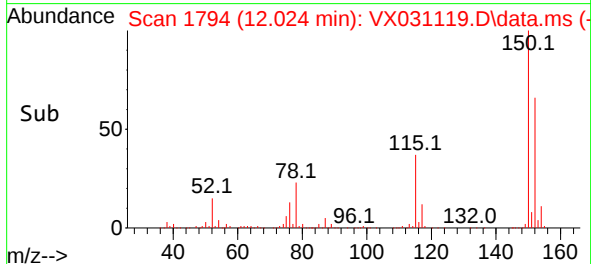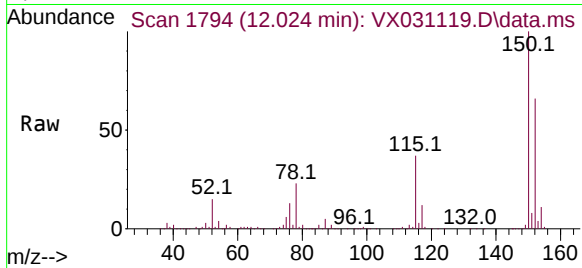

#74
N-ethyl acetate
Concen: 0.267 ug/l
RT: 10.774 min Scan# 1589
Delta R.T. -0.074 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 43 Resp: 1008
Ion Ratio Lower Upper
43 100
70 0.0 32.3 48.5#
55 23.9 18.4 27.6
61 0.0 19.2 28.8#


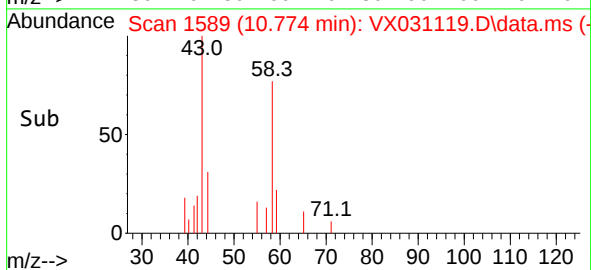

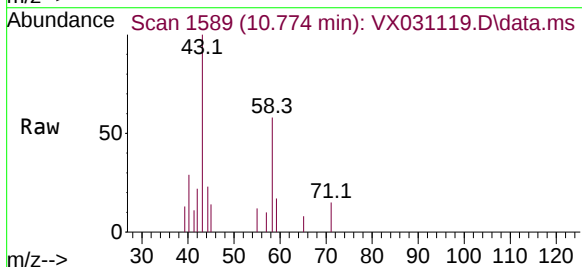


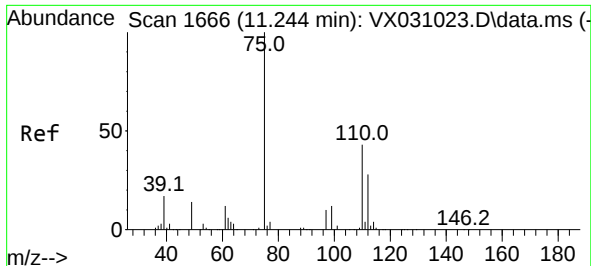

#76
1,2,3-Trichloropropane
Concen: 21.031 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
SB-12


Tgt Ion: 75 Resp: 77106
Ion Ratio Lower Upper
75 100
77 1.4 19.8 59.3#

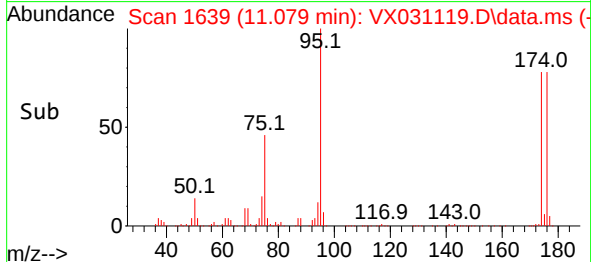

#81
trans-1,4-Dichloro-2-butene
Concen: 66.096 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.055 min
Lab File: VX031119.D
Acq: 04 Sep 2022 06:18

Tgt Ion: 75 Resp: 77106
Ion Ratio Lower Upper
75 100
53 0.0 74.2 111.4#
89 0.0 34.8 52.2#


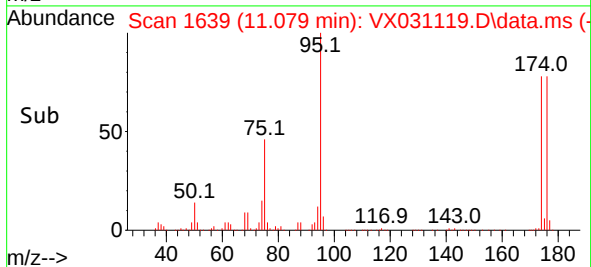

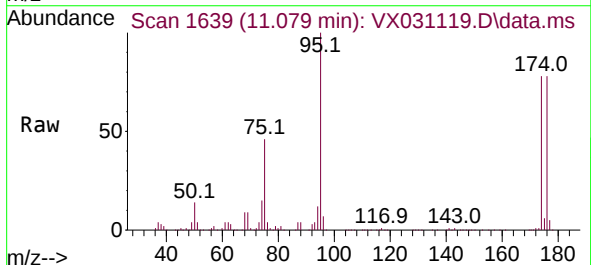


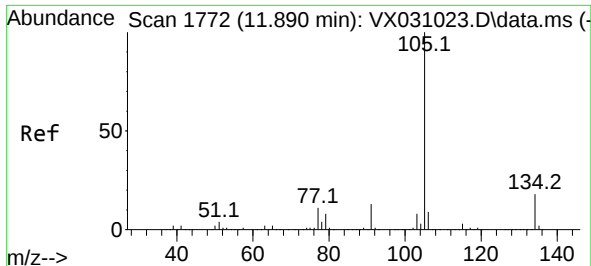

#85
 sec-Butylbenzene
 Concen: 0.662 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. -0.140 min
 Lab File: VX031119.D
 Acq: 04 Sep 2022 06:18

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-12

Tgt Ion:105 Resp: 9081
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.0 30.0#

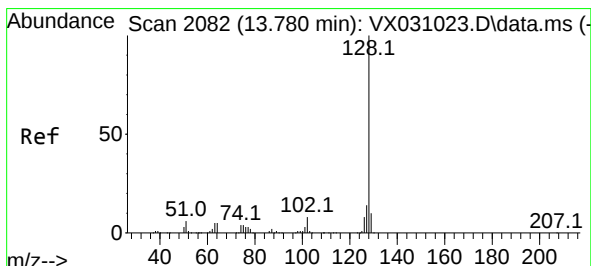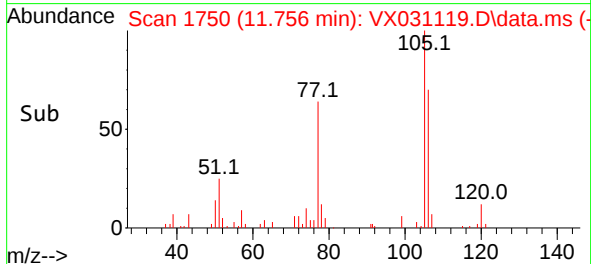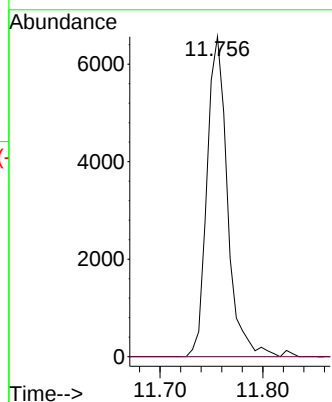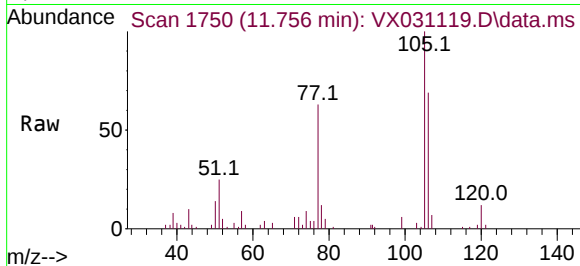

#95
 Naphthalene
 Concen: 21.921 ug/l
 RT: 13.780 min Scan# 2082
 Delta R.T. 0.006 min
 Lab File: VX031119.D
 Acq: 04 Sep 2022 06:18

Tgt Ion:128 Resp: 308154
 Ion Ratio Lower Upper
 128 100
 127 12.8 10.2 15.2
 129 11.1 8.6 13.0

