

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
 Data File : VX031085.D
 Acq On : 03 Sep 2022 16:16
 Operator : JC/MD
 Sample : N4357-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE120D2-20220822

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M

Title : SW846 8260

Signal : TIC: VX031085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	196	204	213	rBV3	119385	232317	2.98%	1.658%
2	5.391	694	706	721	rBV2	146816	428136	5.50%	3.055%
3	5.556	721	733	747	rBV2	222663	634467	8.15%	4.528%
4	5.958	788	799	817	rBV	146154	378459	4.86%	2.701%
5	6.763	921	931	944	rBV	325229	766492	9.84%	5.470%
6	7.129	980	991	1012	rBV	3566195	7786854	100.00%	55.570%
7	8.653	1234	1241	1250	rBV	747372	1184783	15.22%	8.455%
8	9.275	1337	1343	1352	rBV	78411	113149	1.45%	0.807%
9	10.055	1465	1471	1483	rBV	681451	898763	11.54%	6.414%
10	11.079	1634	1639	1650	rBV	600032	780713	10.03%	5.571%
11	12.024	1789	1794	1802	rBV	642531	808537	10.38%	5.770%




Sum of corrected areas: 14012670

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031085.D
Acq On : 03 Sep 2022 16:16
Operator : JC/MD
Sample : N4357-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20220822

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

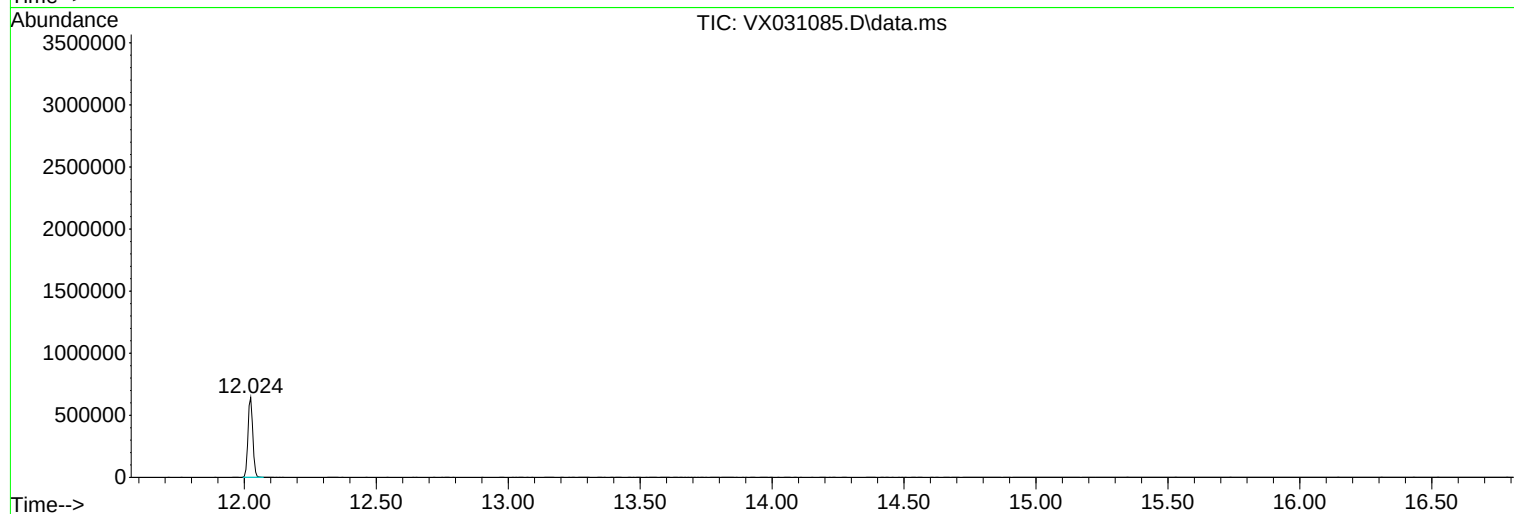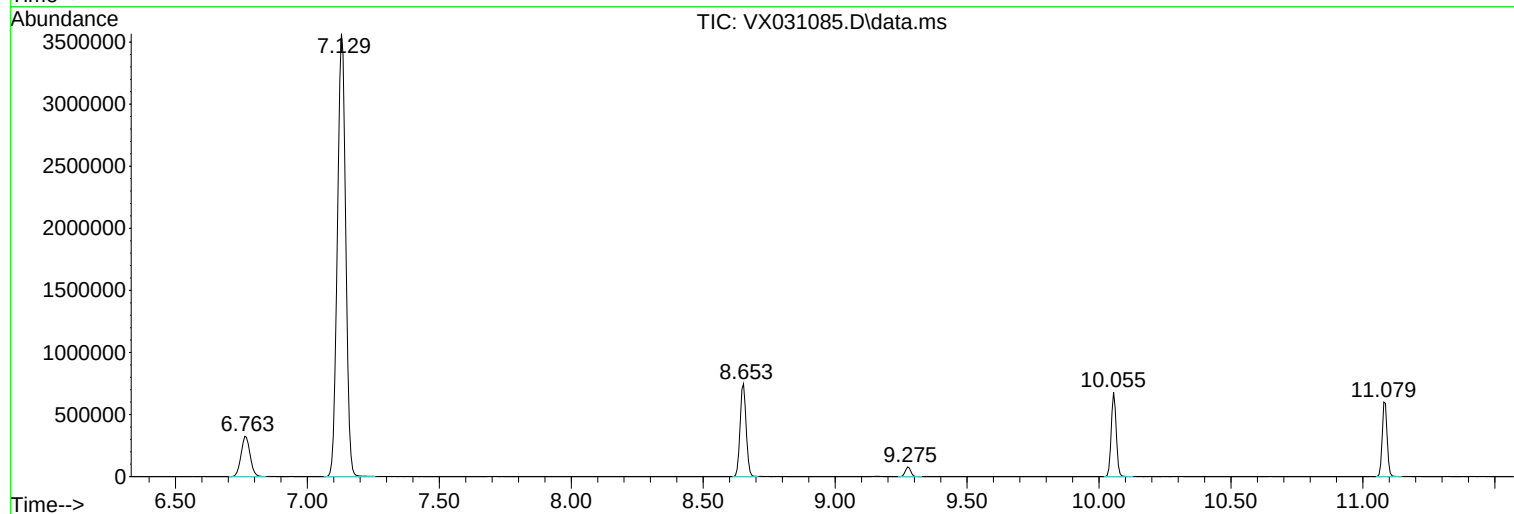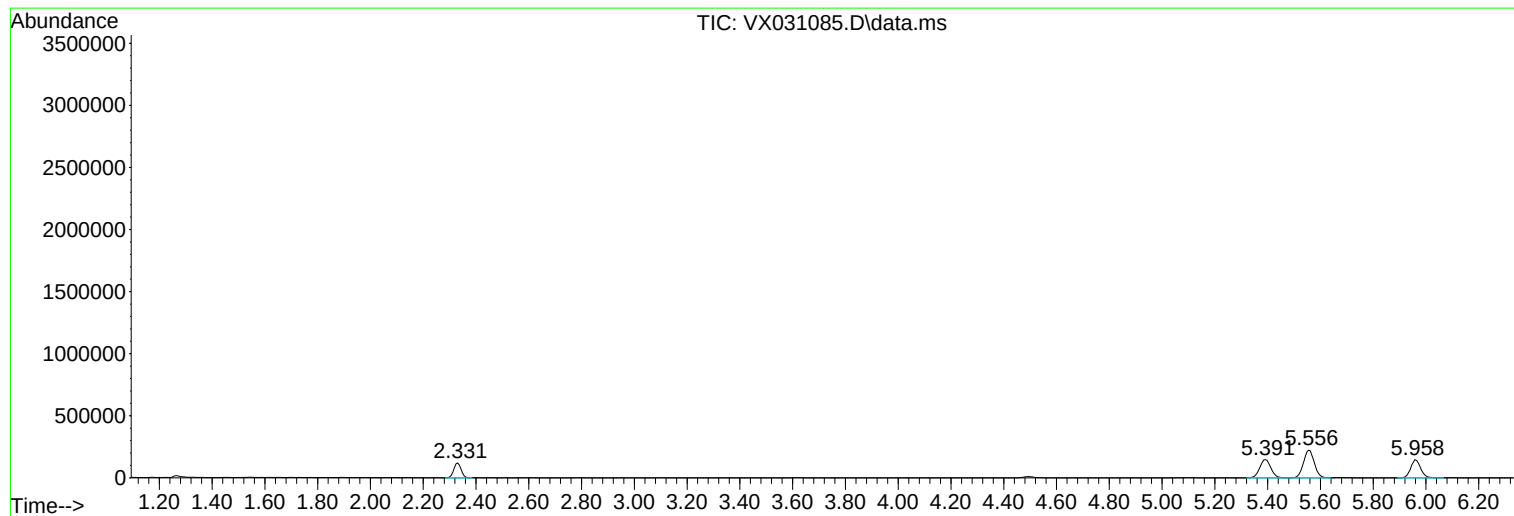

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031085.D
Acq On : 03 Sep 2022 16:16
Operator : JC/MD
Sample : N4357-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20220822

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031085.D
Acq On : 03 Sep 2022 16:16
Operator : JC/MD
Sample : N4357-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20220822

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------