

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031087.D
Acq On : 03 Sep 2022 17:03
Operator : JC/MD
Sample : N4357-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D2-20220823

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M

Title : SW846 8260

Signal : TIC: VX031087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	25	29	43	rBV	12878	29206	2.13%	0.387%
2	2.331	195	204	211	rBV	84338	158624	11.59%	2.099%
3	5.391	693	706	722	rBV	148689	435531	31.83%	5.765%
4	5.556	722	733	746	rVV	221012	632338	46.22%	8.369%
5	5.958	789	799	818	rBV	140685	375266	27.43%	4.967%
6	6.763	920	931	942	rBV	325065	770255	56.30%	10.195%
7	7.129	980	991	1005	rBV	623660	1368115	100.00%	18.108%
8	8.653	1233	1241	1248	rBV	764975	1166231	85.24%	15.436%
9	8.720	1248	1252	1262	rVB	16641	27773	2.03%	0.368%
10	9.275	1336	1343	1352	rVB	139061	205931	15.05%	2.726%
11	10.055	1465	1471	1486	rBV	642103	866876	63.36%	11.474%
12	11.085	1634	1640	1652	rBV	558741	734236	53.67%	9.718%
13	12.024	1788	1794	1800	rBV	657991	784984	57.38%	10.390%




Sum of corrected areas: 7555366

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031087.D
Acq On : 03 Sep 2022 17:03
Operator : JC/MD
Sample : N4357-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D2-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

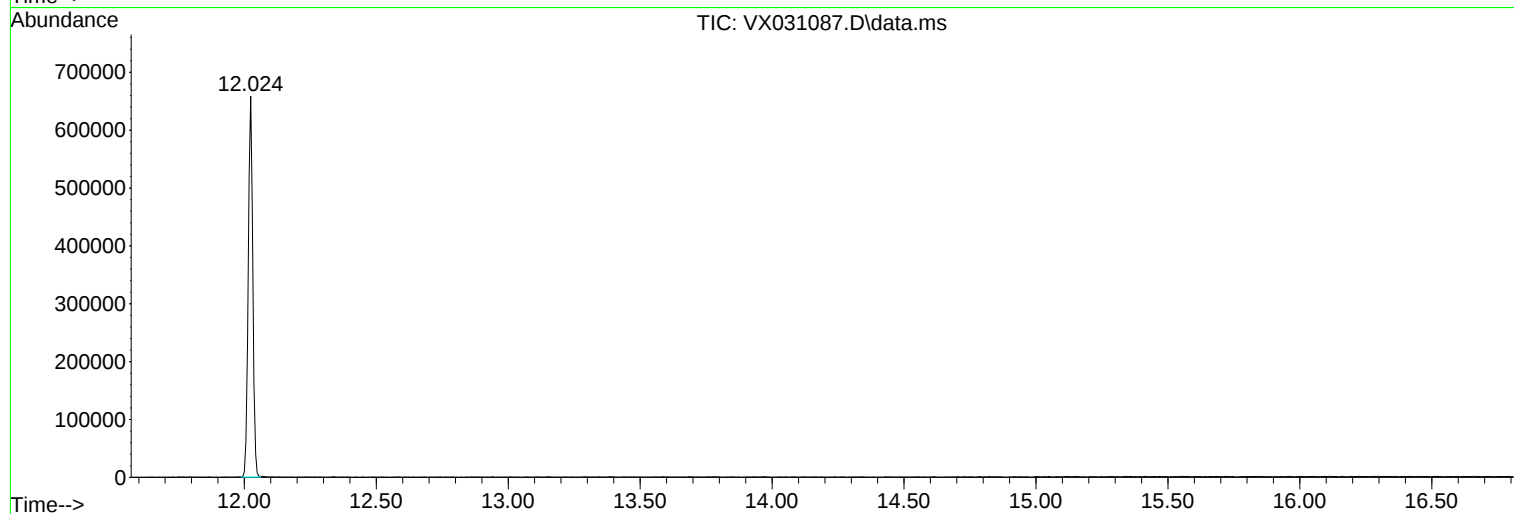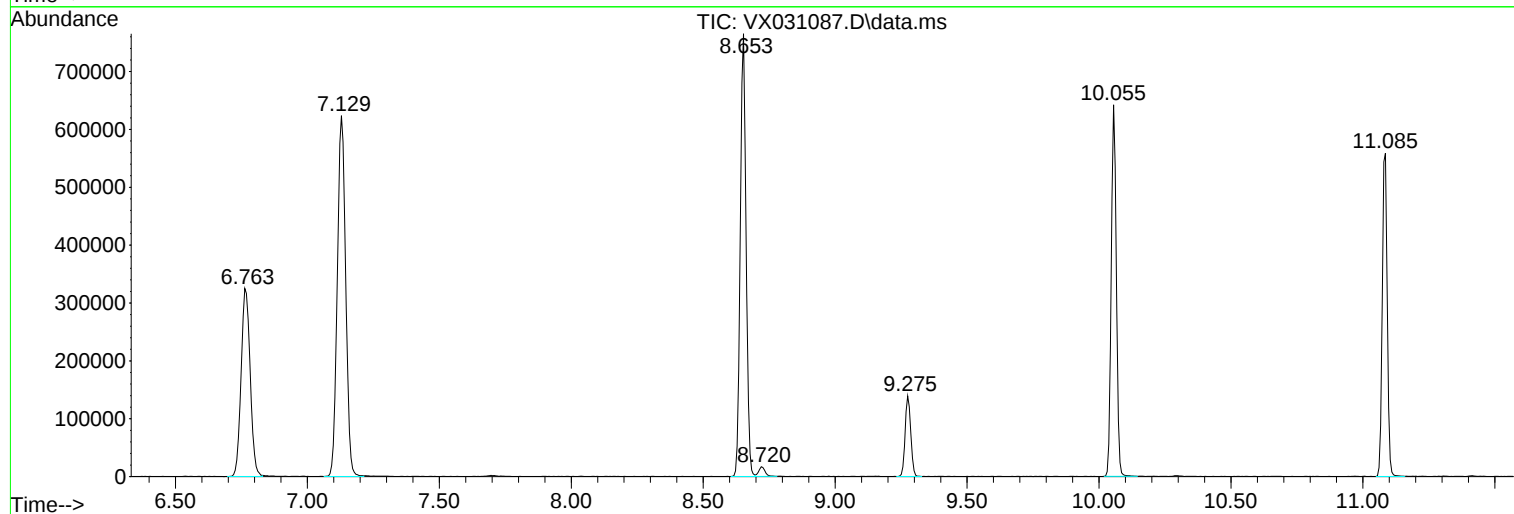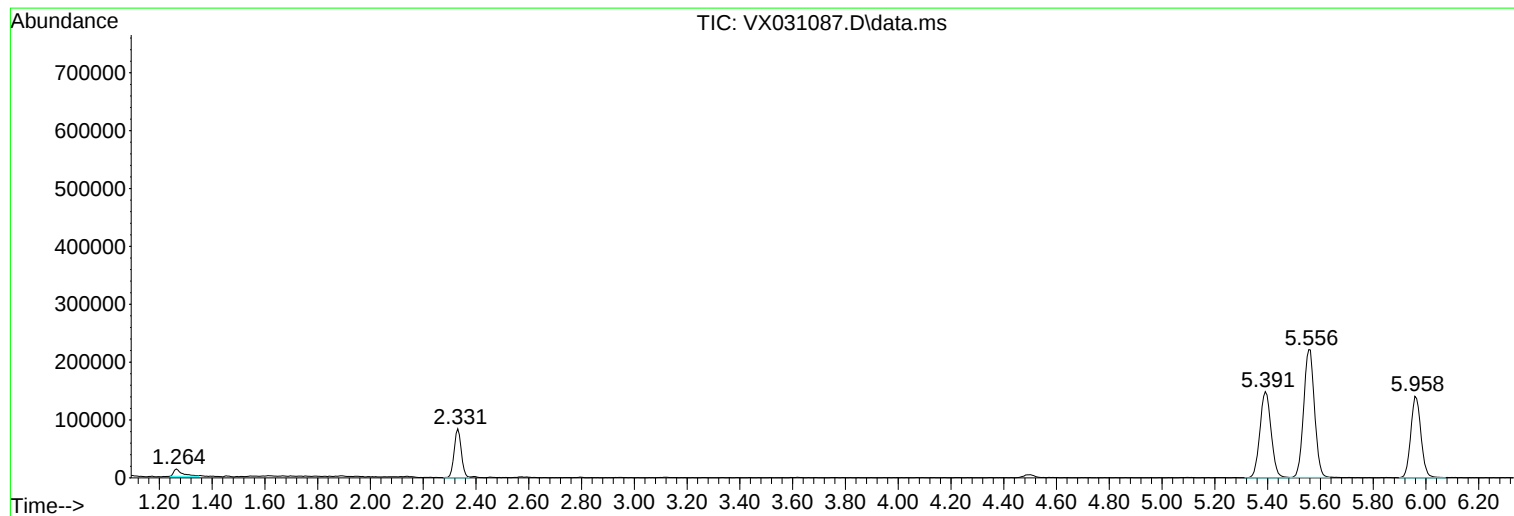

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031087.D
Acq On : 03 Sep 2022 17:03
Operator : JC/MD
Sample : N4357-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D2-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031087.D
Acq On : 03 Sep 2022 17:03
Operator : JC/MD
Sample : N4357-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D2-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc