

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
 Data File : VX031094.D
 Acq On : 03 Sep 2022 19:47
 Operator : JC/MD
 Sample : N4357-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE125D3-20220823

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M

Title : SW846 8260

Signal : TIC: VX031094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	193	204	218	rBV	483332	902466	49.25%	10.925%
2	5.391	693	706	721	rBV2	134884	398663	21.76%	4.826%
3	5.556	721	733	745	rBV	209565	580028	31.66%	7.022%
4	5.958	790	799	812	rBV	129876	346556	18.91%	4.195%
5	6.763	921	931	947	rBV	292443	710459	38.77%	8.601%
6	7.129	982	991	1013	rBV	854514	1832292	100.00%	22.181%
7	8.653	1234	1241	1249	rBV	706947	1090246	59.50%	13.198%
8	9.275	1337	1343	1350	rBV	107304	151335	8.26%	1.832%
9	10.055	1465	1471	1484	rBV	623905	819895	44.75%	9.925%
10	11.085	1634	1640	1648	rBV	547492	704692	38.46%	8.531%
11	12.024	1789	1794	1806	rVB	572815	723889	39.51%	8.763%




Sum of corrected areas: 8260521

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031094.D
Acq On : 03 Sep 2022 19:47
Operator : JC/MD
Sample : N4357-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

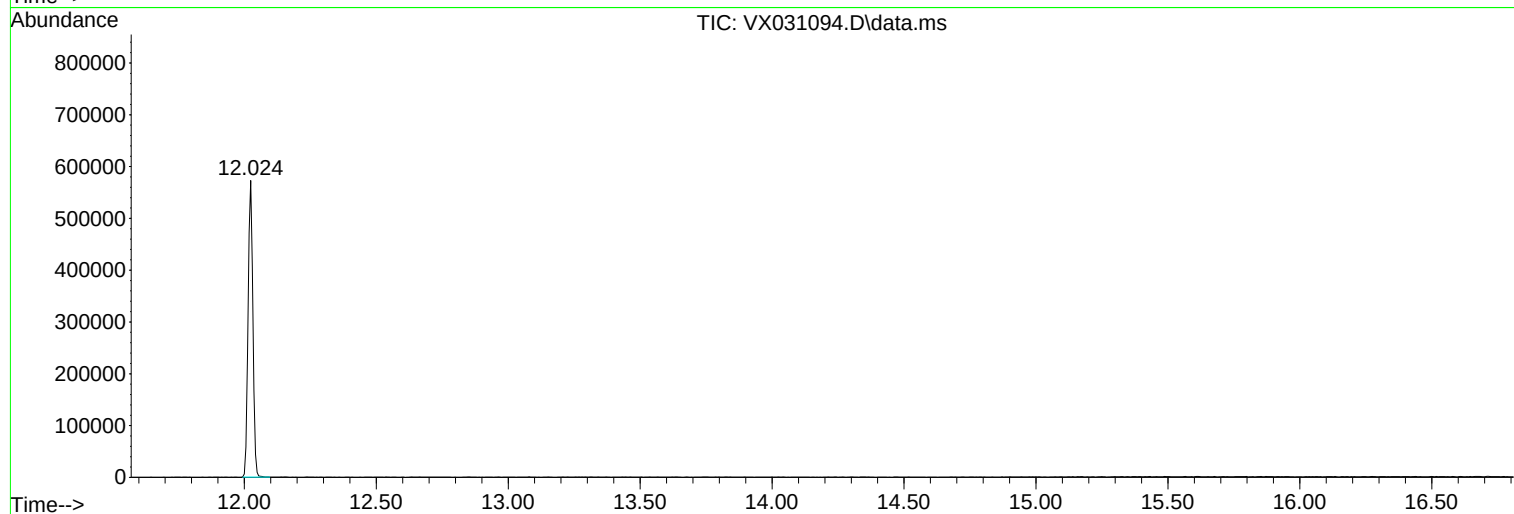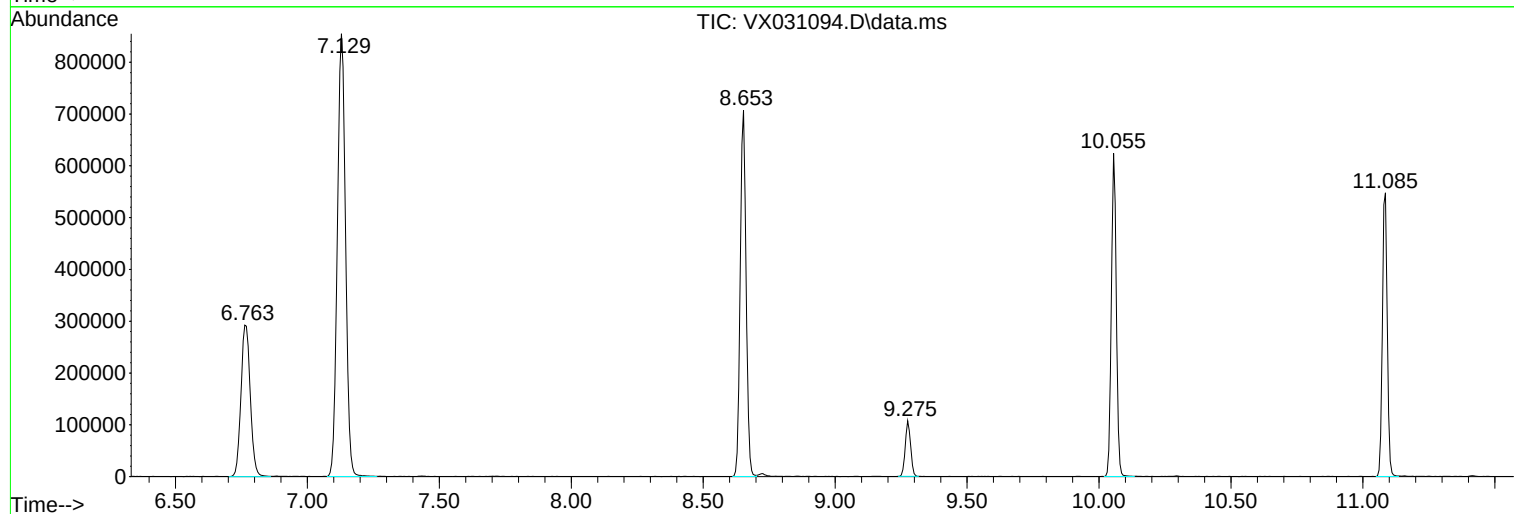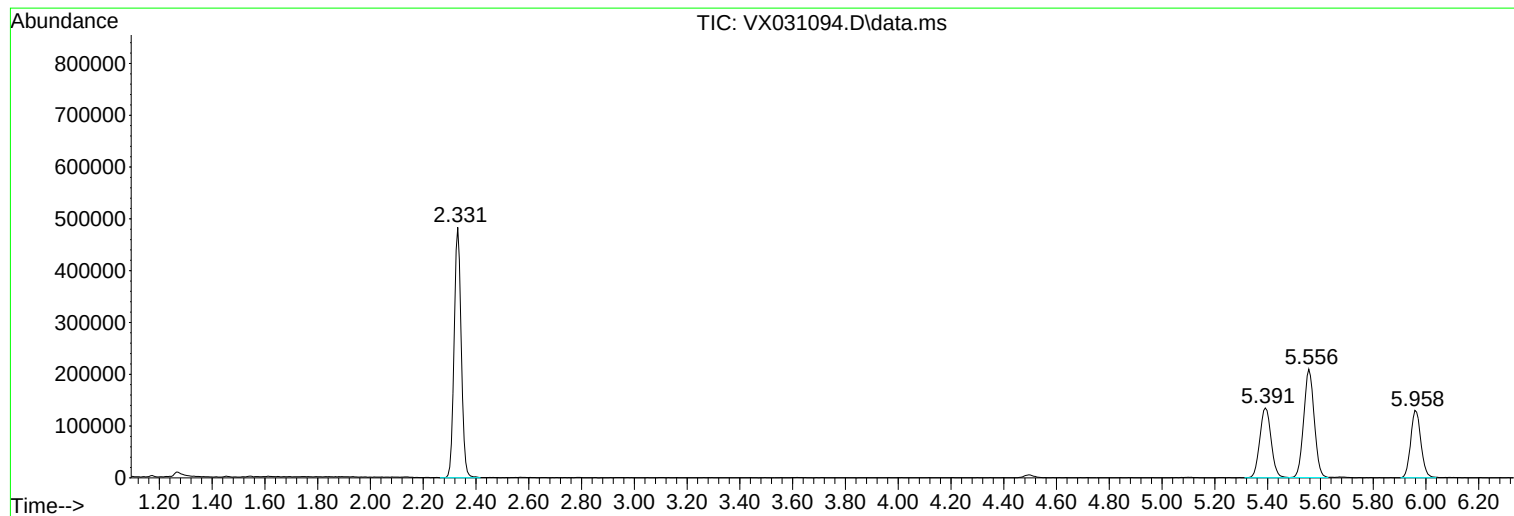

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031094.D
Acq On : 03 Sep 2022 19:47
Operator : JC/MD
Sample : N4357-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031094.D
Acq On : 03 Sep 2022 19:47
Operator : JC/MD
Sample : N4357-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------