

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031095.D
Acq On : 03 Sep 2022 20:11
Operator : JC/MD
Sample : N4357-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT150S1-20220823

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Title : SW846 8260

Signal : TIC: VX031095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	24	29	38	rBV2	9746	21751	1.94%	0.375%
2	5.391	694	706	720	rBV	141893	408561	36.51%	7.052%
3	5.556	722	733	746	rVB	212181	588516	52.60%	10.158%
4	5.958	787	799	813	rBV	133612	358909	32.08%	6.195%
5	6.763	918	931	942	rBV	297933	719800	64.33%	12.424%
6	7.135	983	992	1006	rVB2	76341	171794	15.35%	2.965%
7	8.653	1234	1241	1250	rBV	743537	1118909	100.00%	19.313%
8	9.275	1337	1343	1349	rBV2	12875	19001	1.70%	0.328%
9	10.055	1462	1471	1483	rBV	632904	839641	75.04%	14.492%
10	11.085	1634	1640	1649	rBV	603759	747632	66.82%	12.904%
11	12.024	1788	1794	1807	rBV	695637	799158	71.42%	13.794%




Sum of corrected areas: 5793672

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031095.D
Acq On : 03 Sep 2022 20:11
Operator : JC/MD
Sample : N4357-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT150S1-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

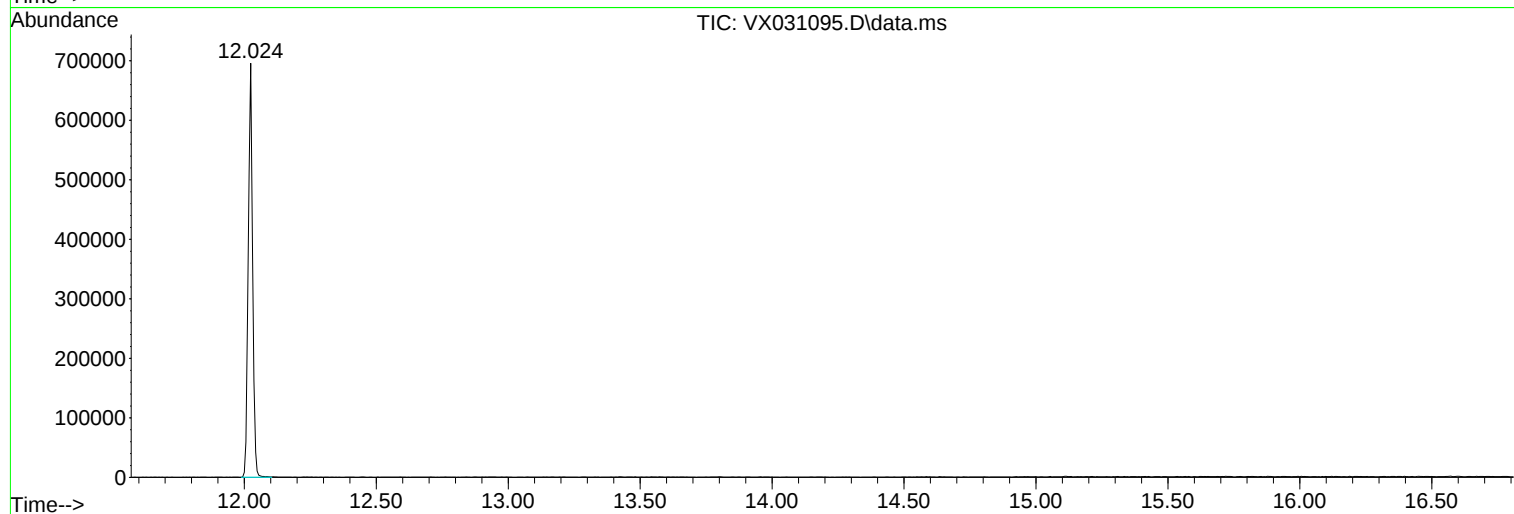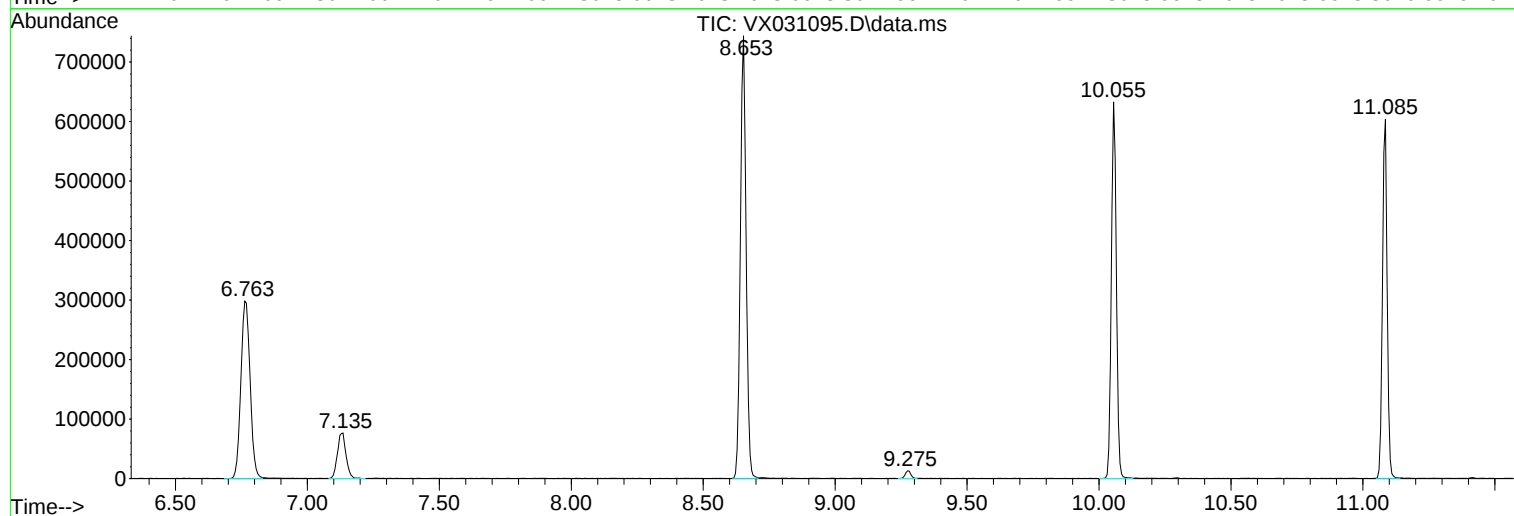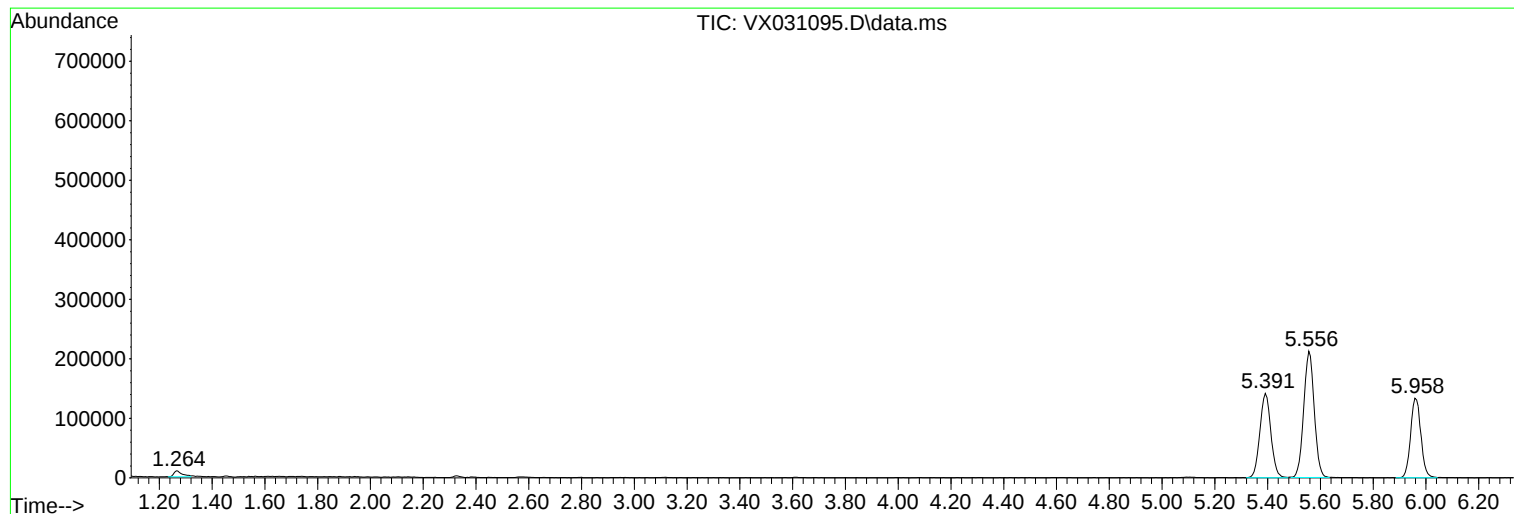

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031095.D
Acq On : 03 Sep 2022 20:11
Operator : JC/MD
Sample : N4357-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT150S1-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031095.D
Acq On : 03 Sep 2022 20:11
Operator : JC/MD
Sample : N4357-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT150S1-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------