

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
 Data File : VX031096.D
 Acq On : 03 Sep 2022 20:34
 Operator : JC/MD
 Sample : N4357-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TT180D1-20220823

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M

Title : SW846 8260

Signal : TIC: VX031096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	25	29	41	rBV	9895	22524	1.35%	0.309%
2	2.325	194	203	211	rBV3	18651	37950	2.27%	0.521%
3	5.391	693	706	719	rBV2	145746	423901	25.40%	5.815%
4	5.556	722	733	747	rVB2	216974	607989	36.43%	8.340%
5	5.964	787	800	812	rBV	137304	367903	22.05%	5.047%
6	6.763	922	931	946	rBV	307331	742429	44.49%	10.185%
7	7.129	979	991	1013	rBV	781520	1668766	100.00%	22.892%
8	8.653	1233	1241	1250	rBV	729391	1146327	68.69%	15.725%
9	10.055	1465	1471	1482	rBV	631621	833521	49.95%	11.434%
10	11.079	1634	1639	1648	rBV	560678	731515	43.84%	10.035%
11	12.024	1788	1794	1803	rBV	578843	706956	42.36%	9.698%




Sum of corrected areas: 7289781

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031096.D
Acq On : 03 Sep 2022 20:34
Operator : JC/MD
Sample : N4357-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D1-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

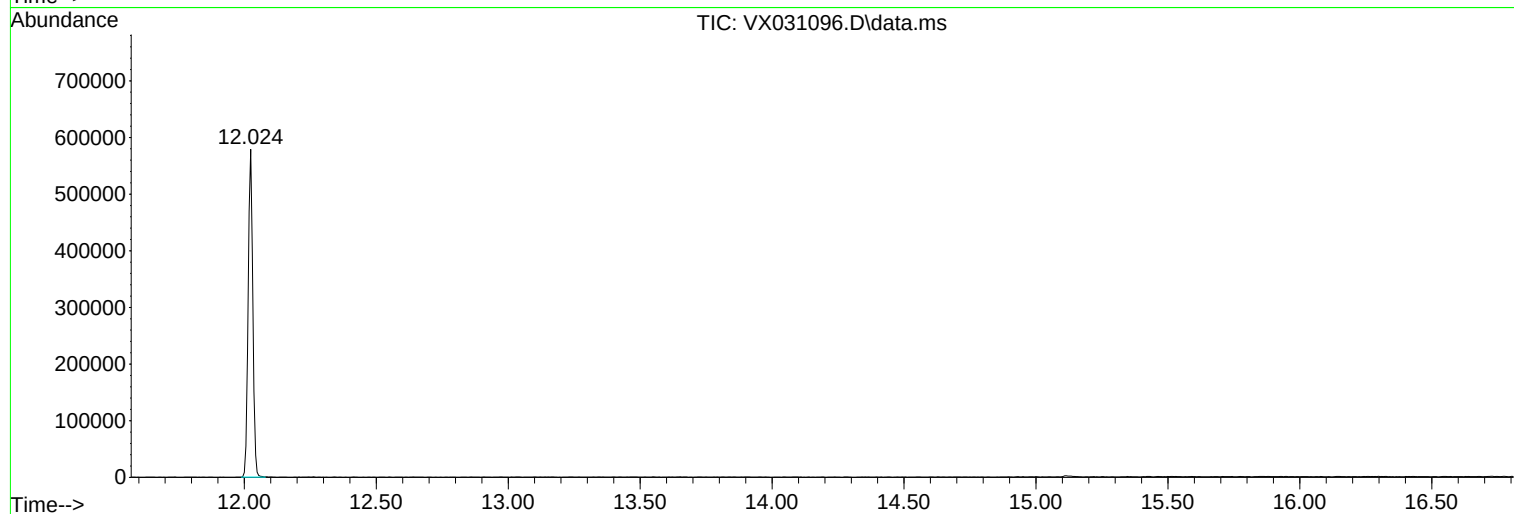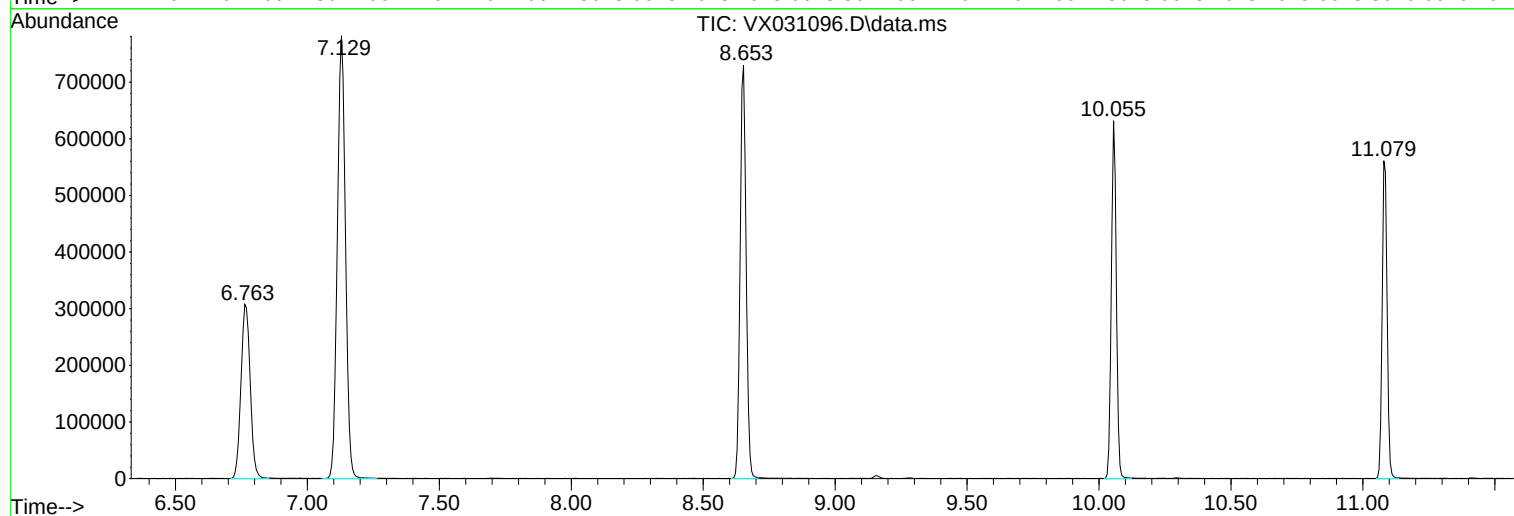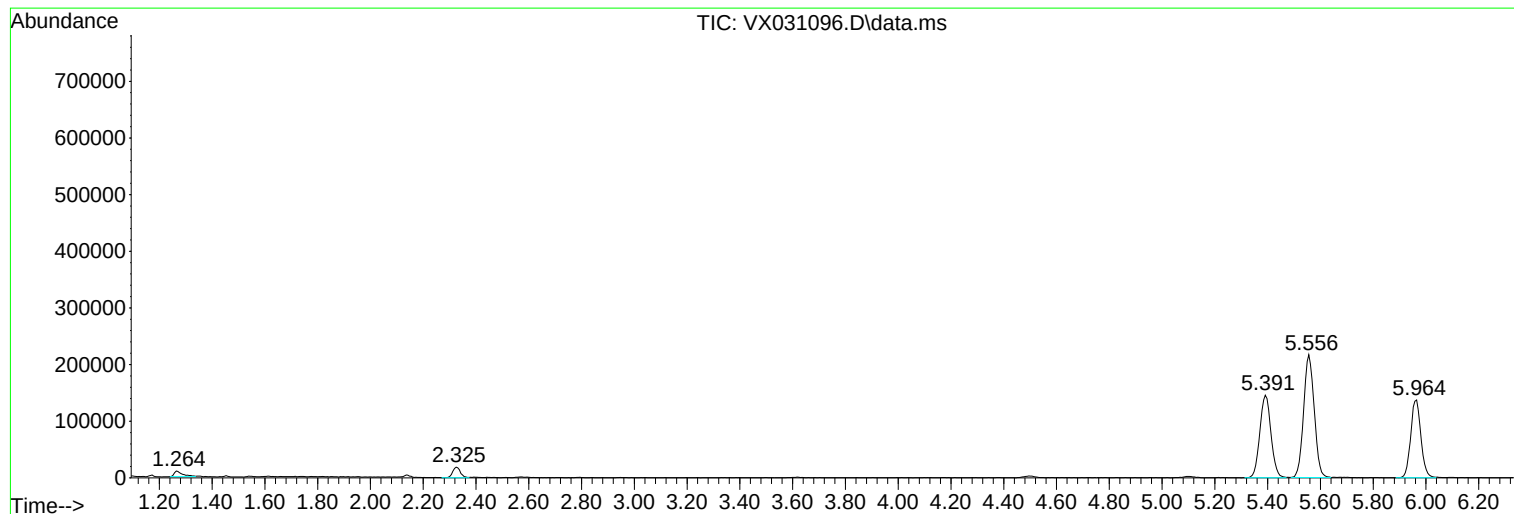

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031096.D
Acq On : 03 Sep 2022 20:34
Operator : JC/MD
Sample : N4357-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D1-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031096.D
Acq On : 03 Sep 2022 20:34
Operator : JC/MD
Sample : N4357-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D1-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------