

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
 Data File : VX031101.D
 Acq On : 03 Sep 2022 22:31
 Operator : JC/MD
 Sample : N4357-13 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE105D2-20220823

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M

Title : SW846 8260

Signal : TIC: VX031101.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	25	31	43	rBV4	5593	15717	1.46%	0.249%
2	2.947	295	305	312	rBV2	18907	45736	4.24%	0.726%
3	5.391	694	706	718	rBV	139135	396597	36.80%	6.293%
4	5.556	722	733	746	rVV2	211400	587569	54.52%	9.324%
5	5.964	789	800	814	rBV	127606	342852	31.81%	5.440%
6	6.763	922	931	943	rBV	302523	714161	66.27%	11.332%
7	7.129	982	991	1004	rBV	426511	911649	84.59%	14.466%
8	8.653	1234	1241	1251	rBV	694201	1077708	100.00%	17.101%
9	10.055	1465	1471	1485	rBV	620513	820160	76.10%	13.015%
10	11.085	1634	1640	1650	rBV	522803	691727	64.19%	10.977%
11	12.024	1788	1794	1803	rBV	572537	698012	64.77%	11.076%




Sum of corrected areas: 6301888

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031101.D
Acq On : 03 Sep 2022 22:31
Operator : JC/MD
Sample : N4357-13 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE105D2-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

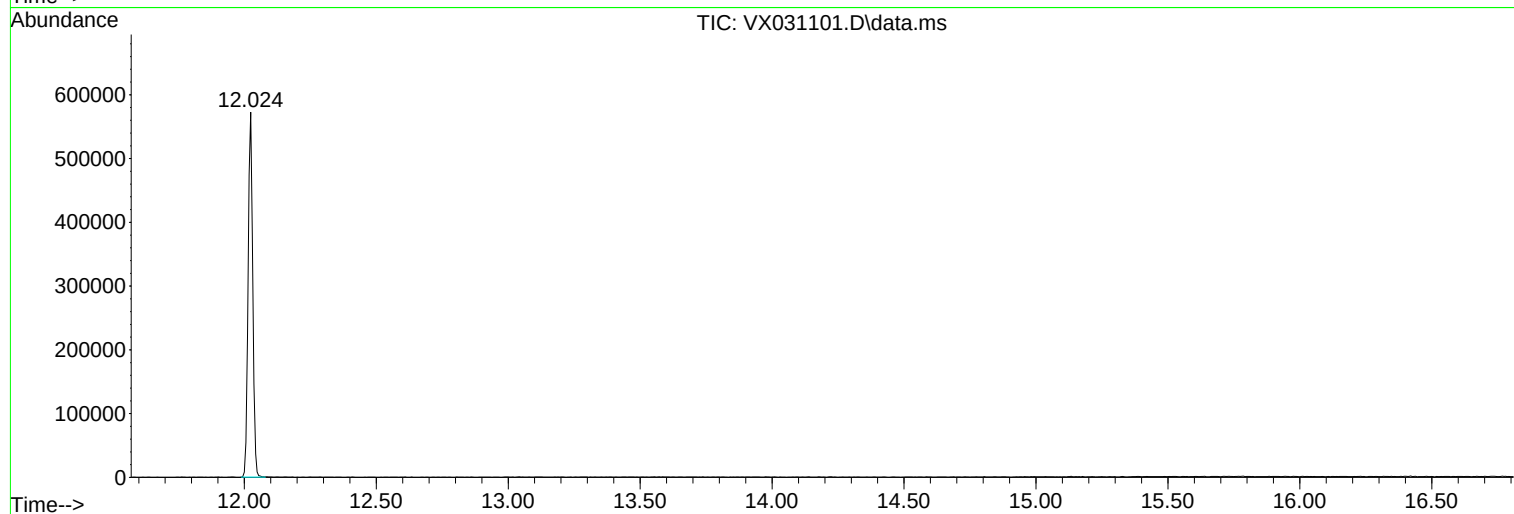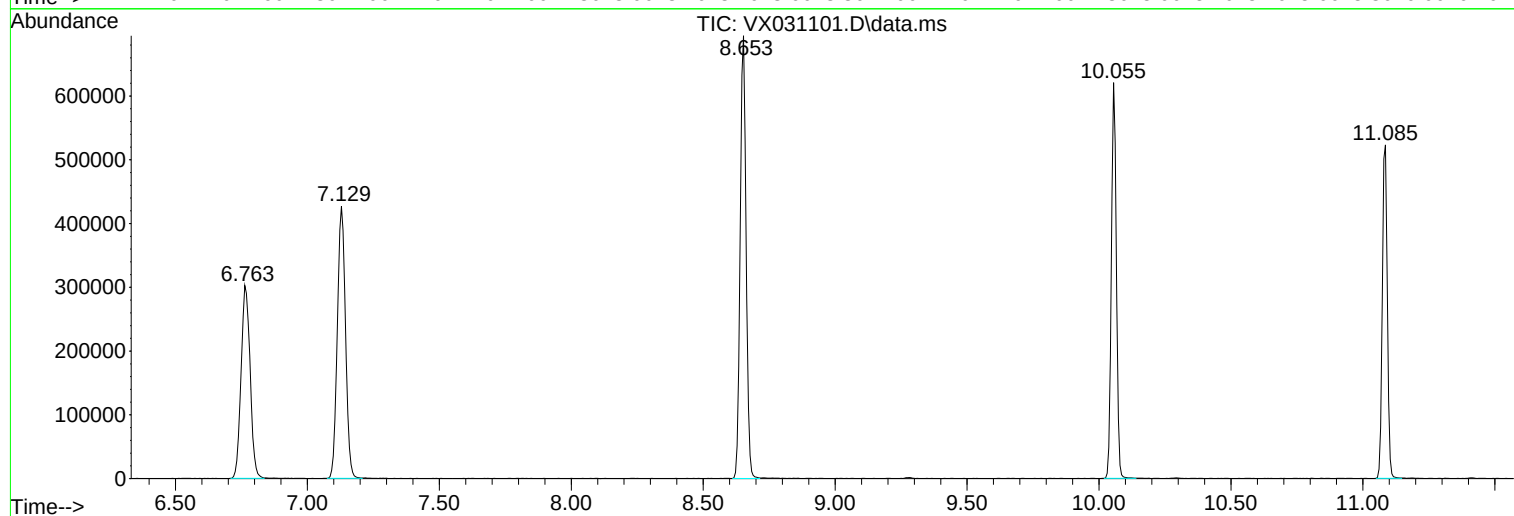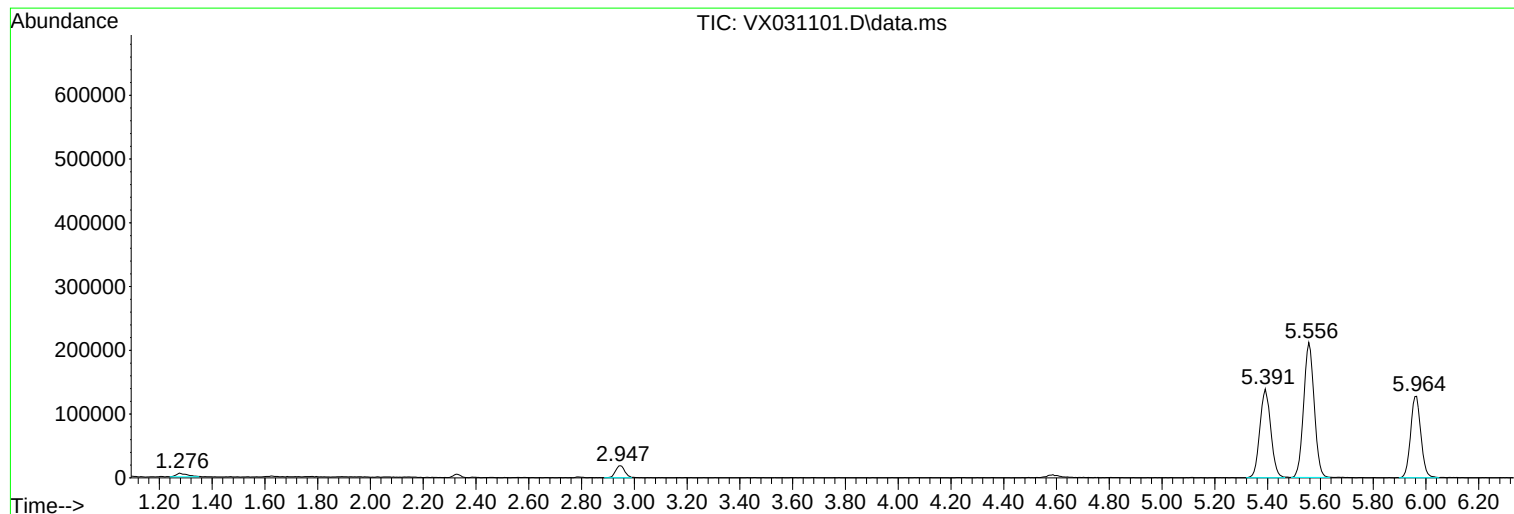

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031101.D
Acq On : 03 Sep 2022 22:31
Operator : JC/MD
Sample : N4357-13 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE105D2-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031101.D
Acq On : 03 Sep 2022 22:31
Operator : JC/MD
Sample : N4357-13 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE105D2-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------