
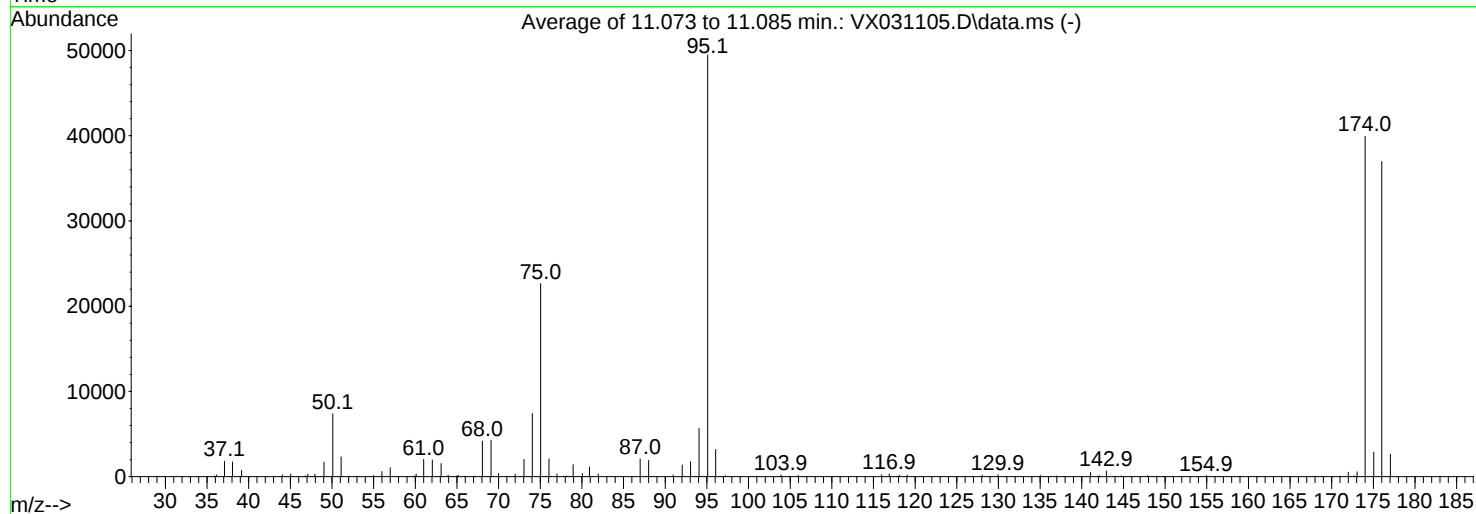


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090322\
Data File : VX031105.D
Acq On : 04 Sep 2022 00:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Title : SW846 8260
Last Update : Fri Sep 02 02:49:21 2022

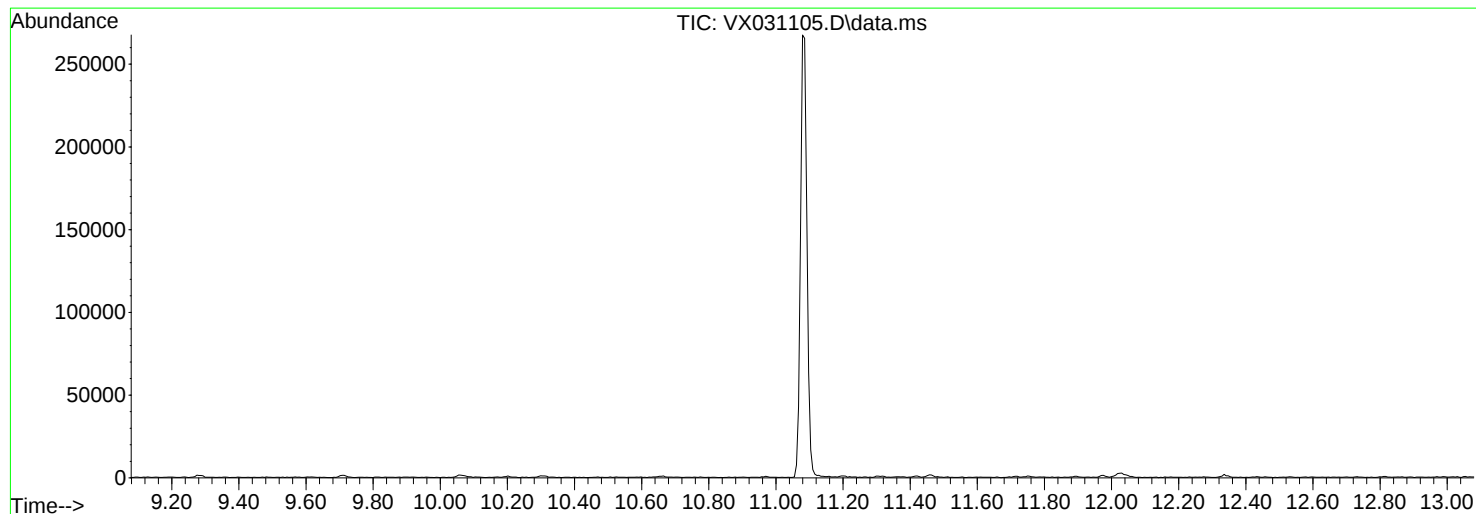

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	14.9	7382	FAIL*
75	95	30	60	45.8	22651	PASS
95	95	100	100	100.0	49491	PASS
96	95	5	9	6.4	3185	PASS
173	174	0.00	2	1.4	556	PASS
174	95	50	100	80.7	39939	PASS
175	174	5	9	7.2	2871	PASS
176	174	95	101	92.6	36981	FAIL*
177	176	5	9	7.1	2624	PASS