


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX090418\
 Data File : VX004338.D
 Acq On : 04 Sep 2018 10:43
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
 Title : SW846 8260
 Last Update : Thu Aug 23 05:39:44 2018

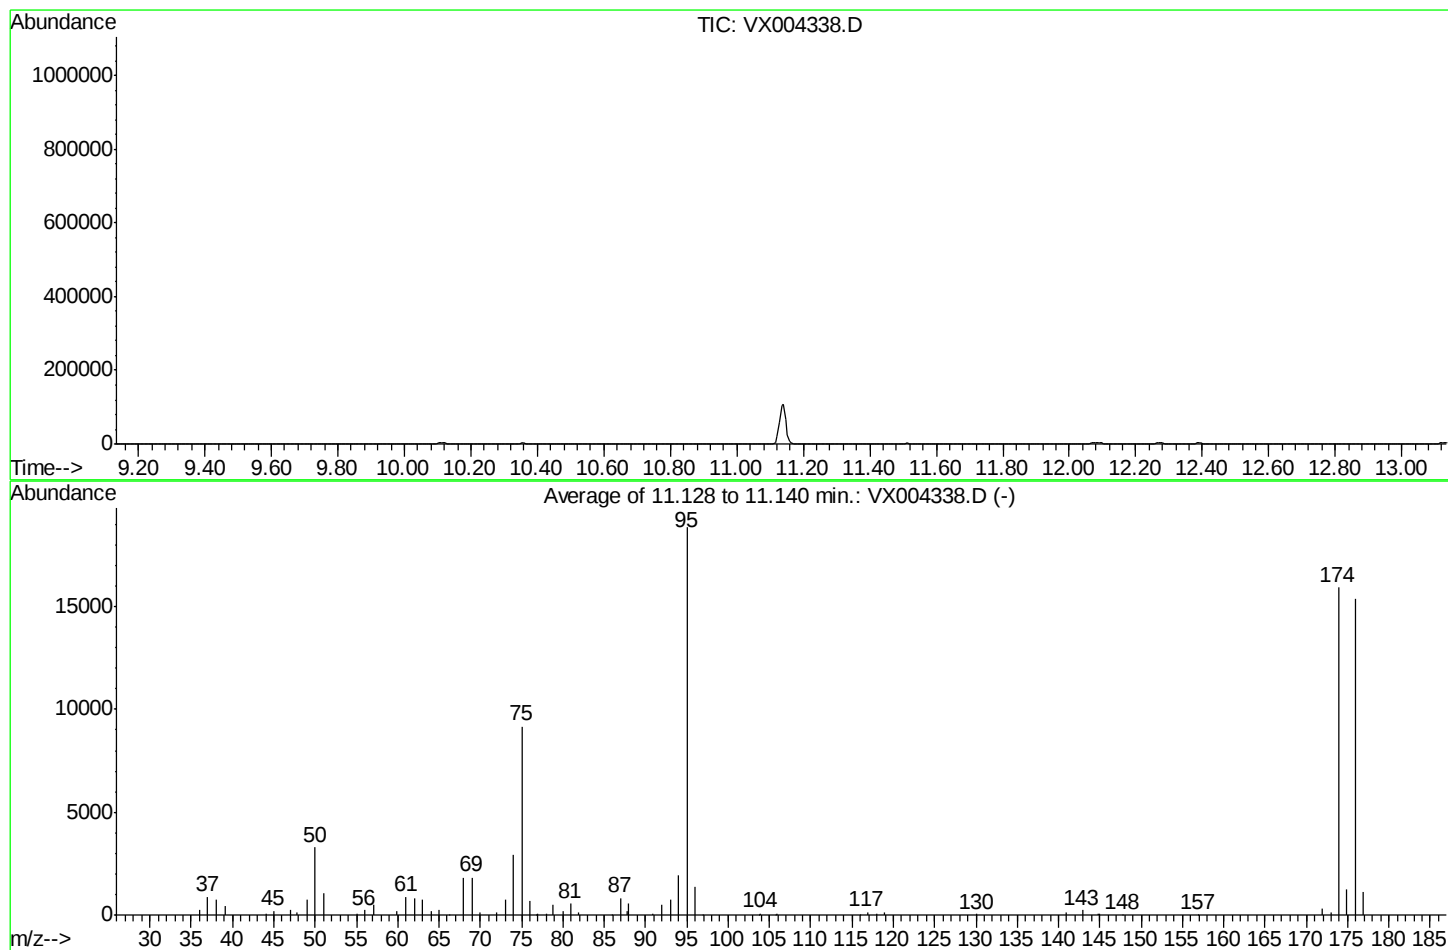

AutoFind: Scans 1729, 1730, 1731; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	3273	PASS
75	95	30	60	48.6	9164	PASS
95	95	100	100	100.0	18850	PASS
96	95	5	9	7.2	1351	PASS
173	174	0.00	2	0.9	141	PASS
174	95	50	100	84.5	15927	PASS
175	174	5	9	7.6	1216	PASS
176	174	95	101	96.4	15349	PASS
177	176	5	9	7.3	1115	PASS