


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX090419\
 Data File : VX012066.D
 Acq On : 04 Sep 2019 21:49
 Operator : SY/SP
 Sample : BFB
 Misc : 5.00µ/5.0mL/MSVOA X/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X090319S.M
 Title : SW846 8260
 Last Update : Tue Sep 03 15:26:48 2019

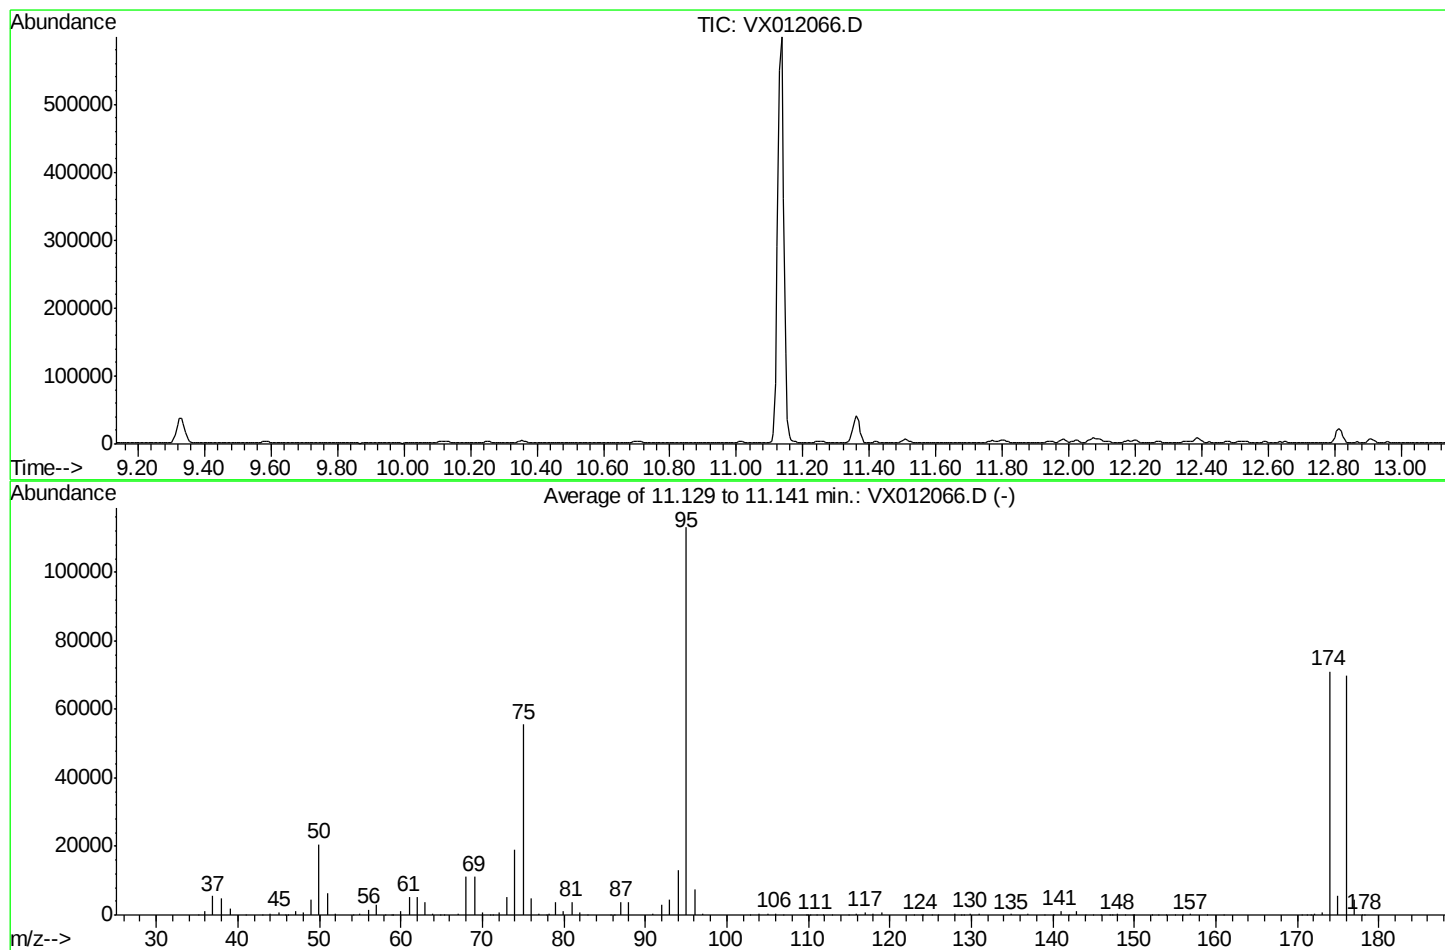

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	20554	PASS
75	95	30	60	49.1	55503	PASS
95	95	100	100	100.0	113133	PASS
96	95	5	9	6.6	7451	PASS
173	174	0.00	2	0.8	601	PASS
174	95	50	100	62.9	71154	PASS
175	174	5	9	7.9	5655	PASS
176	174	95	101	98.3	69920	PASS
177	176	5	9	6.4	4462	PASS