


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX090519\
 Data File : VX012091.D
 Acq On : 05 Sep 2019 10:24
 Operator : SY/SP
 Sample : BFB
 Misc : 5.00µ/5.0mL/MSVOA X/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X090319S.M
 Title : SW846 8260
 Last Update : Tue Sep 03 15:26:48 2019

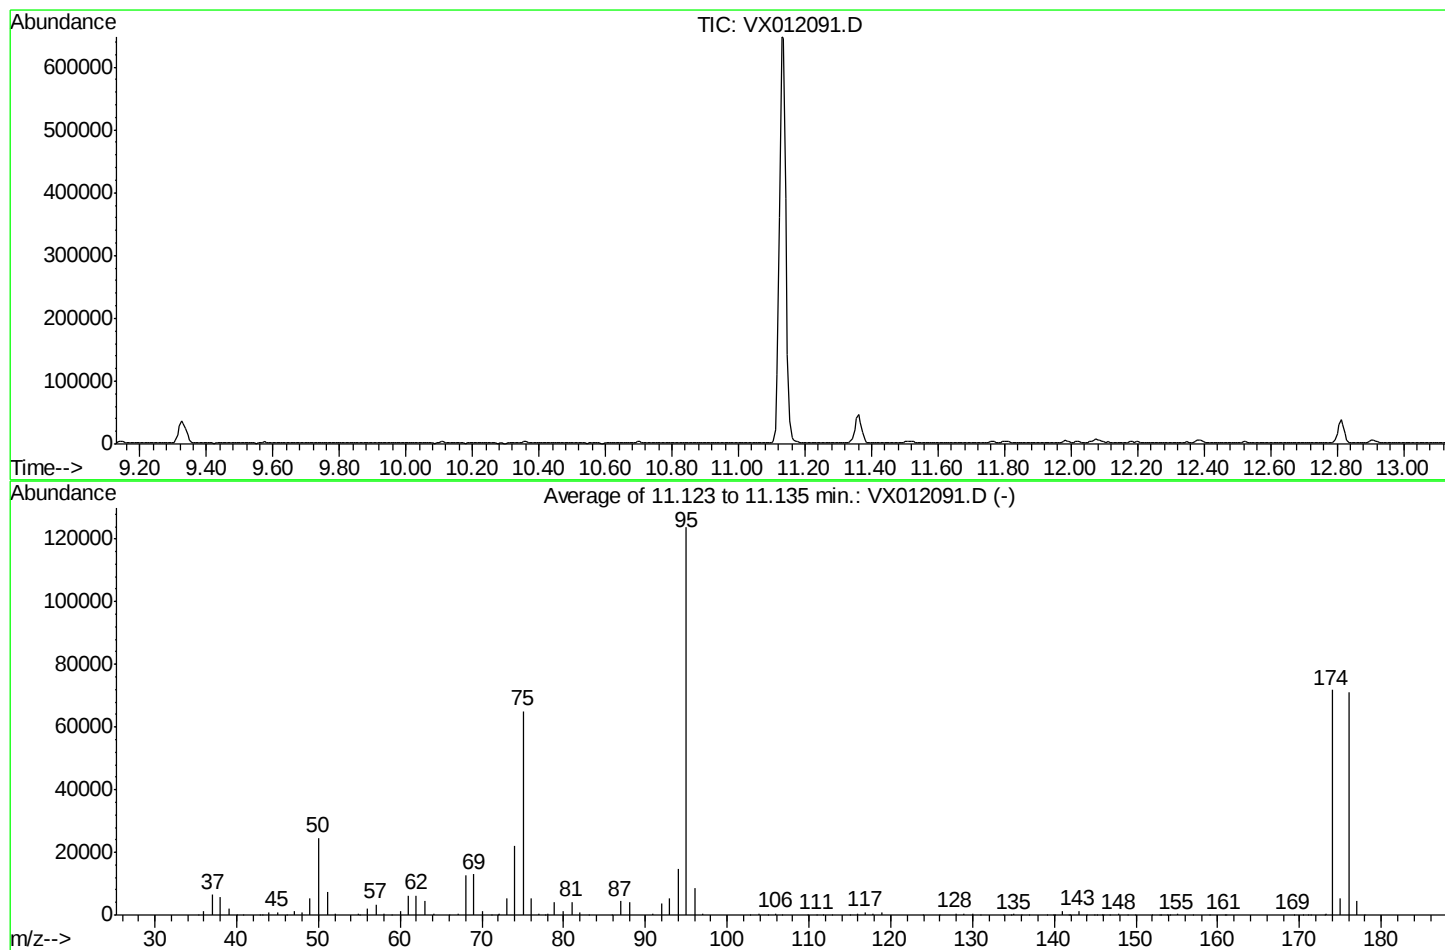

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	24621	PASS
75	95	30	60	52.5	64968	PASS
95	95	100	100	100.0	123746	PASS
96	95	5	9	6.9	8491	PASS
173	174	0.00	2	0.7	486	PASS
174	95	50	100	58.0	71754	PASS
175	174	5	9	7.7	5508	PASS
176	174	95	101	98.9	70957	PASS
177	176	5	9	6.4	4554	PASS