


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX090519\
 Data File : VX012117.D
 Acq On : 05 Sep 2019 23:11
 Operator : SY/SP
 Sample : BFB
 Misc : 5.00µ/5.0mL/MSVOA X/SOIL
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X090319S.M
 Title : SW846 8260
 Last Update : Tue Sep 03 15:26:48 2019

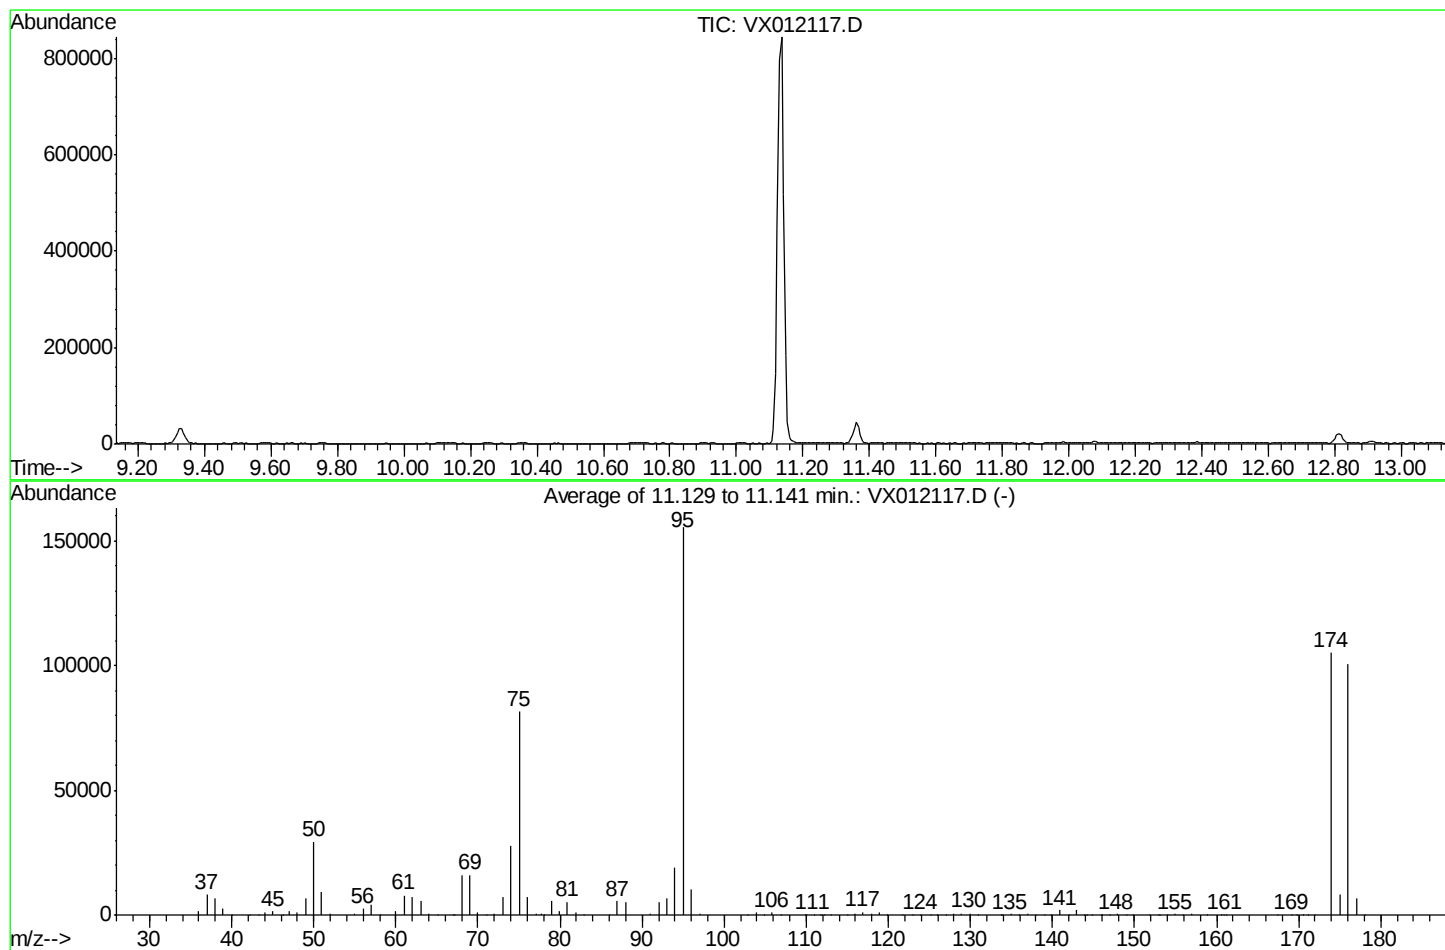

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	29378	PASS
75	95	30	60	52.4	81402	PASS
95	95	100	100	100.0	155333	PASS
96	95	5	9	6.6	10259	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	67.7	105085	PASS
175	174	5	9	8.1	8467	PASS
176	174	95	101	95.5	100338	PASS
177	176	5	9	6.7	6688	PASS